

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082118\
 Data File : BF108362.D
 Acq On : 22 Aug 2018 2:37
 Operator : JU/SJ
 Sample : J4275-11 5X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-01-082018-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.231	489	492	497	rVB	24166	24737	1.95%	0.220%
2	5.619	555	558	570	rBV	629522	591024	46.59%	5.248%
3	6.613	724	727	738	rBV	701949	643812	50.75%	5.717%
4	6.772	750	754	757	rBV	678938	640805	50.52%	5.690%
5	7.001	790	793	797	rBV	1078789	969748	76.45%	8.611%
6	7.160	816	820	823	rBV	578652	501318	39.52%	4.451%
7	7.560	884	888	895	rBV	463328	391889	30.89%	3.480%
8	8.289	1008	1012	1015	rBV	1380755	1199751	94.58%	10.653%
9	9.360	1190	1194	1201	rBV	806920	711632	56.10%	6.319%
10	9.748	1257	1260	1264	rBV	59338	52413	4.13%	0.465%
11	10.048	1307	1311	1315	rBV2	1431023	1268480	100.00%	11.263%
12	10.836	1442	1445	1455	rVB	327146	306595	24.17%	2.722%
13	11.542	1562	1565	1569	rBV	1163964	1083470	85.41%	9.620%
14	12.766	1769	1773	1776	rBV	31681	31995	2.52%	0.284%
15	12.995	1806	1812	1817	rBV	34275	43959	3.47%	0.390%
16	13.124	1831	1834	1838	rBV	593793	515990	40.68%	4.582%
17	13.371	1872	1876	1881	rVB4	15894	22887	1.80%	0.203%
18	13.807	1947	1950	1952	rBV	27265	24504	1.93%	0.218%
19	14.195	2012	2016	2019	rBV	1095117	1035073	81.60%	9.191%
20	14.218	2019	2020	2023	rVB	54039	44539	3.51%	0.395%
21	14.330	2037	2039	2044	rBV6	14110	17219	1.36%	0.153%
22	14.607	2083	2086	2089	rBV	44031	45707	3.60%	0.406%
23	15.013	2152	2155	2158	rBV	43230	58059	4.58%	0.516%
24	15.042	2158	2160	2166	rVB	71197	77621	6.12%	0.689%
25	15.324	2206	2208	2212	rVB3	43862	43472	3.43%	0.386%
26	15.754	2275	2281	2287	rVB	620739	847556	66.82%	7.526%
27	16.207	2355	2358	2364	rVB	44424	68054	5.37%	0.604%


Sum of corrected areas: 11262309

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082118\
Data File : BF108362.D
Acq On : 22 Aug 2018 2:37
Operator : JU/SJ
Sample : J4275-11 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-082018-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

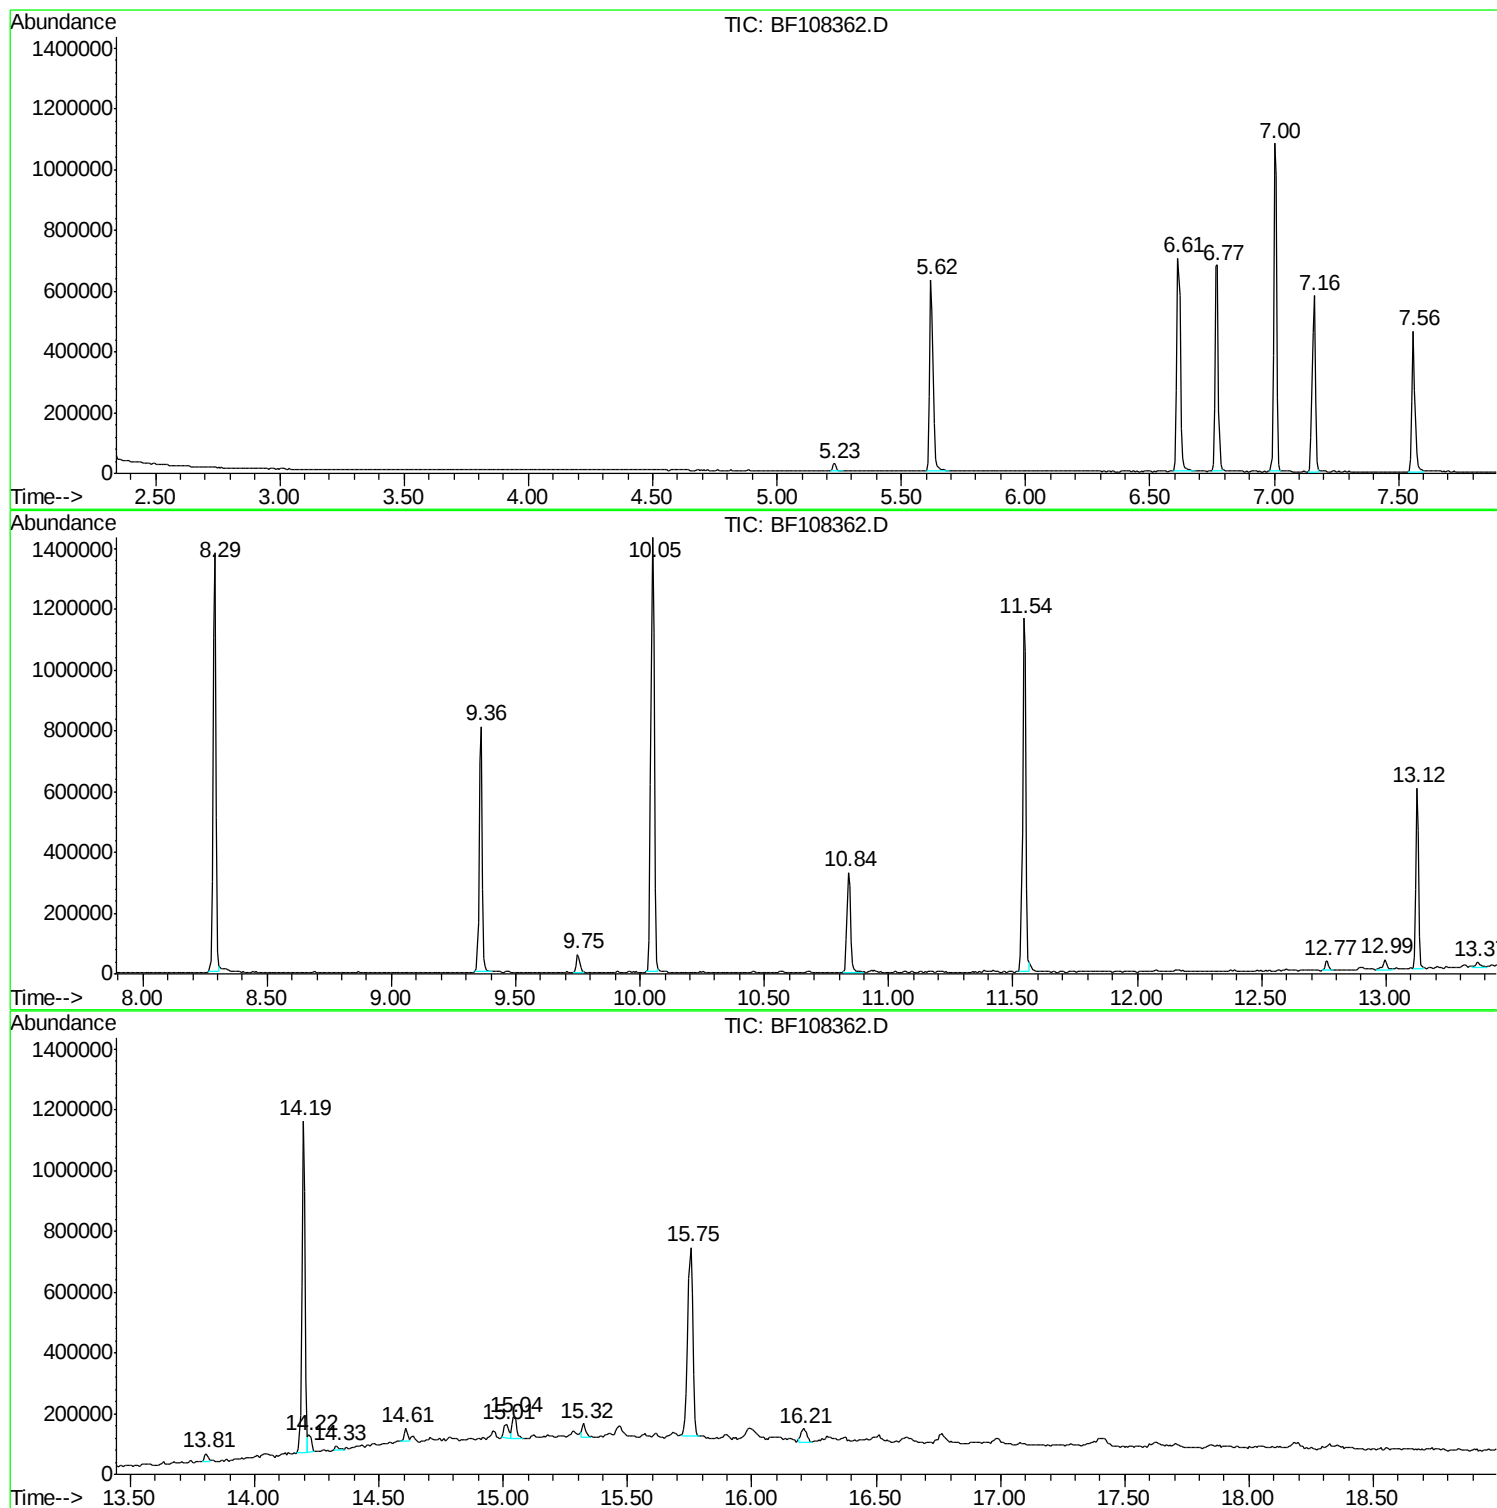

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082118\
Data File : BF108362.D
Acq On : 22 Aug 2018 2:37
Operator : JU/SJ
Sample : J4275-11 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-082018-B










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.77 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.77	13.22 ng	640805	1,4-Dichlorobenzene-d4	7.00

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	10
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

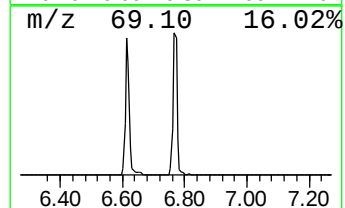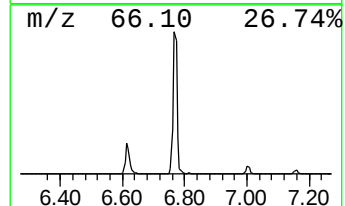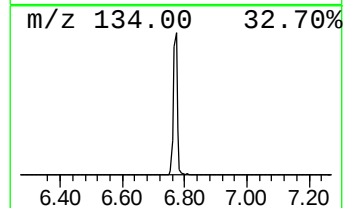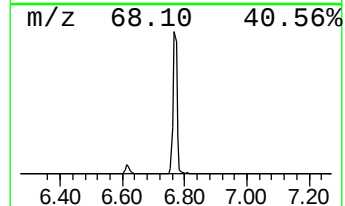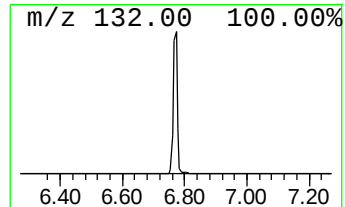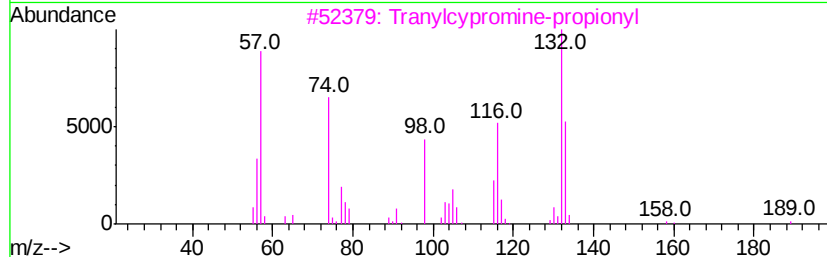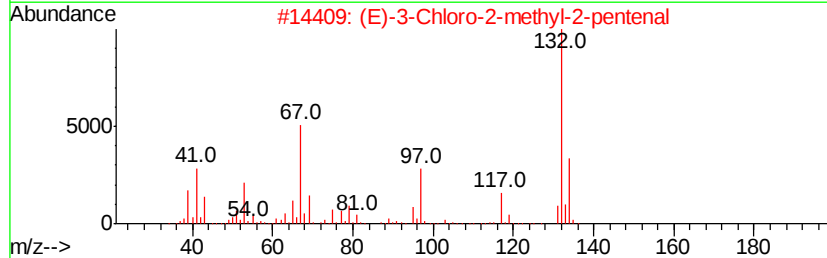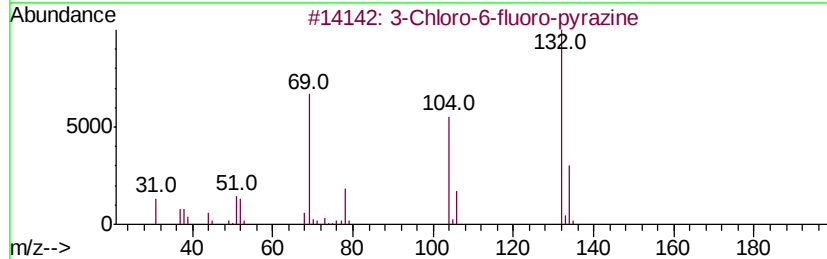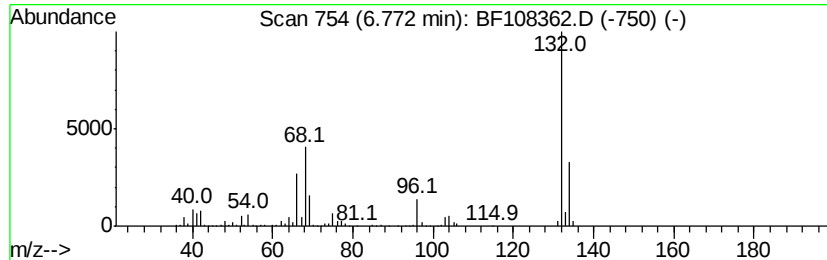

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082118\
Data File : BF108362.D
Acq On : 22 Aug 2018 2:37
Operator : JU/SJ
Sample : J4275-11 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-082018-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.77	6.77	13.2	ng	640805	1	7.00	969748	20.0