


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082118\
Data File : BF108325.D
Acq On : 21 Aug 2018 8:25
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 22 11:01:45 2018

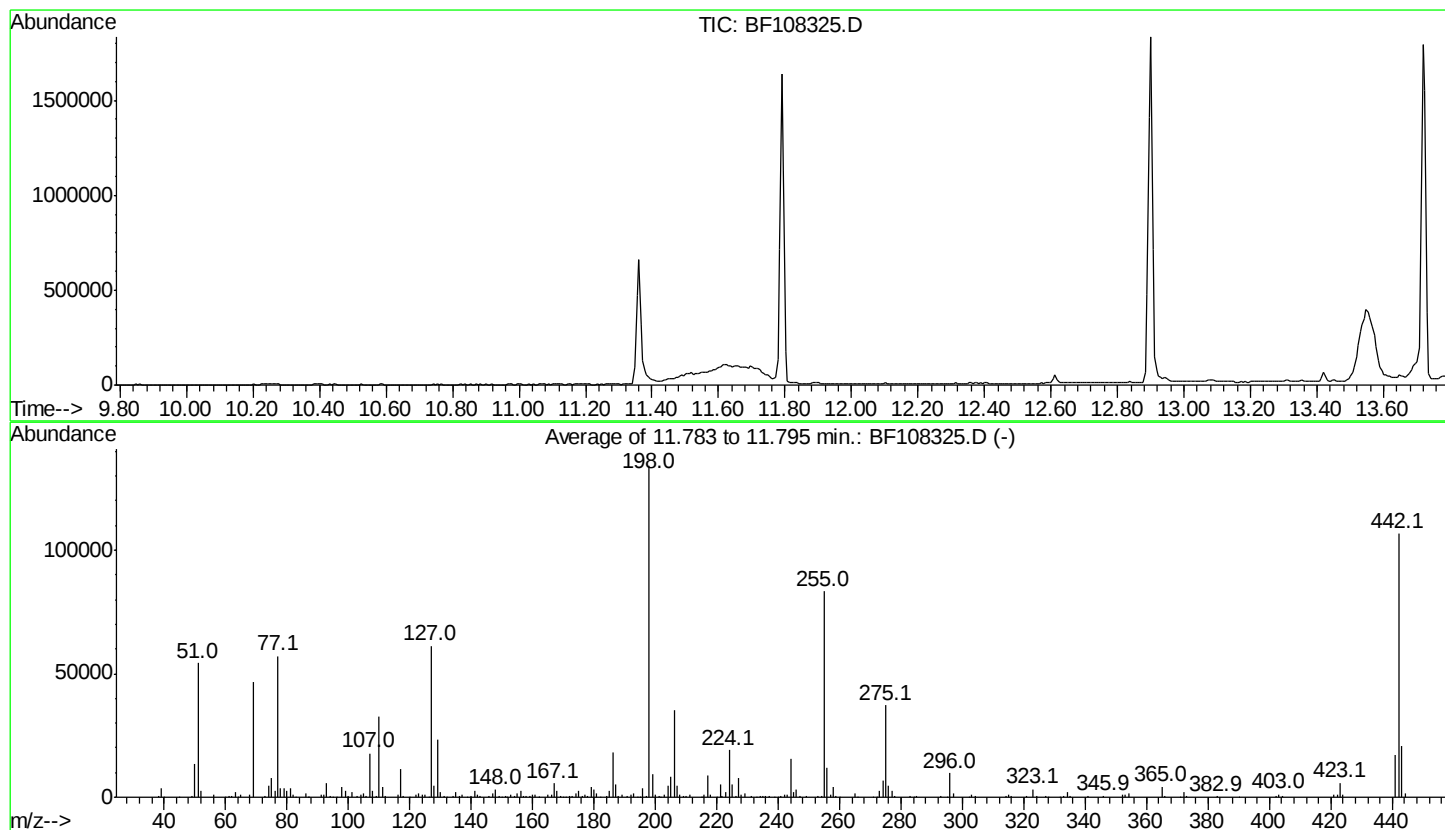

AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	54173	PASS
68	69	0.00	2	1.8	841	PASS
69	198	0.00	100	34.9	46822	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.6	61168	PASS
197	198	0.00	2	0.4	523	PASS
198	198	100	100	100.0	134197	PASS
199	198	5	9	6.9	9246	PASS
275	198	10	60	27.7	37216	PASS
365	198	1	100	3.3	4416	PASS
441	198	0.01	100	12.9	17318	PASS
442	198	50	100	79.4	106597	PASS
443	442	15	24	19.4	20681	PASS