


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082118\
Data File : BF108342.D
Acq On : 21 Aug 2018 17:00
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 22 11:01:45 2018

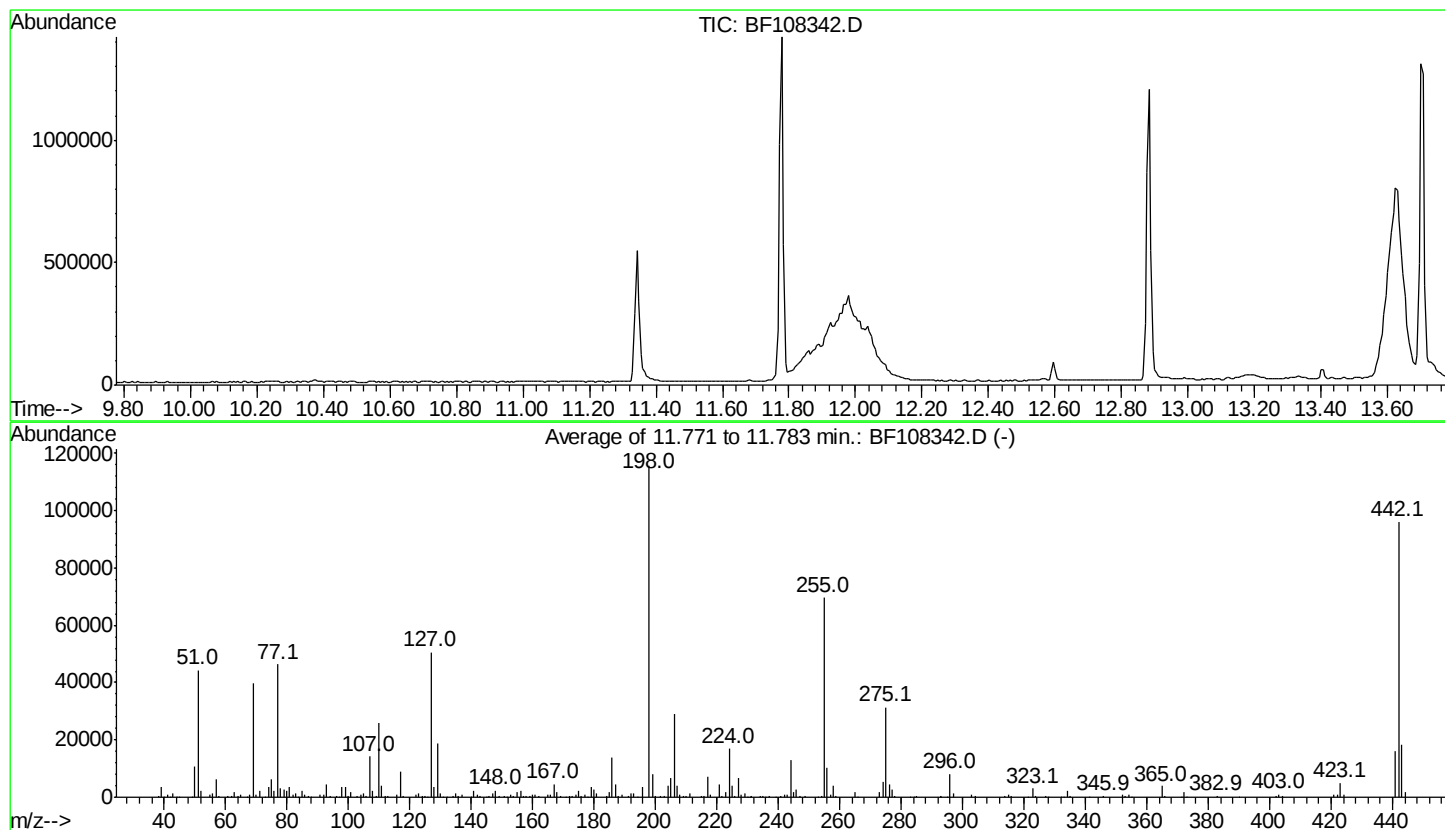

AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	44269	PASS
68	69	0.00	2	1.9	755	PASS
69	198	0.00	100	34.2	39605	PASS
70	69	0.00	2	1.9	753	PASS
127	198	10	80	43.7	50608	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	115712	PASS
199	198	5	9	6.8	7907	PASS
275	198	10	60	27.1	31373	PASS
365	198	1	100	3.4	3963	PASS
441	198	0.01	100	13.8	15976	PASS
442	198	50	100	83.0	96042	PASS
443	442	15	24	18.9	18147	PASS