


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082118\
 Data File : BF108368.D
 Acq On : 22 Aug 2018 5:21
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 22 11:01:45 2018

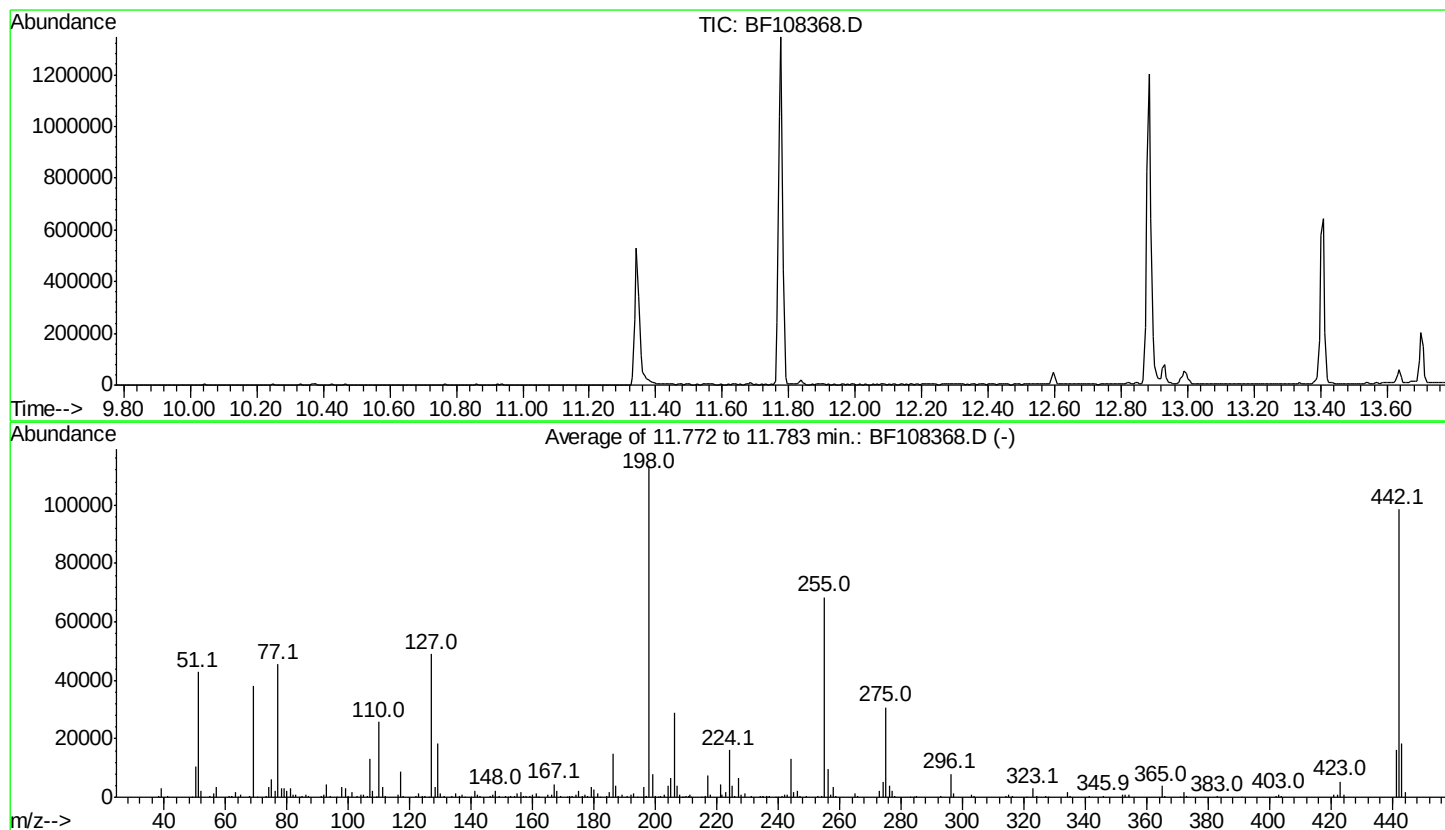

AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	42753	PASS
68	69	0.00	2	1.3	508	PASS
69	198	0.00	100	33.7	38245	PASS
70	69	0.00	2	0.3	109	PASS
127	198	10	80	43.1	48941	PASS
197	198	0.00	2	0.4	473	PASS
198	198	100	100	100.0	113536	PASS
199	198	5	9	6.9	7791	PASS
275	198	10	60	27.1	30821	PASS
365	198	1	100	3.4	3867	PASS
441	198	0.01	100	14.4	16346	PASS
442	198	50	100	86.8	98573	PASS
443	442	15	24	18.8	18498	PASS