

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF082120\
 Data File : BF121364.D
 Acq On : 21 Aug 2020 12:38
 Operator : JU/CG
 Sample : PB131046BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB131046BL

Quant Time: Aug 21 13:04:26 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF081920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 20 04:56:10 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.69	152	179303	20.00	ng	0.00
21) Naphthalene-d8	7.97	136	689822	20.00	ng	0.00
39) Acenaphthene-d10	9.73	164	358257	20.00	ng	0.00
64) Phenanthrene-d10	11.21	188	681698	20.00	ng	0.00
76) Chrysene-d12	13.85	240	568516	20.00	ng	0.00
86) Perylene-d12	15.26	264	552248	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	1076196	98.42	ng	0.02
7) Phenol-d6	6.35	99	1315673	94.25	ng	0.00
23) Nitrobenzene-d5	7.26	82	921980	75.59	ng	0.00
42) 2,4,6-Tribromophenol	10.52	330	377190	90.35	ng	0.00
45) 2-Fluorobiphenyl	9.06	172	1517520	80.65	ng	0.00
79) Terphenyl-d14	12.80	244	1546997	53.17	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.26	70	120286	16.022	ng	# 78
25) Isophorone	7.26	82	920816	41.484	ng	# 65
50) Dimethylphthalate	9.73	163	75746	2.906	ng	# 1
51) 2,6-Dinitrotoluene	9.73	165	45528	8.179	ng	# 29
57) 2,4-Dinitrotoluene	9.73	165	45528	6.704	ng	# 24
58) Fluorene	10.52	166	13997	Below Cal		# 89
67) 4-Bromophenyl-phenylether	10.52	248	21166	2.799	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF082120\
Data File : BF121364.D
Acq On : 21 Aug 2020 12:38
Operator : JU/CG
Sample : PB131046BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB131046BL

Quant Time: Aug 21 13:04:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF081920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 20 04:56:10 2020
Response via : Initial Calibration

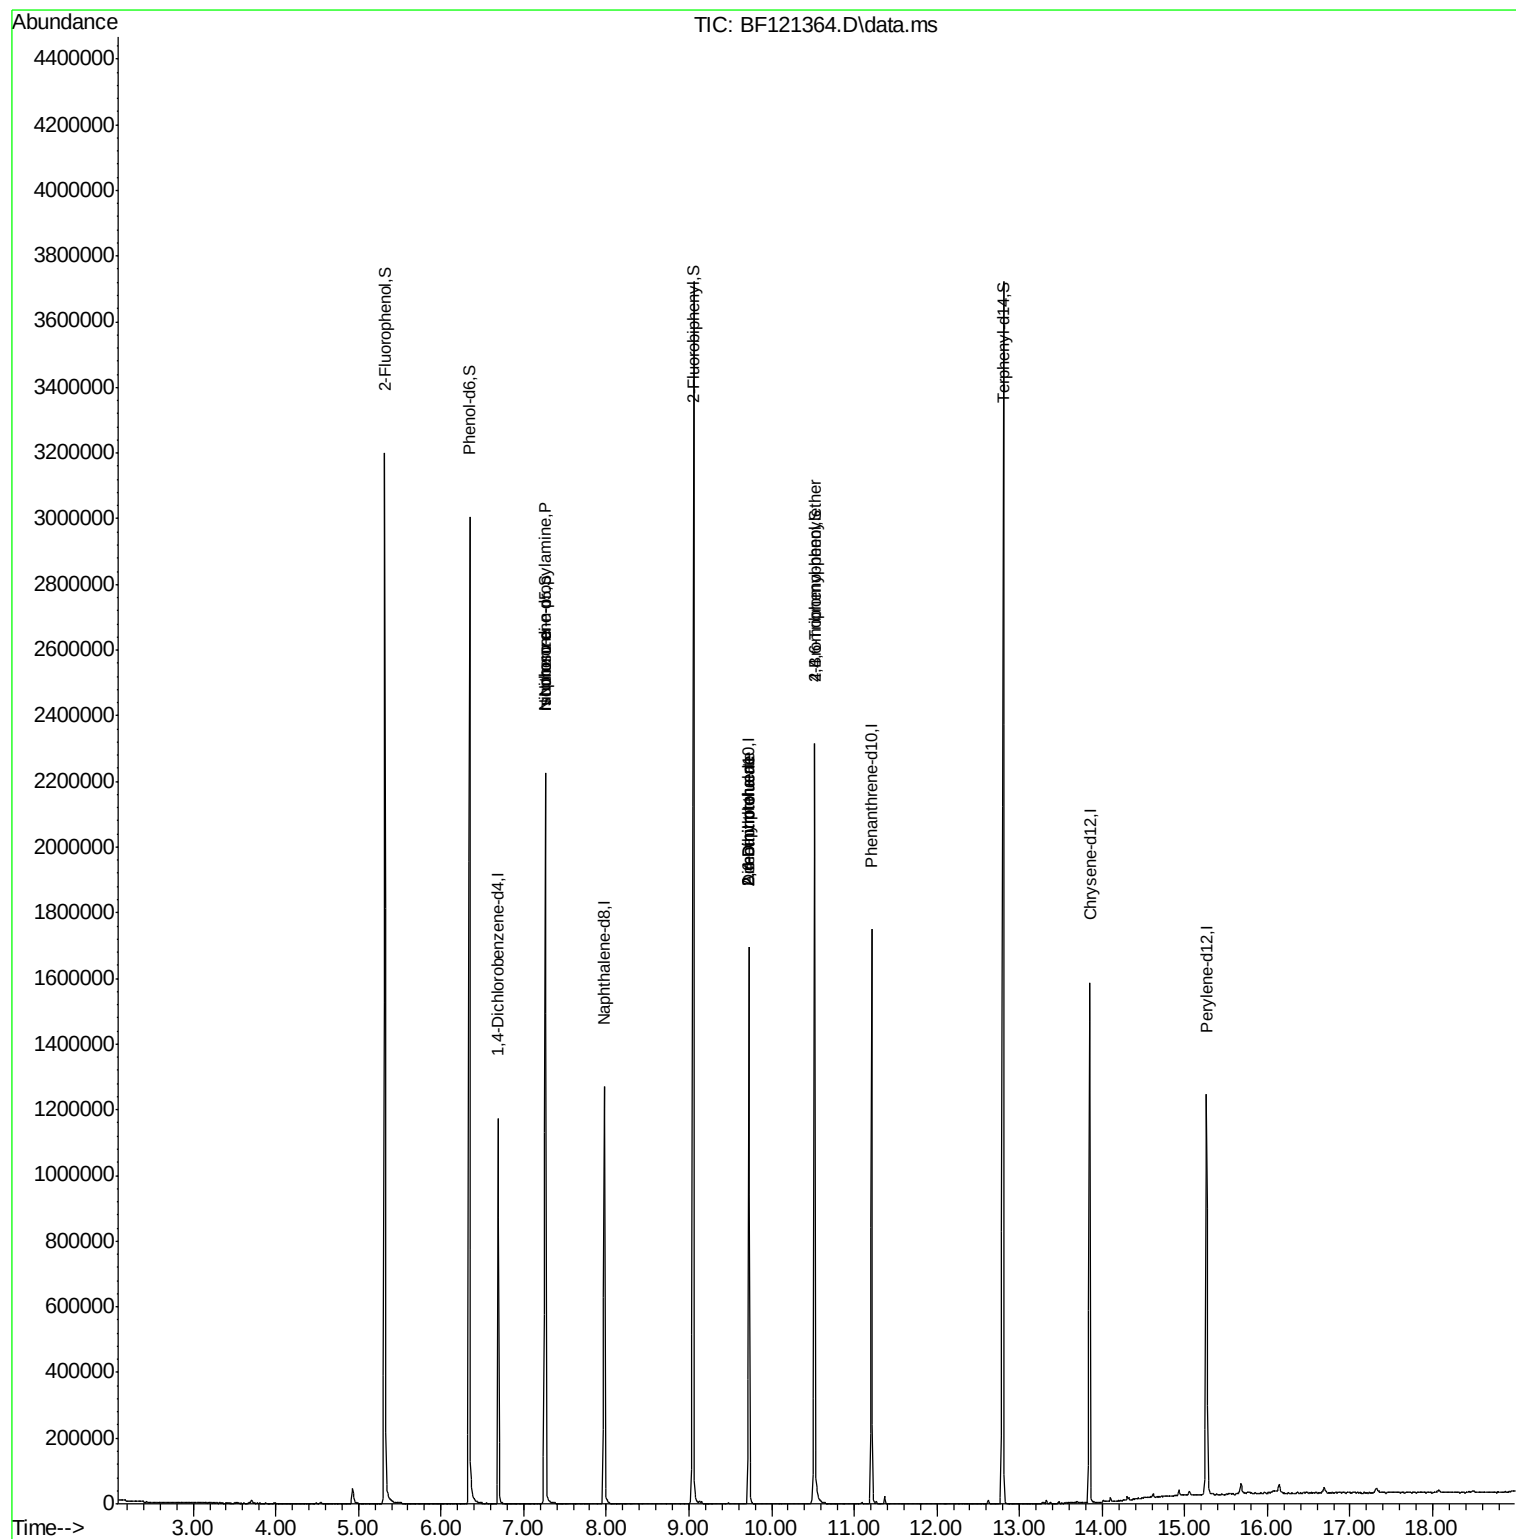

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

Instrument :

BNA_F

ClientSampleId :

PB131046BL