
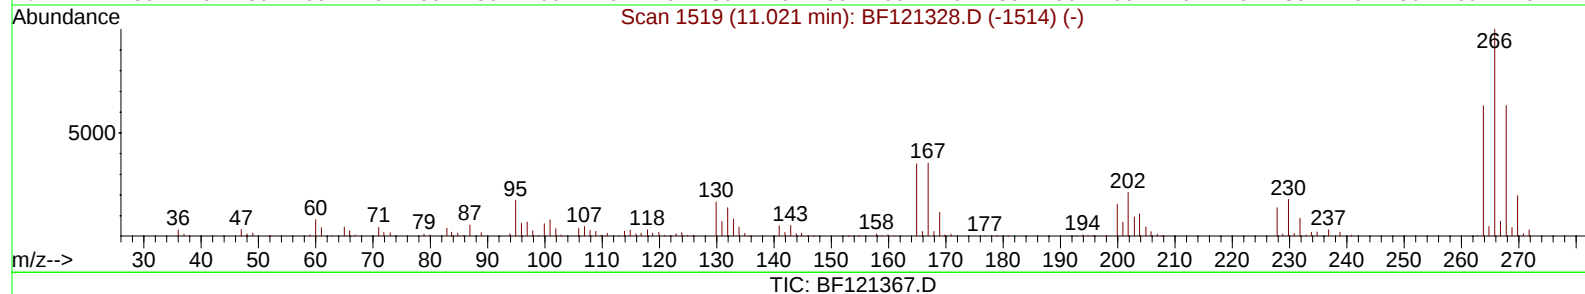
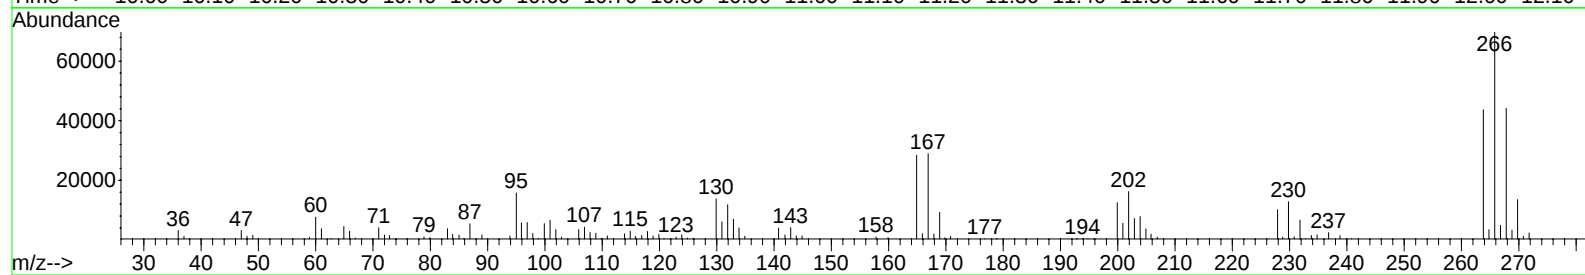


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082120\
Data File : BF121367.D
Acq On : 21 Aug 2020 14:47
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 18:46:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF081920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 20 04:56:10 2020
Response via : Initial Calibration

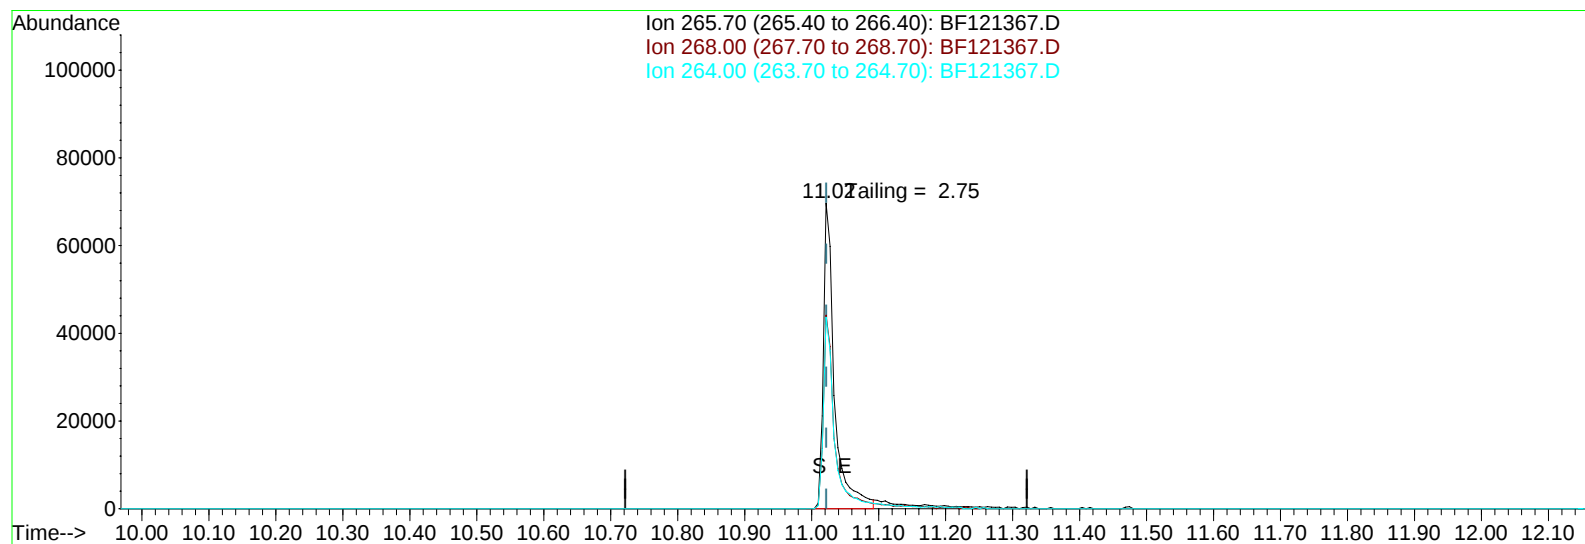

(70) Pentachlorophenol (C)




11.021min (-0.000) 104455.65ng

response 85572

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	63.31
264.00	63.10	62.66
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082120\
 Data File : BF121367.D
 Acq On : 21 Aug 2020 14:47
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 18:46:24 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF081920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 20 04:56:10 2020
 Response via : Initial Calibration

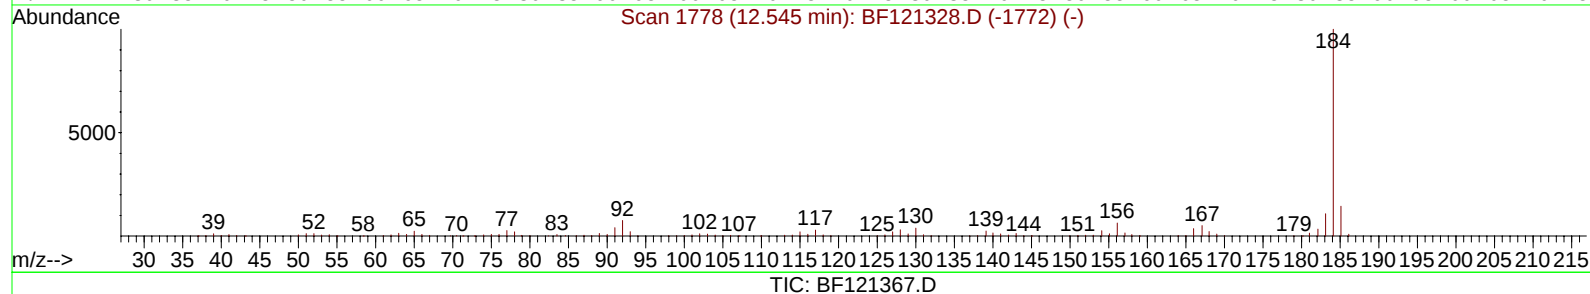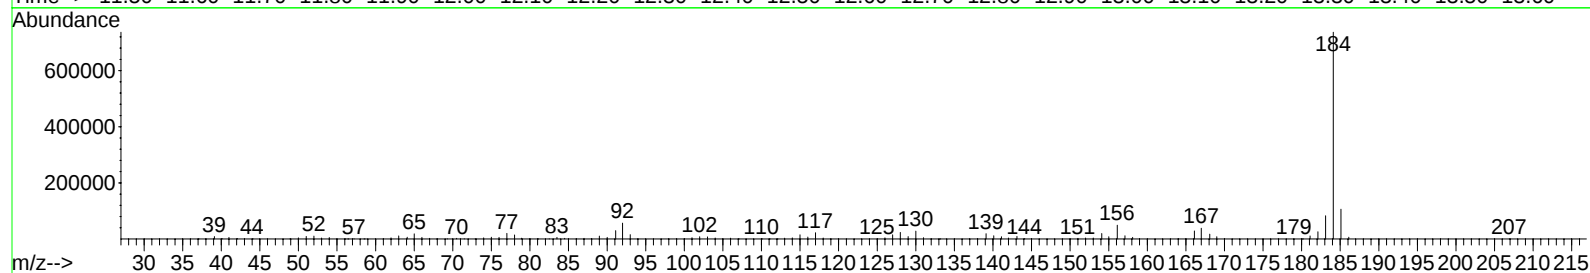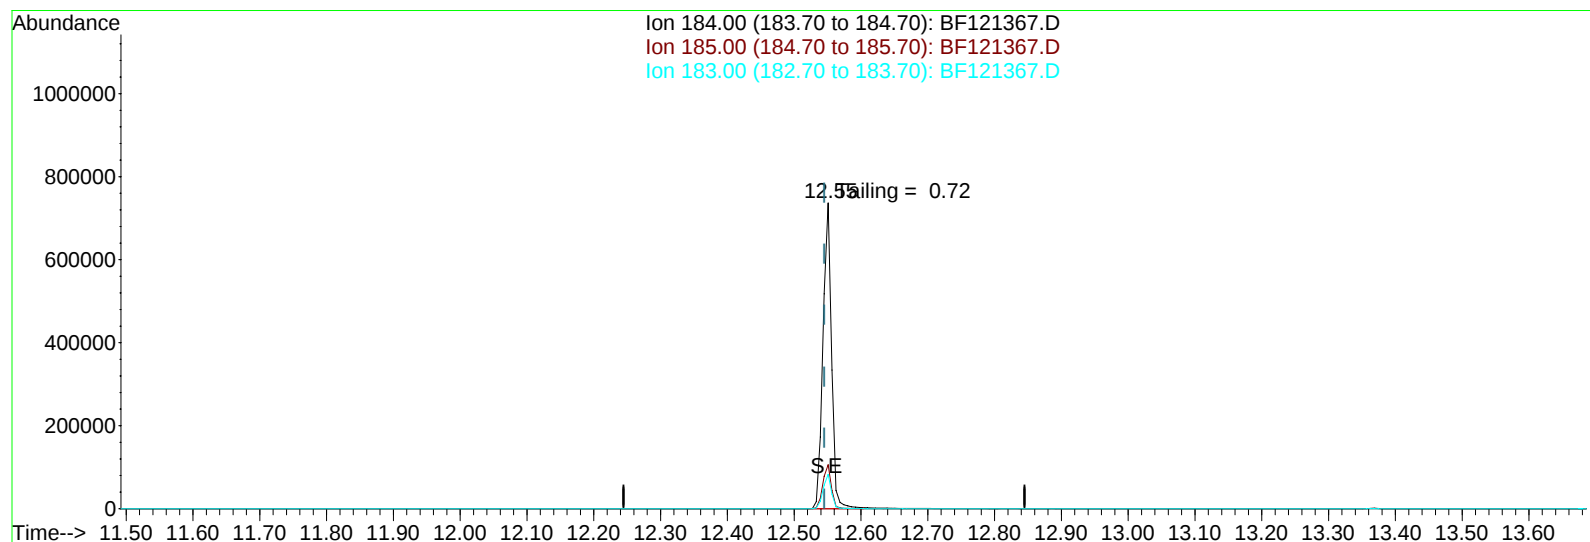

(77) Benzidine

12.551min (+0.006) 0.00ng

response 666278

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	14.40
183.00	10.90	11.24
0.00	0.00	0.00