

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082120\
 Data File : BF121372.D
 Acq On : 21 Aug 2020 17:42
 Operator : JU/CG
 Sample : L3719-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 20200507-DISCRETE-005

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.898	475	478	489	rVB	38758	52723	1.83%	0.224%
2	5.310	543	548	564	rBV	2517854	2536710	88.09%	10.783%
3	6.339	718	723	740	rBV	2441751	2597758	90.21%	11.042%
4	6.533	753	756	767	rBV	27239	42147	1.46%	0.179%
5	6.692	779	783	793	rVB	1187913	935812	32.50%	3.978%
6	7.257	874	879	891	rBV	1691399	1790242	62.17%	7.610%
7	7.975	997	1001	1016	rBV	1425316	1249741	43.40%	5.312%
8	9.051	1179	1184	1187	rBV	3063851	2879532	100.00%	12.240%
9	9.445	1247	1251	1258	rBV	367925	294058	10.21%	1.250%
10	9.663	1283	1288	1294	rBV3	15203	29714	1.03%	0.126%
11	9.727	1294	1299	1302	rBV	1551629	1431160	49.70%	6.083%
12	10.516	1428	1433	1443	rBV	1918872	1910561	66.35%	8.121%
13	11.210	1546	1551	1554	rBV	1707163	1520345	52.80%	6.462%
14	12.798	1816	1821	1824	rBV	2631678	2733331	94.92%	11.618%
15	13.292	1898	1905	1908	rBV	23916	32057	1.11%	0.136%
16	13.368	1913	1918	1921	rBV2	27438	34426	1.20%	0.146%
17	13.704	1971	1975	1990	rBV	254272	478478	16.62%	2.034%
18	13.845	1995	1999	2003	rVB	1562180	1378727	47.88%	5.860%
19	14.015	2024	2028	2030	rBV	39020	35531	1.23%	0.151%
20	14.321	2077	2080	2082	rVB	39154	34949	1.21%	0.149%
21	14.351	2082	2085	2093	rVB5	17023	30249	1.05%	0.129%
22	14.615	2124	2130	2134	rBV2	54408	70741	2.46%	0.301%
23	14.927	2180	2183	2188	rBV	47860	49606	1.72%	0.211%
24	15.256	2234	2239	2248	rBV	1052355	1250067	43.41%	5.314%
25	15.680	2307	2311	2316	rVB	39136	48366	1.68%	0.206%
26	15.768	2320	2326	2328	rBV6	21423	46623	1.62%	0.198%
27	16.139	2385	2389	2394	rVB2	21368	32474	1.13%	0.138%


Sum of corrected areas: 23526128

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082120\
Data File : BF121372.D
Acq On : 21 Aug 2020 17:42
Operator : JU/CG
Sample : L3719-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20200507-DISCRETE-005

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF081920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

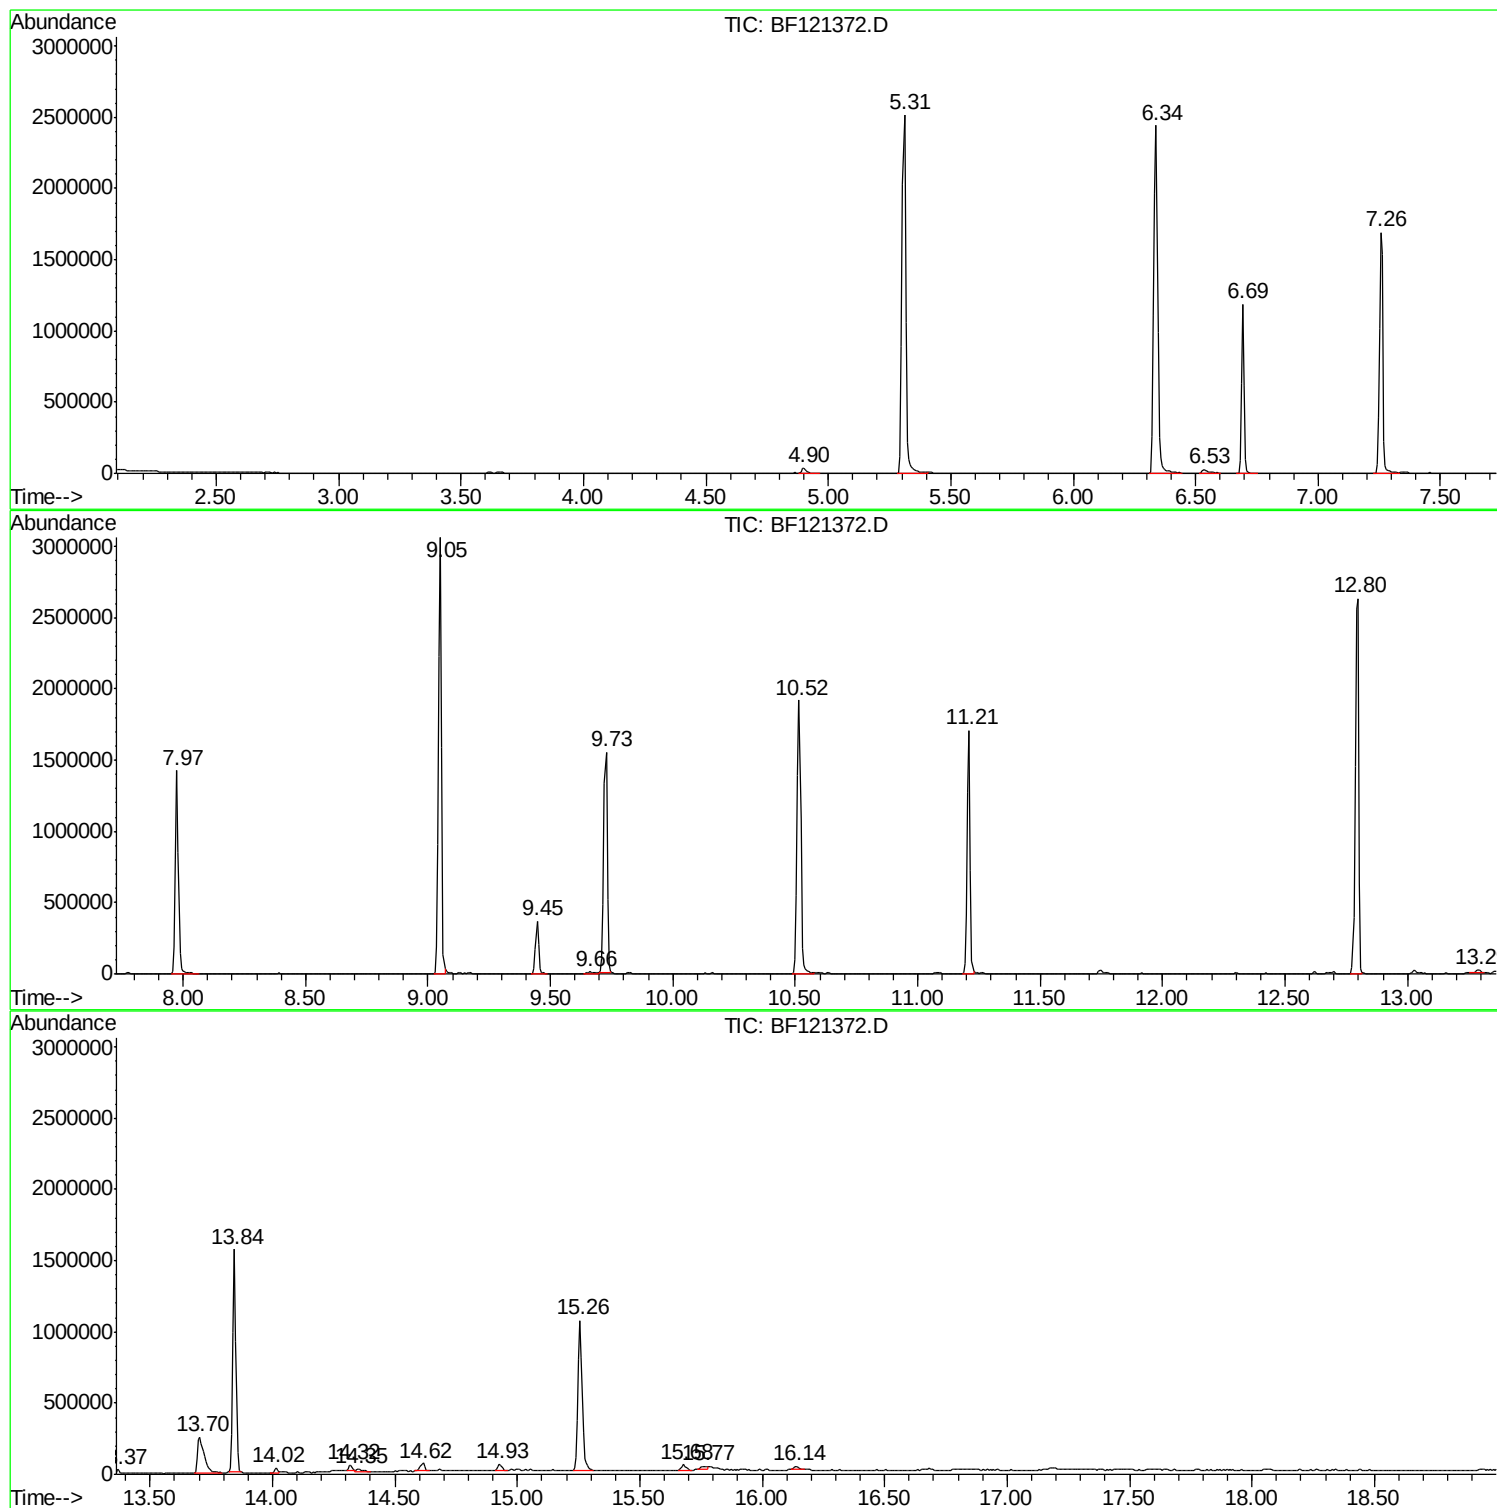

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082120\
Data File : BF121372.D
Acq On : 21 Aug 2020 17:42
Operator : JU/CG
Sample : L3719-02
Misc :
ALS Vial : 6 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
20200507-DISCRETE-005

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF081920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Trichloroacetic acid, hexad... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
13.70	6.94 ng	478478	Chrysene-d12	13.84	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	94
2	1-Heneicosanol	312	C21H44O	015594-90-8	93
3	Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	91
4	Nonadecyl pentafluoropropionate	430	C22H39F5O2	1000351-88-8	91
5	1-Docosene	308	C22H44	001599-67-3	91

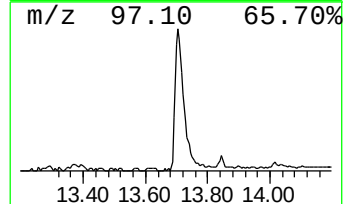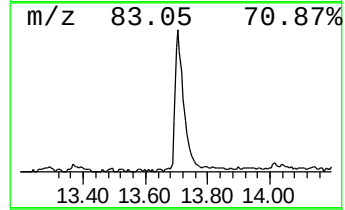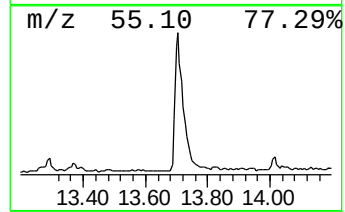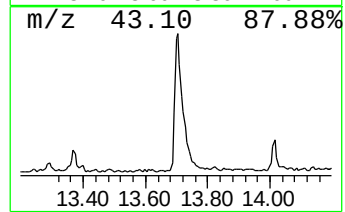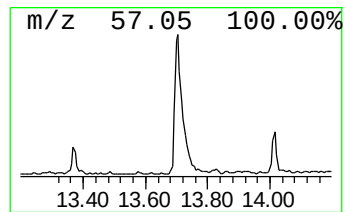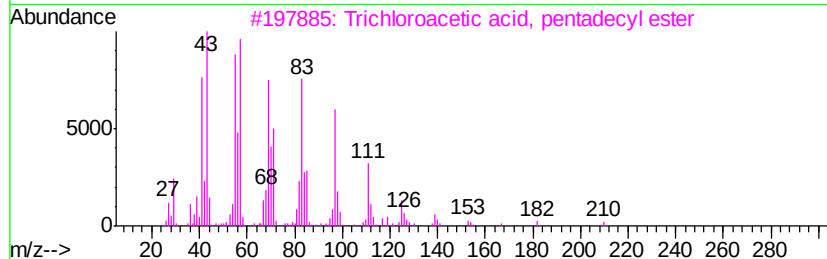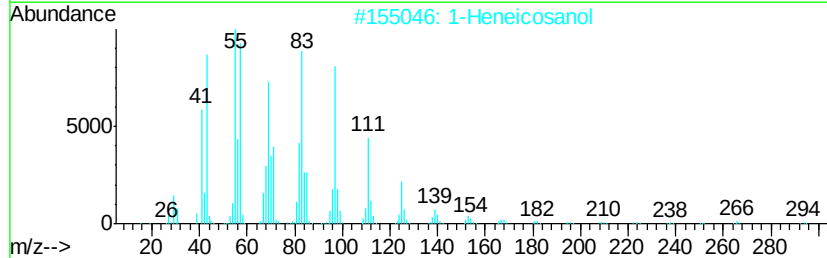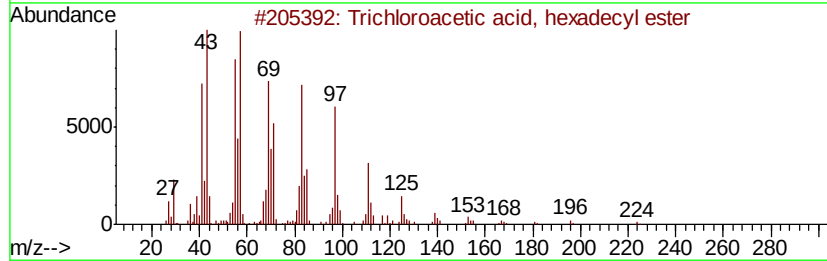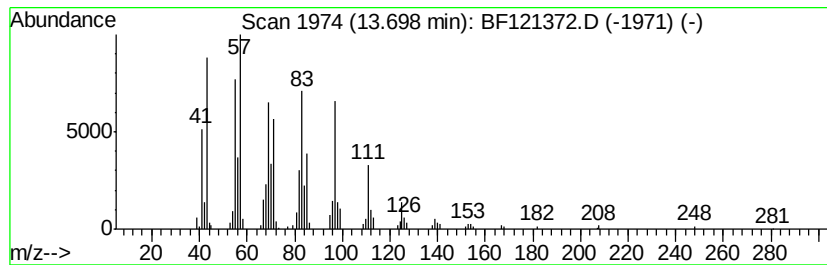

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082120\
Data File : BF121372.D
Acq On : 21 Aug 2020 17:42
Operator : JU/CG
Sample : L3719-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20200507-DISCRETE-005

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
Trichloroacetic a...	13.70	6.9	ng	478478	5	13.84	1378730	20.0