


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082120\
 Data File : BF121357.D
 Acq On : 21 Aug 2020 9:00
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 20 04:56:10 2020

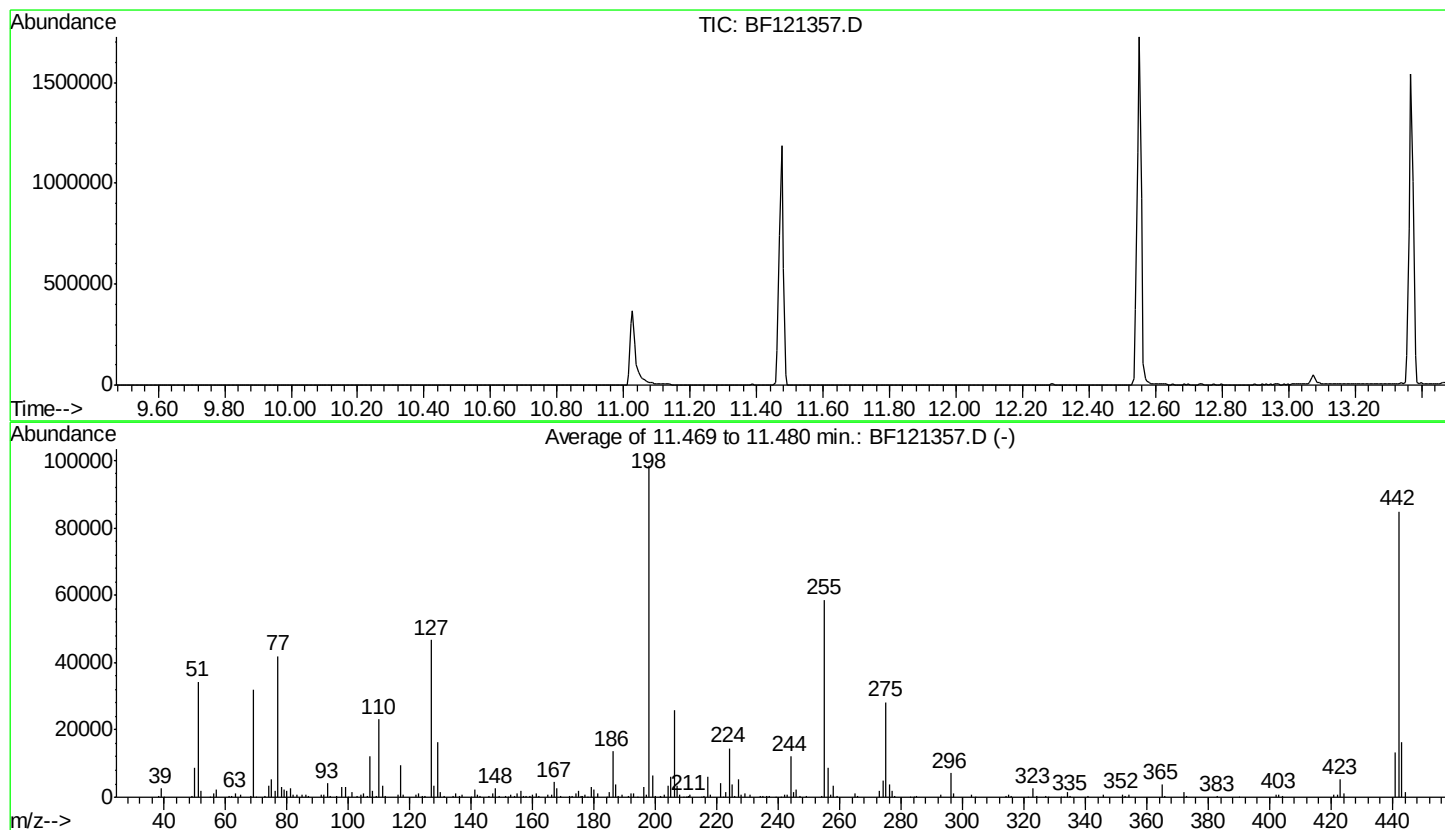

AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	34385	PASS
68	69	0.00	2	1.3	406	PASS
69	198	0.00	100	32.6	32063	PASS
70	69	0.00	2	0.4	117	PASS
127	198	10	80	47.5	46728	PASS
197	198	0.00	2	0.6	636	PASS
198	198	100	100	100.0	98464	PASS
199	198	5	9	6.6	6528	PASS
275	198	10	60	28.6	28144	PASS
365	198	1	100	3.7	3662	PASS
441	198	0.01	100	13.4	13168	PASS
442	198	50	100	86.3	84954	PASS
443	442	15	24	19.0	16183	PASS