
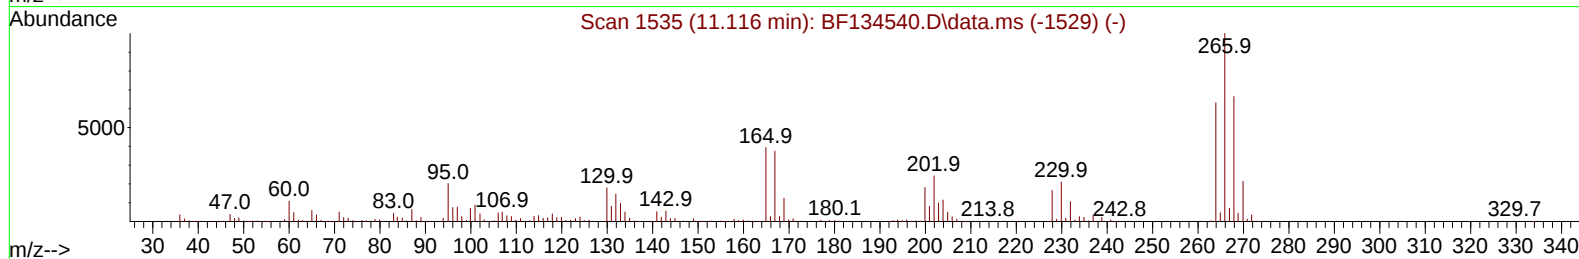
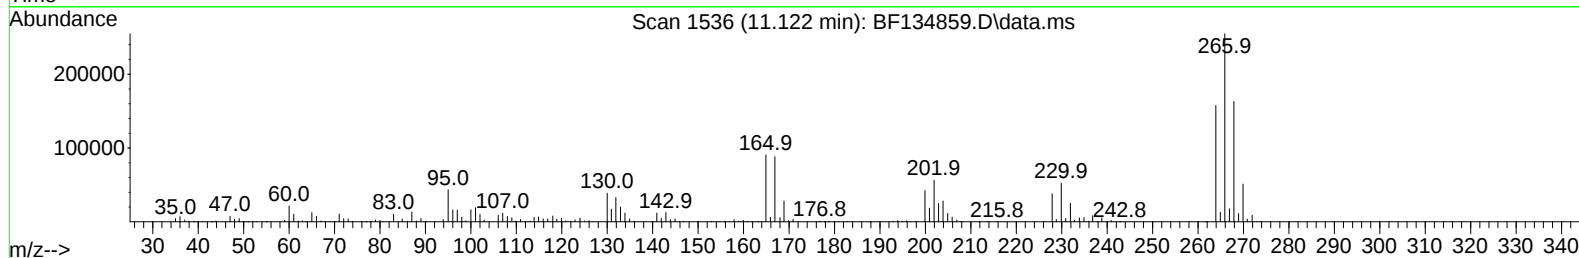


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF082123\  
Data File : BF134859.D  
Acq On : 21 Aug 2023 10:21  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 12:03:58 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF080123.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Aug 04 09:29:15 2023  
Response via : Initial Calibration

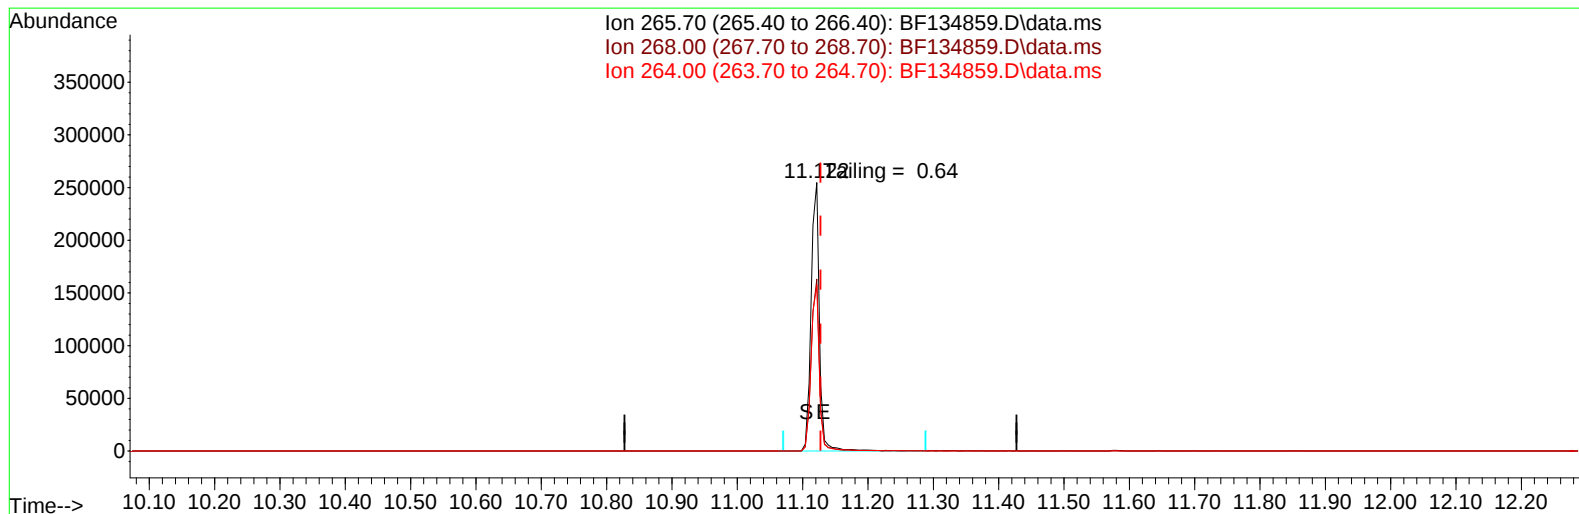

TIC: BF134859.D\data.ms

**(70) Pentachlorophenol (C)**




11.122min (-0.006) 259437.45 ng m

response 226540

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 66.10  | 64.02  |
| 264.00 | 59.70  | 61.86  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF082123\  
Data File : BF134859.D  
Acq On : 21 Aug 2023 10:21  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 12:03:58 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF080123.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Aug 04 09:29:15 2023  
Response via : Initial Calibration

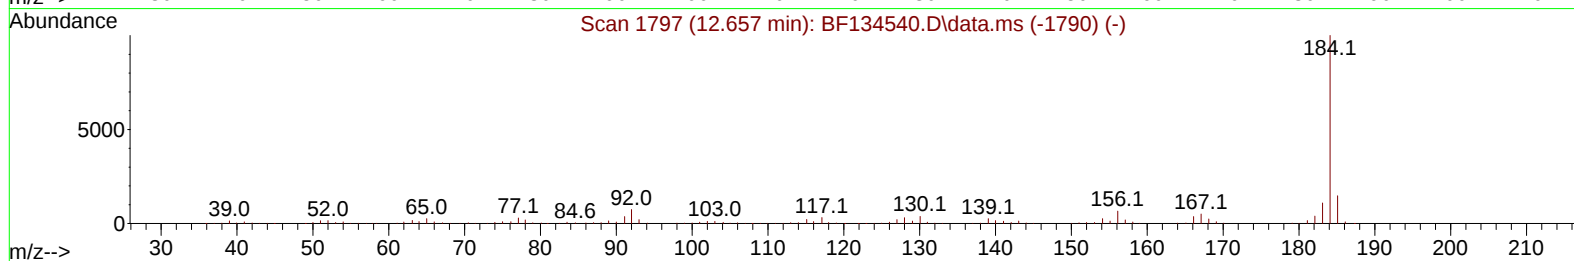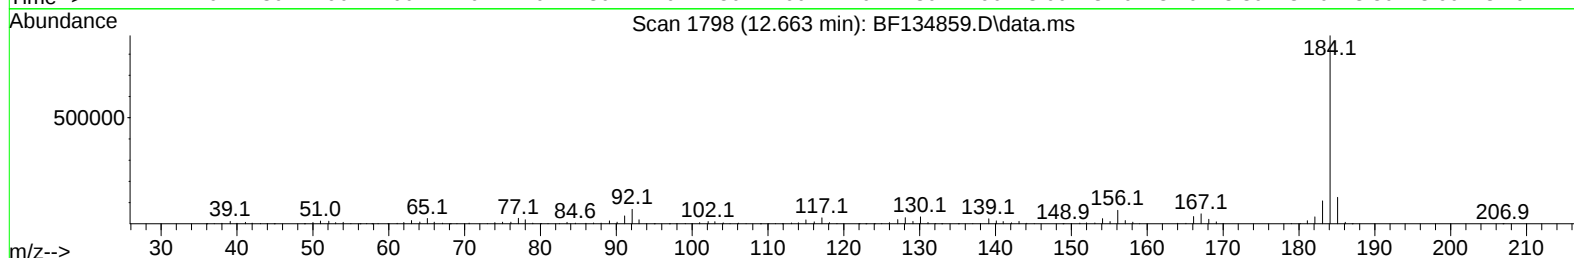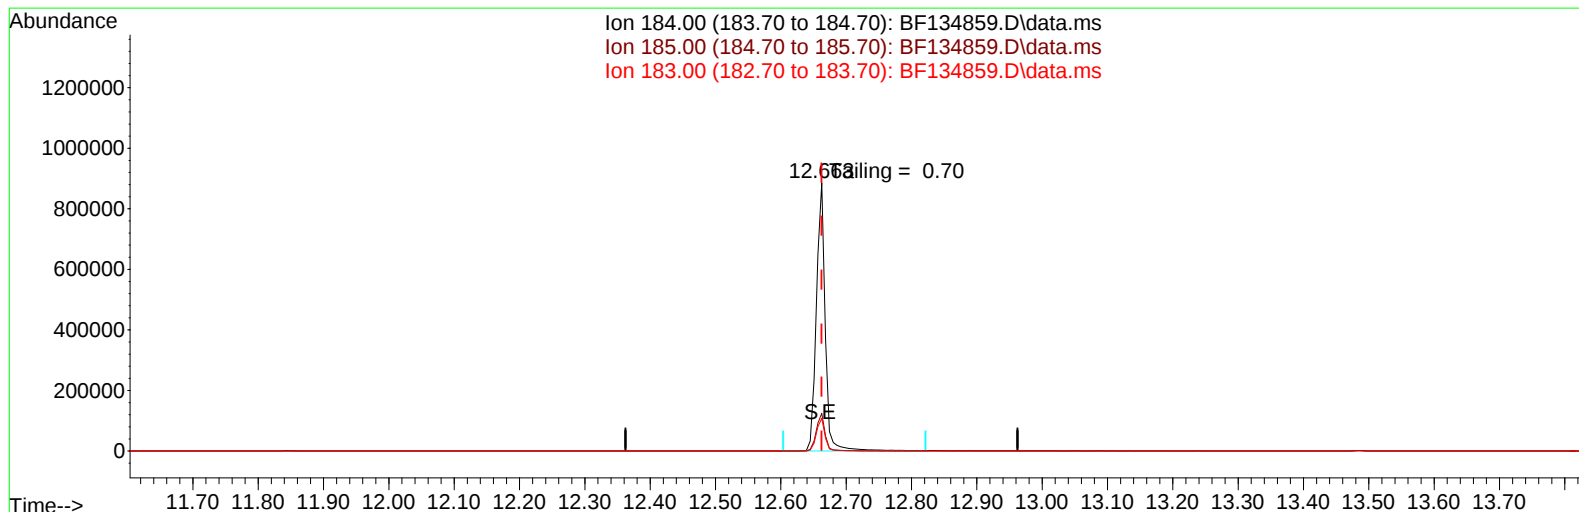

TIC: BF134859.D\data.ms

**(77) Benzidine**

12.663min (+ 0.000) 95811.01 ng

response 840261

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.00  | 14.09  |
| 183.00 | 10.80  | 12.18  |
| 0.00   | 0.00   | 0.00   |