

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082123\
 Data File : BF134861.D
 Acq On : 21 Aug 2023 11:24
 Operator : CG\JU
 Sample : PB154909BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB154909BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF134861.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.146	6	10	16	rVB	62268	89680	1.56%	0.239%
2	5.440	564	570	573	rBV	4343681	4745739	82.33%	12.656%
3	6.434	733	739	742	rBV	3784203	4869799	84.48%	12.987%
4	6.792	796	800	803	rBV	1586304	1275572	22.13%	3.402%
5	7.357	889	896	899	rBV	2937155	3282641	56.95%	8.754%
6	8.069	1012	1017	1020	rBV	1927585	1790961	31.07%	4.776%
7	9.151	1194	1201	1204	rBV	5435143	5764519	100.00%	15.373%
8	9.822	1310	1315	1319	rBV	2105447	2066738	35.85%	5.512%
9	10.622	1444	1451	1454	rBV	3654651	3821157	66.29%	10.190%
10	11.316	1565	1569	1572	rBV	2466612	2053894	35.63%	5.477%
11	12.916	1835	1841	1844	rBV	5121415	5364379	93.06%	14.306%
12	13.963	2015	2019	2032	rVB	1293233	1187406	20.60%	3.167%
13	15.433	2263	2269	2275	rBV	917182	1185679	20.57%	3.162%




Sum of corrected areas: 37498164

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082123\
Data File : BF134861.D
Acq On : 21 Aug 2023 11:24
Operator : CG\JU
Sample : PB154909BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154909BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

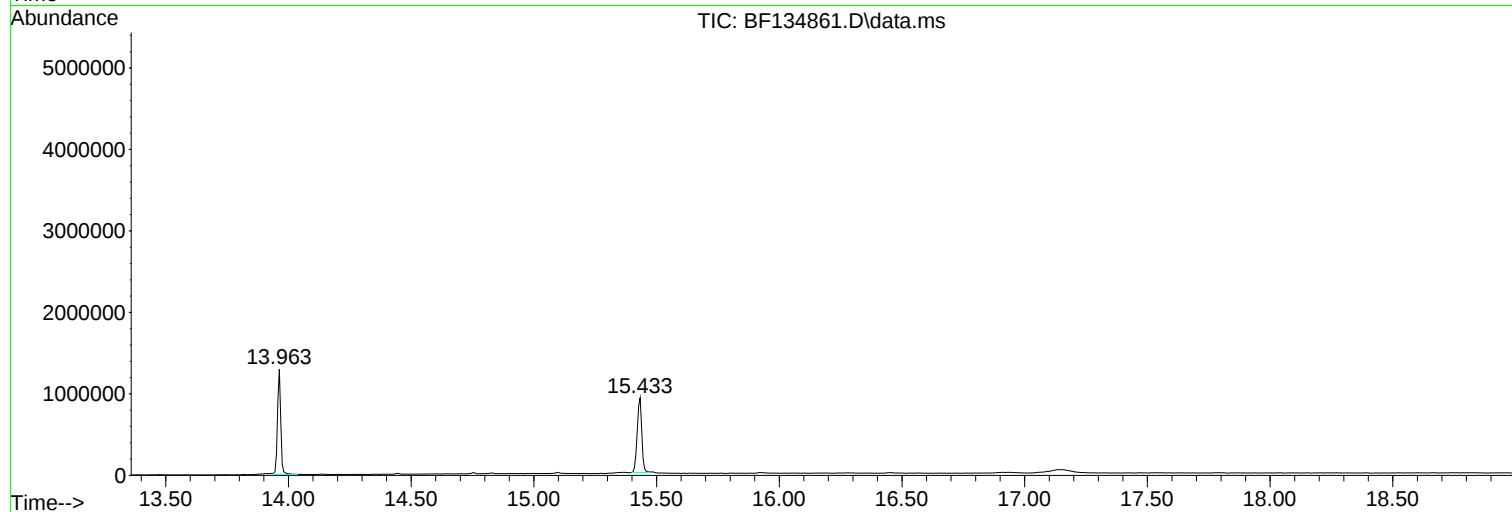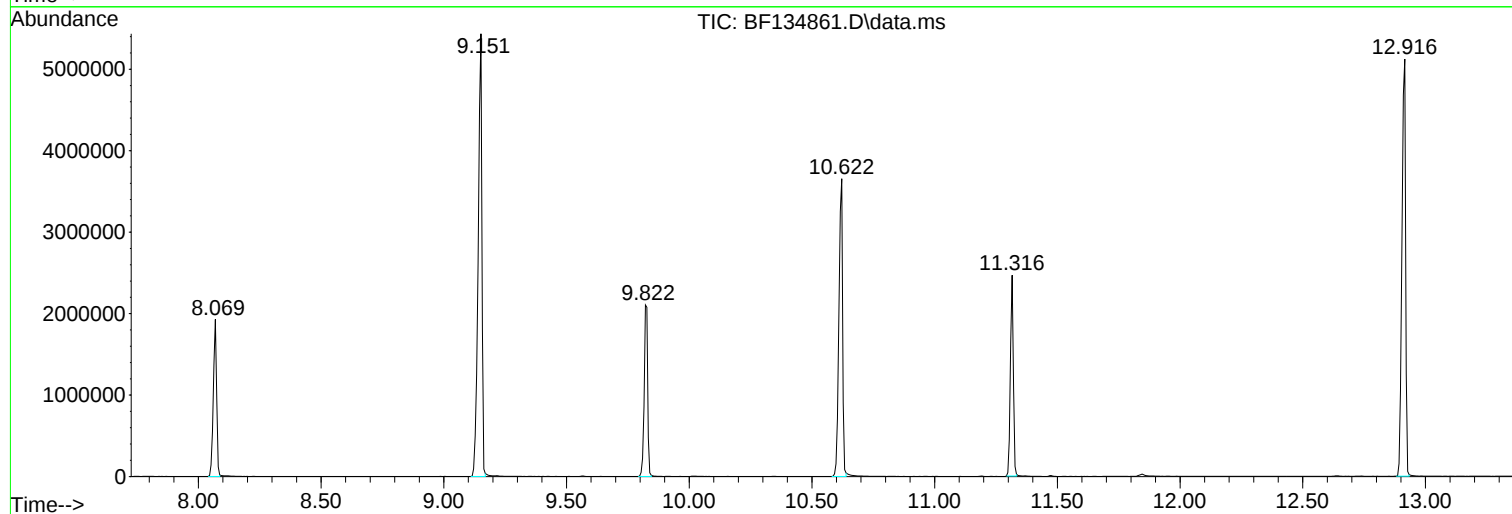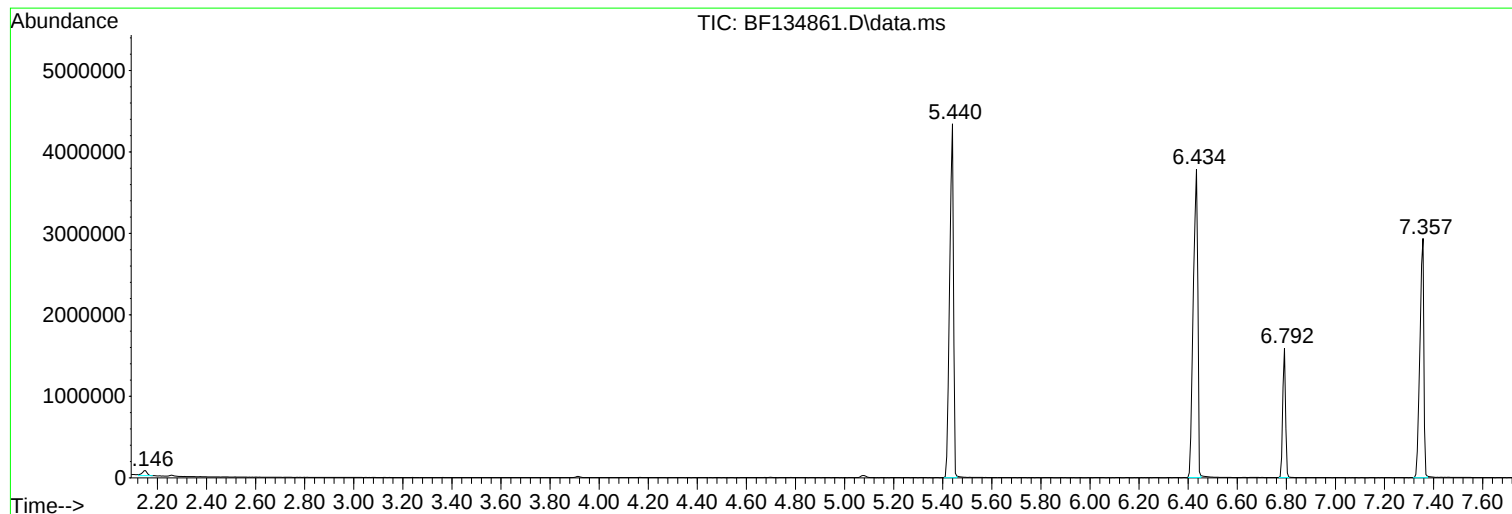

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082123\
Data File : BF134861.D
Acq On : 21 Aug 2023 11:24
Operator : CG\JU
Sample : PB154909BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154909BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082123\
Data File : BF134861.D
Acq On : 21 Aug 2023 11:24
Operator : CG\JU
Sample : PB154909BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154909BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------