

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082123\
 Data File : BF134865.D
 Acq On : 21 Aug 2023 13:45
 Operator : CG\JU
 Sample : 04086-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 B-PP13B

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF134865.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.428	563	568	571	rBV	2722472	2539575	85.72%	11.101%
2	6.428	733	738	741	rBV	2570032	2588456	87.37%	11.315%
3	6.622	768	771	782	rBV	70796	76200	2.57%	0.333%
4	6.792	796	800	803	rBV	1264492	1016660	34.31%	4.444%
5	7.351	890	895	898	rBV	1837133	1596292	53.88%	6.978%
6	8.069	1013	1017	1020	rBV	1666222	1382790	46.67%	6.045%
7	9.145	1195	1200	1203	rBV	3440914	2962771	100.00%	12.951%
8	9.263	1217	1220	1225	rVB	45836	39820	1.34%	0.174%
9	9.822	1311	1315	1319	rBV	1775902	1635083	55.19%	7.148%
10	10.616	1445	1450	1453	rBV	2208265	1930407	65.16%	8.439%
11	11.316	1565	1569	1572	rBV	1966740	1628079	54.95%	7.117%
12	11.380	1576	1580	1584	rVB2	36375	38536	1.30%	0.168%
13	11.851	1655	1660	1674	rBV	333431	389518	13.15%	1.703%
14	12.639	1790	1794	1805	rBV	80724	101313	3.42%	0.443%
15	12.910	1835	1840	1843	rBV	2988910	2622435	88.51%	11.464%
16	13.816	1989	1994	2003	rBV3	124985	169551	5.72%	0.741%
17	13.963	2015	2019	2028	rBV	1266890	1097985	37.06%	4.800%
18	15.433	2263	2269	2275	rBV	845562	1060689	35.80%	4.637%




Sum of corrected areas: 22876160

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082123\
Data File : BF134865.D
Acq On : 21 Aug 2023 13:45
Operator : CG\JU
Sample : 04086-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B-PP13B

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

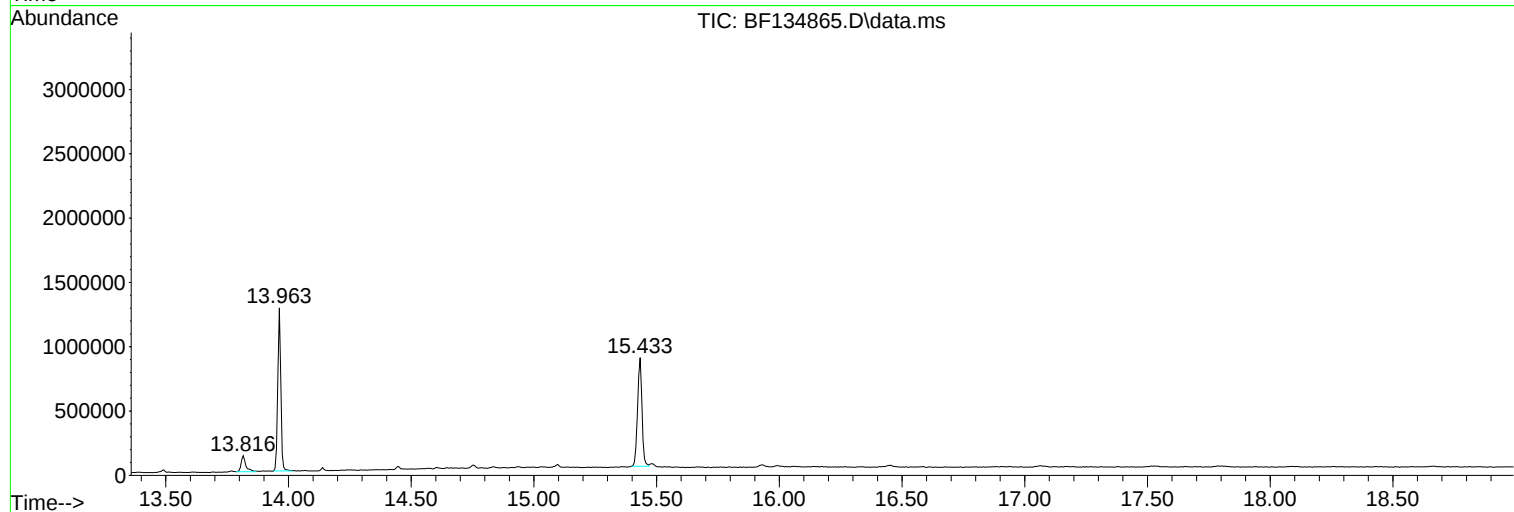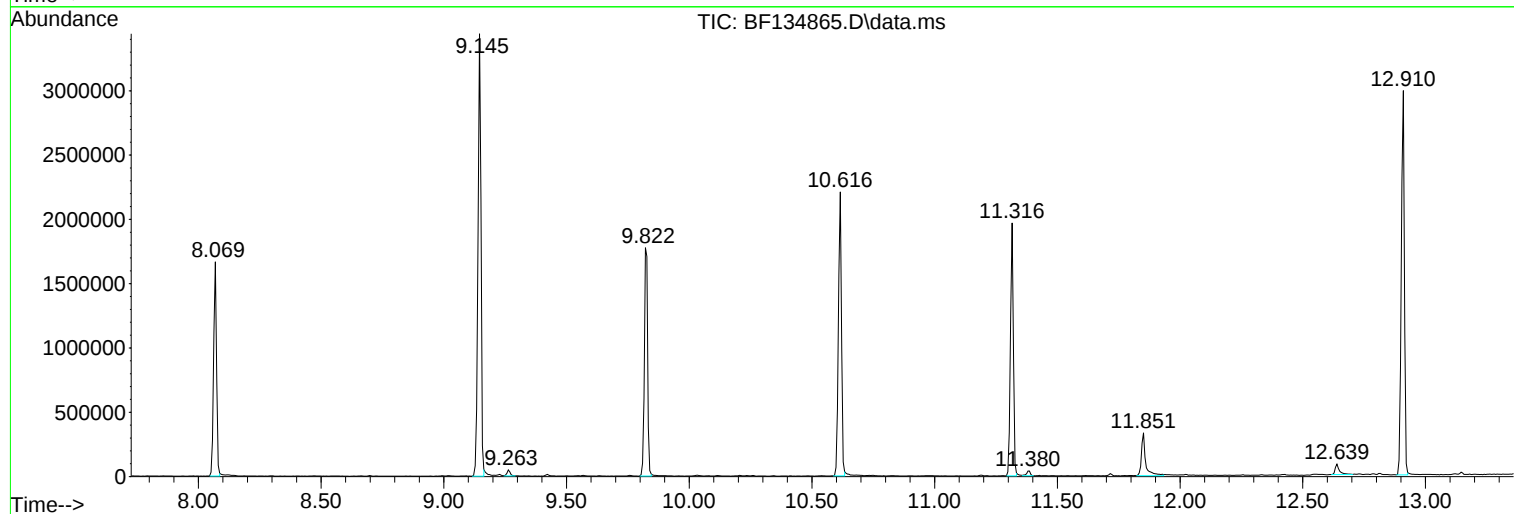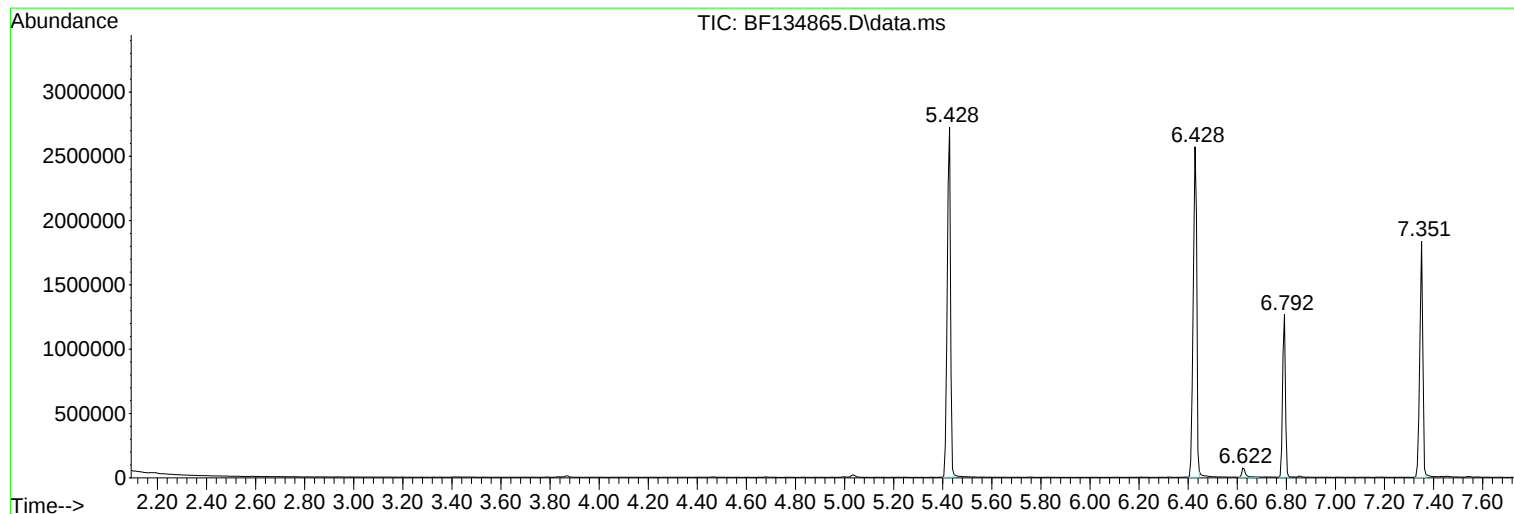

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082123\
Data File : BF134865.D
Acq On : 21 Aug 2023 13:45
Operator : CG\JU
Sample : 04086-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B-PP13B

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082123\
Data File : BF134865.D
Acq On : 21 Aug 2023 13:45
Operator : CG\JU
Sample : 04086-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B-PP13B

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------