
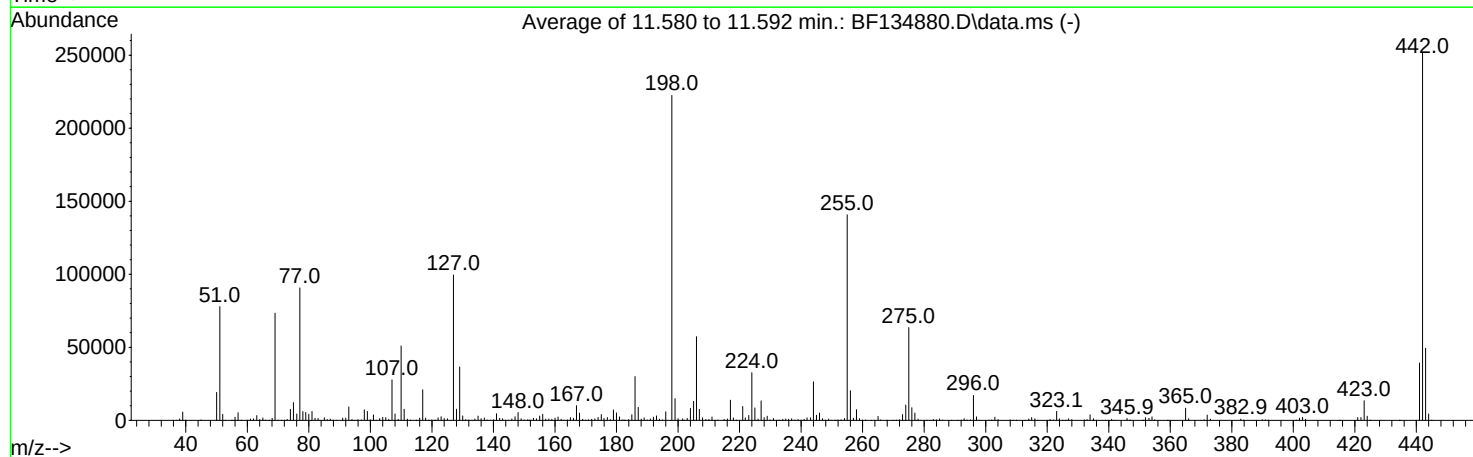


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082223\
Data File : BF134880.D
Acq On : 22 Aug 2023 11:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Aug 22 19:33:25 2023

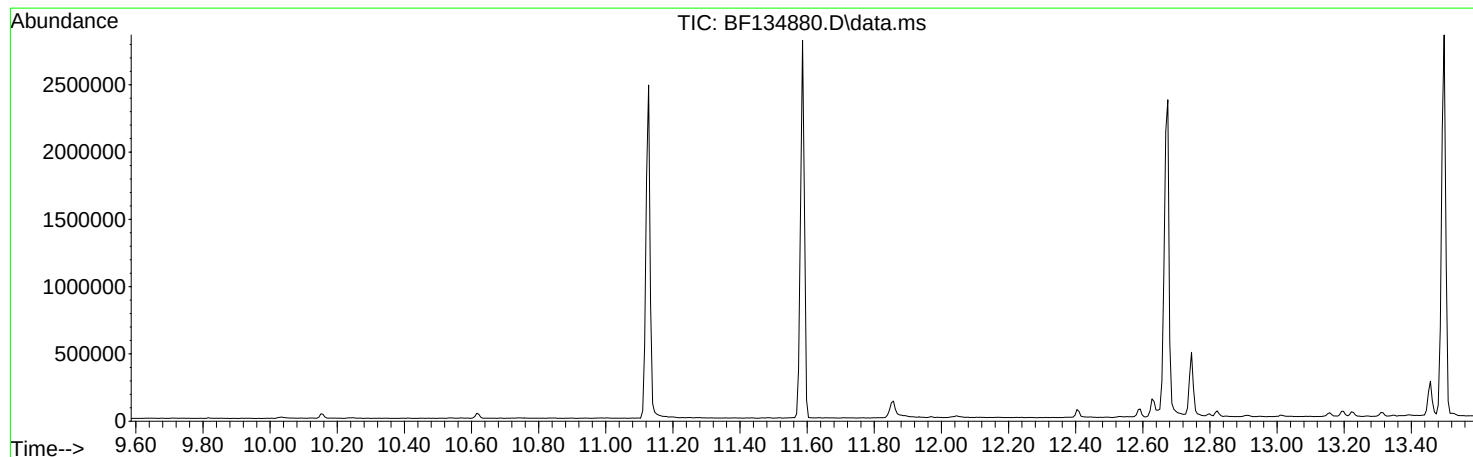




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	77882	PASS
68	69	0.00	2	1.9	1411	PASS
69	198	0.00	100	33.0	73387	PASS
70	69	0.00	2	0.4	285	PASS
127	198	10	80	44.8	99563	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	222464	PASS
199	198	5	9	6.7	14934	PASS
275	198	10	60	28.6	63592	PASS
365	198	1	100	3.8	8360	PASS
441	198	0.01	100	17.7	39368	PASS
442	442	50	100	100.0	251821	PASS
443	442	15	24	19.6	49453	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082223\
Data File : BF134880.D
Acq On : 22 Aug 2023 11:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 23 05:53:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 22 19:33:25 2023
Response via : Initial Calibration

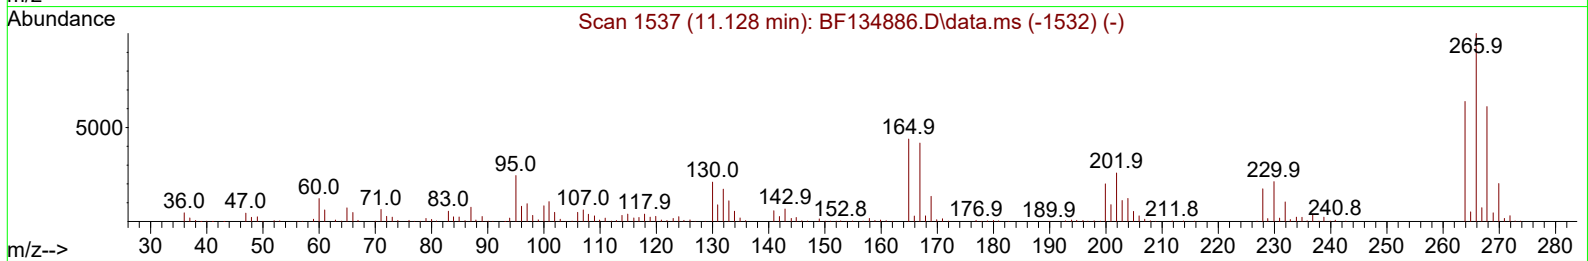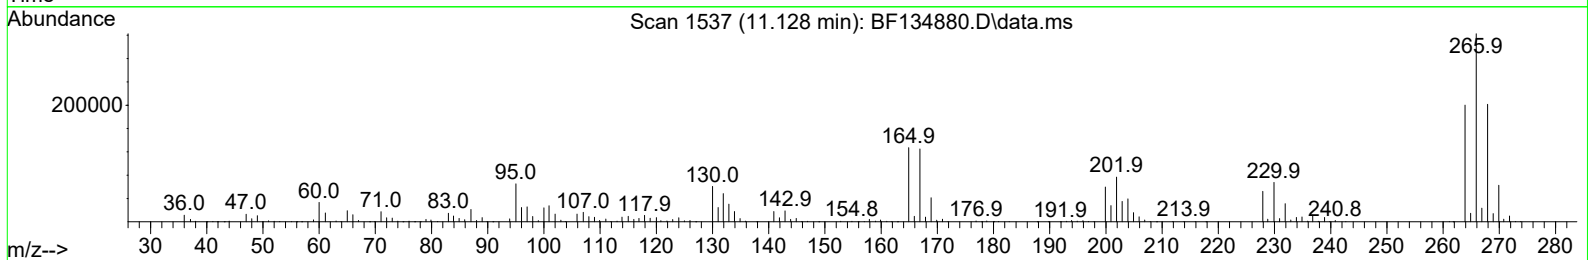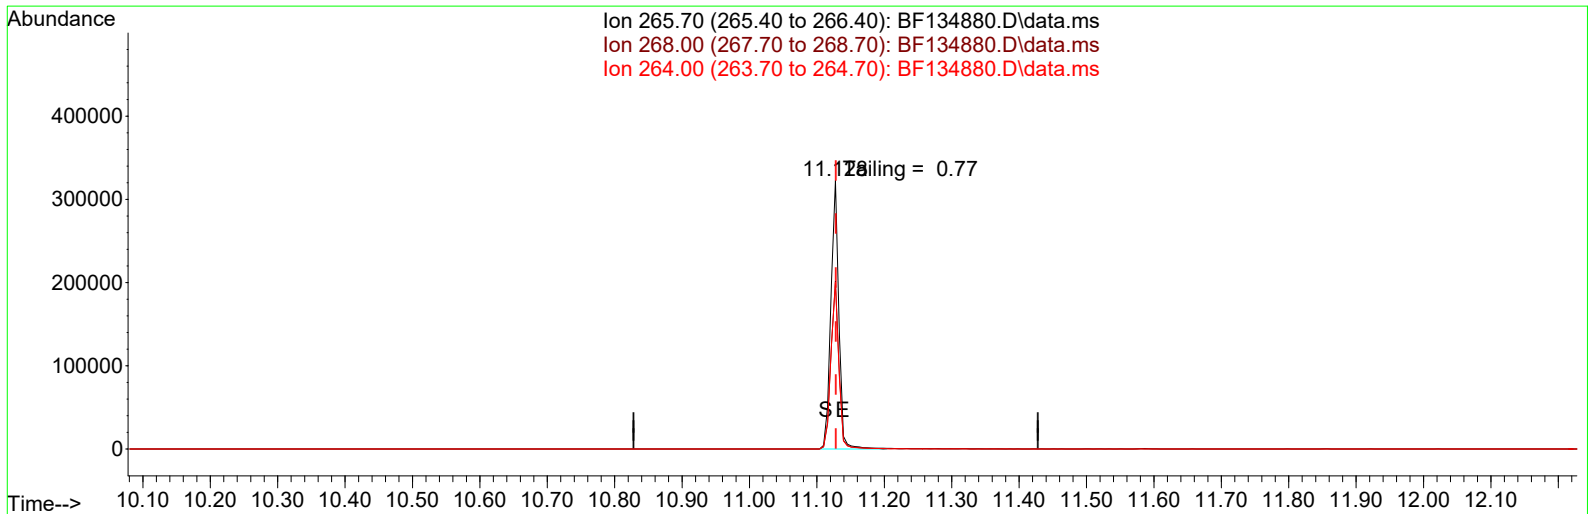

TIC: BF134880.D\data.ms

(70) Pentachlorophenol (C)

11.128min (-0.000) 196339.93 ng




response 268215

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	62.47
264.00	63.80	62.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082223\
Data File : BF134880.D
Acq On : 22 Aug 2023 11:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 23 05:53:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 22 19:33:25 2023
Response via : Initial Calibration

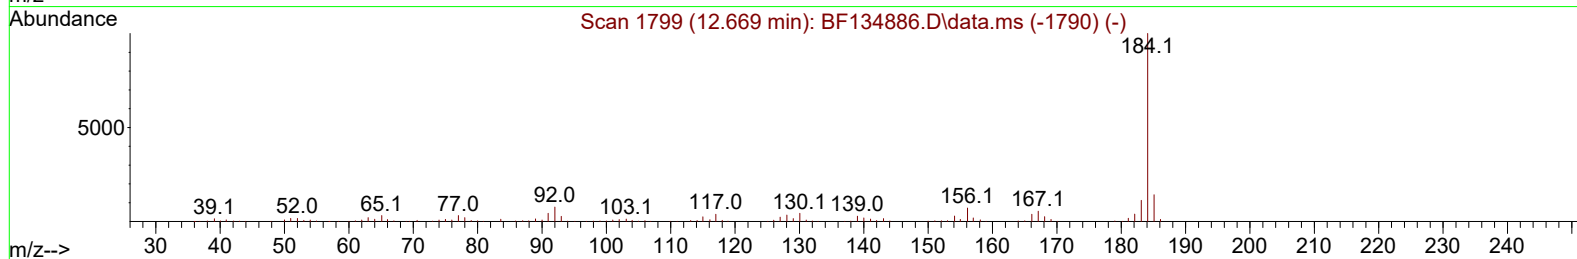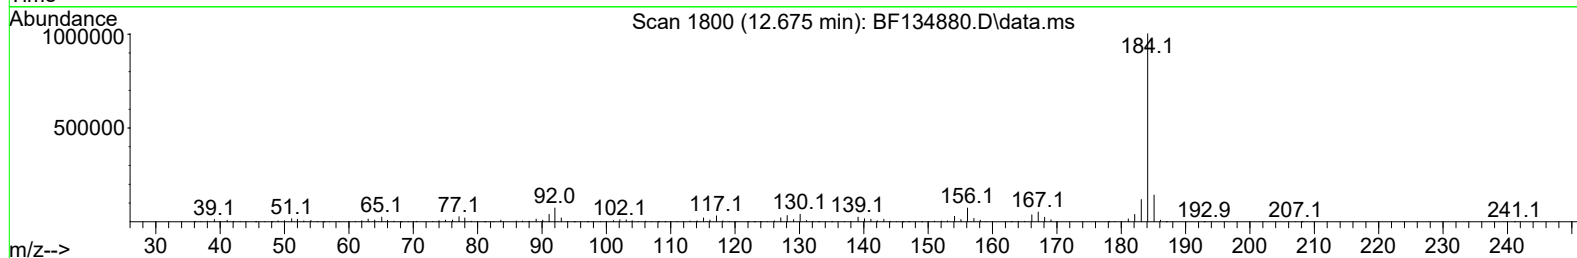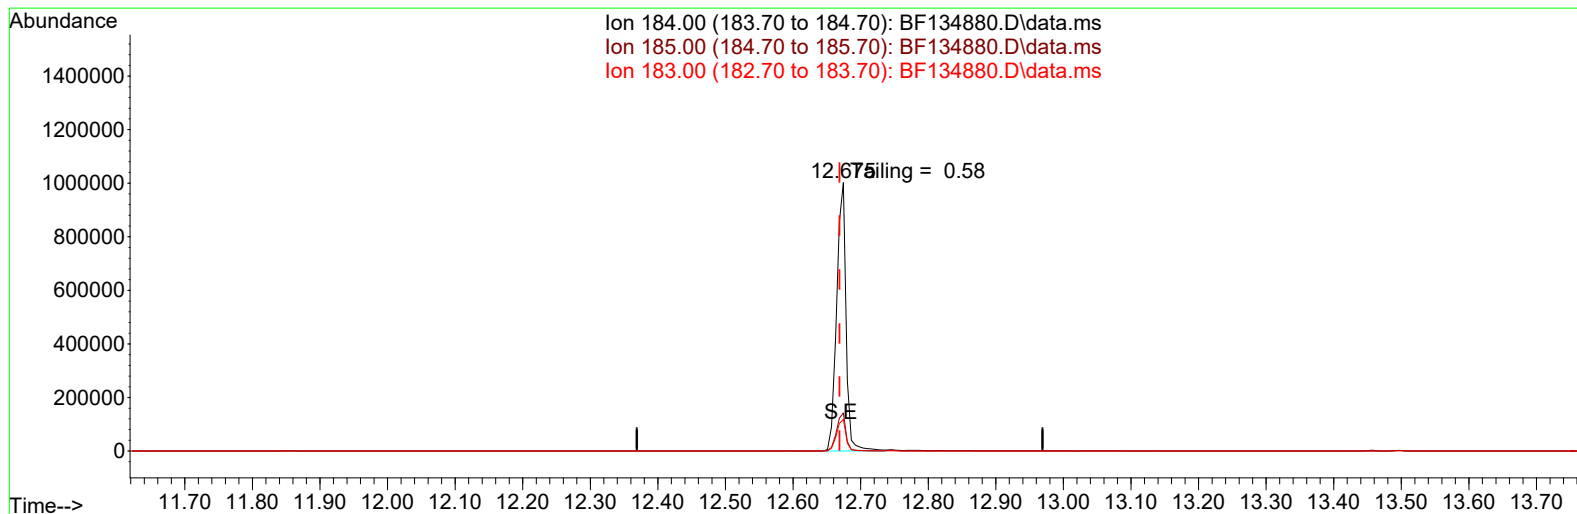

TIC: BF134880.D\data.ms

(77) Benzidine

12.675min (+ 0.006) 51040.21 ng

response 976353

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.19
183.00	11.20	11.82
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/22/2023	BNA_F	<u>BF134880.D</u>
Compound Name	Response	Retention Time
DDT	480434	13.498
DDD	12877	13.198
DDE	243	12.863
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13120	493554	2.66

Instrument :
BNA_F
ClientSampleId :
DFTPP