

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082318\
 Data File : BF108449.D
 Acq On : 24 Aug 2018 5:04
 Operator : JU/SJ
 Sample : J4535-10
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RA-081618-FL-042

Quant Time: Aug 24 05:38:25 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 22 11:01:45 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.00	152	148041	20.00	ng	0.00
21) Naphthalene-d8	8.28	136	535965	20.00	ng	0.00
38) Acenaphthene-d10	10.05	164	227873	20.00	ng	0.00
63) Phenanthrene-d10	11.54	188	321152	20.00	ng	0.00
75) Chrysene-d12	14.21	240	260876	20.00	ng	0.00
86) Perylene-d12	15.77	264	225792	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	682145	83.42	ng	0.00
7) Phenol-d6	6.62	99	921986	84.85	ng	-0.01
23) Nitrobenzene-d5	7.56	82	610487	63.56	ng	-0.01
41) 2,4,6-Tribromophenol	10.84	330	150606	66.26	ng	0.00
44) 2-Fluorobiphenyl	9.36	172	1052547	74.16	ng	0.00
78) Terphenyl-d14	13.14	244	668688	65.17	ng	0.01
Target Compounds						
25) Isophorone	7.56	82	608886	33.259	ng	# 64
49) Dimethylphthalate	9.75	163	63370	3.992	ng	# 95
53) 2,4-Dinitrophenol	10.25	184	451	7.352	ng	# 1
55) 4-Nitrophenol	10.14	139	5991	2.177	ng	# 47
64) 4,6-Dinitro-2-methylphenol	10.65	198	730	5.896	ng	# 1
65) n-Nitrosodiphenylamine	10.70	169	54132	5.704	ng	# 36
70) Phenanthrene	11.57	178	78766	5.200	ng	# 87
77) Pyrene	13.02	202	33951	2.056	ng	# 15

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082318\
Data File : BF108449.D
Acq On : 24 Aug 2018 5:04
Operator : JU/SJ
Sample : J4535-10
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RA-081618-FL-042

Quant Time: Aug 24 05:38:25 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 22 11:01:45 2018
Response via : Initial Calibration

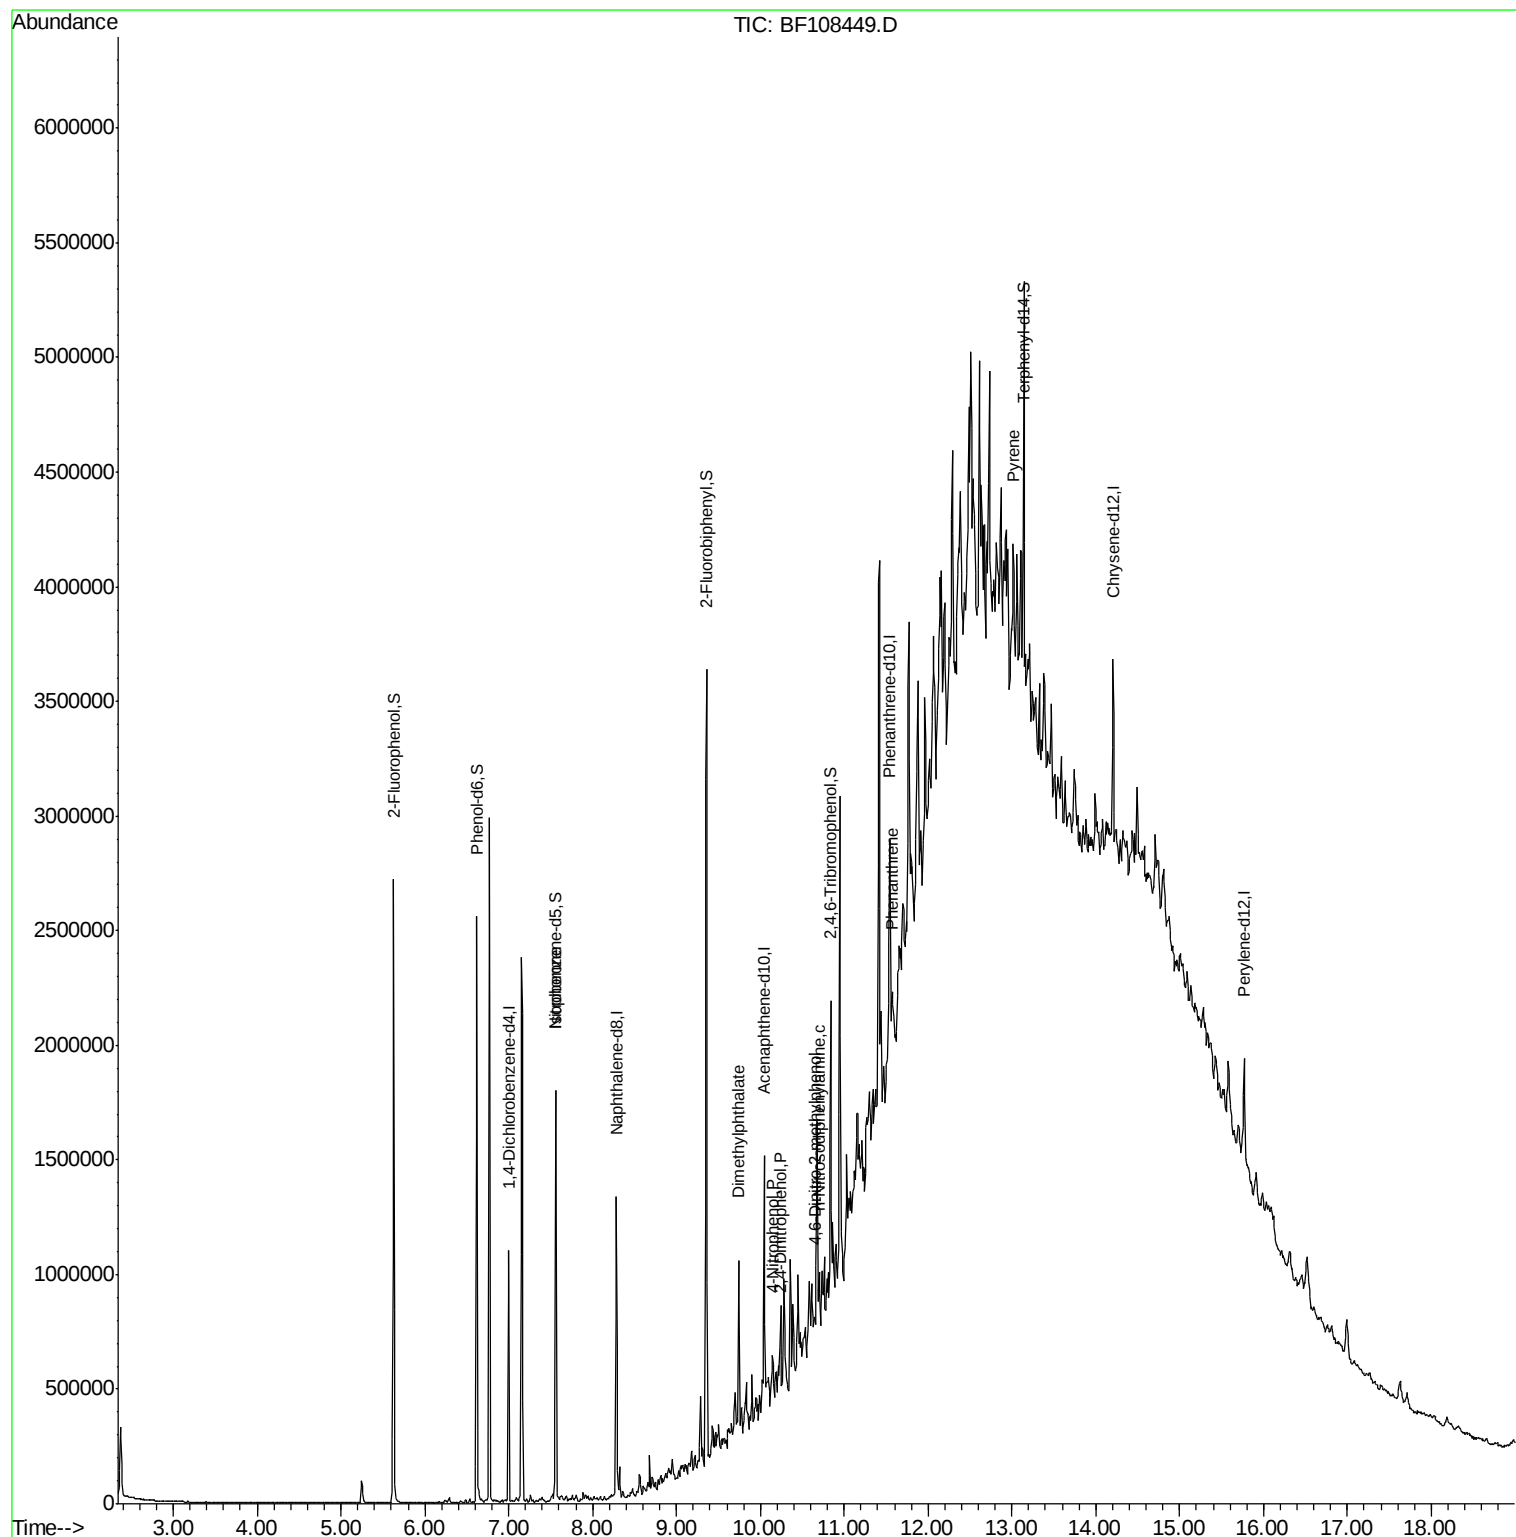






#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.00 min Scan# 793
Delta R.T. -0.01 min
Lab File: BF108449.D
Acq: 24 Aug 2018 5:04

Instrument :
BNA_F
ClientSampleId :
RA-081618-FL-042




Tgt Ion:152 Resp: 148041
Ion Ratio Lower Upper
152 100
150 153.4 124.6 186.8
115 58.2 50.1 75.1

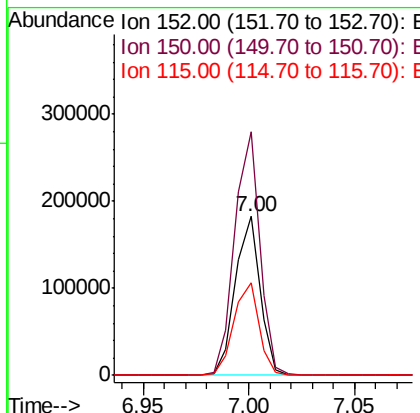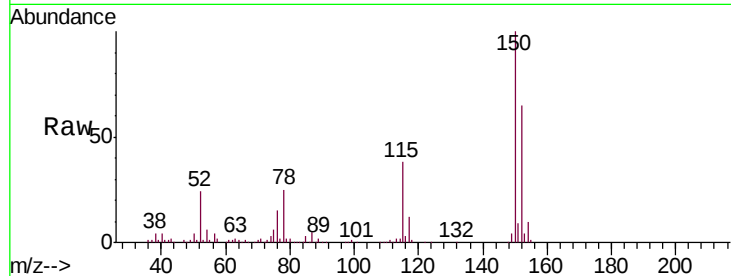


#5

2-Fluorophenol
Concen: 83.422 ng
RT: 5.63 min Scan# 560
Delta R.T. -0.00 min
Lab File: BF108449.D
Acq: 24 Aug 2018 5:04

Tgt Ion:112 Resp: 682145
Ion Ratio Lower Upper
112 100
64 67.6 47.9 71.9
63 35.8 23.7 35.5#

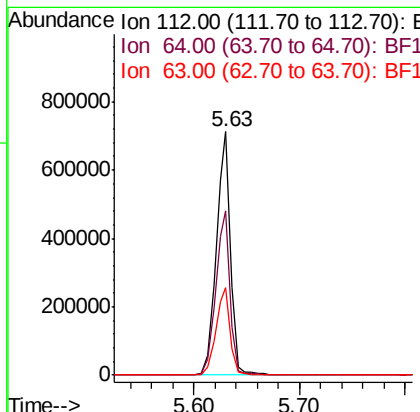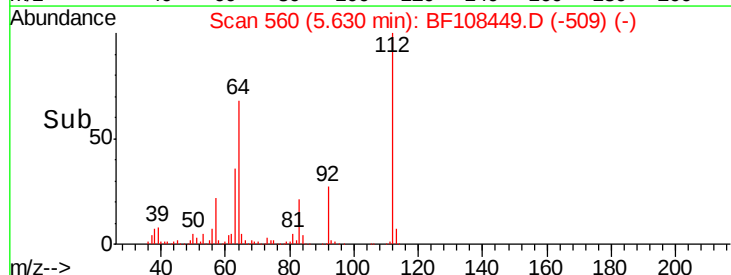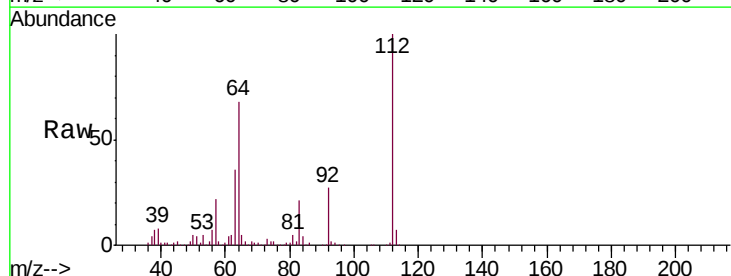

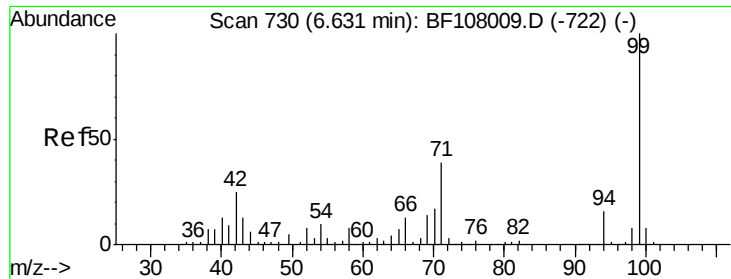

#7

Phenol-d6

Concen: 84.849 ng

RT: 6.62 min Scan# 728

Delta R.T. -0.01 min

Lab File: BF108449.D

Acq: 24 Aug 2018 5:04

Instrument :

BNA_F

ClientSampleId :

RA-081618-FL-042


Tgt Ion: 99 Resp: 921986

Ion Ratio Lower Upper

99 100

42 23.0 14.5 21.7#




71 37.3 25.4 38.0



Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

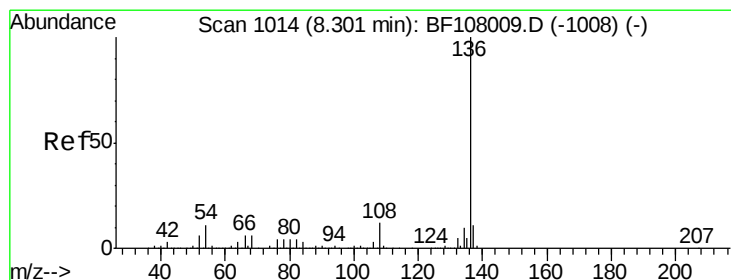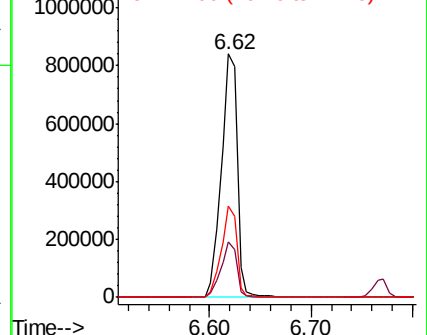

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.28 min Scan# 1011

Delta R.T. -0.01 min

Lab File: BF108449.D

Acq: 24 Aug 2018 5:04

Tgt Ion: 136 Resp: 535965


Ion Ratio Lower Upper

136 100

137 11.2 8.9 13.3

54 9.7 6.6 9.8

68 6.0 5.0 7.4


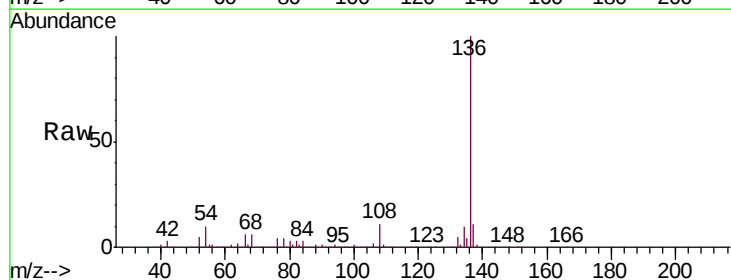



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1



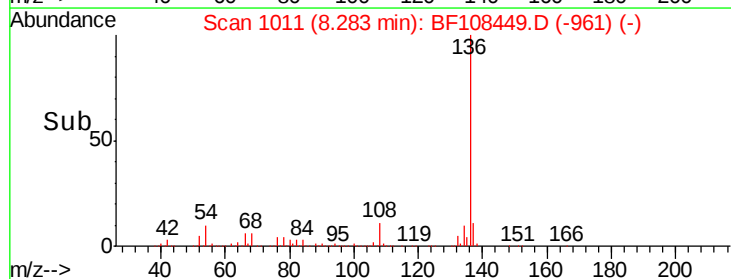
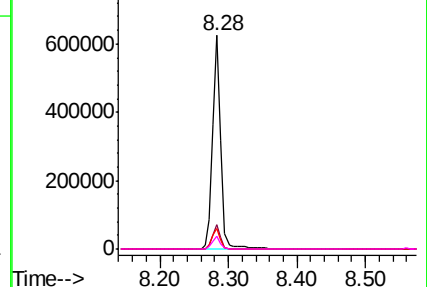




#23
 Nitrobenzene-d5
 Concen: 63.560 ng
 RT: 7.56 min Scan# 888
 Delta R.T. -0.01 min
 Lab File: BF108449.D
 Acq: 24 Aug 2018 5:04




Instrument :
 BNA_F
 ClientSampleId :
 RA-081618-FL-042


Tgt Ion	Ratio	Lower	Upper
82	100		
128	41.3	36.1	54.1
54	58.4	41.4	62.2

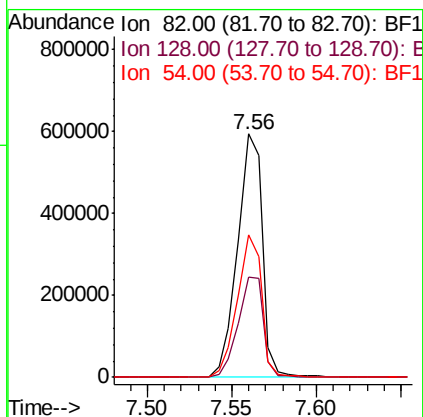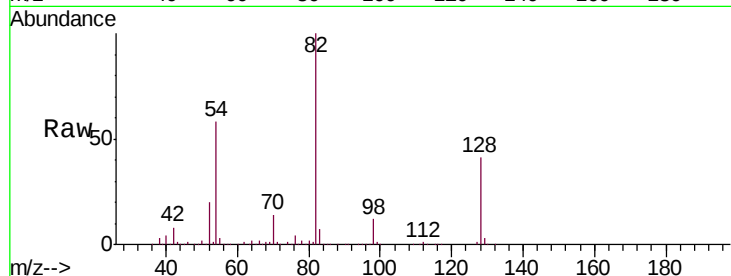

#25
 Isophorone
 Concen: 33.259 ng
 RT: 7.56 min Scan# 888
 Delta R.T. -0.27 min
 Lab File: BF108449.D
 Acq: 24 Aug 2018 5:04

Tgt Ion	Ratio	Lower	Upper
82	100		
95	0.1	5.2	7.8#
138	0.0	14.9	22.3#

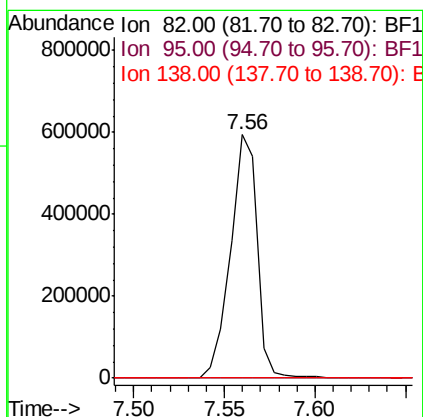



#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.05 min Scan# 1311

Delta R.T. -0.01 min

Lab File: BF108449.D

Acq: 24 Aug 2018 5:04

Instrument :

BNA_F

ClientSampleId :

RA-081618-FL-042


Tgt Ion:164 Resp: 227873

Ion Ratio Lower Upper

164 100

162 101.9 86.1 129.1




160 47.0 38.3 57.5

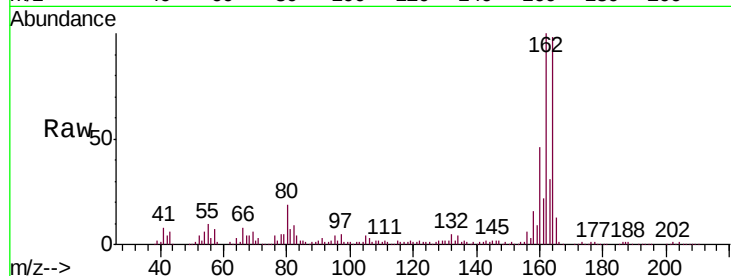

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

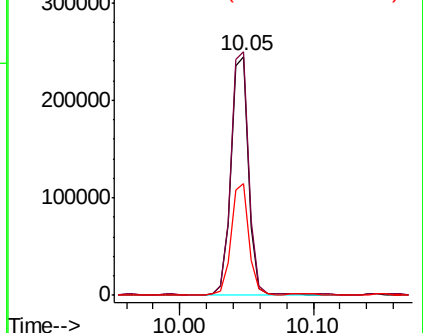

#41

2,4,6-Tribromophenol

Concen: 66.259 ng

RT: 10.84 min Scan# 1446

Delta R.T. -0.01 min

Lab File: BF108449.D

Acq: 24 Aug 2018 5:04


Tgt Ion:330 Resp: 150606

Ion Ratio Lower Upper

330 100

332 97.6 77.0 115.6



141 33.2 29.9 44.9




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E




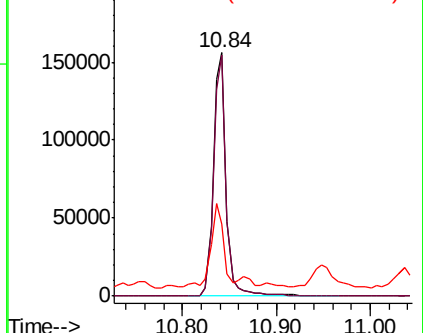




#44
 2-Fluorobiphenyl
 Concen: 74.157 ng
 RT: 9.36 min Scan# 1194
 Delta R.T. -0.01 min
 Lab File: BF108449.D
 Acq: 24 Aug 2018 5:04




Instrument :
 BNA_F
 ClientSampleId :
 RA-081618-FL-042


Tgt Ion:172 Resp: 1052547
 Ion Ratio Lower Upper
 172 100
 171 36.2 29.7 44.5
 170 23.9 19.6 29.4

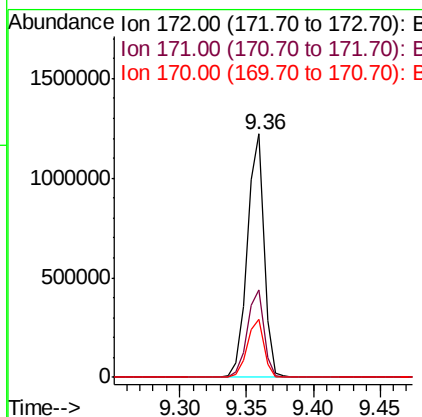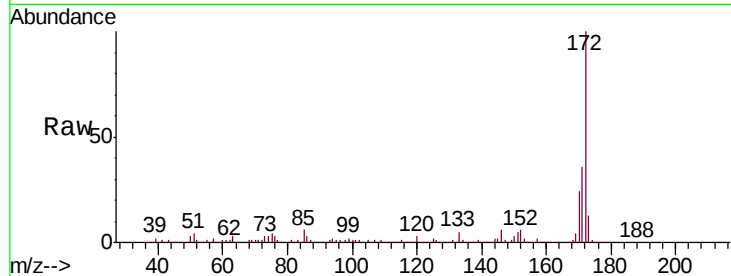

#49
 Dimethylphthalate
 Concen: 3.992 ng
 RT: 9.75 min Scan# 1260
 Delta R.T. -0.02 min
 Lab File: BF108449.D
 Acq: 24 Aug 2018 5:04

Tgt Ion:163 Resp: 63370
 Ion Ratio Lower Upper
 163 100
 194 9.4 2.7 4.1#
 164 10.5 8.2 12.2



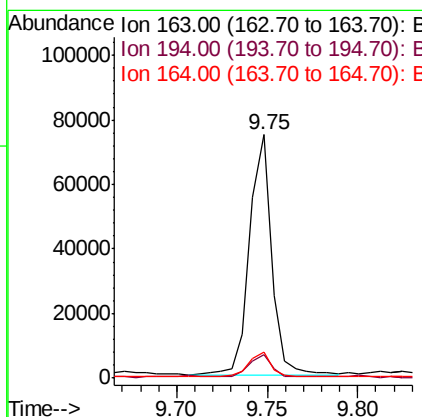
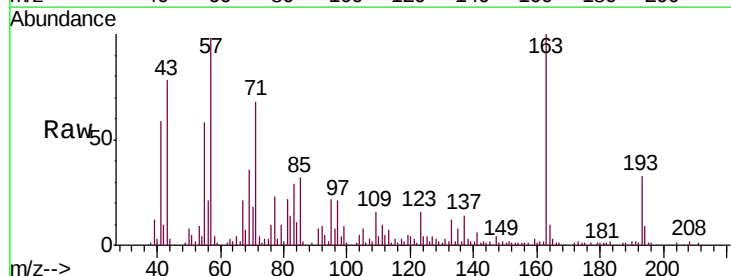


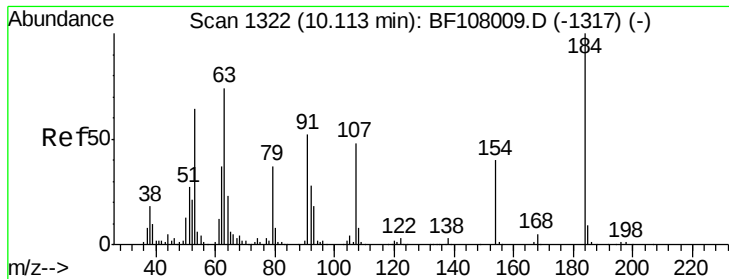

#53
 2,4-Dinitrophenol
 Concen: 7.352 ng
 RT: 10.25 min Scan# 1346
 Delta R.T. 0.15 min
 Lab File: BF108449.D
 Acq: 24 Aug 2018 5:04




Instrument :
 BNA_F
 ClientSampleId :
 RA-081618-FL-042


Tgt Ion:184 Resp: 451
 Ion Ratio Lower Upper
 184 100
 63 288.5 54.2 81.2#
 154 373.2 184.0 276.0#

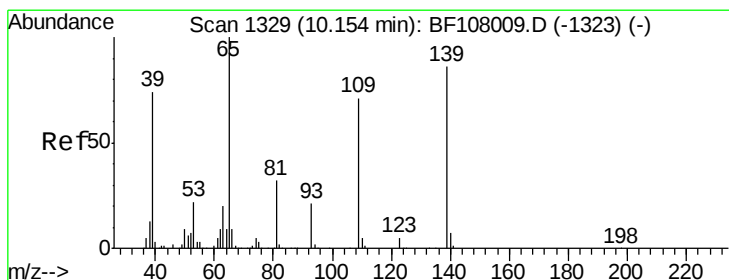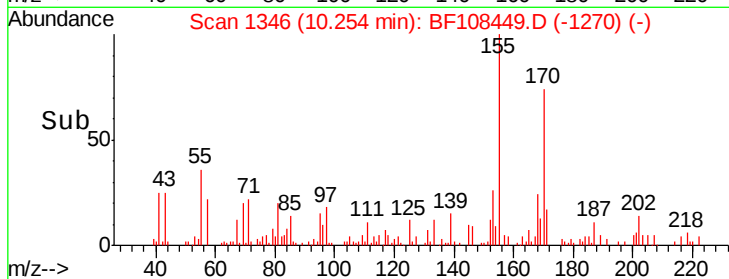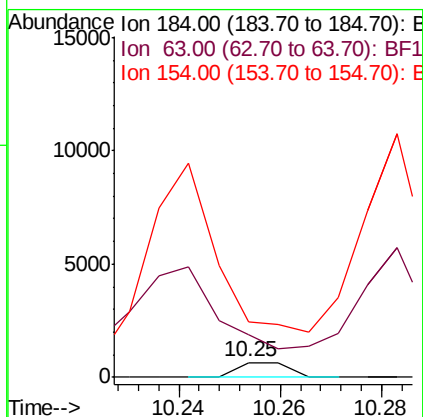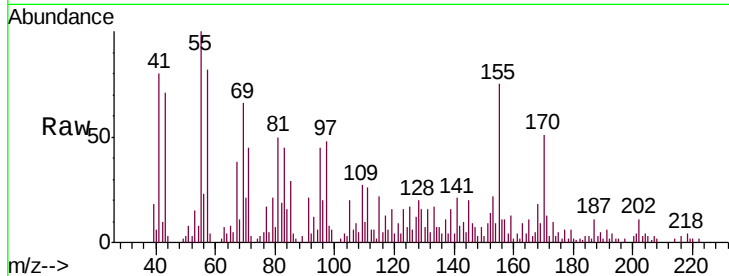

#55
 4-Nitrophenol
 Concen: 2.177 ng
 RT: 10.14 min Scan# 1327
 Delta R.T. -0.01 min
 Lab File: BF108449.D
 Acq: 24 Aug 2018 5:04

Tgt Ion:139 Resp: 5991
 Ion Ratio Lower Upper
 139 100
 109 143.2 48.4 88.4#
 65 69.1 72.6 112.6#


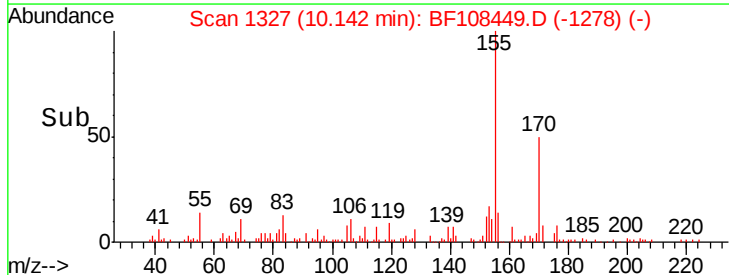
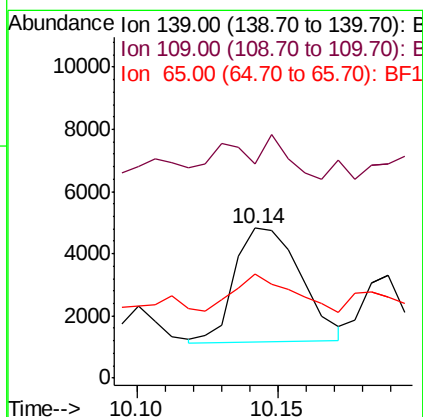
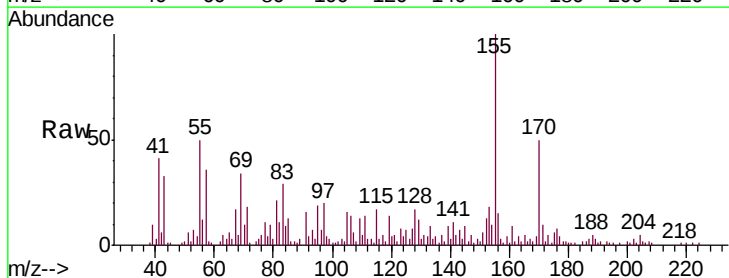


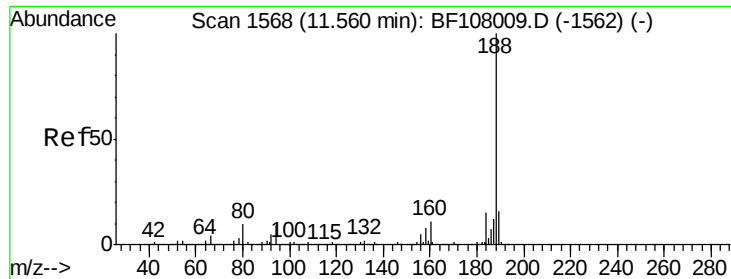

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.54 min Scan# 1565
Delta R.T. -0.01 min
Lab File: BF108449.D
Acq: 24 Aug 2018 5:04




Instrument :
BNA_F
ClientSampleId :
RA-081618-FL-042


Tgt Ion:188 Resp: 321152
Ion Ratio Lower Upper
188 100
94 10.0 8.5 12.7
80 11.8 9.2 13.8

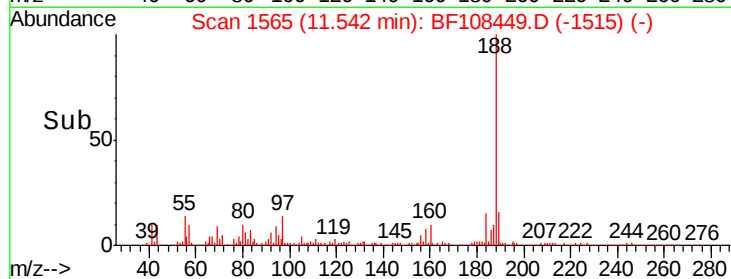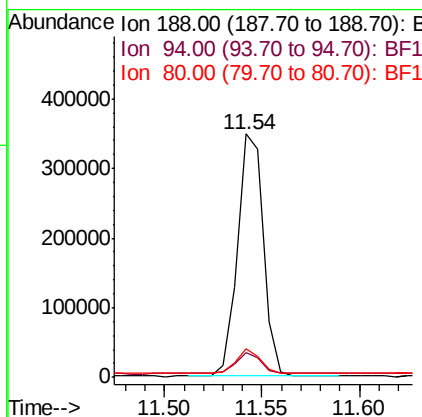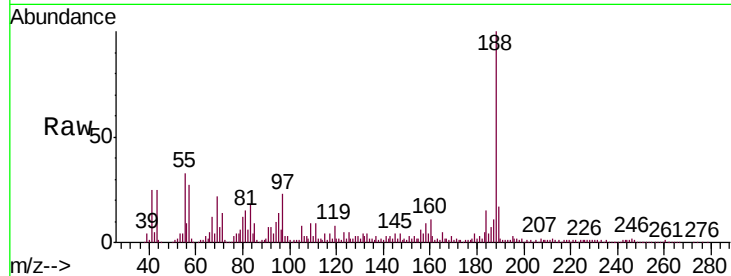

#64
4,6-Dinitro-2-methylphenol
Concen: 5.896 ng
RT: 10.65 min Scan# 1414
Delta R.T. 0.01 min
Lab File: BF108449.D
Acq: 24 Aug 2018 5:04

Tgt Ion:198 Resp: 730
Ion Ratio Lower Upper
198 100
51 359.5 37.7 77.7#
105 1867.4 36.3 76.3#



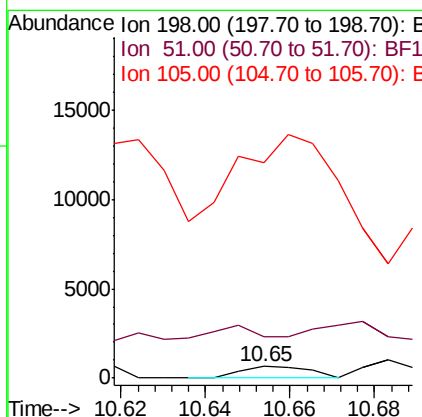



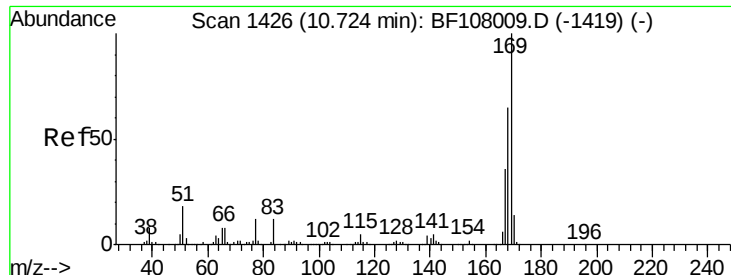

#65
 n-Nitrosodiphenylamine
 Concen: 5.704 ng
 RT: 10.70 min Scan# 1422
 Delta R.T. -0.01 min
 Lab File: BF108449.D
 Acq: 24 Aug 2018 5:04




Instrument :
 BNA_F
 ClientSampleId :
 RA-081618-FL-042


Tgt Ion:169 Resp: 54132
 Ion Ratio Lower Upper
 169 100
 168 8.2 54.4 81.6#
 167 9.4 29.8 44.6#

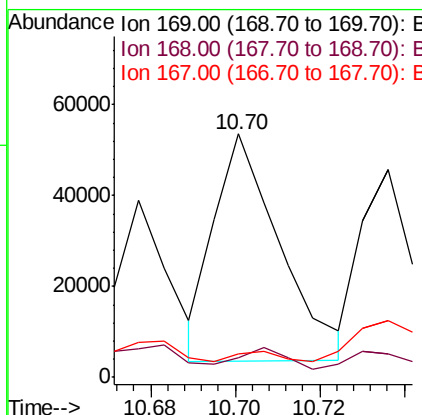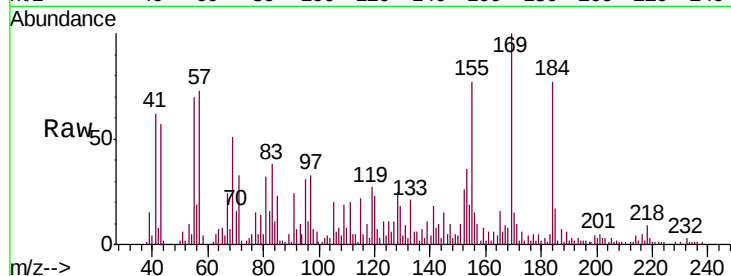

#70
 Phenanthrene
 Concen: 5.200 ng
 RT: 11.57 min Scan# 1569
 Delta R.T. -0.01 min
 Lab File: BF108449.D
 Acq: 24 Aug 2018 5:04

Tgt Ion:178 Resp: 78766
 Ion Ratio Lower Upper
 178 100
 176 21.4 15.8 23.8
 179 27.2 13.0 19.6#

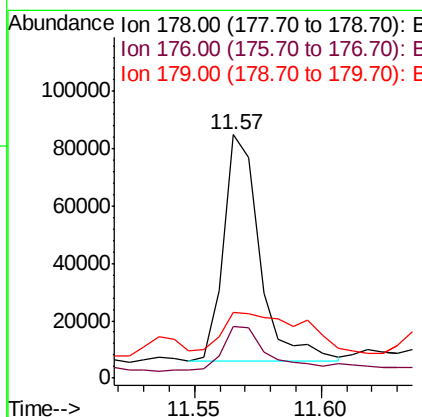

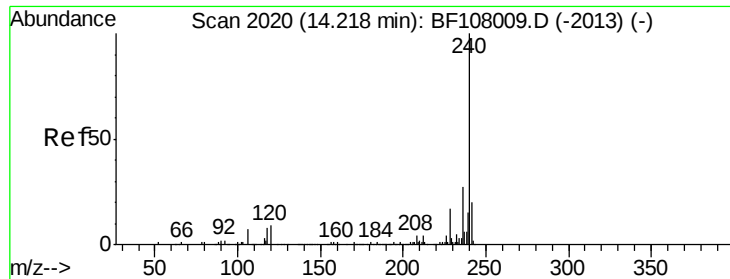

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.21 min Scan# 2018

Delta R.T. 0.01 min

Lab File: BF108449.D

Acq: 24 Aug 2018 5:04

Instrument :

BNA_F

ClientSampleId :

RA-081618-FL-042


Tgt Ion:240 Resp: 260876

Ion Ratio Lower Upper

240 100

120 13.7 9.5 14.3




236 27.6 20.7 31.1

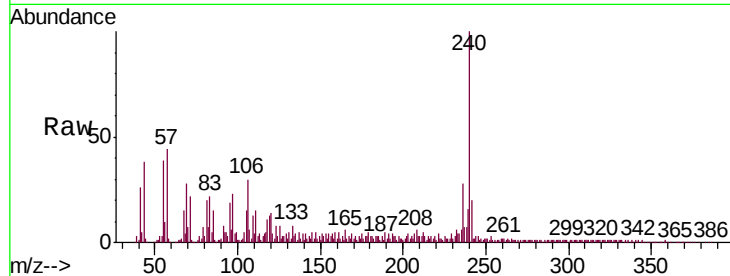

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

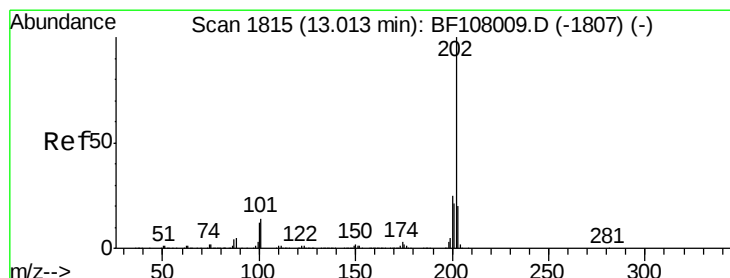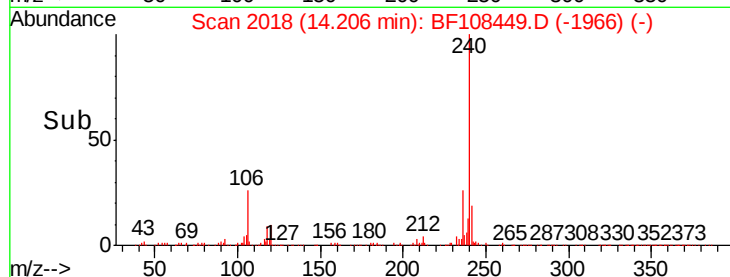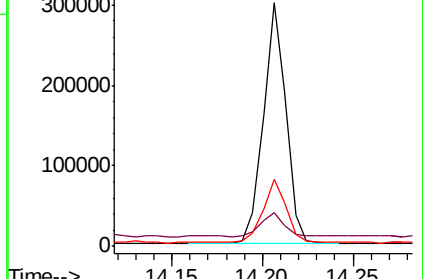

#77

Pyrene

Concen: 2.056 ng

RT: 13.02 min Scan# 1816

Delta R.T. 0.02 min

Lab File: BF108449.D

Acq: 24 Aug 2018 5:04


Tgt Ion:202 Resp: 33951

Ion Ratio Lower Upper

202 100

200 24.4 17.4 26.2



203 98.4 14.3 21.5#

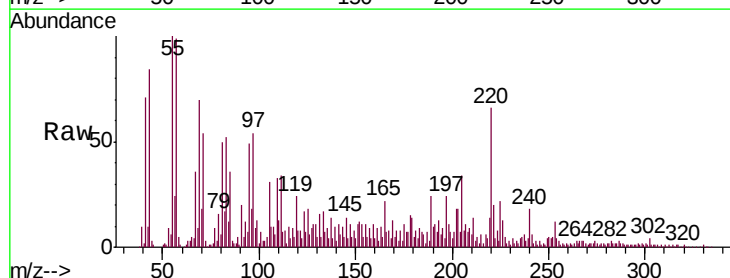


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

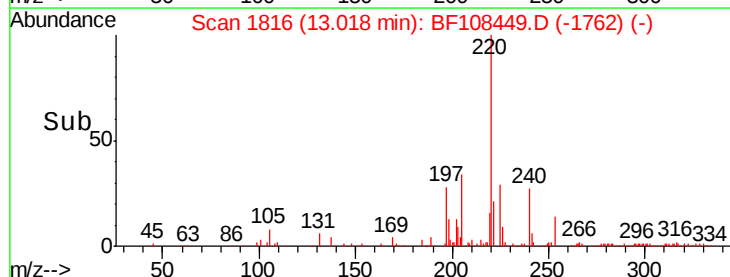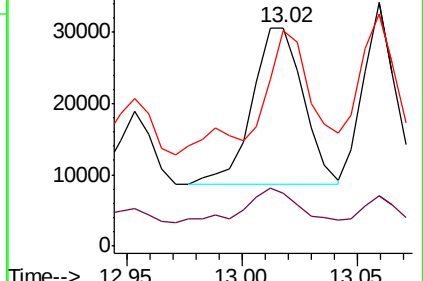

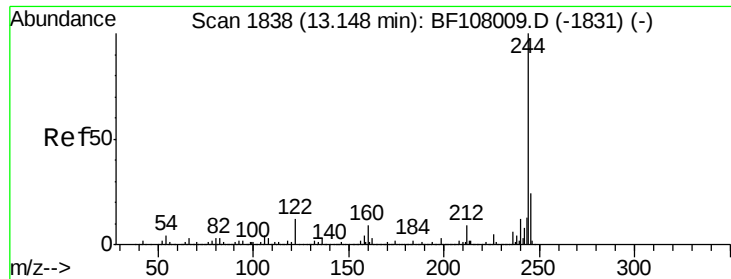

#78

Terphenyl-d14

Concen: 65.172 ng

RT: 13.14 min Scan# 1837

Delta R.T. 0.01 min

Lab File: BF108449.D

Acq: 24 Aug 2018 5:04

Instrument :

BNA_F

ClientSampleId :

RA-081618-FL-042


Tgt Ion:244 Resp: 668688

Ion Ratio Lower Upper

244 100

212 7.7 5.4 8.0




122 9.7 11.0 16.4#



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

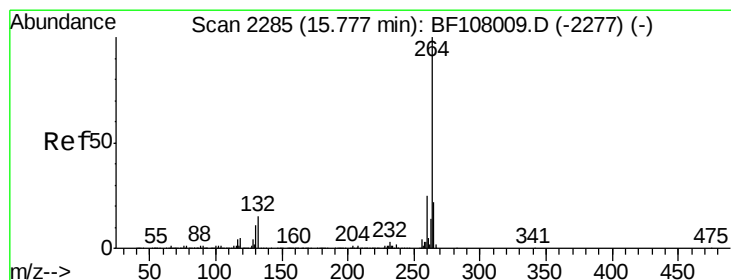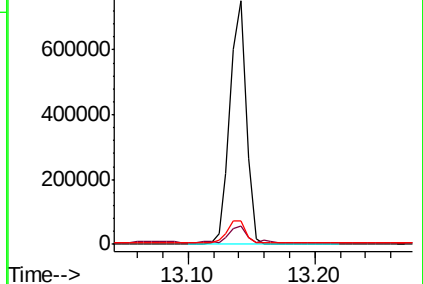

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.77 min Scan# 2284

Delta R.T. 0.01 min

Lab File: BF108449.D

Acq: 24 Aug 2018 5:04


Tgt Ion:264 Resp: 225792

Ion Ratio Lower Upper

264 100

260 23.6 19.2 28.8

265 22.7 17.5 26.3



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

