

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082318\
 Data File : BF108441.D
 Acq On : 24 Aug 2018 00:37
 Operator : JU/SJ
 Sample : J4278-11 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 EO-01-082118-C

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.619	554	558	571	rBV	224746	238819	22.88%	3.246%
2	6.613	723	727	737	rBV	262410	267413	25.62%	3.635%
3	6.766	749	753	760	rVB	311796	263956	25.29%	3.588%
4	7.001	789	793	796	rBV	914068	782092	74.93%	10.630%
5	7.154	815	819	826	rBV	261800	219109	20.99%	2.978%
6	7.554	884	887	894	rBV	147155	160932	15.42%	2.187%
7	8.284	1006	1011	1016	rBV	1207519	981490	94.03%	13.340%
8	9.354	1189	1193	1201	rBV	366356	322309	30.88%	4.381%
9	9.748	1255	1260	1265	rBV	51356	57123	5.47%	0.776%
10	9.954	1291	1295	1299	rVB2	10084	11706	1.12%	0.159%
11	10.042	1304	1310	1320	rBV	1042440	1043831	100.00%	14.188%
12	10.836	1442	1445	1454	rVB	105022	107371	10.29%	1.459%
13	10.936	1457	1462	1466	rVB3	9595	16908	1.62%	0.230%
14	11.542	1561	1565	1568	rBV	919139	871057	83.45%	11.839%
15	11.907	1624	1627	1630	rBV	20077	14846	1.42%	0.202%
16	12.154	1666	1669	1671	rBV2	10713	12025	1.15%	0.163%
17	12.595	1740	1744	1746	rBV	112779	101559	9.73%	1.380%
18	12.619	1746	1748	1753	rVB3	69719	65704	6.29%	0.893%
19	12.701	1760	1762	1766	rVB2	13499	13233	1.27%	0.180%
20	12.760	1769	1772	1775	rBV	54814	50177	4.81%	0.682%
21	12.989	1805	1811	1816	rBV	61919	76239	7.30%	1.036%
22	13.118	1830	1833	1837	rBV	251582	228473	21.89%	3.105%
23	14.195	2011	2016	2019	rBV	779446	809396	77.54%	11.001%
24	15.748	2275	2280	2287	rVB	475678	641630	61.47%	8.721%


Sum of corrected areas: 7357398

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082318\
Data File : BF108441.D
Acq On : 24 Aug 2018 00:37
Operator : JU/SJ
Sample : J4278-11 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EO-01-082118-C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

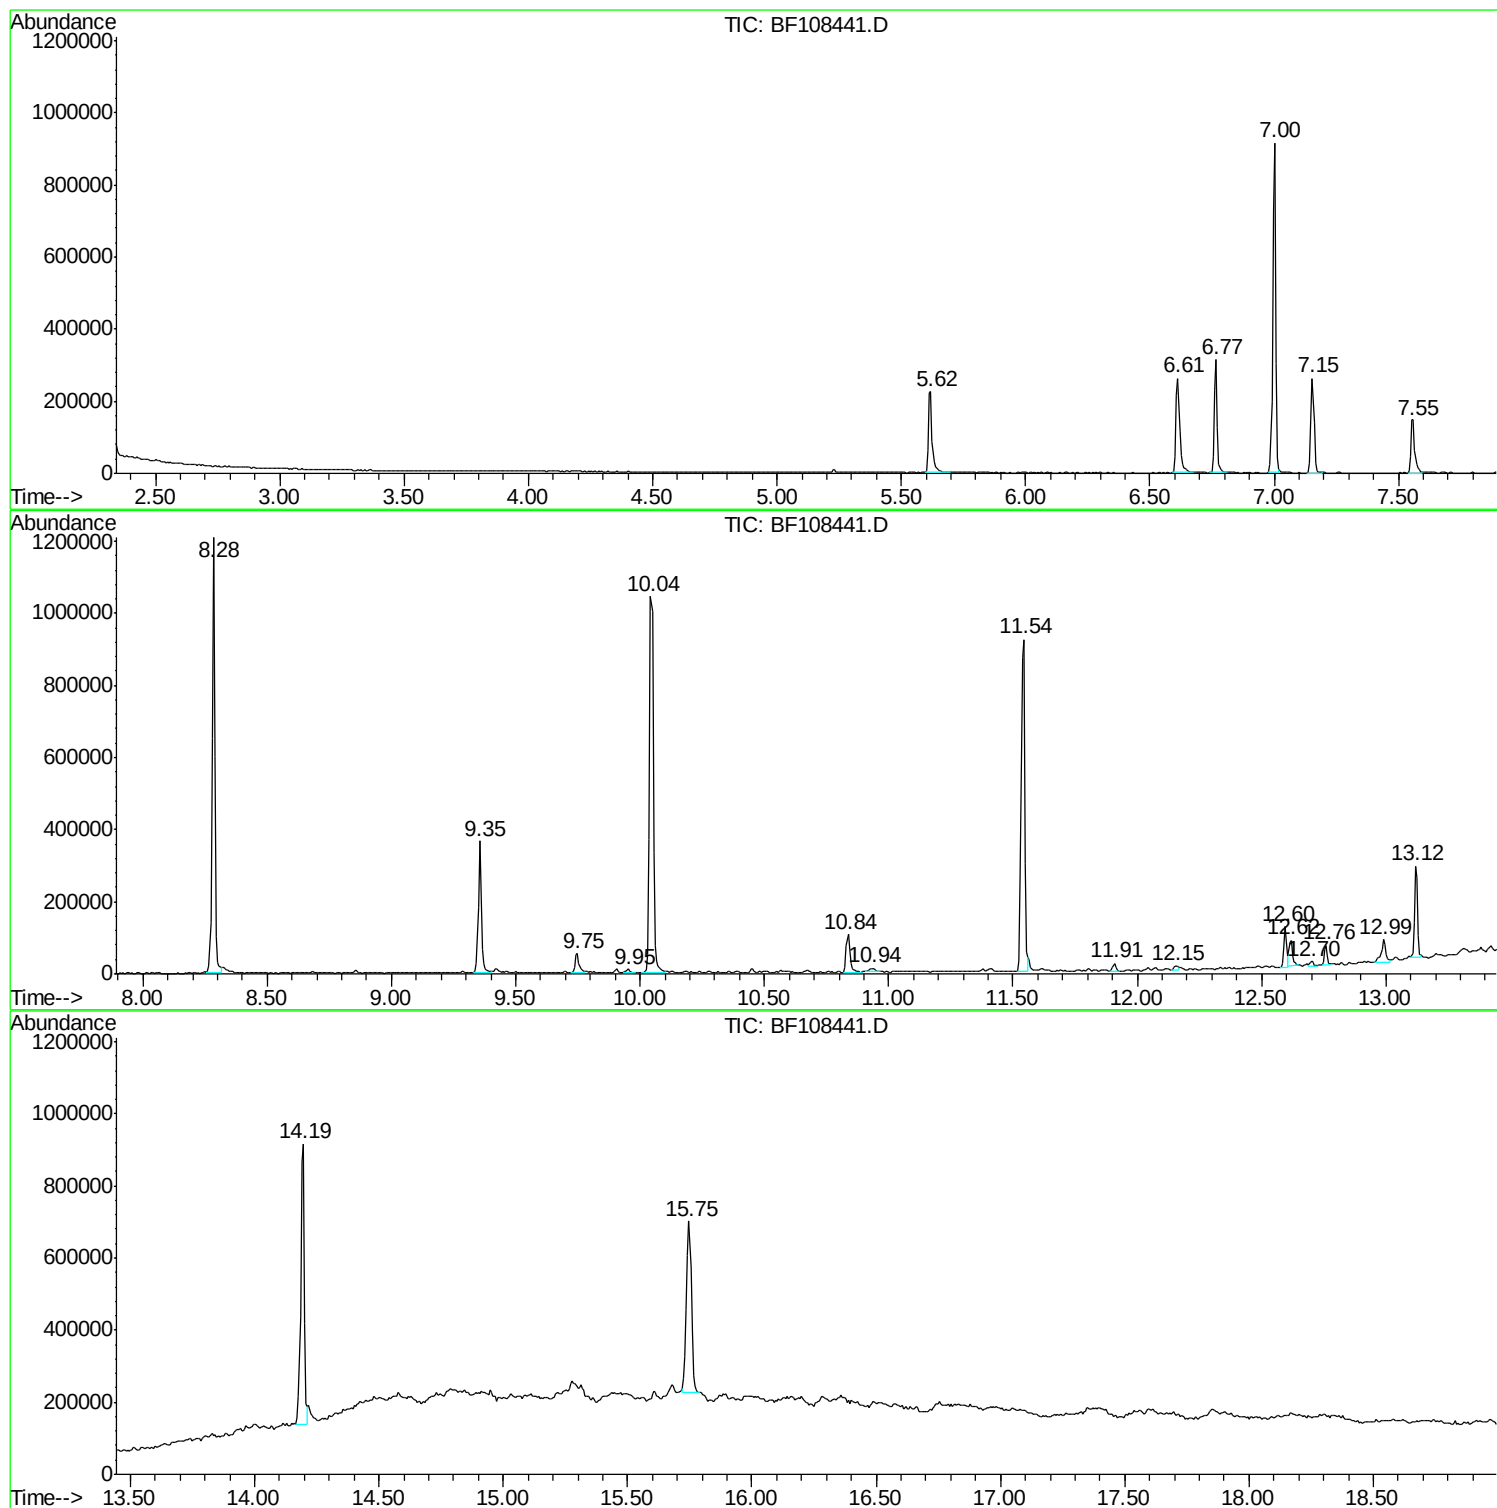

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082318\
Data File : BF108441.D
Acq On : 24 Aug 2018 00:37
Operator : JU/SJ
Sample : J4278-11 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EO-01-082118-C










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.77 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.77	6.75 ng	263956	1,4-Dichlorobenzene-d4	7.00

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3			Tranvlcypromine-propionyl	189	C12H15NO	1000123-86-3	10
4			Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5			2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

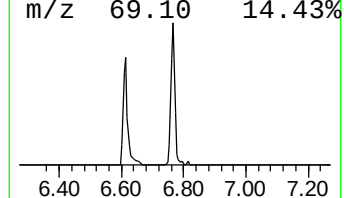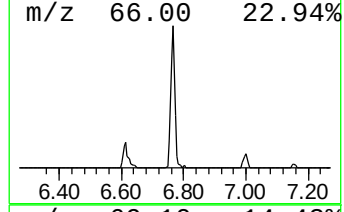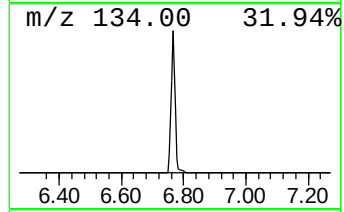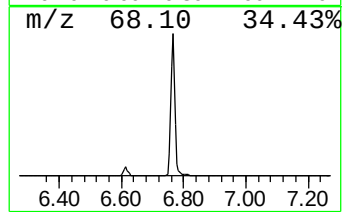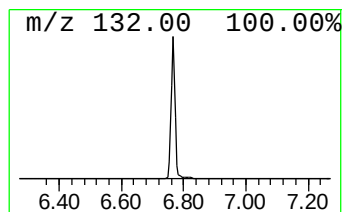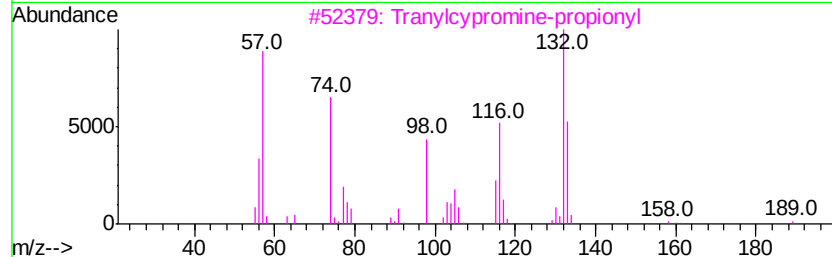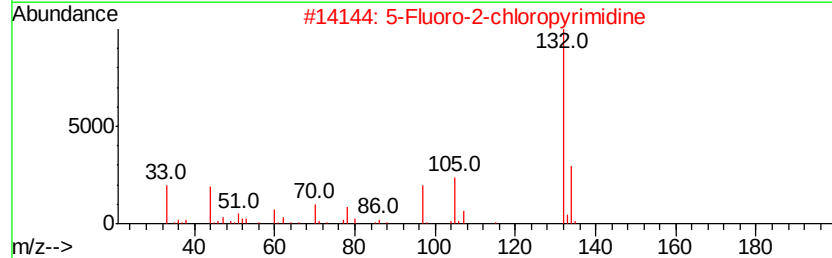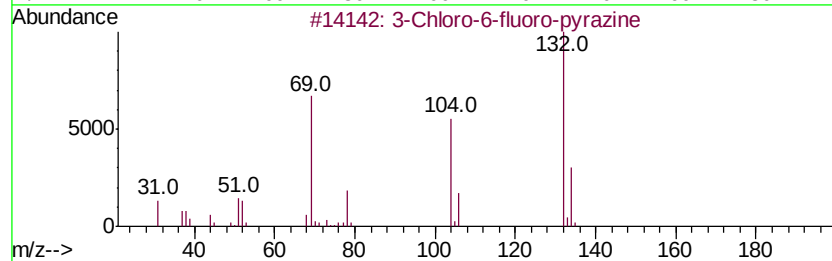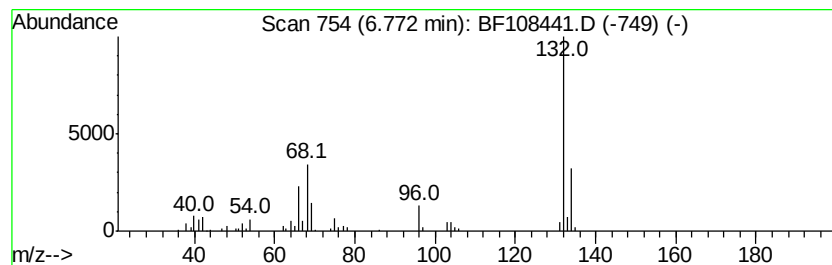

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082318\
Data File : BF108441.D
Acq On : 24 Aug 2018 00:37
Operator : JU/SJ
Sample : J4278-11 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
EO-01-082118-C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Cyclodecene Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.	
12.60	2.33 ng	101559	Phenanthrene-d10	11.54	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Cyclodecene	138	C10H18	003618-12-0	93
2	2-Chloroethyl linoleate	342	C20H35ClO2	025525-76-2	90
3	8-Hexadecyne	222	C16H30	019781-86-3	83
4	3,4-Octadiene, 7-methyl-	124	C9H16	037050-05-8	81
5	Cyclodecene, (Z)-	138	C10H18	000935-31-9	76

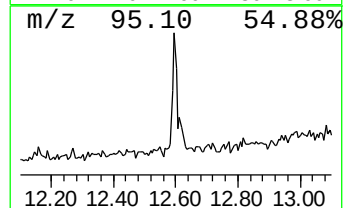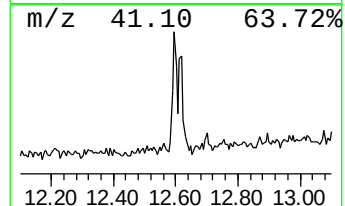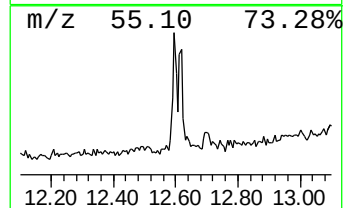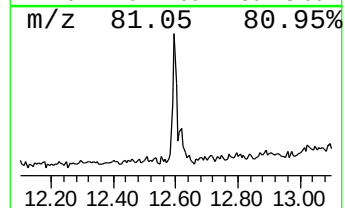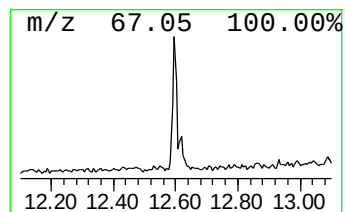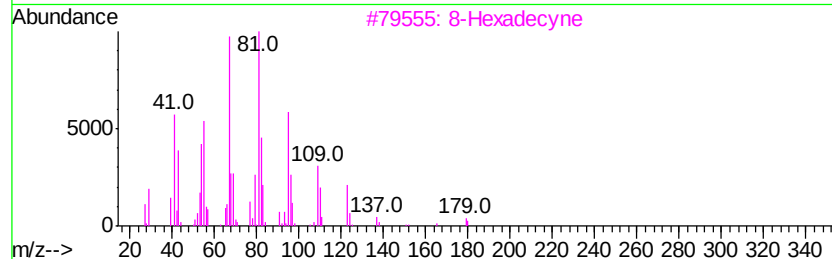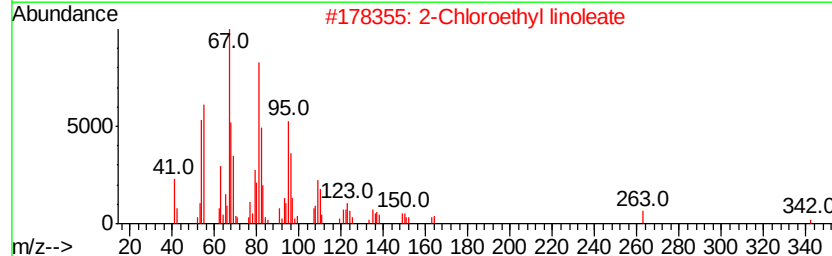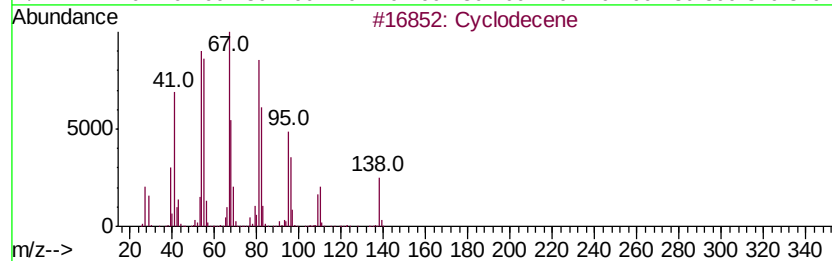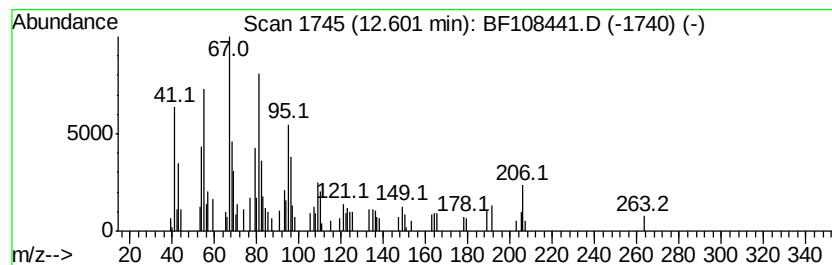

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082318\
Data File : BF108441.D
Acq On : 24 Aug 2018 00:37
Operator : JU/SJ
Sample : J4278-11 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EO-01-082118-C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.77	6.77	6.8	ng	263956	1	7.00	782092	20.0
Cyclodecene	12.60	2.3	ng	101559	4	11.54	871057	20.0