


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082323\
Data File : BF134892.D
Acq On : 23 Aug 2023 08:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Aug 22 19:33:25 2023

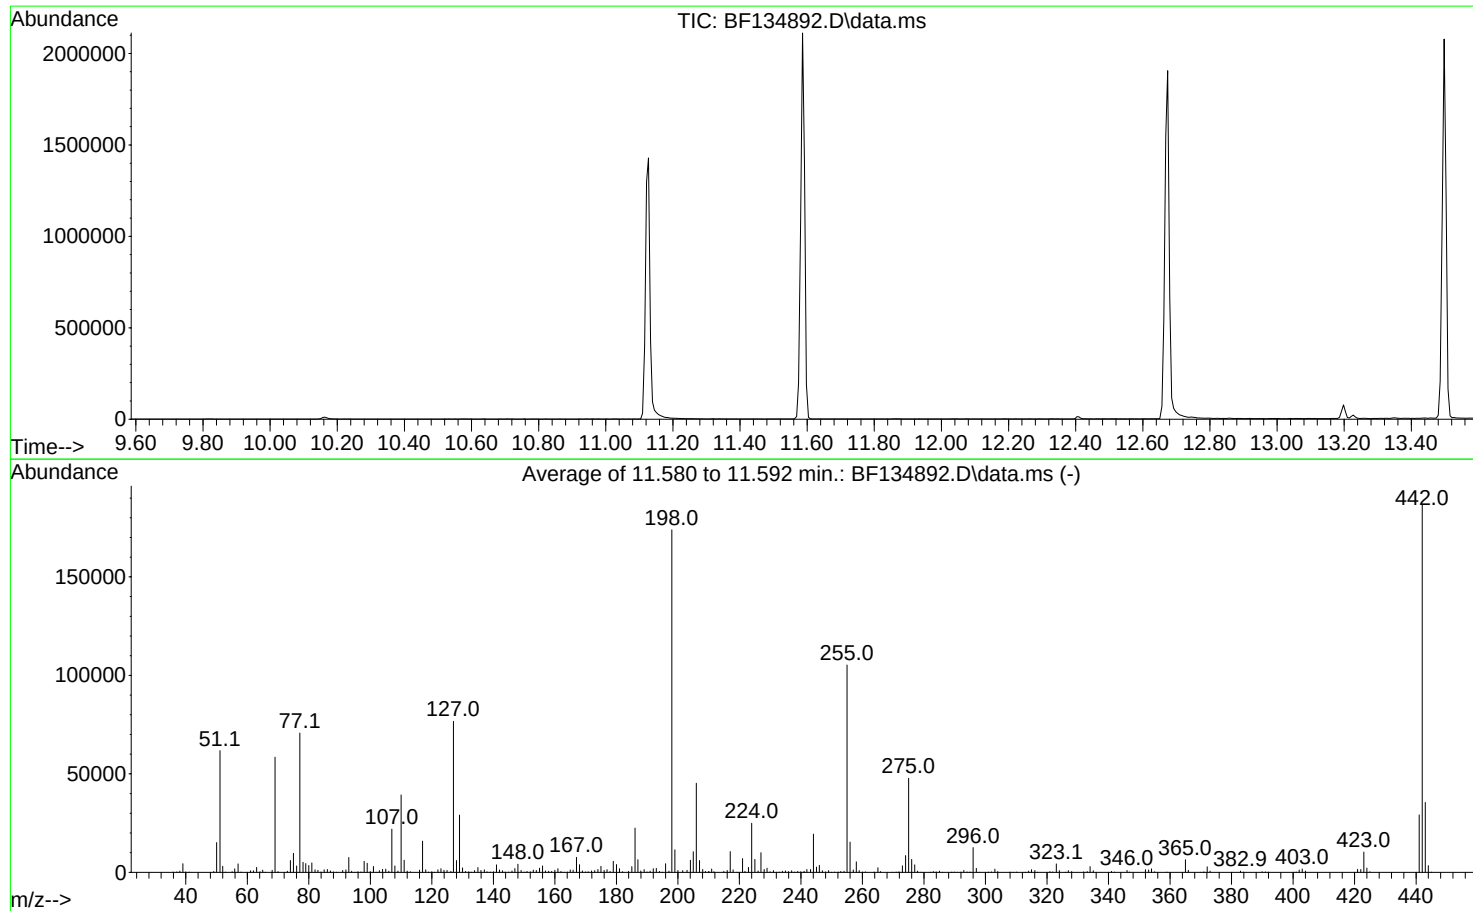




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	61861	PASS
68	69	0.00	2	1.9	1098	PASS
69	198	0.00	100	33.6	58469	PASS
70	69	0.00	2	0.5	276	PASS
127	198	10	80	44.1	76725	PASS
197	198	0.00	2	0.4	670	PASS
198	198	100	100	100.0	173947	PASS
199	198	5	9	6.6	11464	PASS
275	198	10	60	27.5	47763	PASS
365	198	1	100	3.7	6410	PASS
441	198	0.01	100	16.8	29182	PASS
442	442	50	100	100.0	186749	PASS
443	442	15	24	19.0	35527	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082323\
Data File : BF134892.D
Acq On : 23 Aug 2023 08:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 23 10:36:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 22 19:33:25 2023
Response via : Initial Calibration

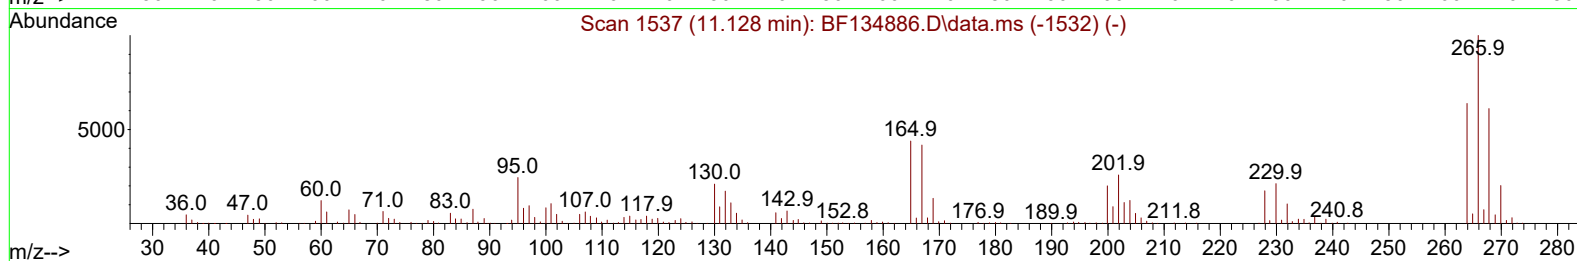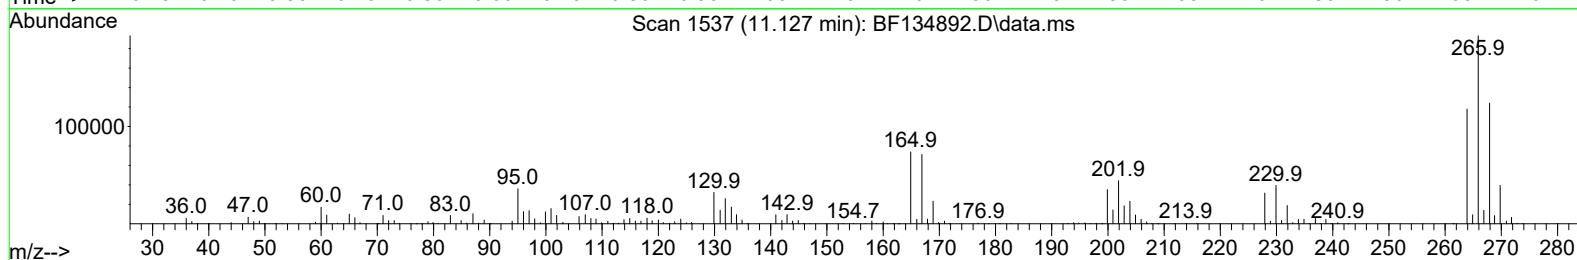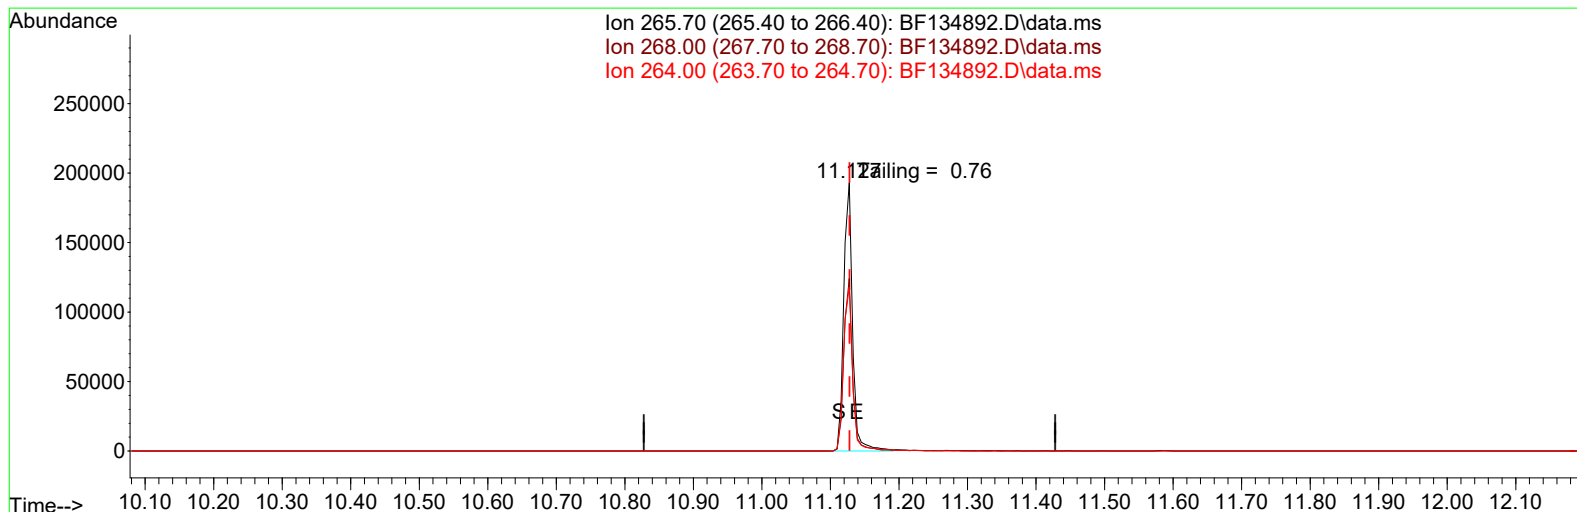

TIC: BF134892.D\data.ms

(70) Pentachlorophenol (C)

11.127min (-0.001) 394721.14 ng




response 171967

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	64.24
264.00	63.80	61.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082323\
Data File : BF134892.D
Acq On : 23 Aug 2023 08:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 23 10:36:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 22 19:33:25 2023
Response via : Initial Calibration

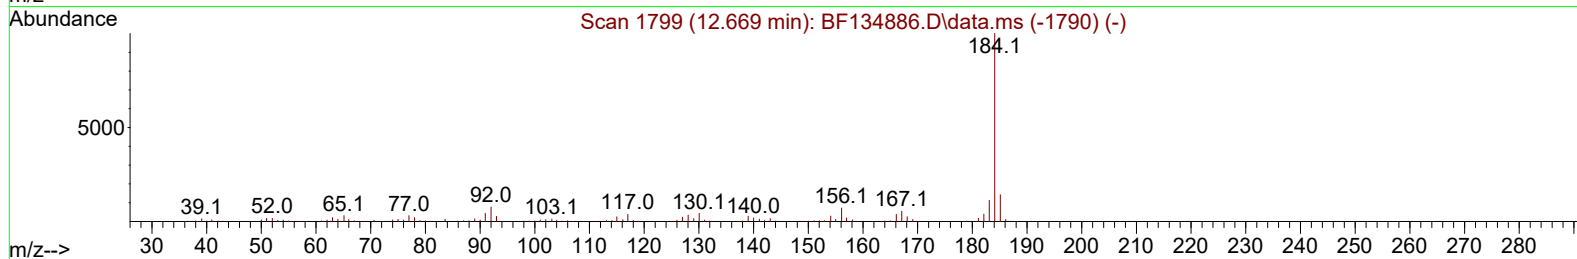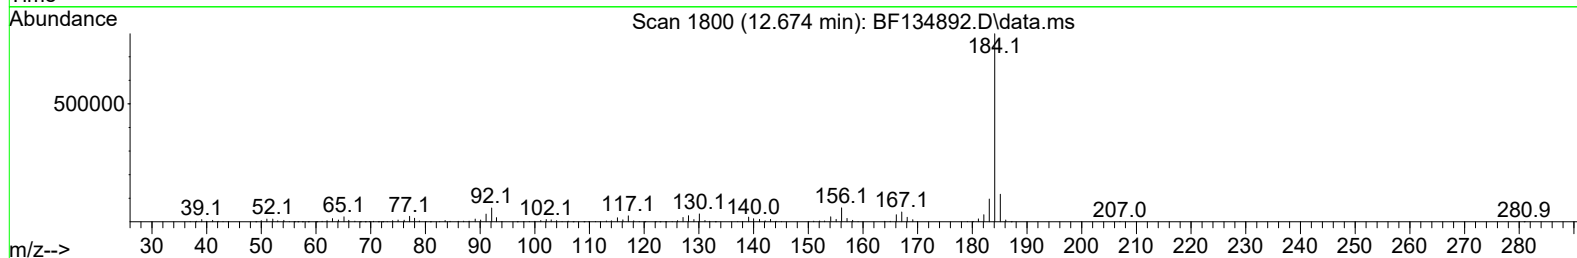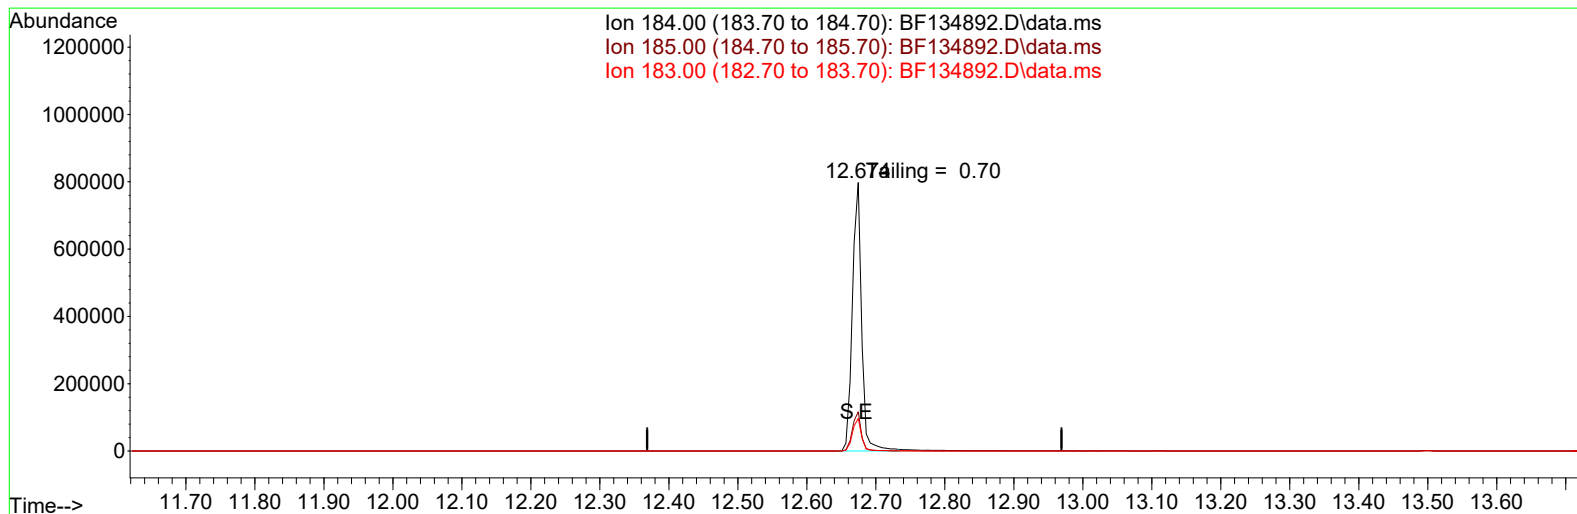

TIC: BF134892.D\data.ms

(77) Benzidine

12.674min (+ 0.005) 9555.40 ng

response 741222

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.63
183.00	11.20	12.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/23/2023	BNA_F	<u>BF134892.D</u>
Compound Name	Response	Retention Time
DDT	345828	13.498
DDD	16098	13.198
DDE	478	12.863
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16576	362404	4.57

Instrument :
BNA_F
ClientSampleId :
DFTPP