
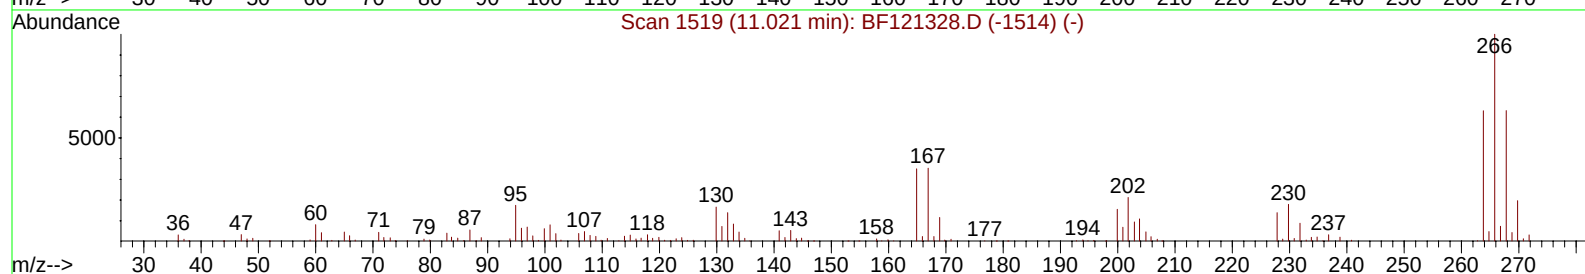
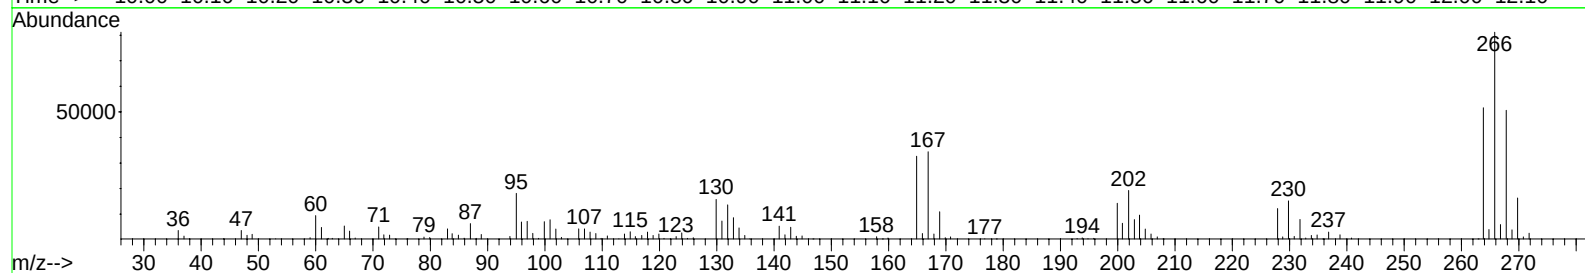


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082420\
 Data File : BF121390.D
 Acq On : 24 Aug 2020 9:22
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 18:58:59 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF081920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 20 04:56:10 2020
 Response via : Initial Calibration

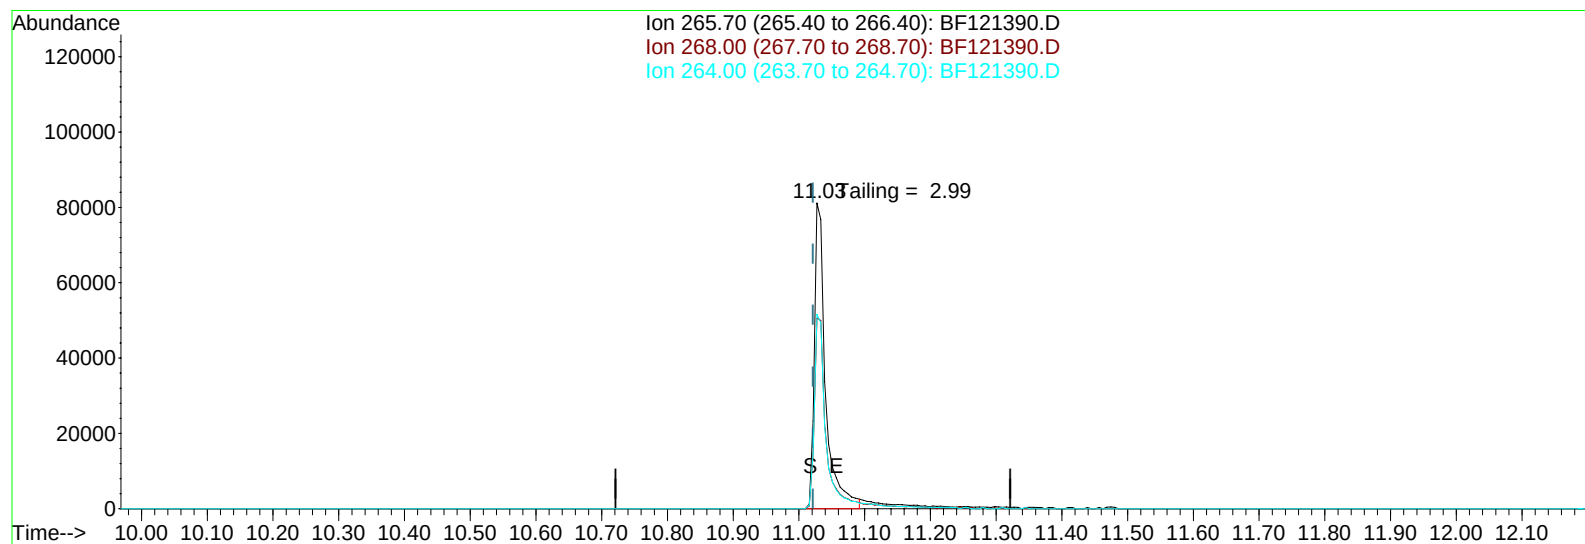

TIC: BF121390.D

(70) Pentachlorophenol (C)




11.027min (+0.006) 134635.13ng

response 104934

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	62.37
264.00	63.10	63.57
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082420\
 Data File : BF121390.D
 Acq On : 24 Aug 2020 9:22
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 18:58:59 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF081920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 20 04:56:10 2020
 Response via : Initial Calibration

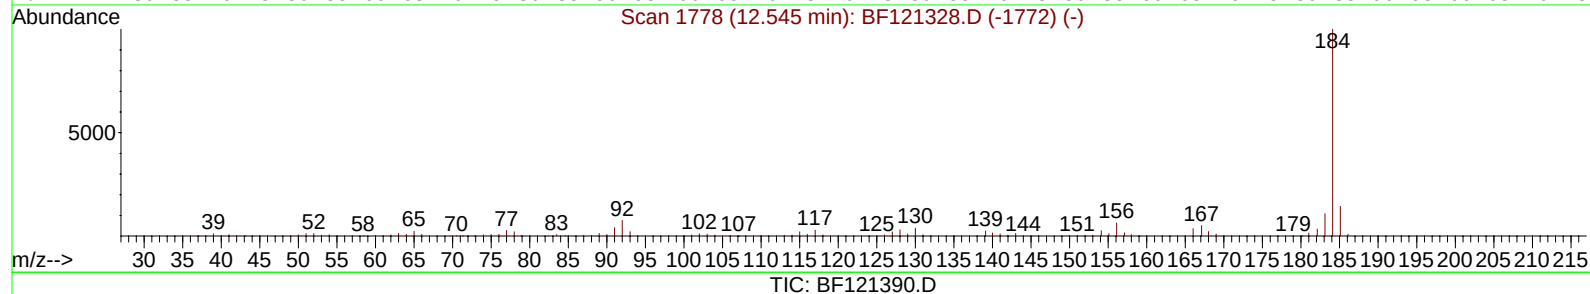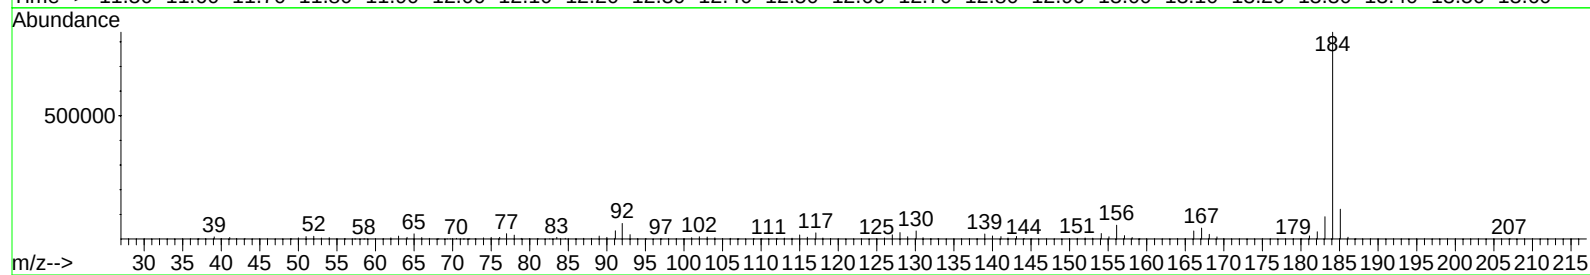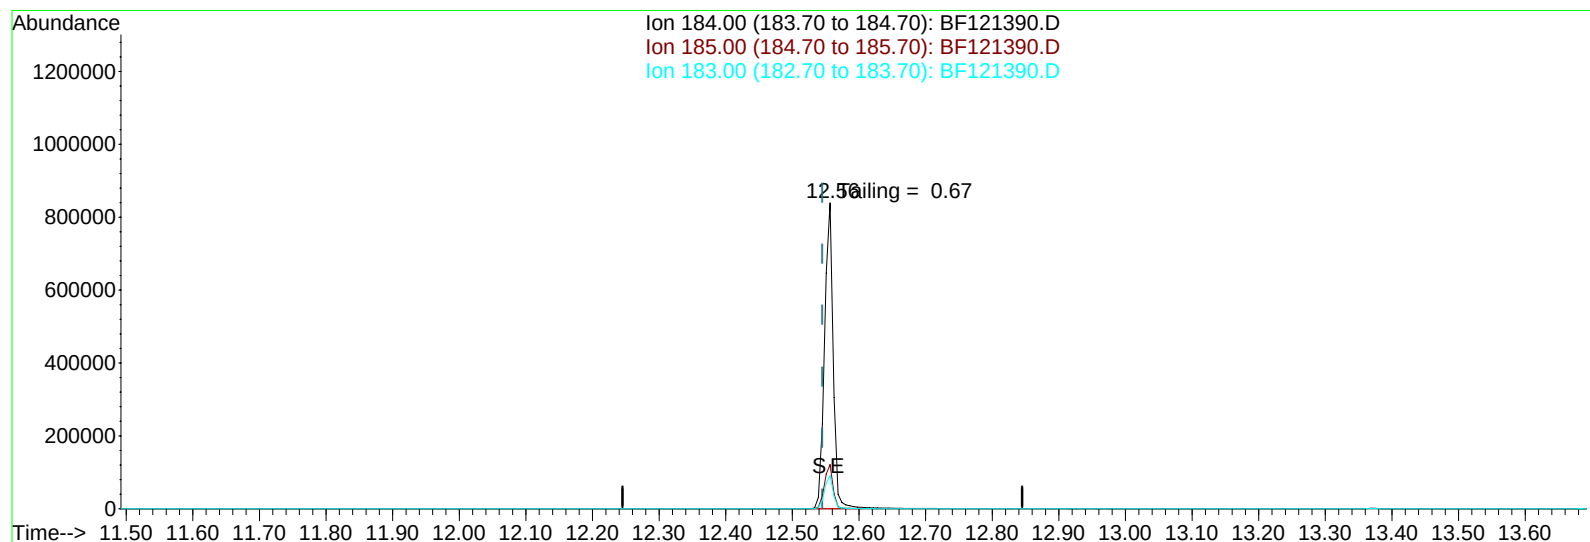

(77) Benzidine

12.557min (+0.012) 88037.82ng

response 766458

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	14.47
183.00	10.90	10.83
0.00	0.00	0.00