
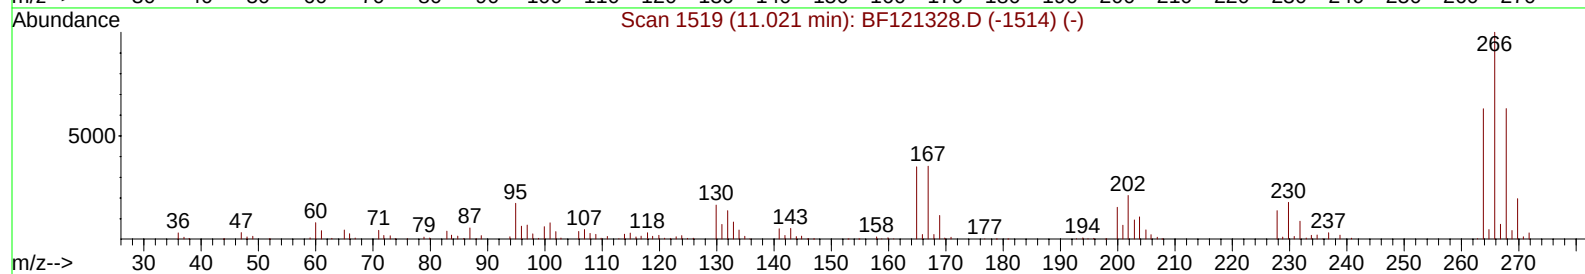
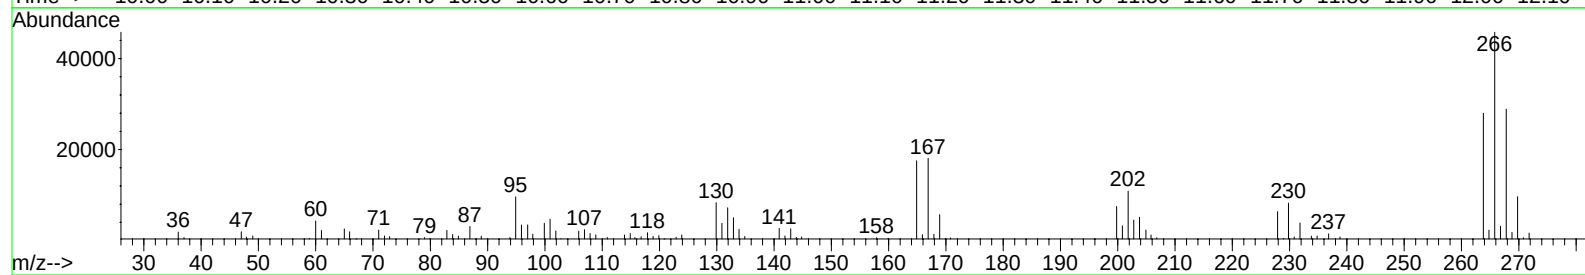


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082420\
Data File : BF121401.D
Acq On : 24 Aug 2020 16:04
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 19:01:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF081920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 20 04:56:10 2020
Response via : Initial Calibration

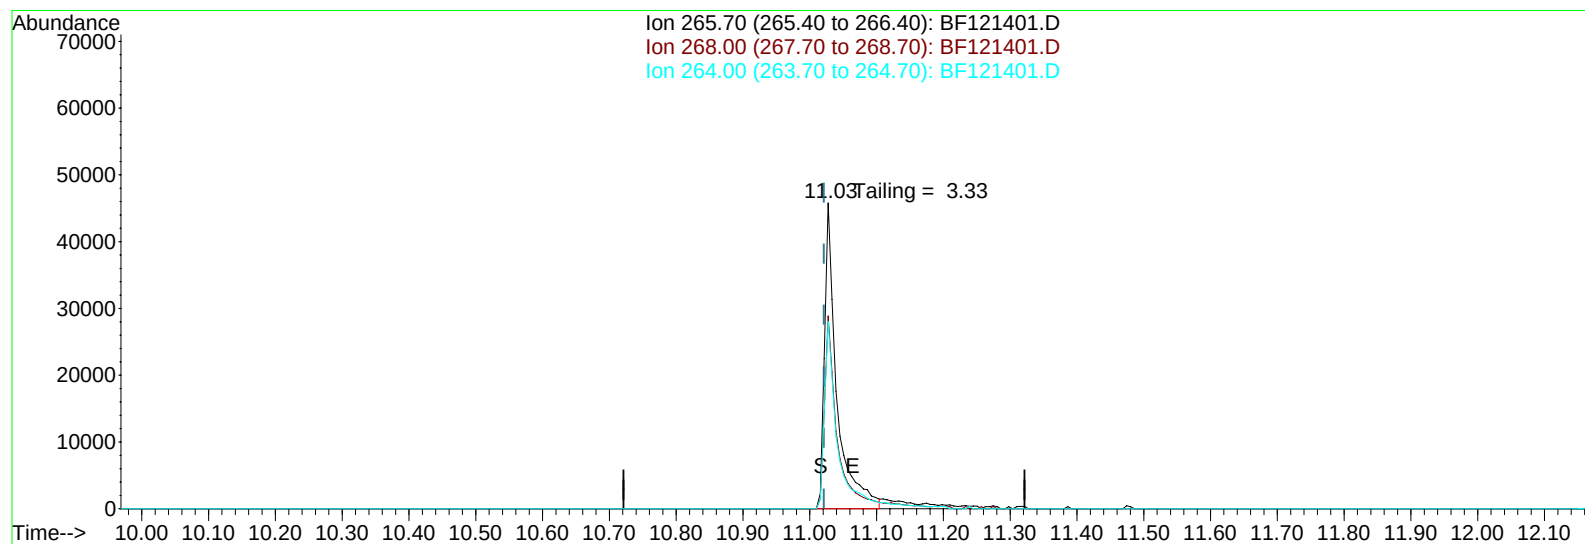

TIC: BF121401.D

(70) Pentachlorophenol (C)




11.028min (+0.006) 45215.10ng

response 62764

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	63.07
264.00	63.10	61.16
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082420\
Data File : BF121401.D
Acq On : 24 Aug 2020 16:04
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 19:01:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF081920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 20 04:56:10 2020
Response via : Initial Calibration

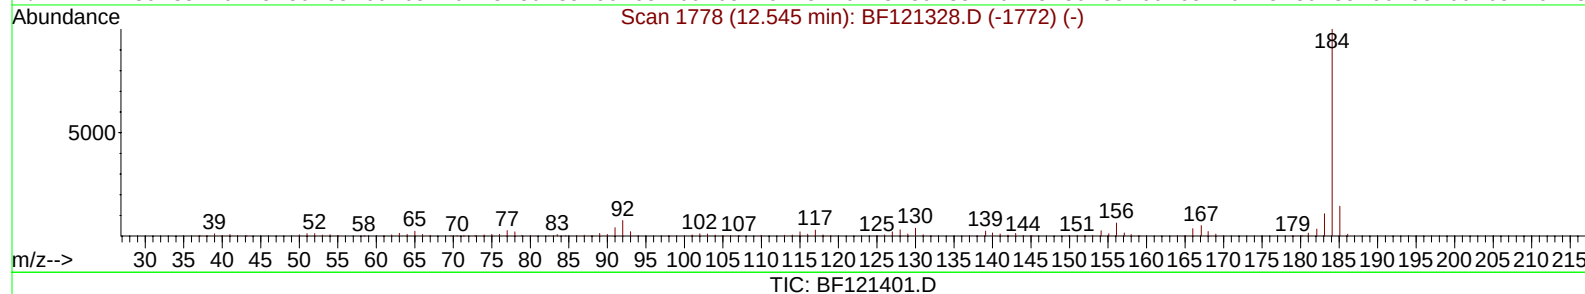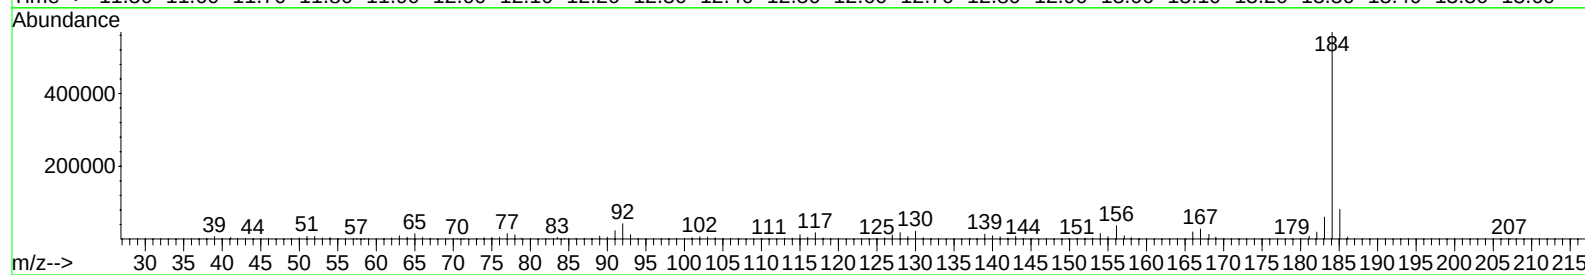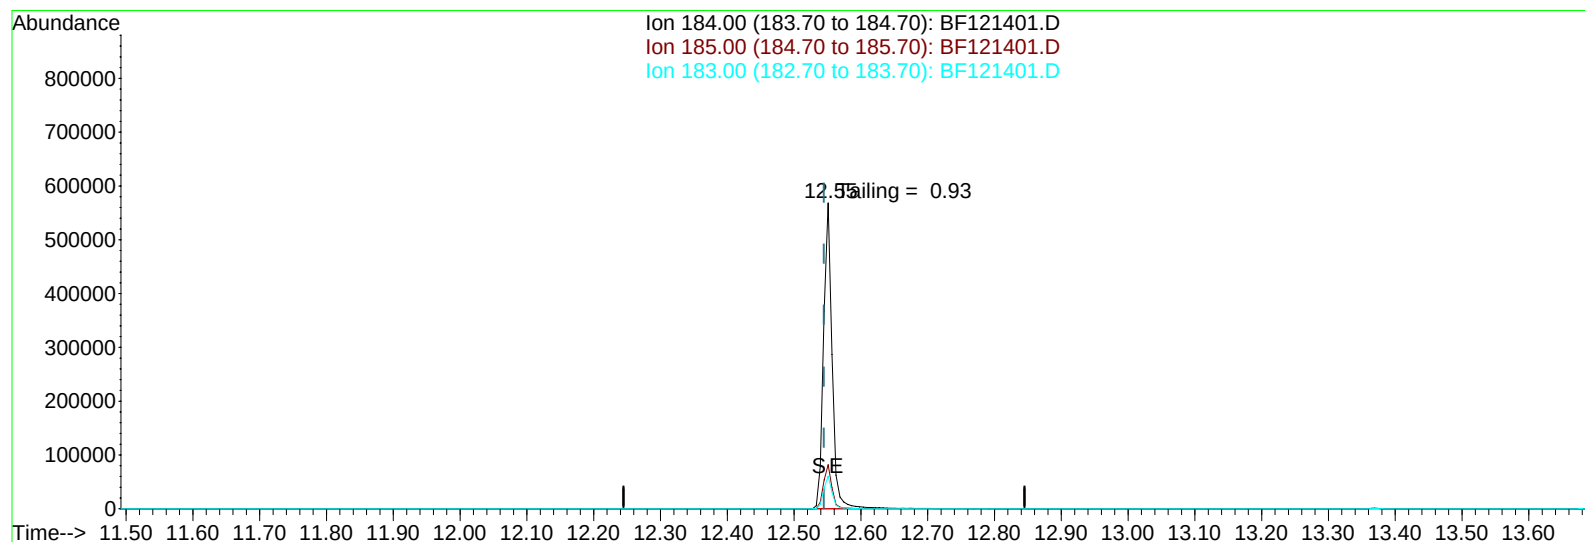

(77) Benzidine

12.551min (+0.006) 0.00ng

response 510601

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	14.39
183.00	10.90	10.67
0.00	0.00	0.00