


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082420\
 Data File : BF121390.D
 Acq On : 24 Aug 2020 9:22
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 20 04:56:10 2020

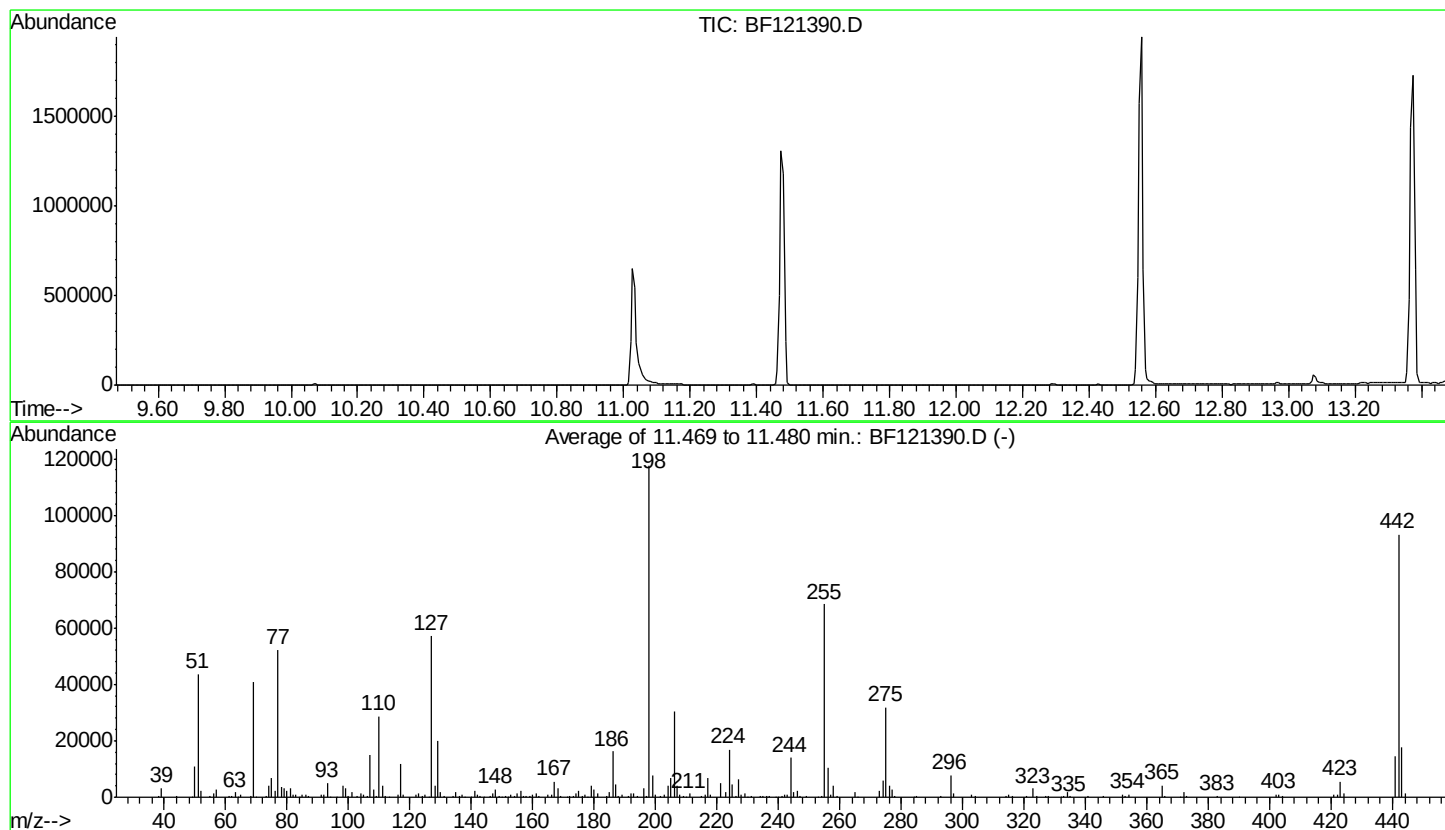

AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	43618	PASS
68	69	0.00	2	1.6	658	PASS
69	198	0.00	100	34.7	40786	PASS
70	69	0.00	2	0.3	109	PASS
127	198	10	80	48.7	57186	PASS
197	198	0.00	2	0.3	365	PASS
198	198	100	100	100.0	117528	PASS
199	198	5	9	6.8	7937	PASS
275	198	10	60	27.1	31801	PASS
365	198	1	100	3.5	4108	PASS
441	198	0.01	100	12.5	14697	PASS
442	198	50	100	79.3	93162	PASS
443	442	15	24	19.1	17749	PASS