

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082423\
 Data File : BF134932.D
 Acq On : 24 Aug 2023 19:24
 Operator : CG\JU
 Sample : 04116-05 2X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-3

Quant Time: Aug 25 01:22:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 22 19:33:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.792	152	95089	20.000	ng	0.00
21) Naphthalene-d8	8.075	136	325765	20.000	ng	0.00
39) Acenaphthene-d10	9.833	164	149781	20.000	ng	0.00
64) Phenanthrene-d10	11.327	188	304443	20.000	ng	0.00
76) Chrysene-d12	13.986	240	215188	20.000	ng	0.00
86) Perylene-d12	15.468	264	168092	20.000	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.422	112	245105	41.104	ng	0.00
7) Phenol-d6	6.428	99	286093	37.547	ng	-0.01
23) Nitrobenzene-d5	7.351	82	154946	26.209	ng	-0.01
42) 2,4,6-Tribromophenol	10.622	330	72327	41.001	ng	0.00
45) 2-Fluorobiphenyl	9.151	172	283709	29.282	ng	0.00
79) Terphenyl-d14	12.921	244	356171	22.765	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propyla...	7.351	70	20325	4.567	ng	# 78
20) 3+4-Methylphenols	7.216	107	53	Below Cal	#	1
25) Isophorone	7.351	82	152337	13.800	ng	# 64
50) Dimethylphthalate	9.833	163	30814	2.890	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082423\
Data File : BF134932.D
Acq On : 24 Aug 2023 19:24
Operator : CG\JU
Sample : 04116-05 2X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-3

Quant Time: Aug 25 01:22:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 22 19:33:25 2023
Response via : Initial Calibration




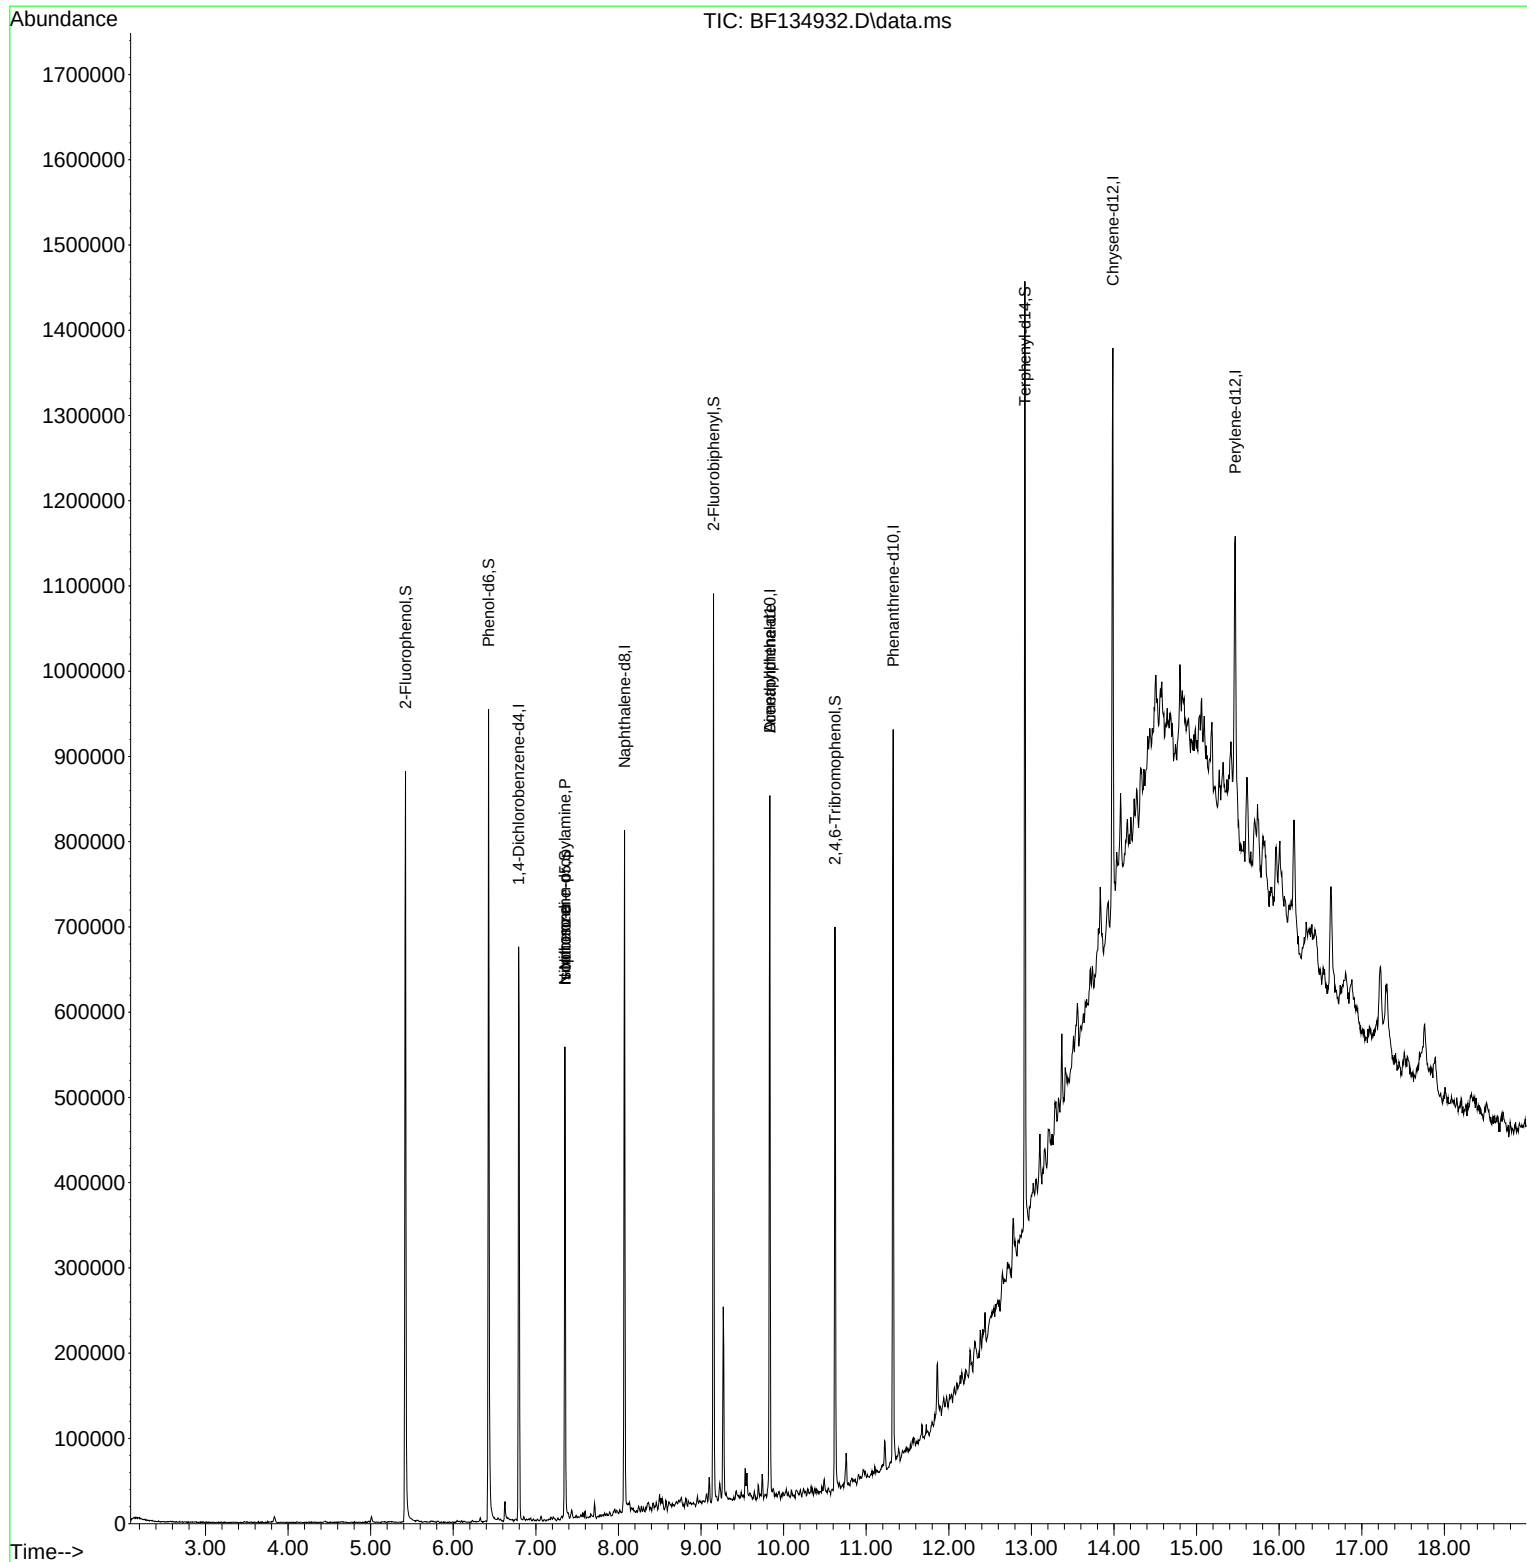




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.792 min Scan# 800
Delta R.T. -0.001 min
Lab File: BF134932.D
Acq: 24 Aug 2023 19:24




Instrument :
BNA_F
ClientSampleId :
TP-3


Tgt Ion:152 Resp: 95089
Ion Ratio Lower Upper
152 100
150 156.4 126.1 189.1
115 66.7 51.1 76.7

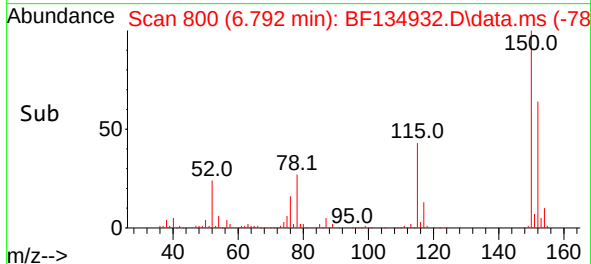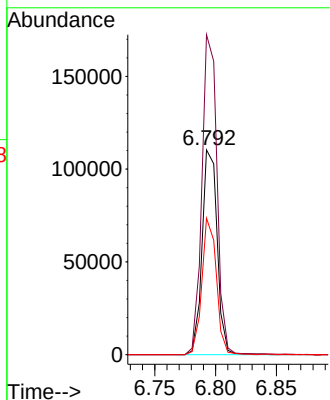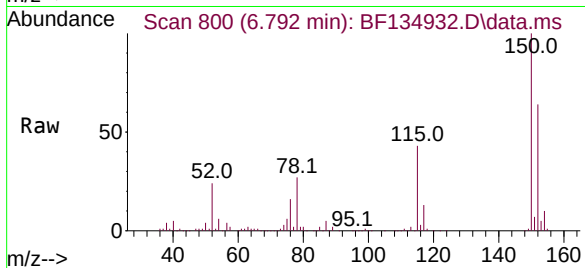

#5
2-Fluorophenol
Concen: 41.104 ng
RT: 5.422 min Scan# 567
Delta R.T. -0.000 min
Lab File: BF134932.D
Acq: 24 Aug 2023 19:24

Tgt Ion:112 Resp: 245105
Ion Ratio Lower Upper
112 100
64 56.7 48.6 73.0
63 30.3 25.7 38.5


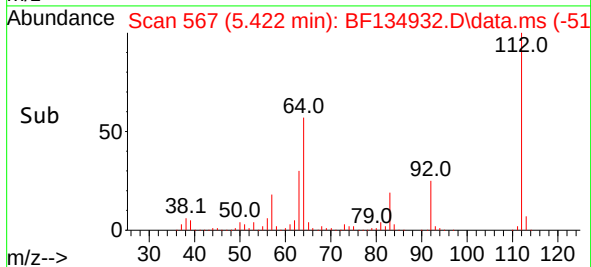
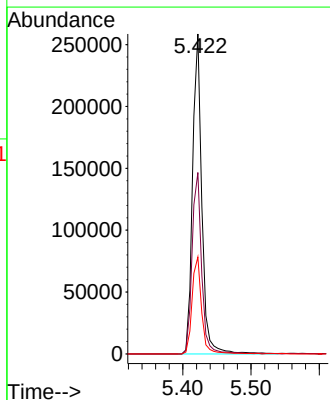
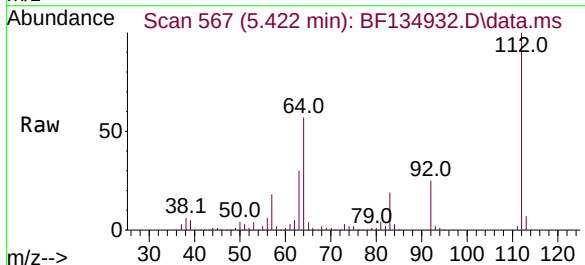


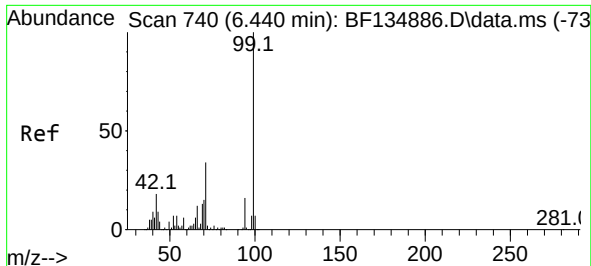

#7
Phenol-d6
Concen: 37.547 ng
RT: 6.428 min Scan# 740
Delta R.T. -0.012 min
Lab File: BF134932.D
Acq: 24 Aug 2023 19:24




Instrument :
BNA_F
ClientSampleId :
TP-3


Tgt Ion:	99	Resp:	286093
Ion	Ratio	Lower	Upper
99	100		
42	18.6	14.6	22.0
71	35.2	27.6	41.4

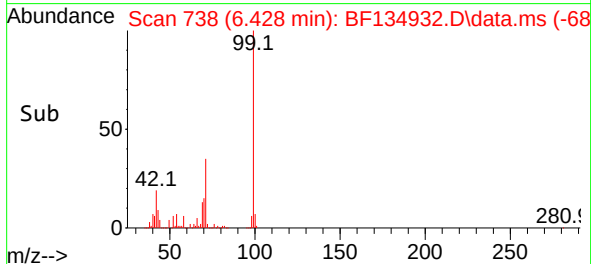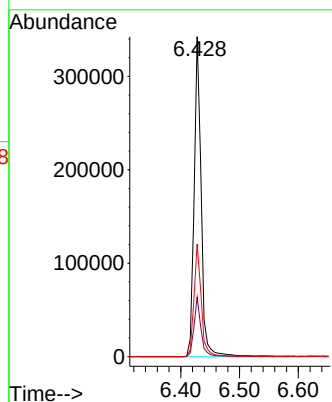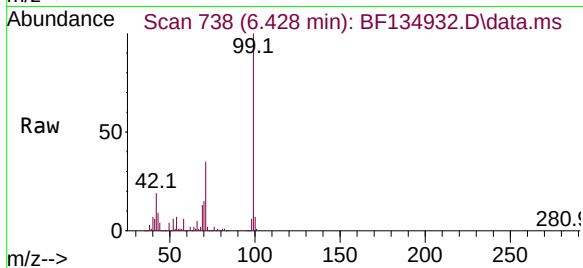

#19
n-Nitroso-di-n-propylamine
Concen: 4.567 ng
RT: 7.351 min Scan# 895
Delta R.T. 0.135 min
Lab File: BF134932.D
Acq: 24 Aug 2023 19:24

Tgt Ion:	70	Resp:	20325
Ion	Ratio	Lower	Upper
70	100		
42	47.8	46.9	70.3
101	0.0	7.5	11.3#
130	2.0	16.9	25.3#


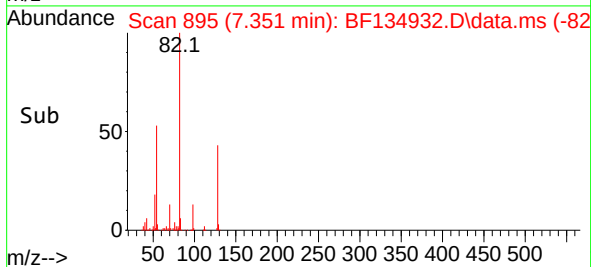
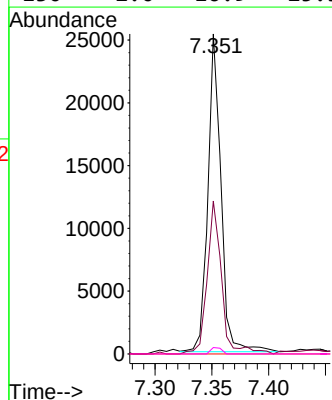
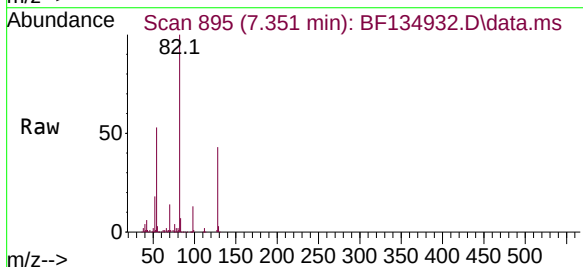


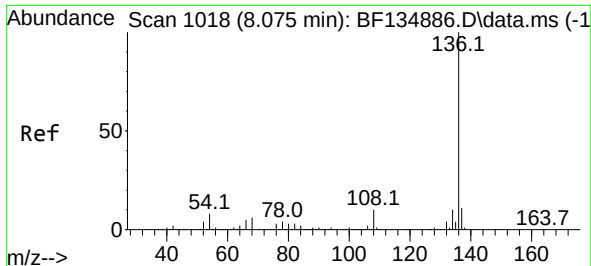

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.075 min Scan# 10
Delta R.T. -0.000 min
Lab File: BF134932.D
Acq: 24 Aug 2023 19:24




Instrument :
BNA_F
ClientSampleId :
TP-3


Tgt Ion:136 Resp: 325765
Ion Ratio Lower Upper
136 100
137 10.7 8.9 13.3
54 7.8 6.6 9.8
68 5.6 5.0 7.4

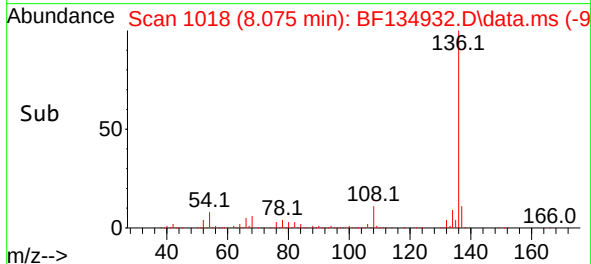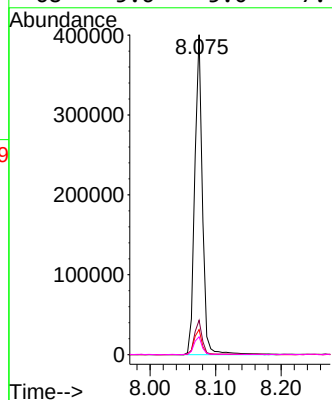

#23
Nitrobenzene-d5
Concen: 26.209 ng
RT: 7.351 min Scan# 895
Delta R.T. -0.012 min
Lab File: BF134932.D
Acq: 24 Aug 2023 19:24

Tgt Ion: 82 Resp: 154946
Ion Ratio Lower Upper
82 100
128 42.6 36.6 54.8
54 52.8 42.6 63.8


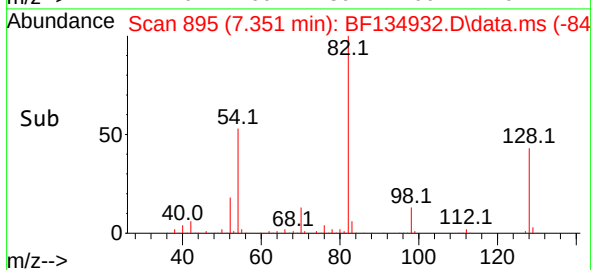
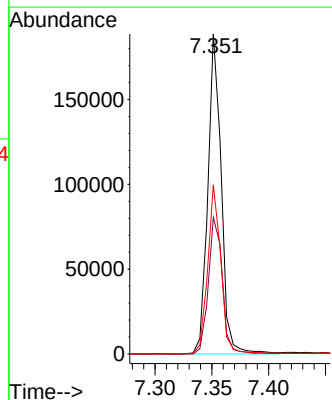
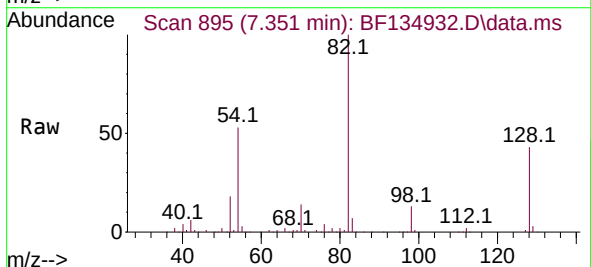


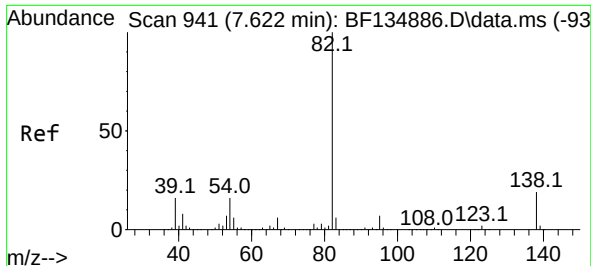

#25
Isophorone
Concen: 13.800 ng
RT: 7.351 min Scan# 89
Delta R.T. -0.271 min
Lab File: BF134932.D
Acq: 24 Aug 2023 19:24




Instrument :
BNA_F
ClientSampleId :
TP-3


Tgt Ion: 82 Resp: 152337
Ion Ratio Lower Upper
82 100
95 0.1 5.9 8.9#
138 0.0 14.9 22.3#

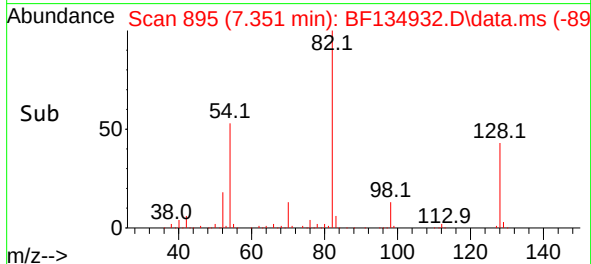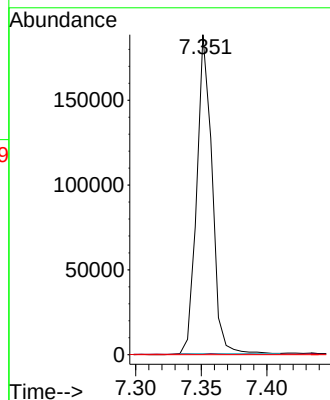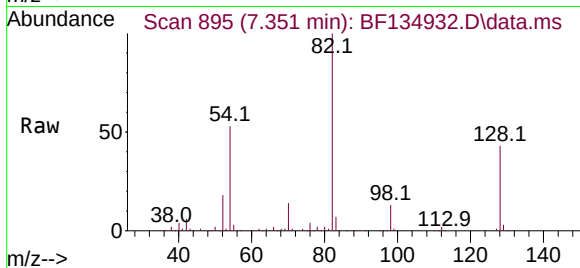

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.833 min Scan# 1317
Delta R.T. -0.000 min
Lab File: BF134932.D
Acq: 24 Aug 2023 19:24

Tgt Ion:164 Resp: 149781
Ion Ratio Lower Upper
164 100
162 103.0 82.6 123.8
160 47.7 37.0 55.4

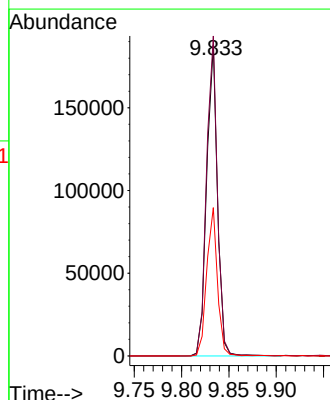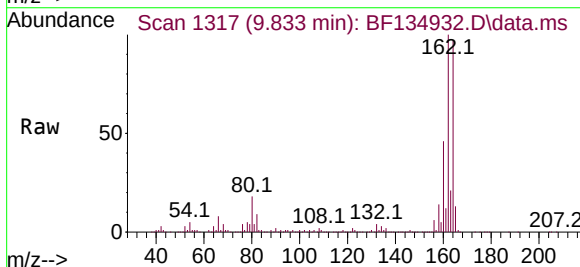



#42

2,4,6-Tribromophenol

Concen: 41.001 ng

RT: 10.622 min Scan# 1452

Delta R.T. -0.006 min

Lab File: BF134932.D

Acq: 24 Aug 2023 19:24

Instrument :

BNA_F

ClientSampleId :

TP-3





Tgt Ion:330 Resp: 72327

Ion Ratio Lower Upper

330 100

332 96.4 76.3 114.5

141 31.7 23.4 35.2

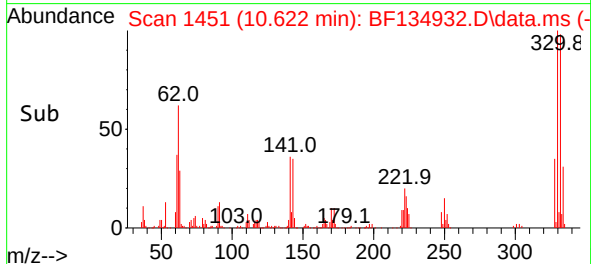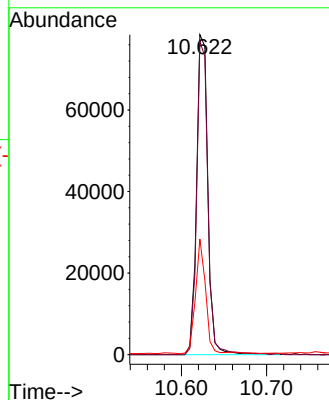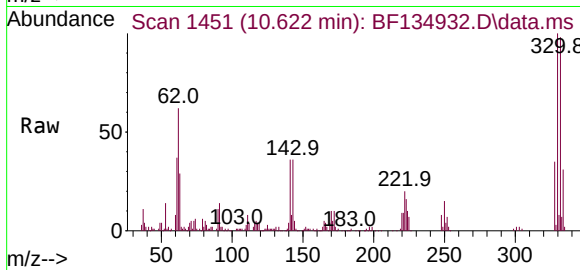

#45

2-Fluorobiphenyl

Concen: 29.282 ng

RT: 9.151 min Scan# 1201

Delta R.T. -0.006 min

Lab File: BF134932.D

Acq: 24 Aug 2023 19:24




Tgt Ion:172 Resp: 283709


Ion Ratio Lower Upper

172 100

171 34.6 29.4 44.0

170 23.1 19.6 29.4



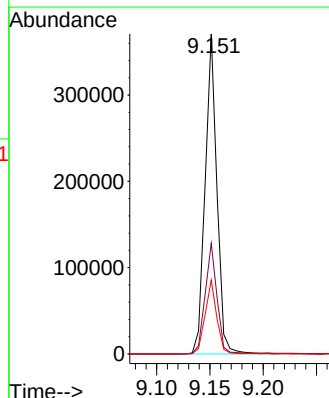
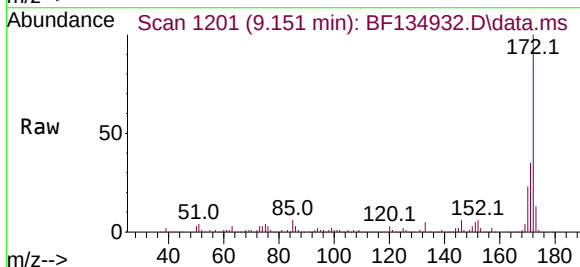


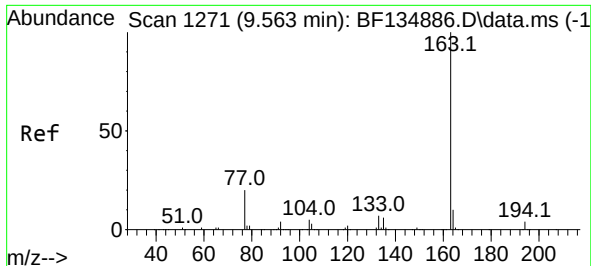

#50
Dimethylphthalate
Concen: 2.890 ng
RT: 9.833 min Scan# 1317
Delta R.T. 0.270 min
Lab File: BF134932.D
Acq: 24 Aug 2023 19:24




Instrument :
BNA_F
ClientSampleId :
TP-3


Tgt Ion:163 Resp: 30814
Ion Ratio Lower Upper
163 100
194 0.0 3.2 4.8#
164 465.7 8.2 12.4#

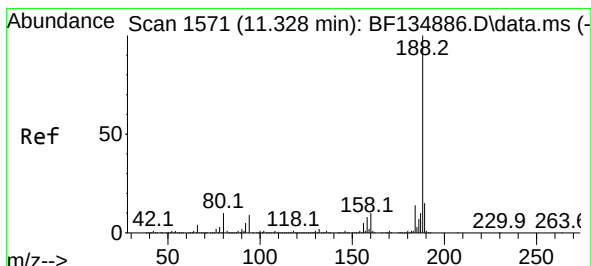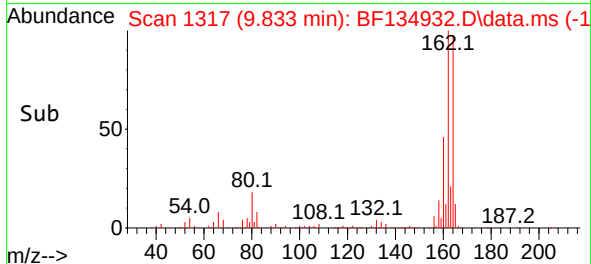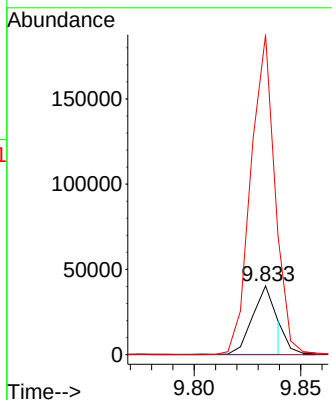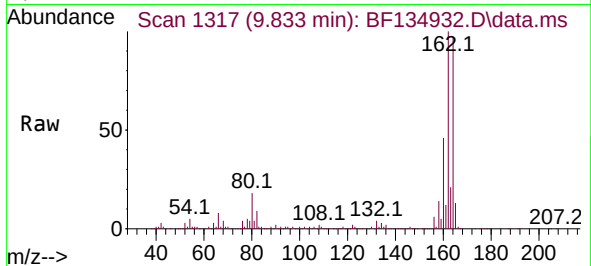

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.327 min Scan# 1571
Delta R.T. -0.000 min
Lab File: BF134932.D
Acq: 24 Aug 2023 19:24

Tgt Ion:188 Resp: 304443
Ion Ratio Lower Upper
188 100
94 9.1 7.5 11.3
80 9.4 7.8 11.6

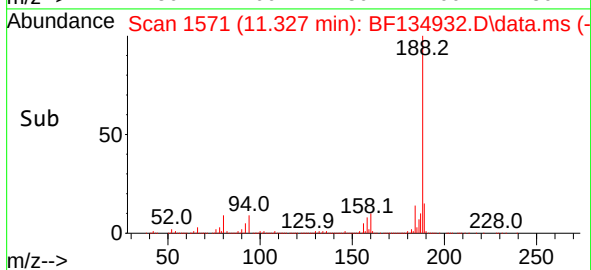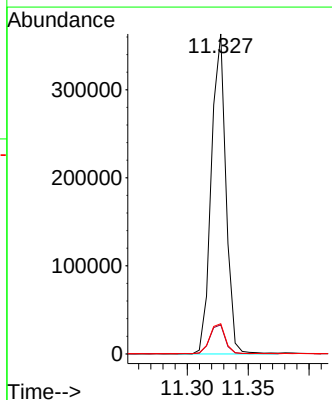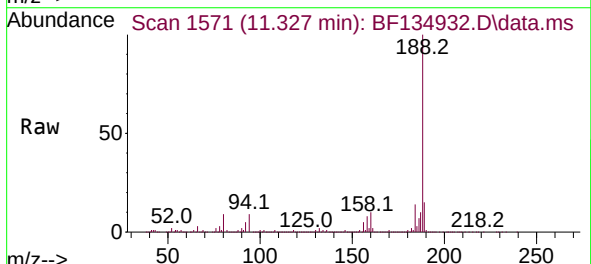



#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.986 min Scan# 20

Delta R.T. 0.006 min

Lab File: BF134932.D

Acq: 24 Aug 2023 19:24

Instrument :

BNA_F

ClientSampleId :

TP-3





Tgt Ion:240 Resp: 215188

Ion Ratio Lower Upper

240 100

120 10.0 8.6 12.8

236 25.9 20.6 31.0

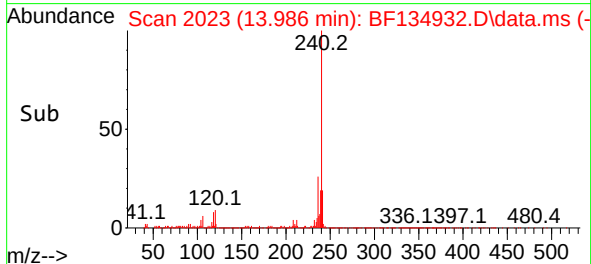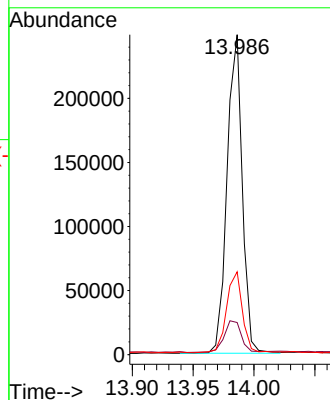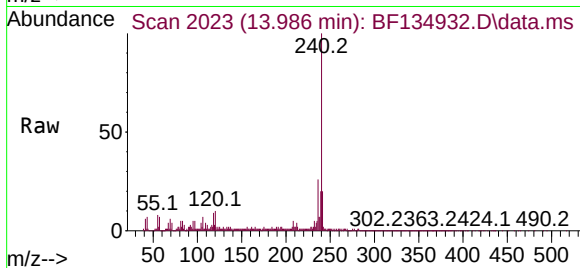

#79

Terphenyl-d14

Concen: 22.765 ng

RT: 12.921 min Scan# 1842

Delta R.T. -0.001 min

Lab File: BF134932.D

Acq: 24 Aug 2023 19:24




Tgt Ion:244 Resp: 356171


Ion Ratio Lower Upper

244 100

212 6.9 5.4 8.0

122 10.6 8.2 12.4

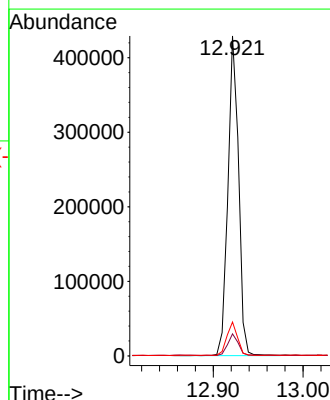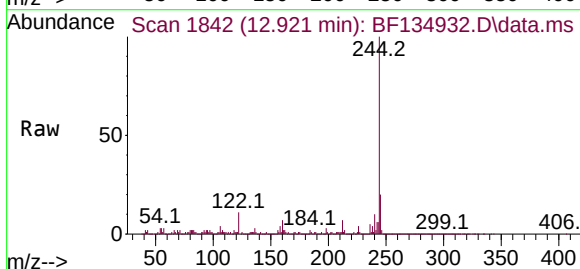



#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.468 min Scan# 21
 Delta R.T. 0.018 min
 Lab File: BF134932.D
 Acq: 24 Aug 2023 19:24

Instrument :
 BNA_F
 ClientSampleId :
 TP-3

Tgt Ion:264 Resp: 168092
 Ion Ratio Lower Upper
 264 100
 260 24.0 19.0 28.6
 265 23.3 17.1 25.7

