
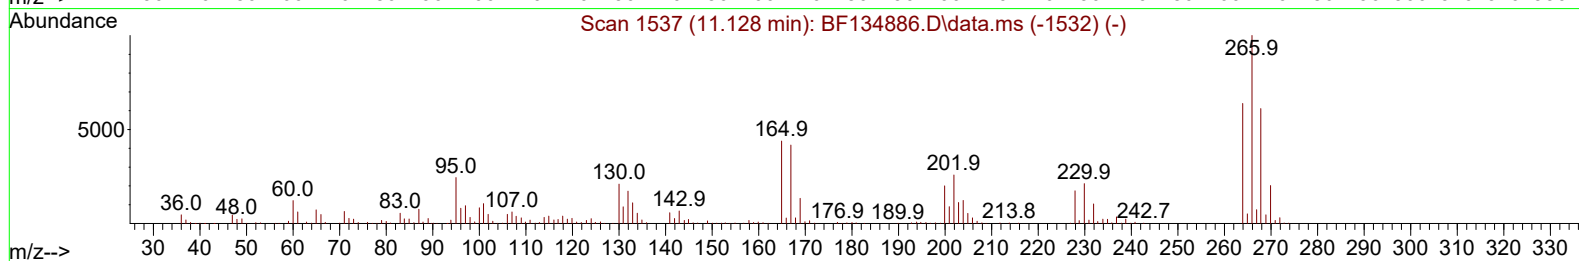
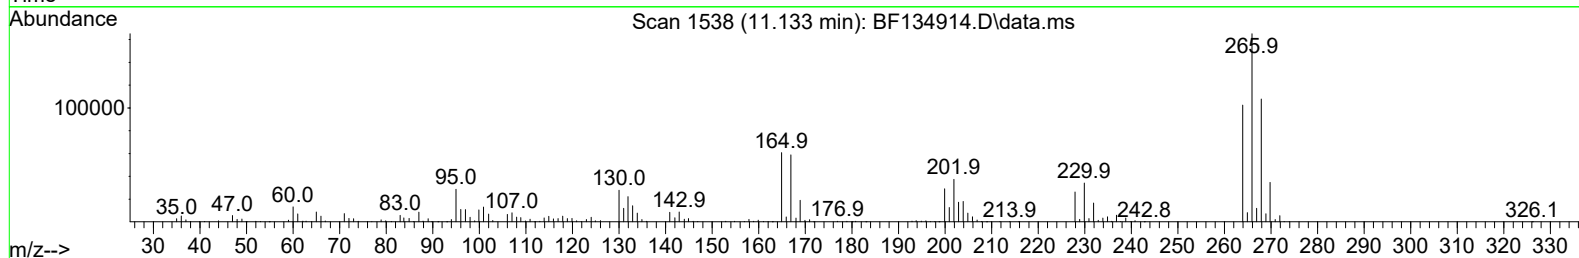


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082423\
Data File : BF134914.D
Acq On : 24 Aug 2023 09:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 10:39:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 22 19:33:25 2023
Response via : Initial Calibration

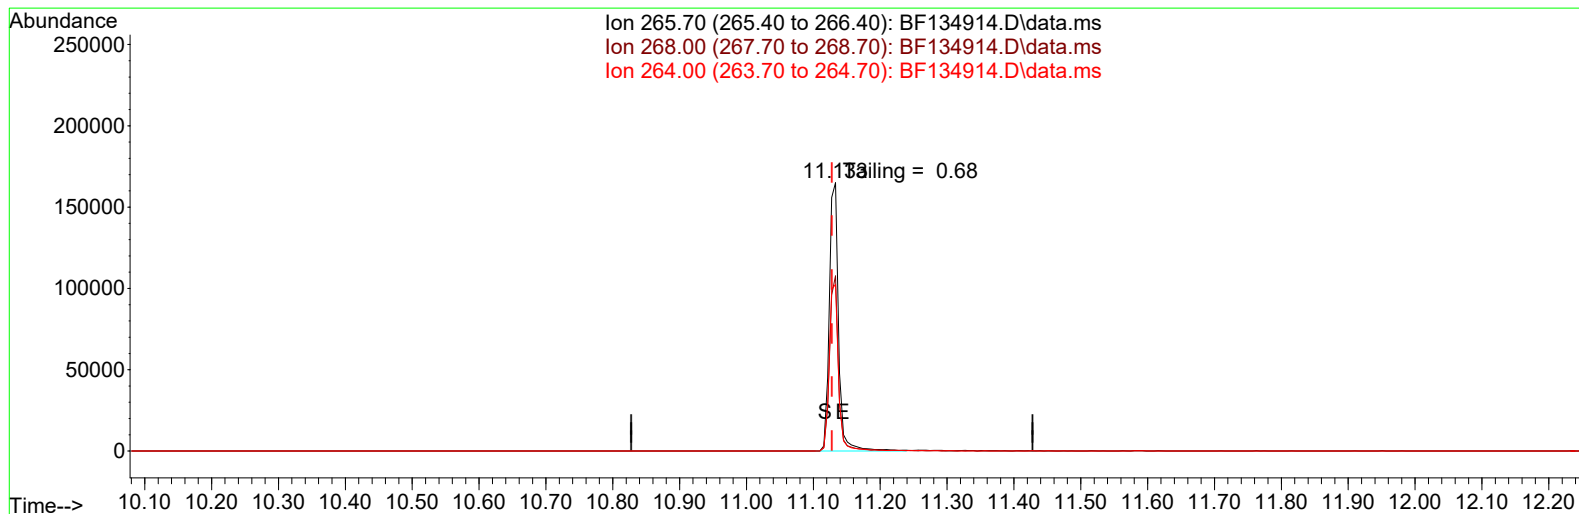

TIC: BF134914.D\data.ms

(70) Pentachlorophenol (C)




11.133min (+ 0.005) 29552.19 ng

response 159518

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	65.29
264.00	63.80	62.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082423\
Data File : BF134914.D
Acq On : 24 Aug 2023 09:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 10:39:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 22 19:33:25 2023
Response via : Initial Calibration

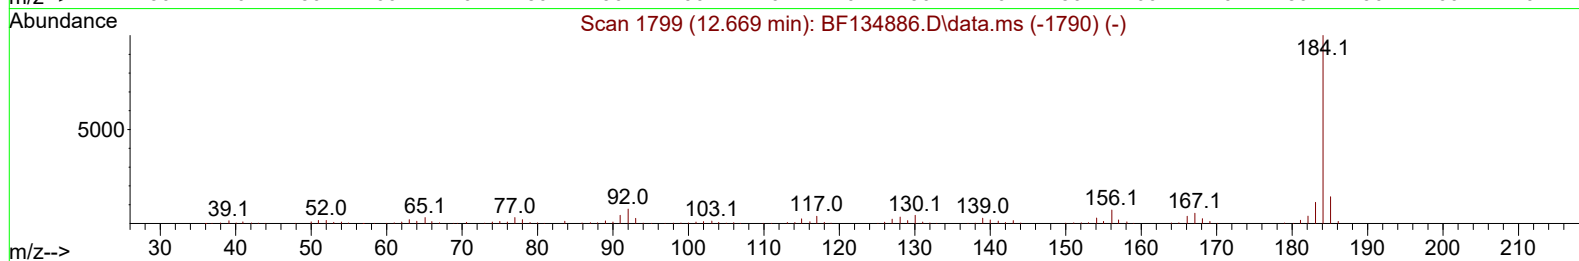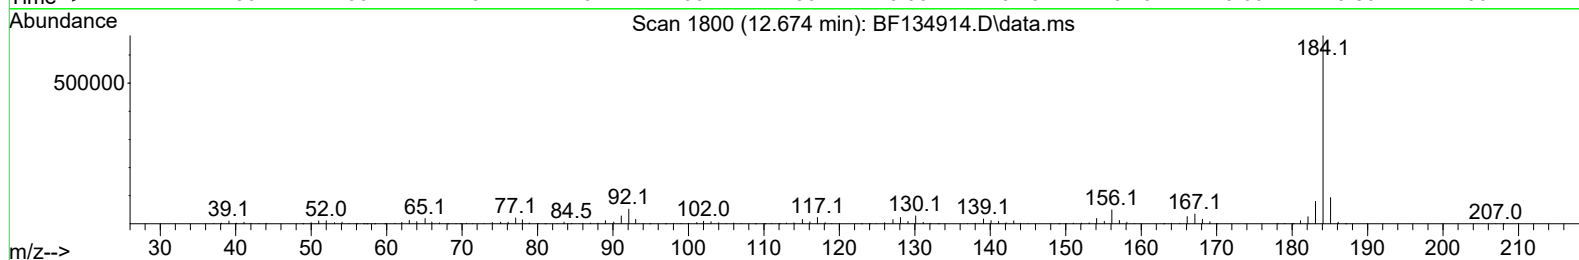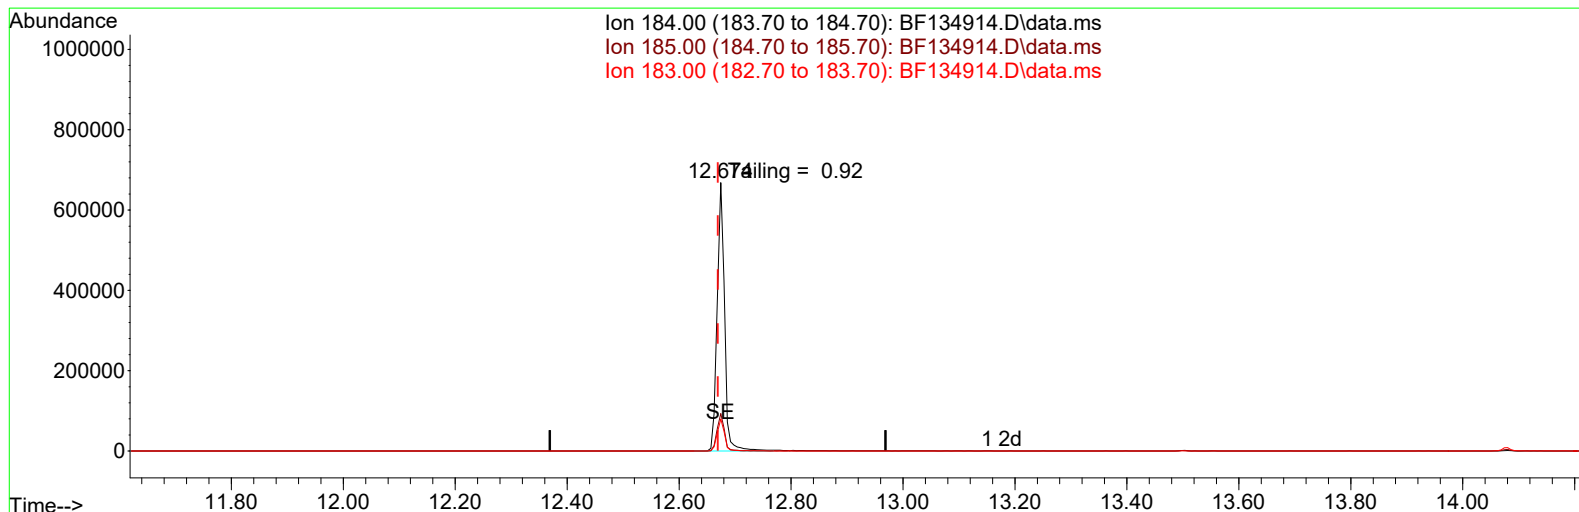

TIC: BF134914.D\data.ms

(77) Benzidine

12.674min (+ 0.005) 331766.64 ng m

response 629795

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.96
183.00	11.20	11.94
0.00	0.00	0.00