

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082423\
Data File : BF134916.D
Acq On : 24 Aug 2023 10:28
Operator : CG\JU
Sample : PB154990BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154990BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF134916.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.116	3	5	15	rVB	47128	59079	1.34%	0.217%
2	5.440	564	570	573	rBV	3656550	3744147	84.84%	13.781%
3	6.440	734	740	742	rBV	3297456	3723669	84.38%	13.706%
4	6.792	797	800	804	rBV	1000694	789441	17.89%	2.906%
5	7.357	890	896	899	rBV	2363343	2493082	56.49%	9.176%
6	8.075	1013	1018	1021	rBV	1183457	1062213	24.07%	3.910%
7	9.157	1196	1202	1205	rBV	4472361	4413220	100.00%	16.244%
8	9.833	1311	1317	1320	rBV	1392429	1198766	27.16%	4.412%
9	10.628	1446	1452	1455	rBV	3171322	2844883	64.46%	10.471%
10	11.327	1566	1571	1574	rBV	1282881	1210705	27.43%	4.456%
11	12.927	1838	1843	1846	rBV	4231962	4014250	90.96%	14.775%
12	13.980	2018	2022	2029	rBV	753697	713679	16.17%	2.627%
13	14.074	2033	2038	2044	rVB	137333	159993	3.63%	0.589%
14	15.457	2268	2273	2280	rBV	580232	741954	16.81%	2.731%




Sum of corrected areas: 27169081

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082423\
Data File : BF134916.D
Acq On : 24 Aug 2023 10:28
Operator : CG\JU
Sample : PB154990BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154990BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

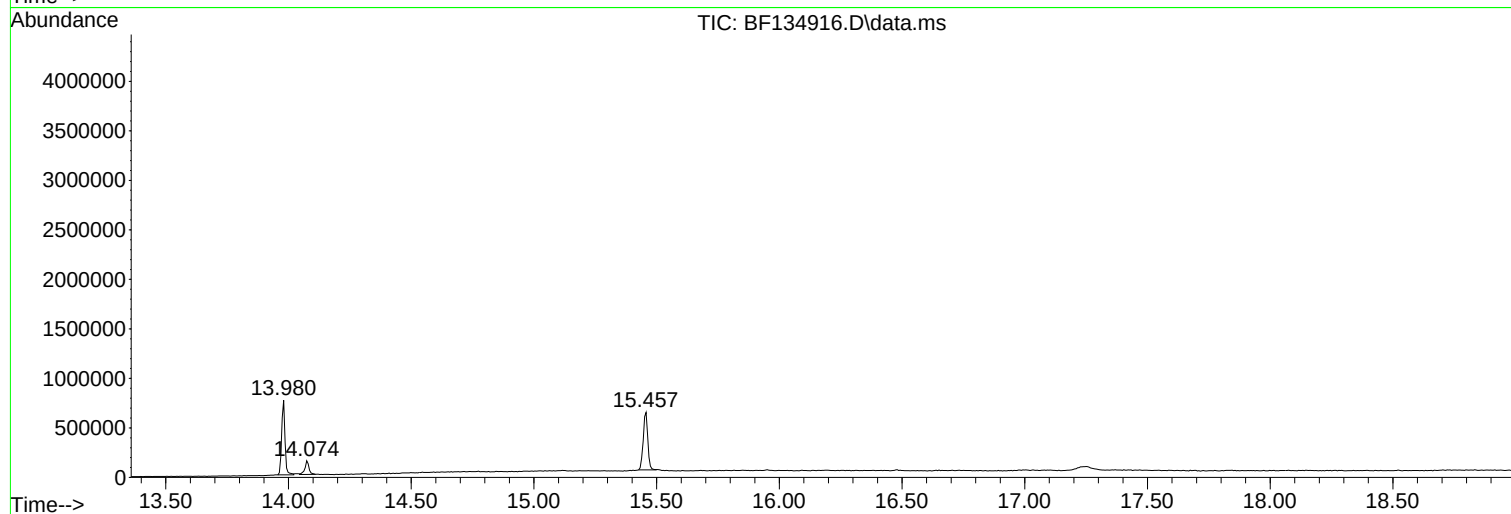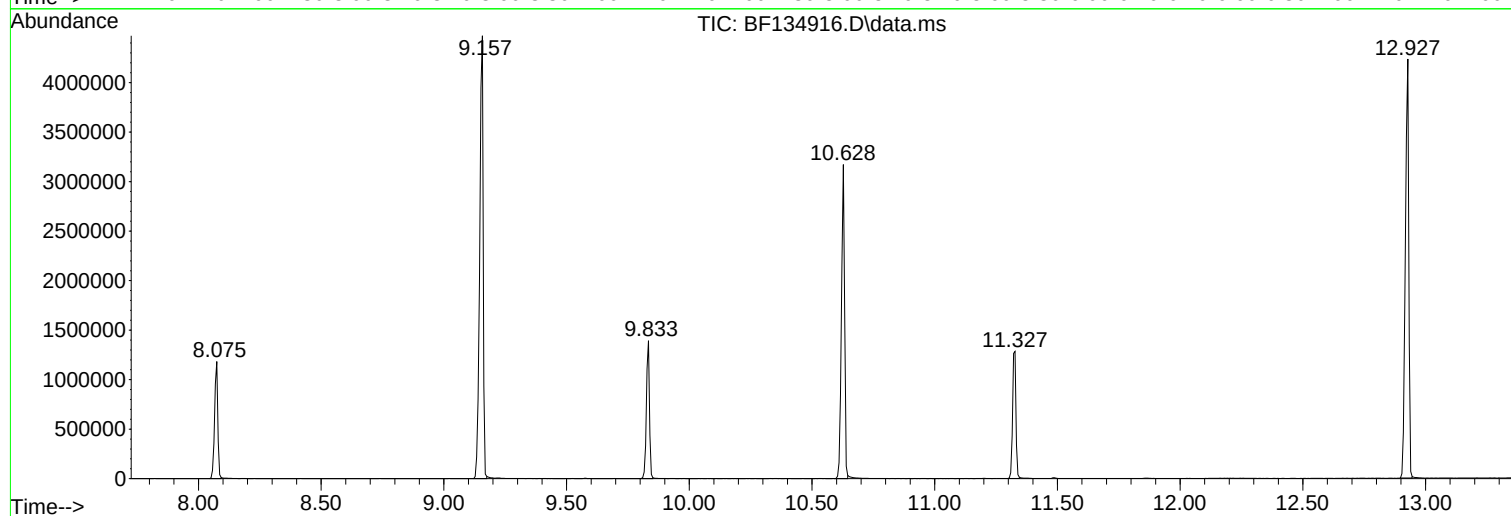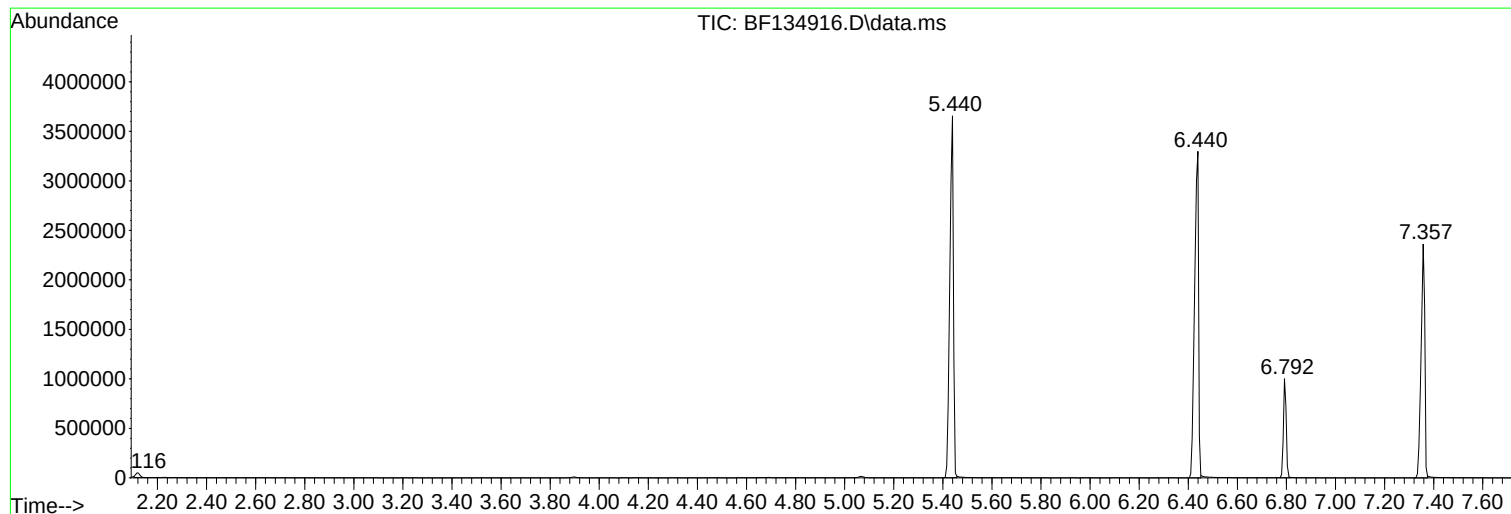

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082423\
Data File : BF134916.D
Acq On : 24 Aug 2023 10:28
Operator : CG\JU
Sample : PB154990BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154990BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.074	4.48 ng	159993	Chrysene-d12	13.980

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	89
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	68
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	64
4			Cobalt,(.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	38
5			(Carbethoxymethyl)-triphenylphos...	428	C22H22BrO2P	001530-45-6	37

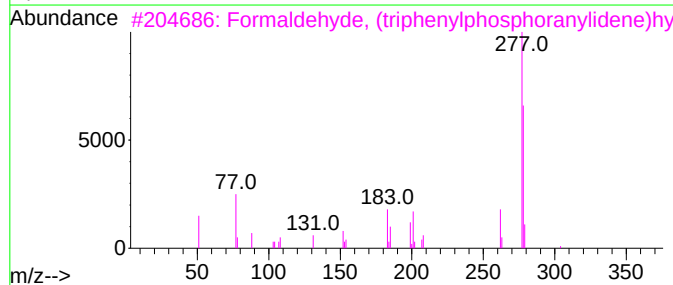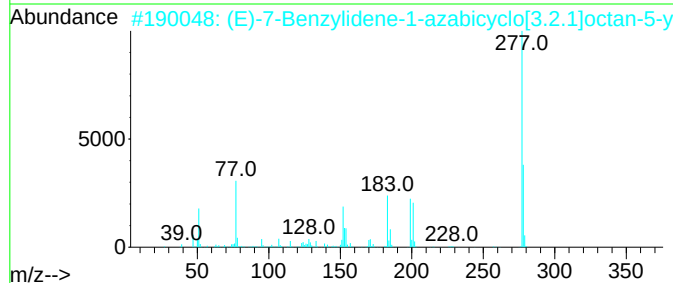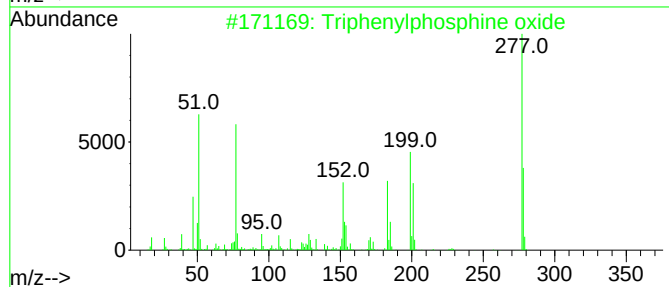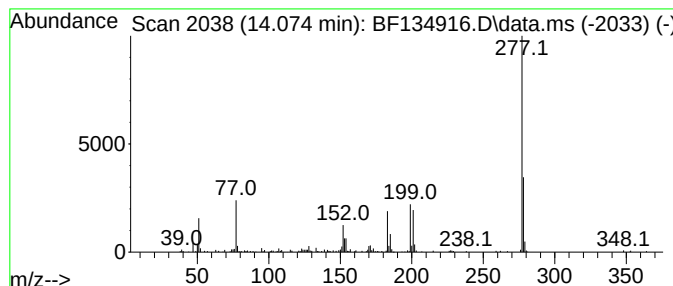

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082423\
Data File : BF134916.D
Acq On : 24 Aug 2023 10:28
Operator : CG\JU
Sample : PB154990BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154990BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.074	4.5	ng	159993	5	13.980	713679	20.0