

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082423\
 Data File : BF134932.D
 Acq On : 24 Aug 2023 19:24
 Operator : CG\JU
 Sample : 04116-05 2X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF134932.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.422	563	567	588	rBV	880773	847865	89.77%	9.556%
2	6.428	734	738	754	rBV	952806	837990	88.73%	9.445%
3	6.628	768	772	777	rBV	23549	27083	2.87%	0.305%
4	6.792	797	800	804	rBV	673108	568416	60.18%	6.407%
5	7.351	892	895	901	rBV	549396	440556	46.65%	4.965%
6	7.710	953	956	960	rVB5	18160	16931	1.79%	0.191%
7	8.075	1012	1018	1021	rBV	800445	651358	68.97%	7.341%
8	8.498	1086	1090	1092	rBV	18524	20270	2.15%	0.228%
9	8.610	1106	1109	1115	rBV8	10295	21718	2.30%	0.245%
10	9.098	1189	1192	1196	rVB2	29744	27239	2.88%	0.307%
11	9.151	1197	1201	1204	rBV	1065094	814179	86.21%	9.177%
12	9.228	1210	1214	1218	rBV4	20380	26703	2.83%	0.301%
13	9.269	1218	1221	1226	rVV	224372	197015	20.86%	2.221%
14	9.533	1264	1266	1268	rBV	34096	31156	3.30%	0.351%
15	9.557	1268	1270	1274	rVB2	27074	22012	2.33%	0.248%
16	9.692	1291	1293	1296	rBV3	16199	15255	1.62%	0.172%
17	9.739	1299	1301	1304	rVB2	29178	25022	2.65%	0.282%
18	9.833	1313	1317	1321	rVB	816444	661364	70.03%	7.454%
19	10.151	1369	1371	1377	rBV7	9428	20104	2.13%	0.227%
20	10.622	1448	1451	1459	rBV	658078	553933	58.65%	6.243%
21	10.757	1470	1474	1478	rVB	37362	39206	4.15%	0.442%
22	11.222	1551	1553	1558	rVB	33947	36938	3.91%	0.416%
23	11.327	1567	1571	1574	rBV	860192	734044	77.72%	8.273%
24	11.863	1659	1662	1666	rBV2	60114	66801	7.07%	0.753%
25	12.921	1839	1842	1846	rBV	1108180	944464	100.00%	10.645%
26	13.986	2019	2023	2028	rBV	654764	644913	68.28%	7.269%
27	15.468	2272	2275	2284	rVB	369066	579897	61.40%	6.536%




Sum of corrected areas: 8872432

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082423\
Data File : BF134932.D
Acq On : 24 Aug 2023 19:24
Operator : CG\JU
Sample : 04116-05 2X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

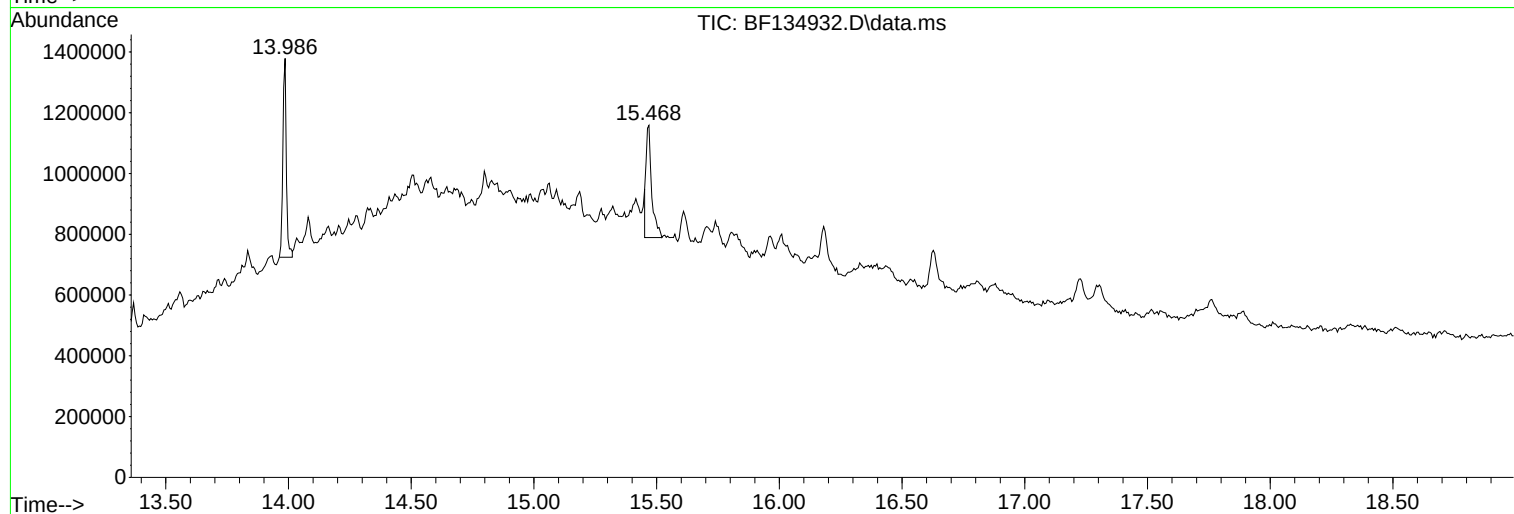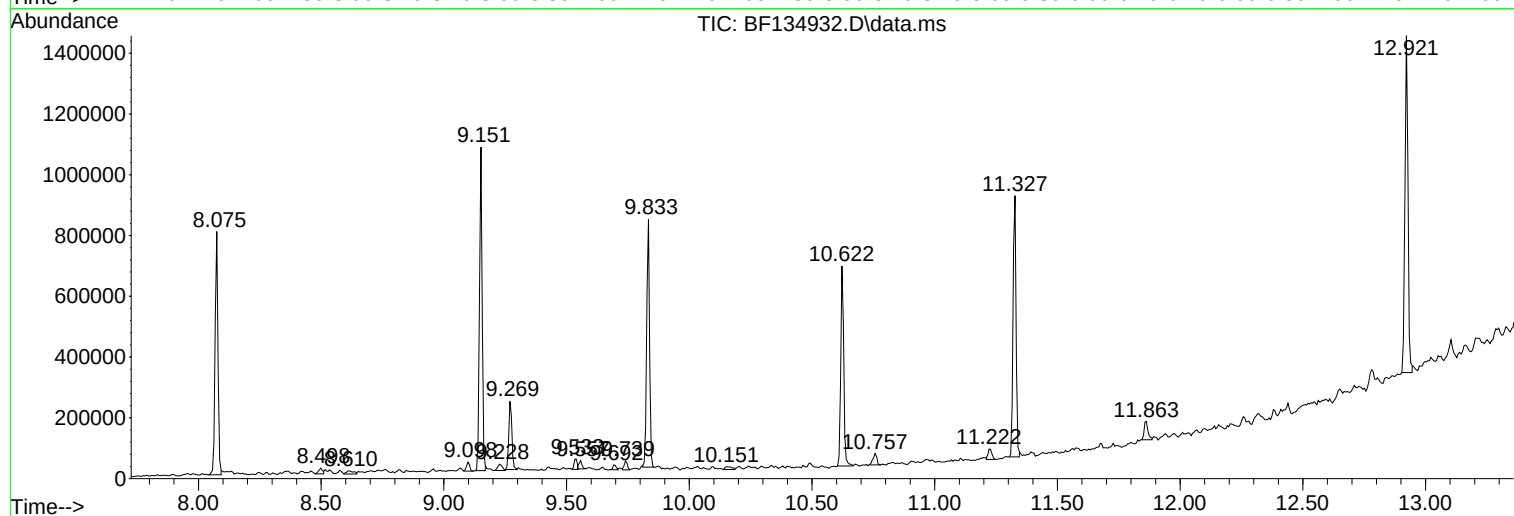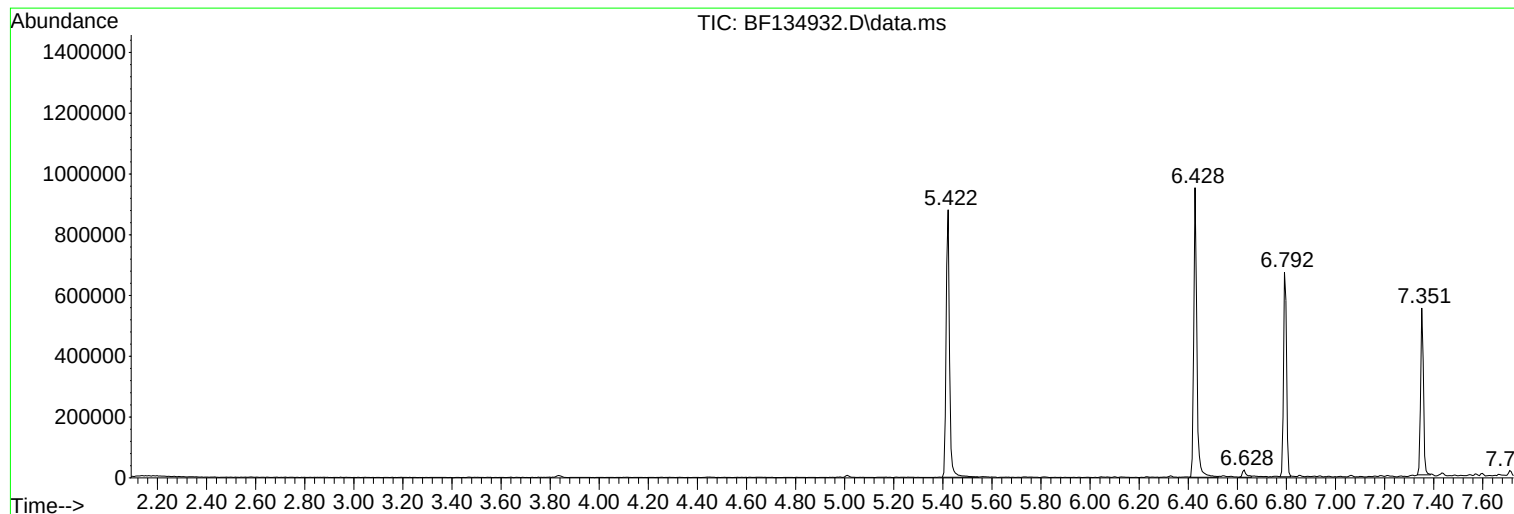

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082423\
Data File : BF134932.D
Acq On : 24 Aug 2023 19:24
Operator : CG\JU
Sample : 04116-05 2X
Misc :
ALS Vial : 19 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
TP-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2,4,7,9-Tetramethyl-5-decyn... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
9.269	5.96 ng	197015	Acenaphthene-d10			9.833
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2,4,7,9-Tetramethyl-5-decyn-4,7-...		226	C14H26O2	000126-86-3	91
2	2-Propenal, 3-(2,2,6-trimethyl-7...		194	C12H18O2	055759-91-6	78
3	Pyridine, 2-butyl-, 1-oxide		151	C9H13NO	031396-32-4	59
4	Metacetamol		151	C8H9NO2	000621-42-1	58
5	Cyclohexanol, 3,3,5-trimethyl-		142	C9H18O	000116-02-9	47

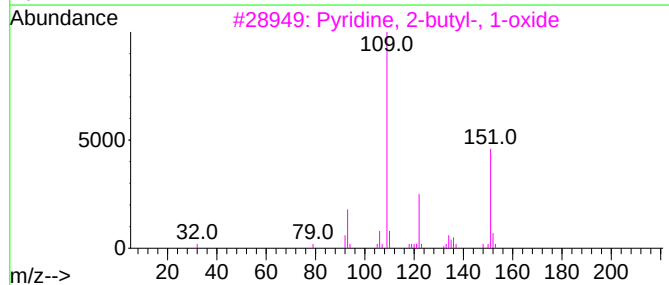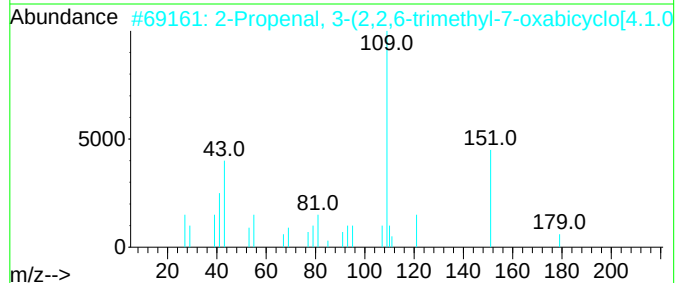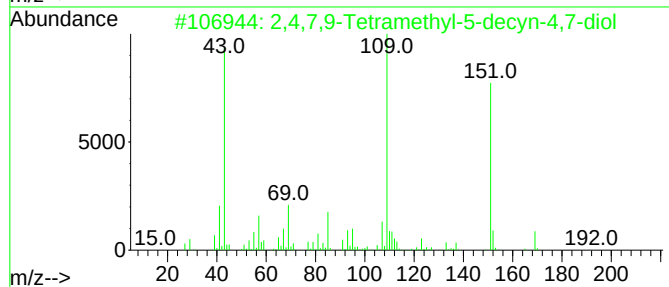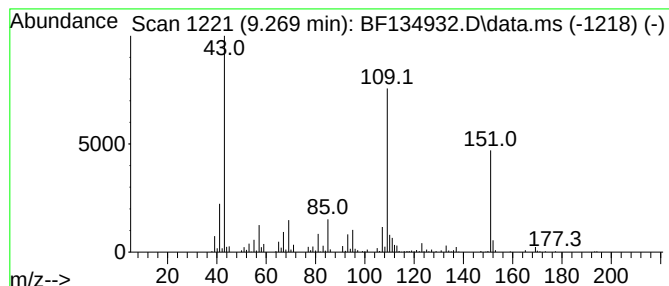

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082423\
Data File : BF134932.D
Acq On : 24 Aug 2023 19:24
Operator : CG\JU
Sample : 04116-05 2X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2,4,7,9-Tetrame...	9.269	6.0	ng	197015	3	9.833	661364	20.0