


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082423\
Data File : BF134914.D
Acq On : 24 Aug 2023 09:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Aug 22 19:33:25 2023

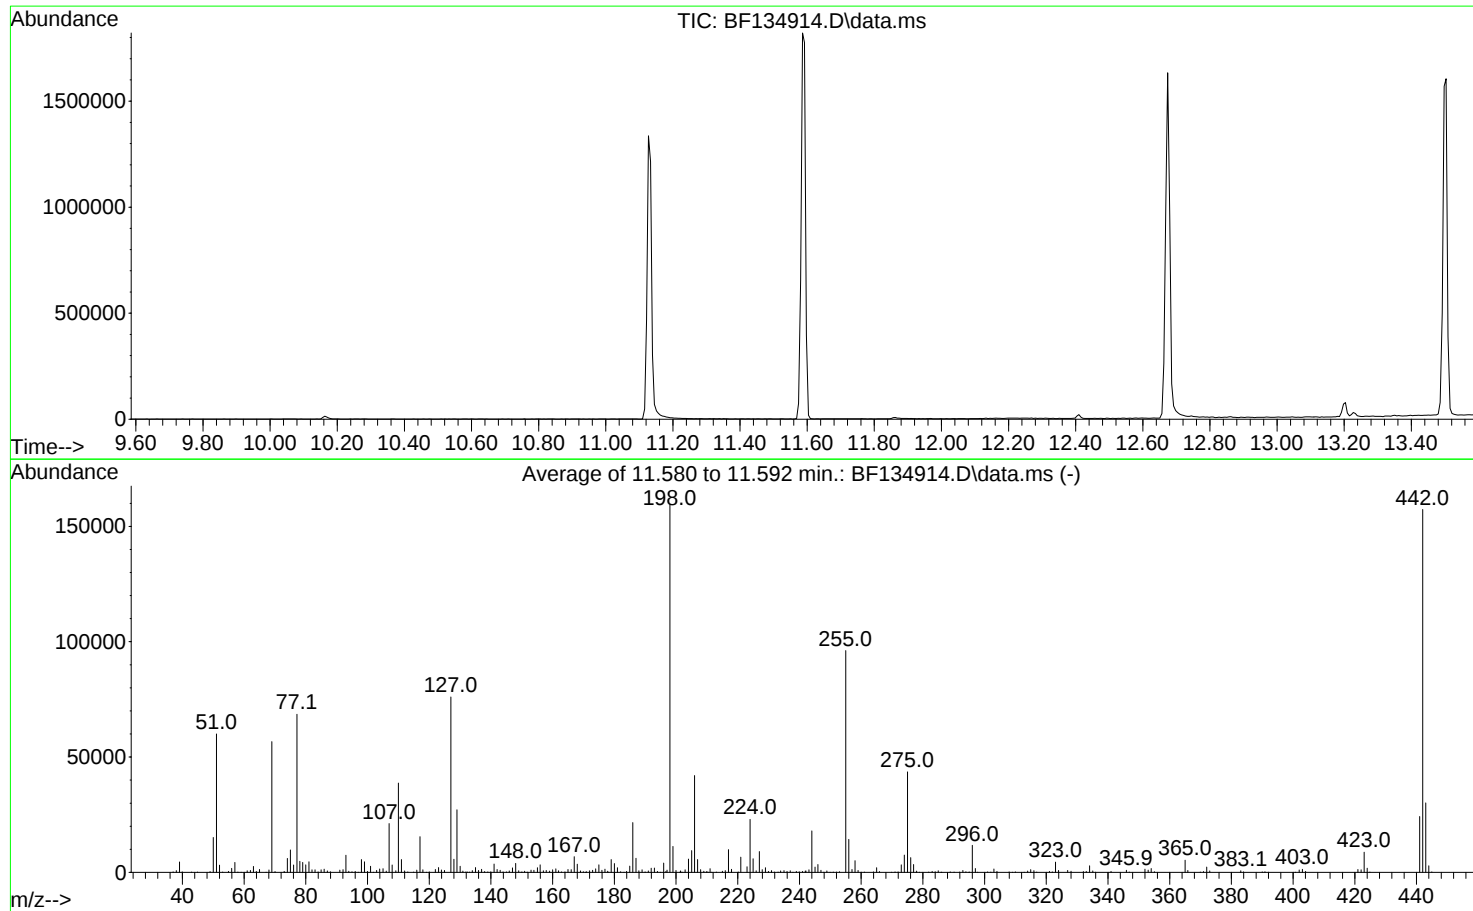




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	59976	PASS
68	69	0.00	2	1.9	1079	PASS
69	198	0.00	100	35.5	56688	PASS
70	69	0.00	2	0.6	327	PASS
127	198	10	80	47.7	76013	PASS
197	198	0.00	2	0.6	1004	PASS
198	198	100	100	100.0	159483	PASS
199	198	5	9	7.1	11271	PASS
275	198	10	60	27.3	43544	PASS
365	198	1	100	3.3	5310	PASS
441	198	0.01	100	15.2	24227	PASS
442	442	50	100	100.0	157323	PASS
443	442	15	24	19.1	30120	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082423\
 Data File : BF134914.D
 Acq On : 24 Aug 2023 09:24
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 24 10:39:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 22 19:33:25 2023
 Response via : Initial Calibration

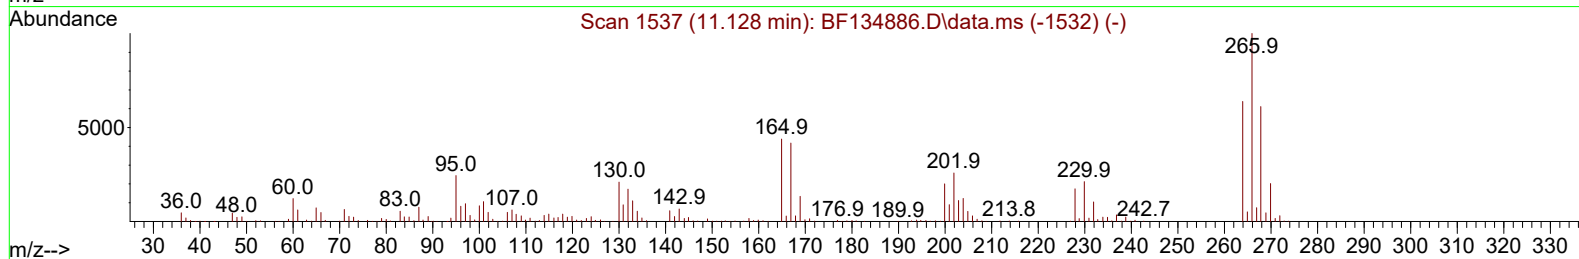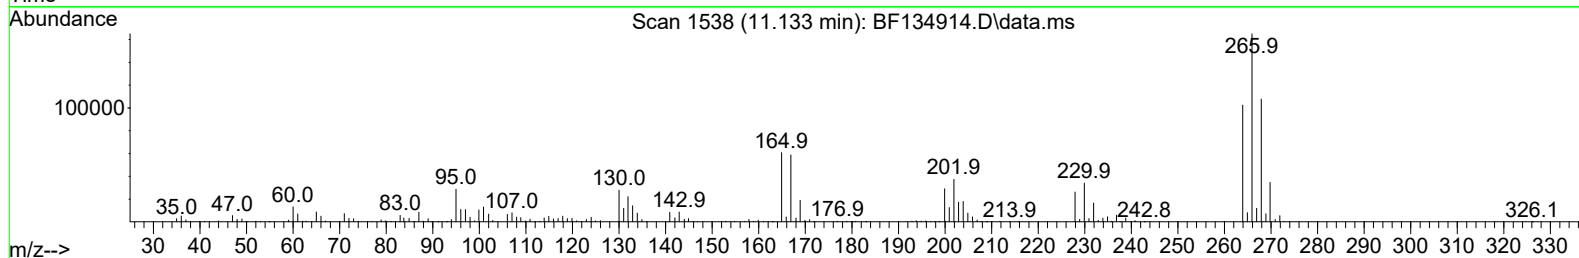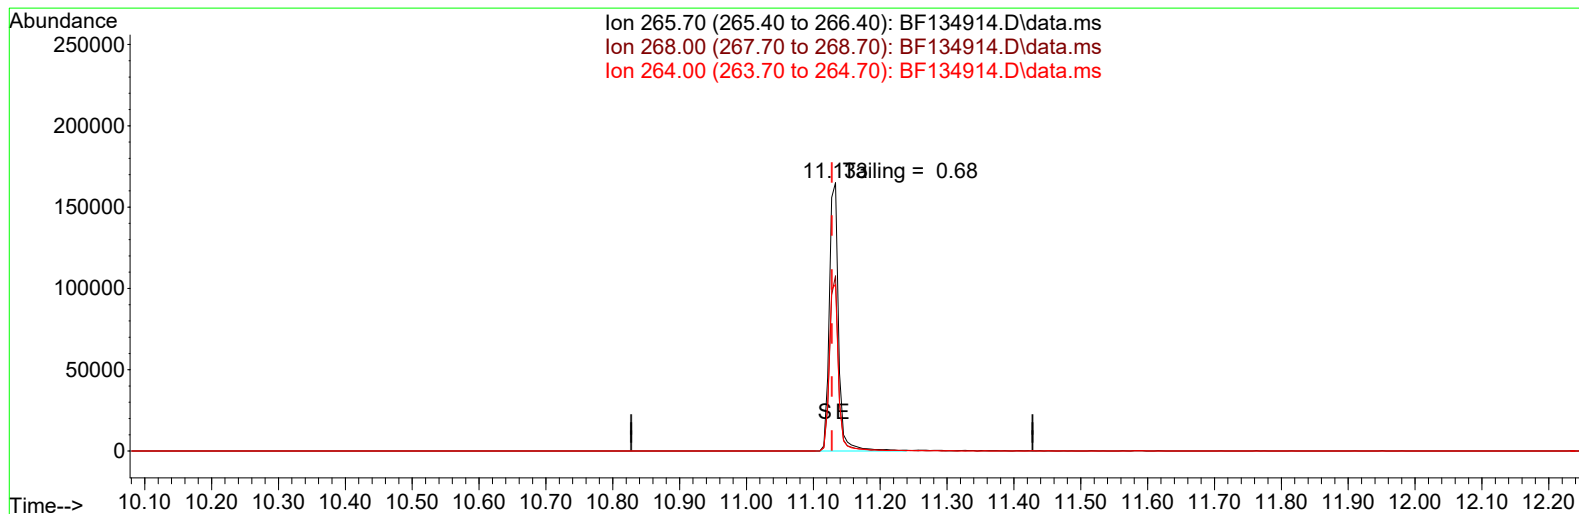

TIC: BF134914.D\data.ms

(70) Pentachlorophenol (C)

11.133min (+ 0.005) 29552.19 ng




response 159518

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	65.29
264.00	63.80	62.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082423\
Data File : BF134914.D
Acq On : 24 Aug 2023 09:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 24 10:39:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 22 19:33:25 2023
Response via : Initial Calibration

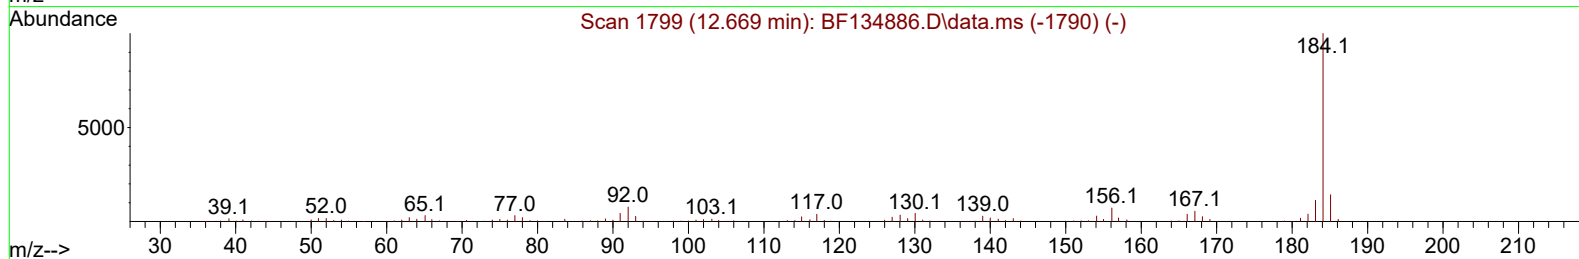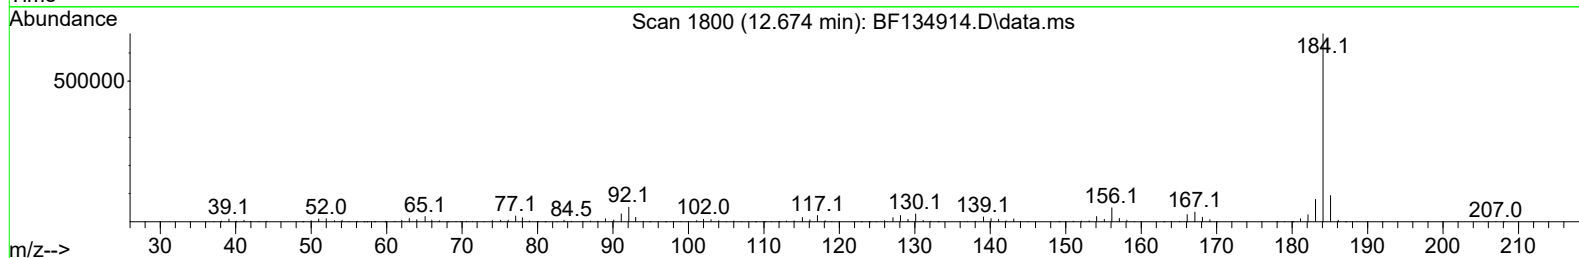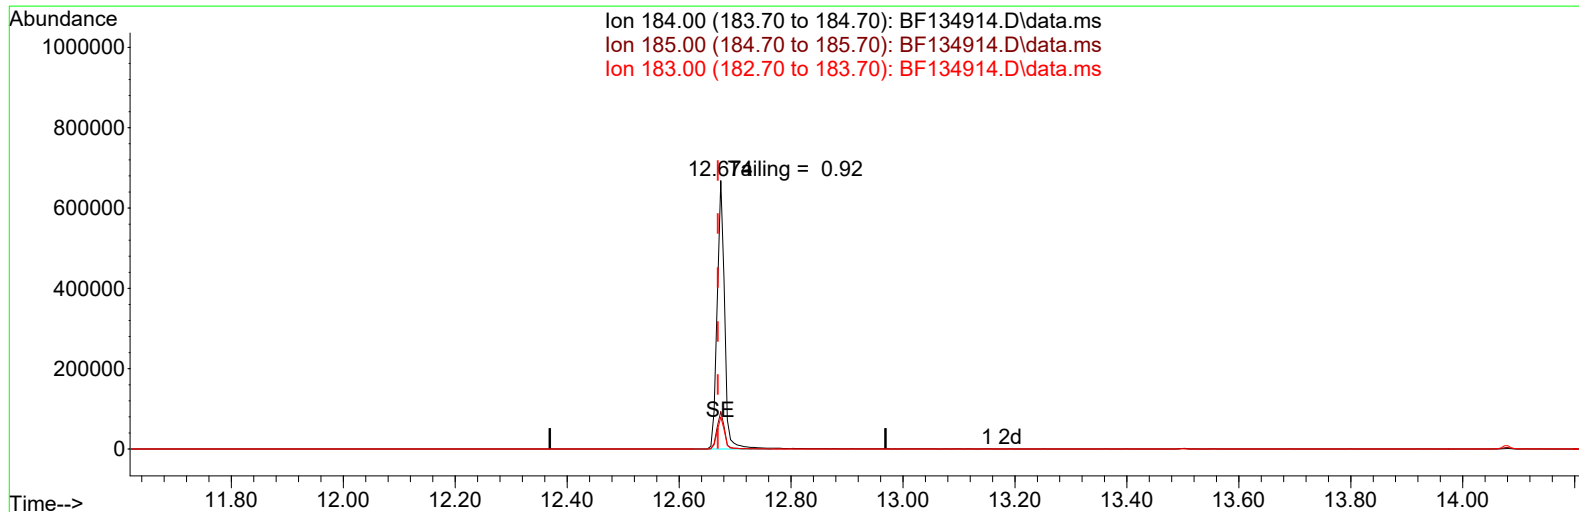

TIC: BF134914.D\data.ms

(77) Benzidine

12.674min (+ 0.005) 331766.64 ng m

response 629795

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.96
183.00	11.20	11.94
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/24/2023	BNA_F	<u>BF134914.D</u>
Compound Name	Response	Retention Time
DDT	292907	13.504
DDD	15820	13.204
DDE	672	12.863
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16492	309399	5.33

Instrument :
BNA_F
ClientSampleId :
DFTPP