


Data Path : Z:\HPCHEM1\BNA_F\Data\BF082515\
 Data File : BF081197.D
 Acq On : 25 Aug 2015 11:53
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 24 13:58:19 2015

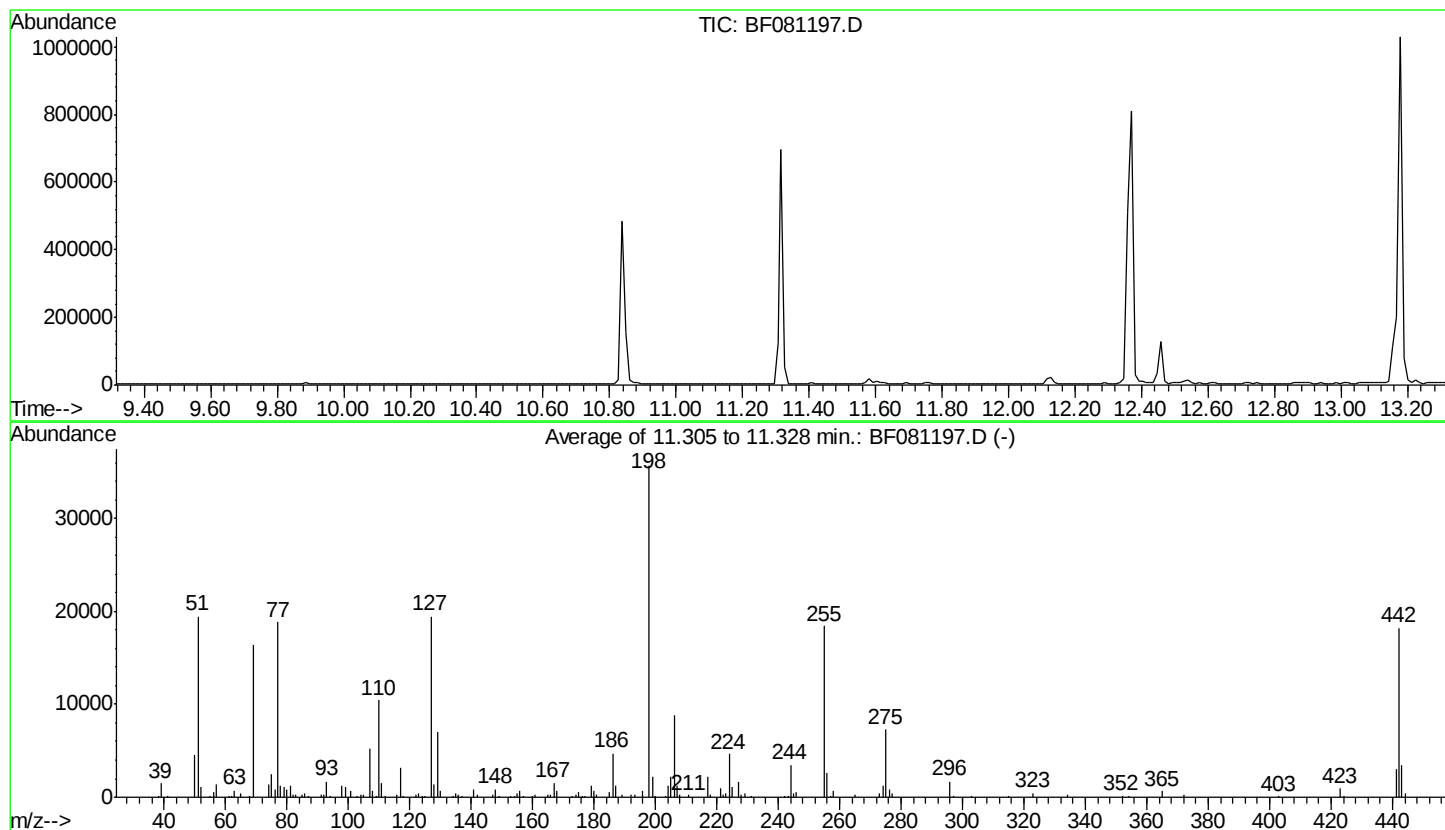

AutoFind: Scans 824, 825, 826; Background Corrected with Scan 821

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.4	19438	PASS
68	69	0.00	2	1.1	187	PASS
69	198	0.00	100	46.0	16435	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.5	19448	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	35699	PASS
199	198	5	9	6.2	2218	PASS
275	198	10	60	20.3	7264	PASS
365	198	1	100	1.9	689	PASS
441	442	0.01	24	16.8	3061	PASS
442	198	50	100	51.1	18231	PASS
443	442	15	24	19.1	3474	PASS