

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082519\
 Data File : BF116552.D
 Acq On : 26 Aug 2019 3:14
 Operator : HP/JU
 Sample : K4510-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-41-COMP

Quant Time: Aug 26 08:31:17 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF082319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 23 13:38:31 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	133794	20.00	ng	0.00
21) Naphthalene-d8	8.16	136	499609	20.00	ng	0.00
39) Acenaphthene-d10	9.92	164	222974	20.00	ng	0.00
64) Phenanthrene-d10	11.40	188	297706	20.00	ng	0.00
76) Chrysene-d12	14.03	240	209653	20.00	ng	0.00
87) Perylene-d12	15.50	264	178516	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.51	112	717239	78.33	ng	0.01
7) Phenol-d6	6.51	99	943567	84.04	ng	0.00
23) Nitrobenzene-d5	7.44	82	552668	60.52	ng	0.00
42) 2,4,6-Tribromophenol	10.70	330	86147	44.99	ng	0.00
45) 2-Fluorobiphenyl	9.24	172	965528	69.73	ng	0.00
79) Terphenyl-d14	12.98	244	636378	56.70	ng	0.00
Target Compounds						
50) Dimethylphthalate	9.62	163	90086	5.791	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082519\
Data File : BF116552.D
Acq On : 26 Aug 2019 3:14
Operator : HP/JU
Sample : K4510-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-41-COMP

Quant Time: Aug 26 08:31:17 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF082319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 23 13:38:31 2019
Response via : Initial Calibration

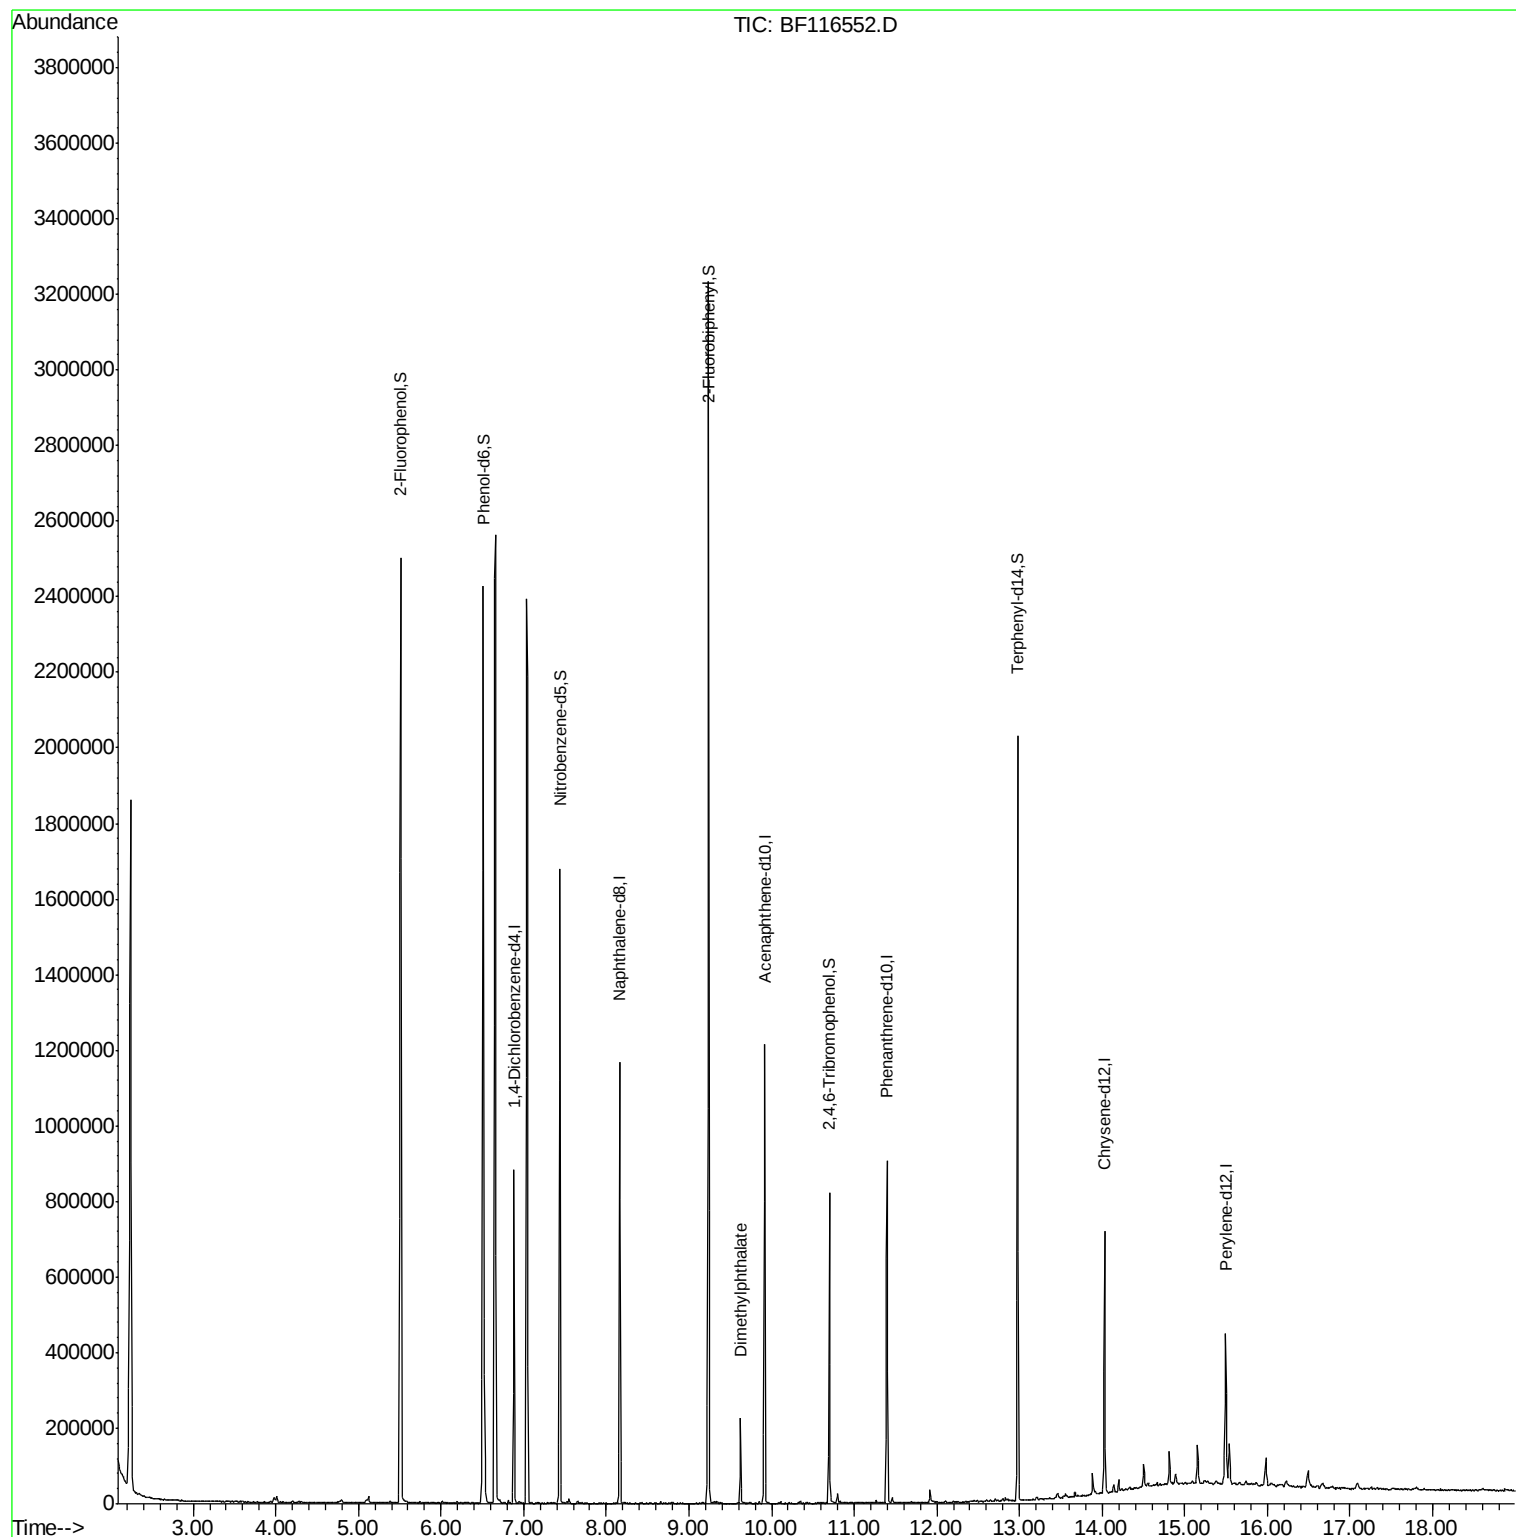

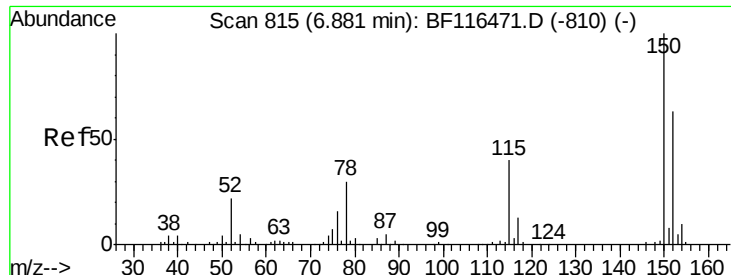


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.89 min Scan# 816
Delta R.T. 0.01 min
Lab File: BF116552.D
Acq: 26 Aug 2019 3:14

Instrument :
BNA_F
ClientSampleId :
SB-41-COMP

Tot Ion:152 Resp: 133794
Ion Ratio Lower Upper
152 100
150 153.8 126.7 190.1
115 59.8 50.9 76.3

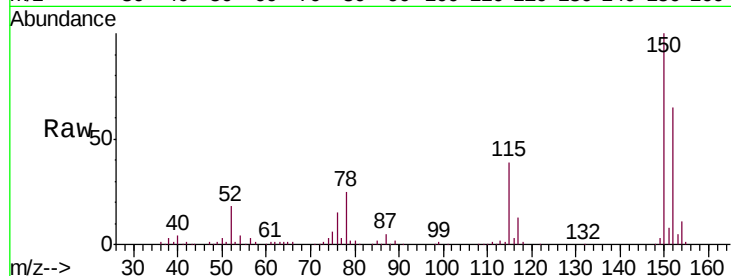


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

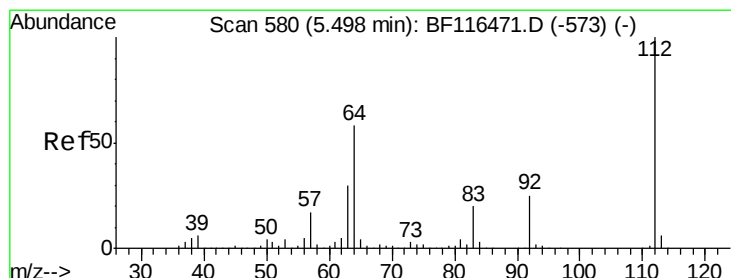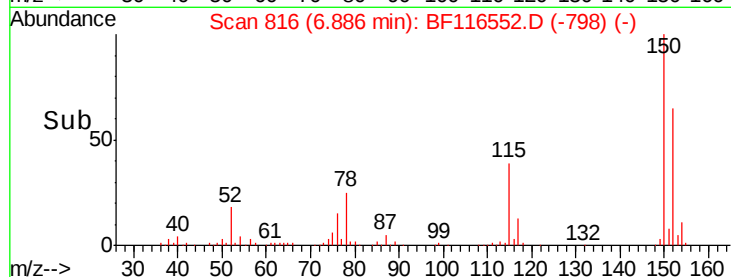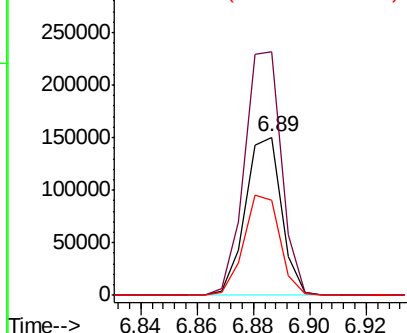



#5


2-Fluorophenol
Concen: 78.329 ng
RT: 5.51 min Scan# 582
Delta R.T. 0.01 min
Lab File: BF116552.D
Acq: 26 Aug 2019 3:14

Tgt Ion:112 Resp: 717239
Ion Ratio Lower Upper
112 100
64 59.7 46.3 69.5
63 31.8 24.2 36.4

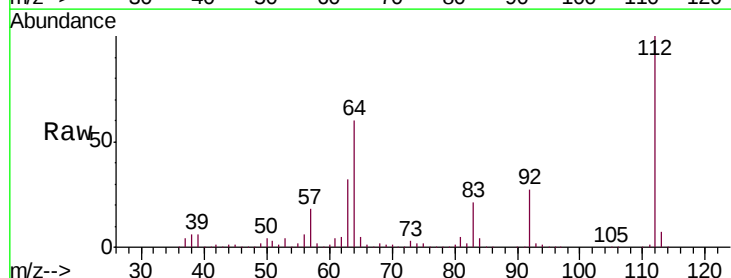

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

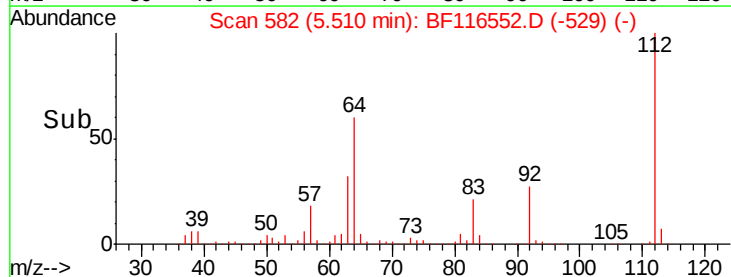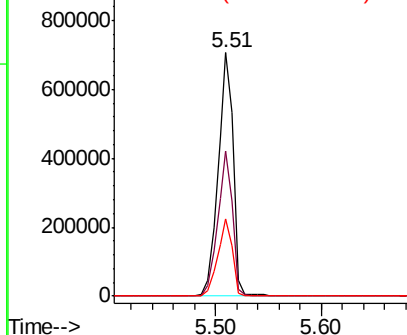

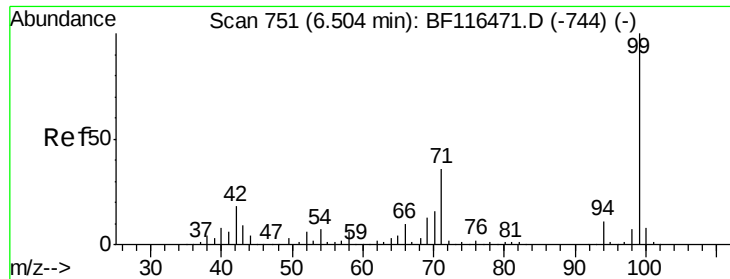

#7

Phenol-d6

Concen: 84.040 ng

RT: 6.51 min Scan# 752

Delta R.T. 0.01 min

Lab File: BF116552.D

Acq: 26 Aug 2019 3:14

Instrument :

BNA_F

ClientSampleId :

SB-41-COMP


Tot Ion: 99 Resp: 943567

Ion Ratio Lower Upper




99 100

42 18.0 14.6 21.8

71 36.8 28.5 42.7

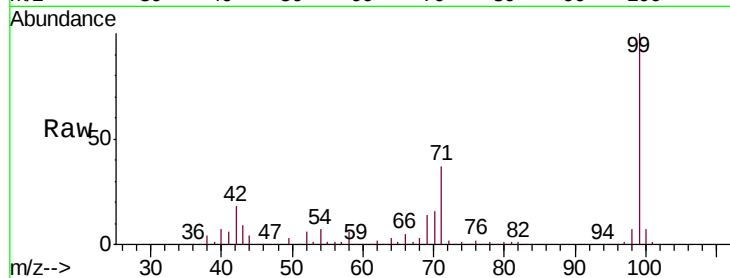

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

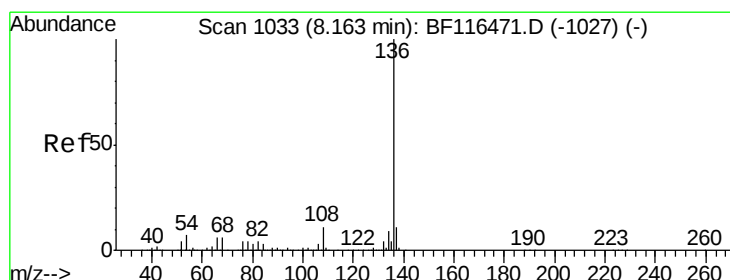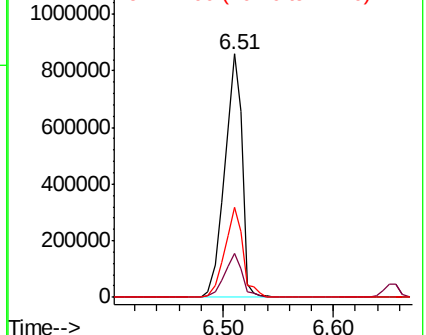

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.16 min Scan# 1033

Delta R.T. -0.00 min

Lab File: BF116552.D

Acq: 26 Aug 2019 3:14

Tgt Ion: 136 Resp: 499609


Ion Ratio Lower Upper

136 100



137 10.9 9.0 13.4


54 6.8 5.8 8.6

68 6.1 5.1 7.7

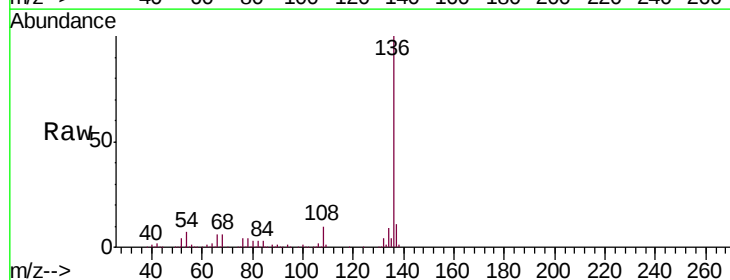

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1




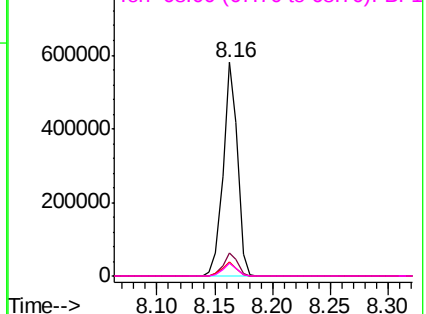




#23
 Nitrobenzene-d5
 Concen: 60.520 ng
 RT: 7.44 min Scan# 910
 Delta R.T. -0.00 min
 Lab File: BF116552.D
 Acq: 26 Aug 2019 3:14




Instrument :
 BNA_F
 ClientSampleId :
 SB-41-COMP


Tot Ion	Ratio	Lower	Upper
82	100		
128	42.5	32.2	48.4
54	44.7	36.5	54.7

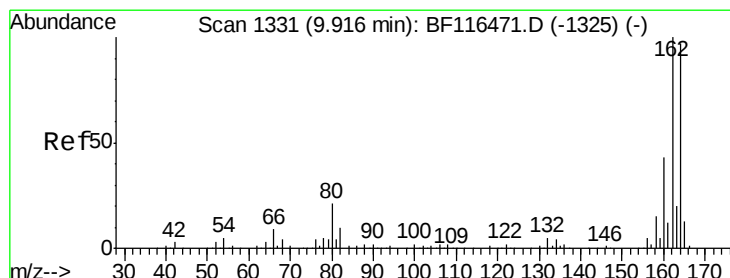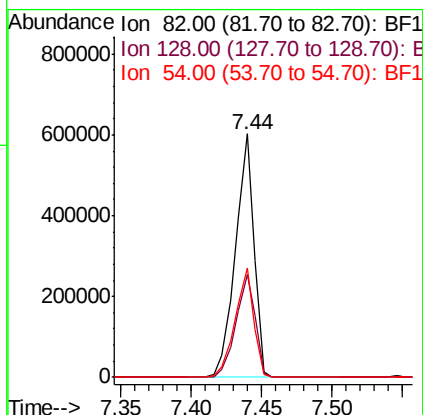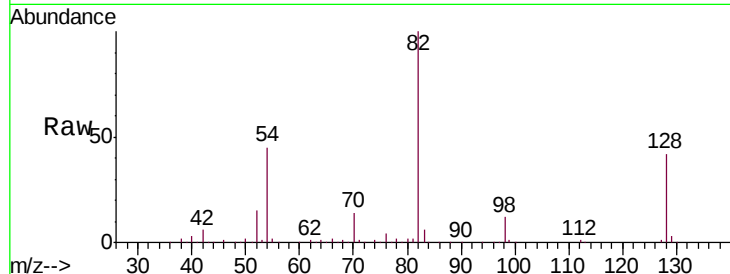

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.92 min Scan# 1331
 Delta R.T. -0.00 min
 Lab File: BF116552.D
 Acq: 26 Aug 2019 3:14

Tgt Ion	Ratio	Lower	Upper
164	100		
162	103.1	82.6	123.8
160	46.1	35.8	53.8

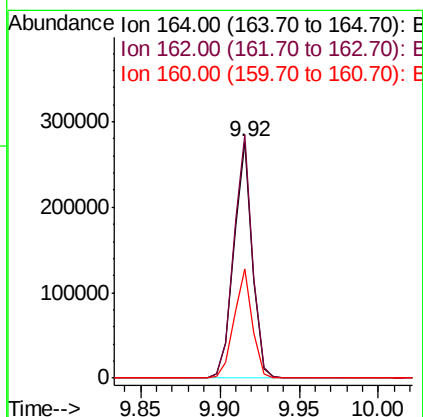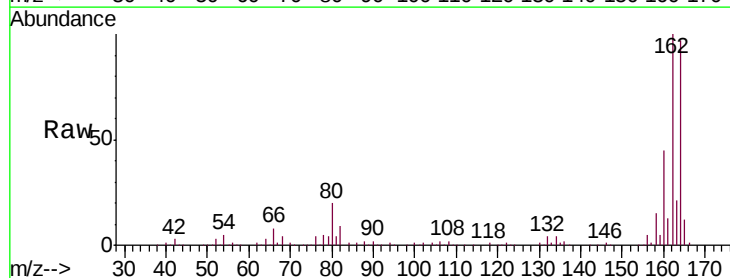







#42
 2,4,6-Tribromophenol
 Concen: 44.994 ng
 RT: 10.70 min Scan# 1464
 Delta R.T. -0.00 min
 Lab File: BF116552.D
 Acq: 26 Aug 2019 3:14

Instrument :
 BNA_F
 ClientSampleId :
 SB-41-COMP

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.8	77.2	115.8
141	38.2	33.3	49.9

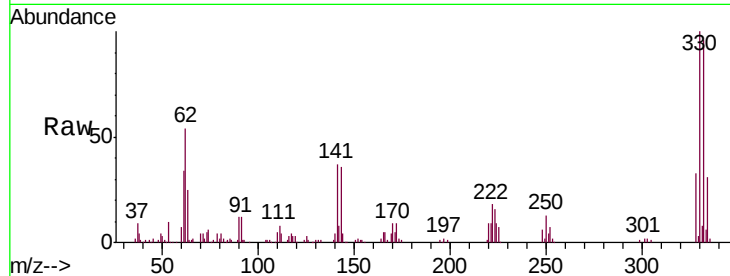


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

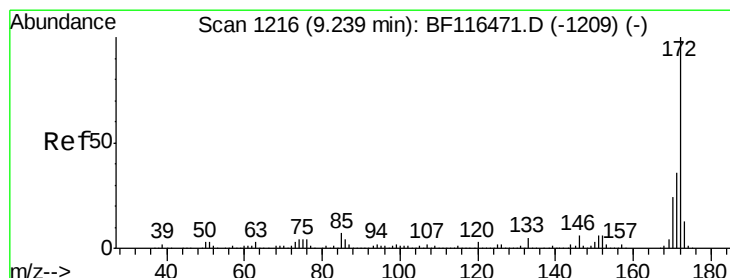
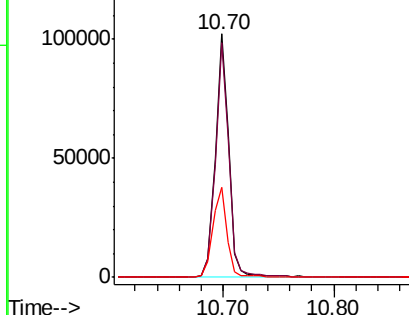



#45
 2-Fluorobiphenyl
 Concen: 69.734 ng
 RT: 9.24 min Scan# 1216
 Delta R.T. -0.00 min
 Lab File: BF116552.D
 Acq: 26 Aug 2019 3:14

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.2	28.9	43.3
170	23.9	19.4	29.0

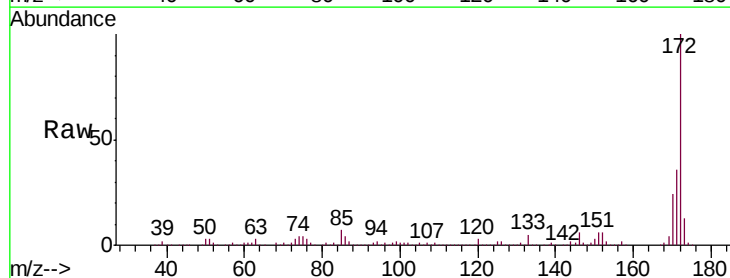

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

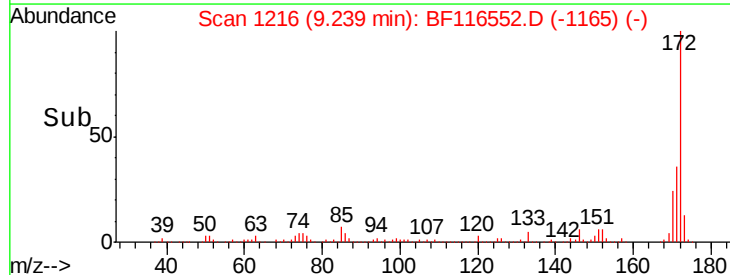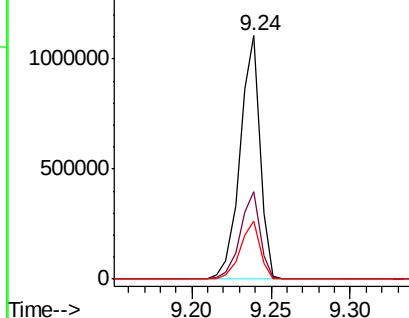


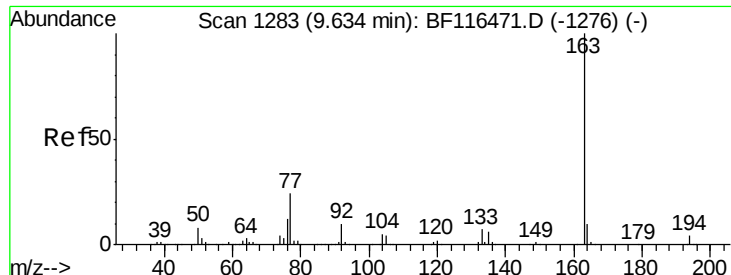




#50
Dimethylphthalate
Concen: 5.791 ng
RT: 9.62 min Scan# 1281
Delta R.T. -0.01 min
Lab File: BF116552.D
Acq: 26 Aug 2019 3:14

Instrument :
BNA_F
ClientSampleId :
SB-41-COMP

Tot Ion:163 Resp: 90086
Ion Ratio Lower Upper
163 100
194 3.7 2.9 4.3
164 10.7 8.2 12.2

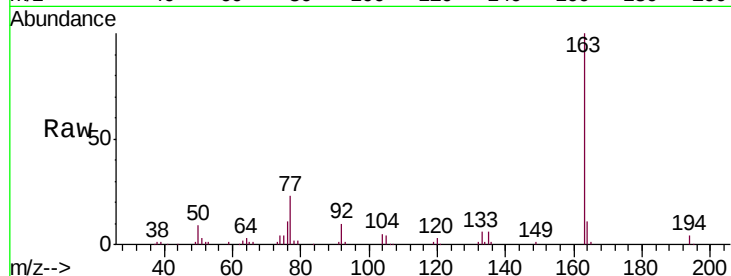


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

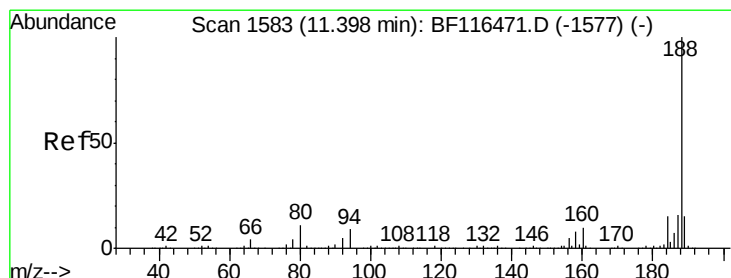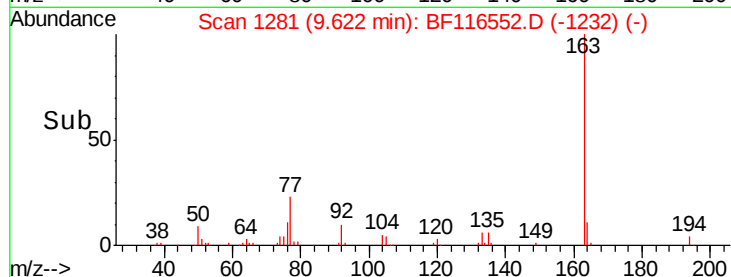
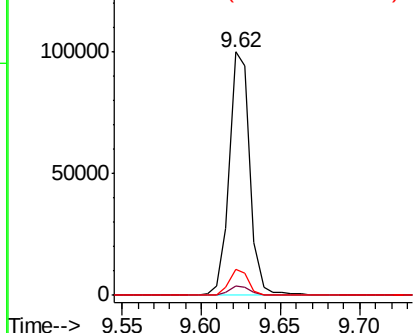



#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.40 min Scan# 1583
Delta R.T. -0.00 min
Lab File: BF116552.D
Acq: 26 Aug 2019 3:14

Tgt Ion:188 Resp: 297706
Ion Ratio Lower Upper
188 100
94 9.3 7.4 11.2
80 10.2 8.6 12.8

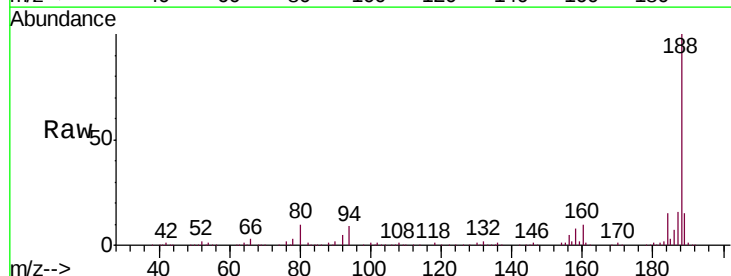

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1



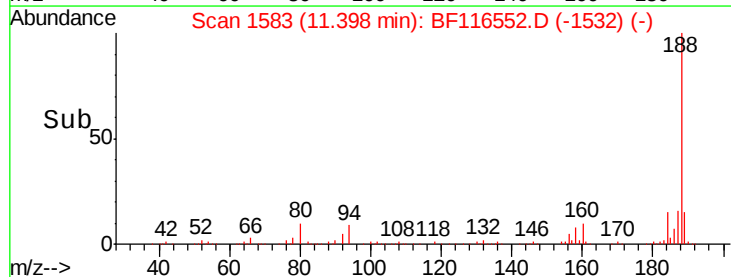
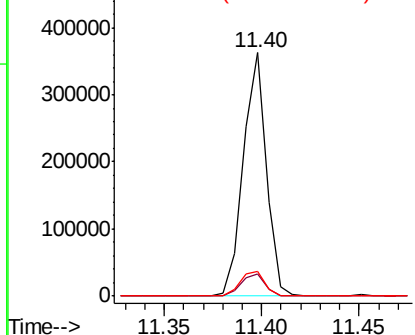




#76
 Chrvsene-d12
 Concen: 20.000 ng
 RT: 14.03 min Scan# 2030
 Delta R.T. -0.01 min
 Lab File: BF116552.D
 Acq: 26 Aug 2019 3:14




Instrument :
 BNA_F
 ClientSampleId :
 SB-41-COMP


Tot Ion	Ratio	Lower	Upper
240	100		
120	12.2	10.5	15.7
236	24.8	20.2	30.2

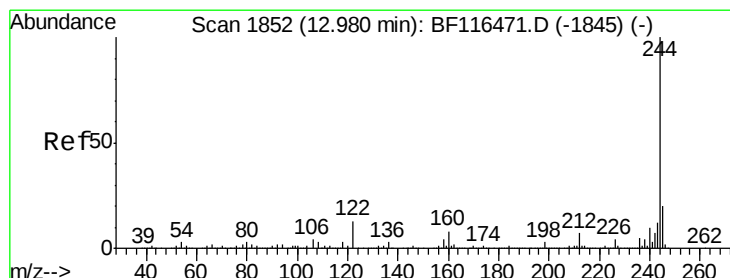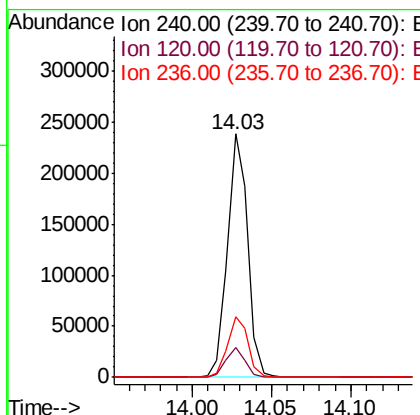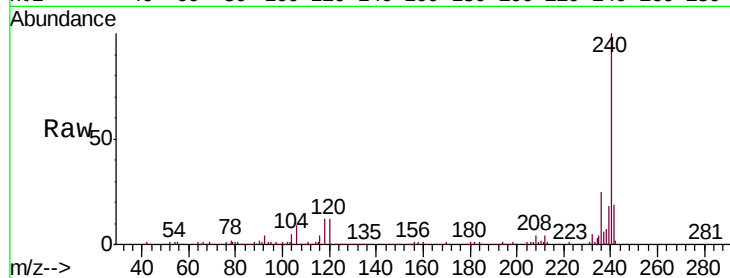

#79
 Terphenyl-d14
 Concen: 56.698 ng
 RT: 12.98 min Scan# 1852
 Delta R.T. -0.00 min
 Lab File: BF116552.D
 Acq: 26 Aug 2019 3:14

Tgt Ion	Ratio	Lower	Upper
244	100		
212	6.9	5.7	8.5
122	11.1	10.2	15.4

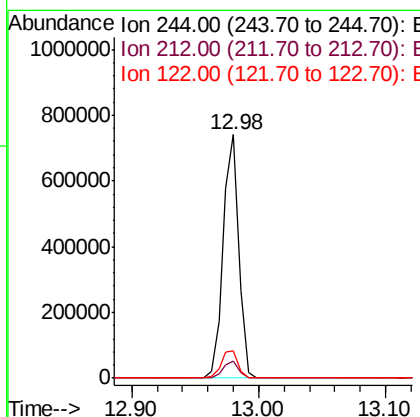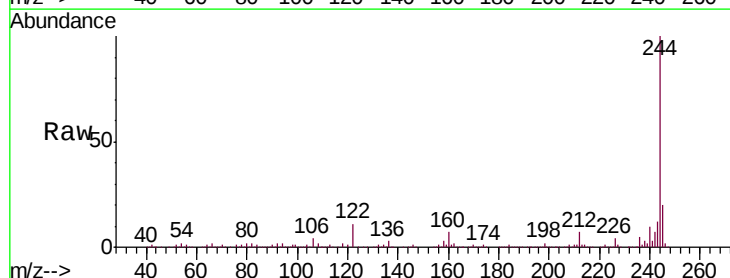


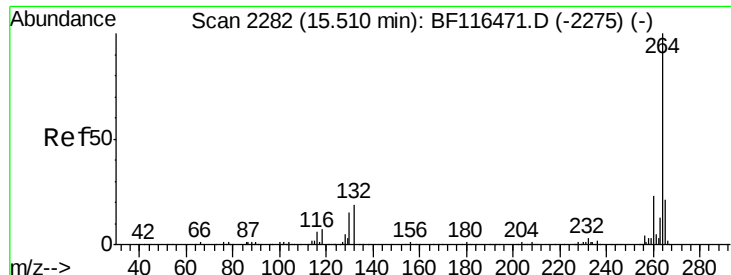

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.50 min Scan# 2280
 Delta R.T. -0.01 min
 Lab File: BF116552.D
 Acq: 26 Aug 2019 3:14

Instrument :
 BNA_F
 ClientSampleId :
 SB-41-COMP

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.9	18.8	28.2
265	20.9	17.1	25.7

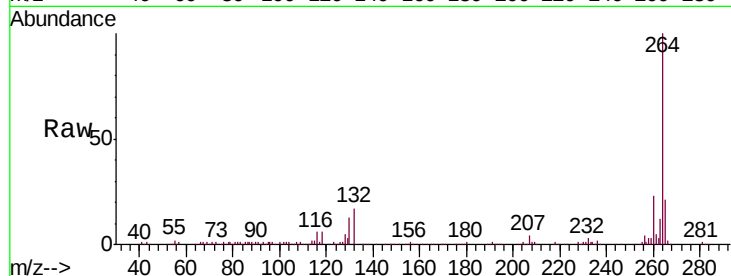

Abundance Ion 264.00 (263.70 to 264.70): E
 200000 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

