


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082519\
 Data File : BF116525.D
 Acq On : 25 Aug 2019 9:54
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 23 13:38:31 2019

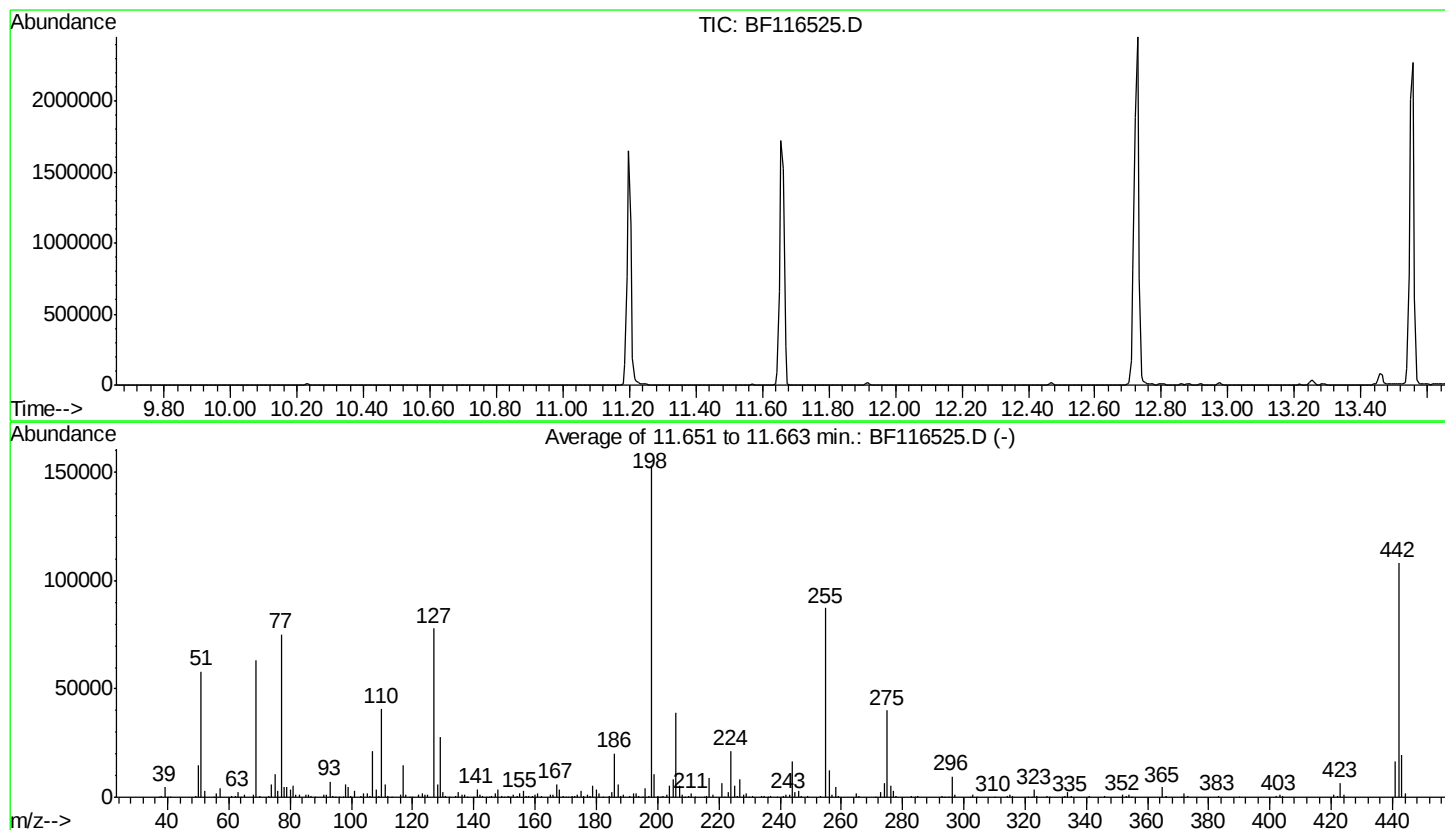

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	58109	PASS
68	69	0.00	2	1.6	1021	PASS
69	198	0.00	100	41.3	63218	PASS
70	69	0.00	2	0.6	402	PASS
127	198	10	80	50.8	77832	PASS
197	198	0.00	2	0.4	581	PASS
198	198	100	100	100.0	153138	PASS
199	198	5	9	6.8	10377	PASS
275	198	10	60	26.2	40082	PASS
365	198	1	100	3.1	4705	PASS
441	198	0.01	100	10.9	16651	PASS
442	198	50	100	70.7	108338	PASS
443	442	15	24	18.2	19677	PASS