
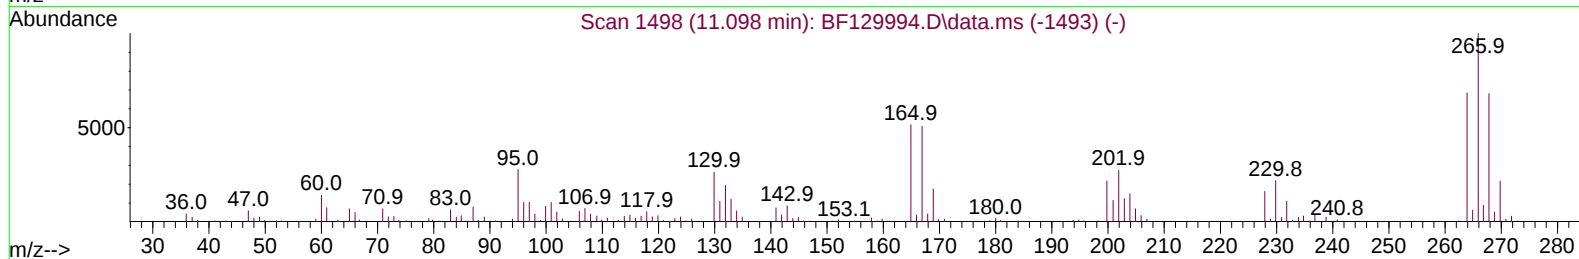
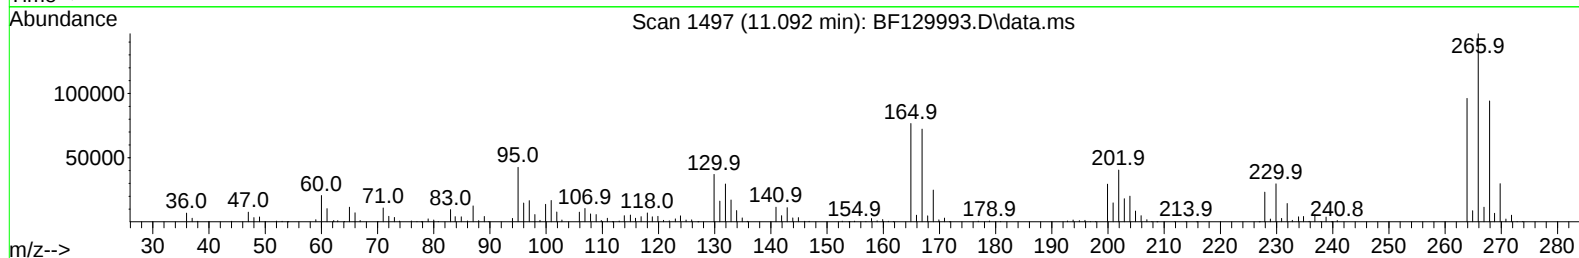


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082522\
Data File : BF129993.D
Acq On : 25 Aug 2022 10:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 17:23:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 14:45:09 2022
Response via : Initial Calibration

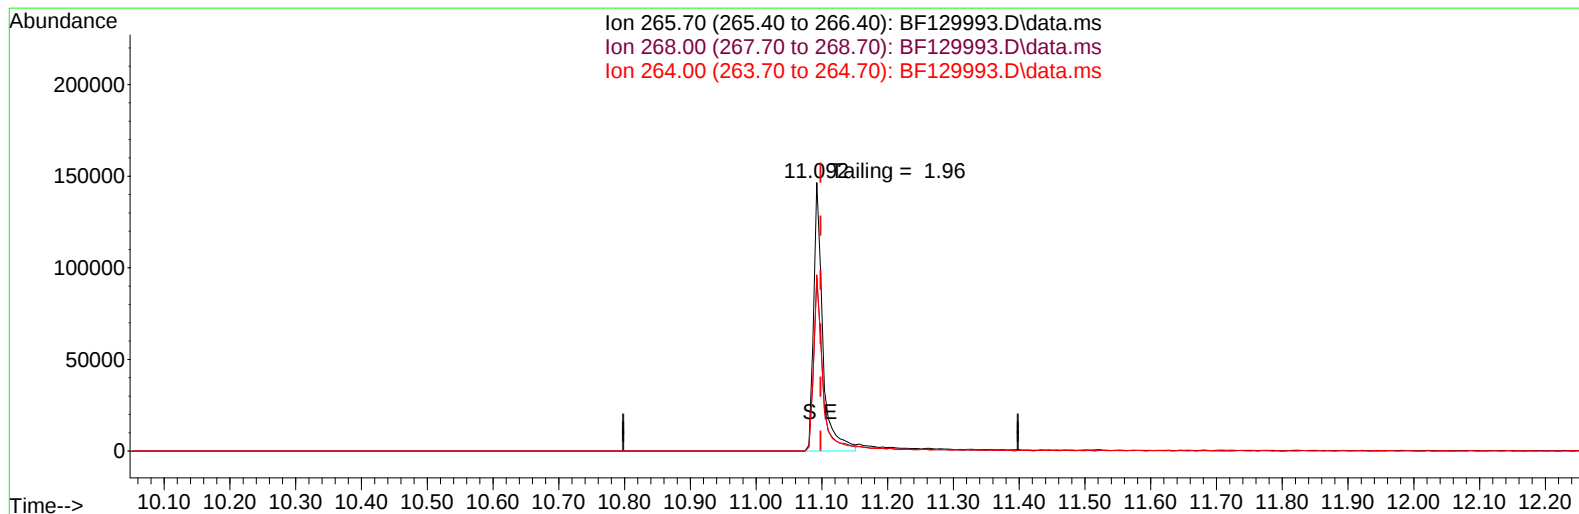

TIC: BF129993.D\data.ms




(70) Pentachlorophenol (C)

11.092min (-0.006) 176679.34 ng

response 153747

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.31
264.00	59.90	65.65
0.00	0.00	0.00

Quant Time: Aug 25 17:23:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 14:45:09 2022
Response via : Initial Calibration

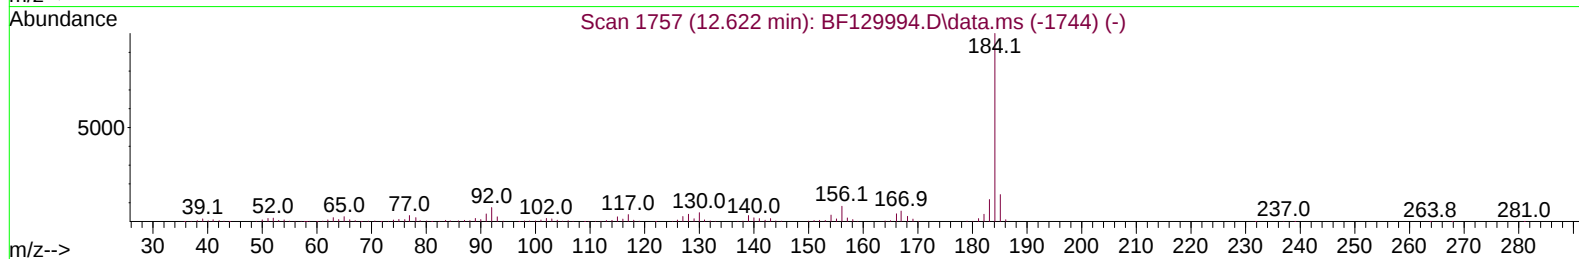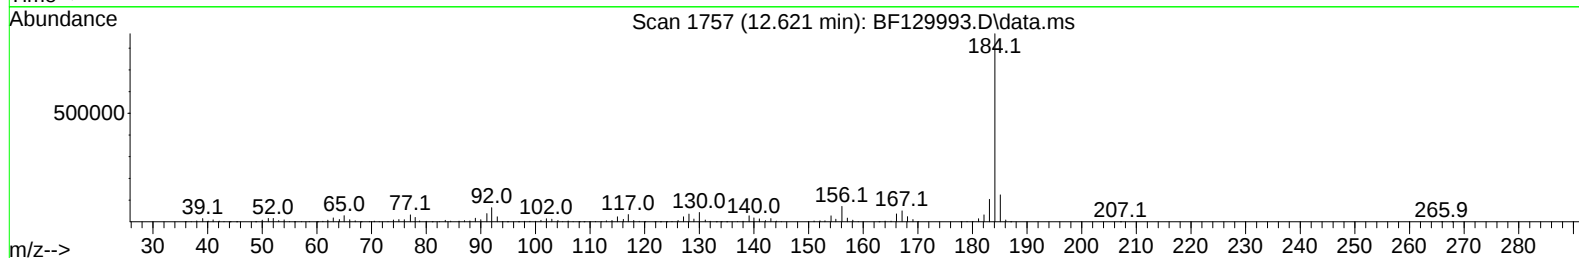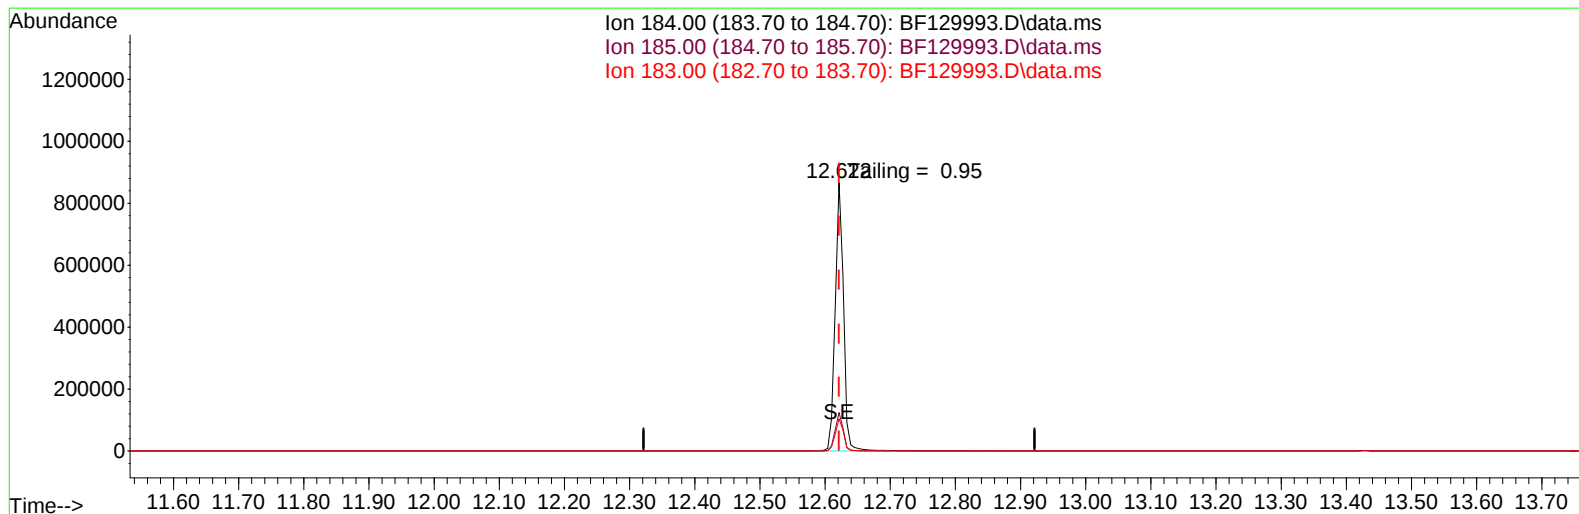

TIC: BF129993.D\data.ms

(77) Benzidine

12.621min (-0.000) 69900.05 ng

response **777516**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.35
183.00	11.80	11.97
0.00	0.00	0.00