

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082522\
 Data File : BF130010.D
 Acq On : 25 Aug 2022 21:08
 Operator : CG\JU
 Sample : N4323-01 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TR-05-082322

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130010.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.740	241	247	254	rBV2	5882	11712	1.43%	0.193%
2	4.963	452	455	467	rBV	29511	39956	4.88%	0.659%
3	5.404	527	530	542	rBV	199884	255972	31.23%	4.221%
4	6.428	701	704	725	rBV	198178	254241	31.02%	4.193%
5	6.757	756	760	767	rBV	689361	594801	72.58%	9.809%
6	7.328	854	857	866	rBV	144722	140646	17.16%	2.320%
7	8.039	974	978	987	rBV	808290	682674	83.30%	11.259%
8	9.110	1156	1160	1163	rBV	313405	247408	30.19%	4.080%
9	9.792	1272	1276	1279	rBV	737624	666169	81.29%	10.986%
10	10.586	1407	1411	1418	rBV	165411	146355	17.86%	2.414%
11	10.680	1424	1427	1432	rVB4	7339	11964	1.46%	0.197%
12	11.280	1525	1529	1532	rBV	905347	742981	90.66%	12.253%
13	11.304	1532	1533	1538	rVV	31301	20801	2.54%	0.343%
14	11.357	1538	1542	1546	rVV	10170	11260	1.37%	0.186%
15	11.657	1590	1593	1597	rBV	19067	15441	1.88%	0.255%
16	11.810	1616	1619	1623	rVB3	11877	11678	1.42%	0.193%
17	11.892	1631	1633	1636	rBV2	13872	13672	1.67%	0.225%
18	12.069	1660	1663	1667	rBV4	8473	11890	1.45%	0.196%
19	12.345	1705	1710	1711	rBV4	37515	45348	5.53%	0.748%
20	12.363	1711	1713	1715	rVB2	30238	24768	3.02%	0.408%
21	12.498	1732	1736	1739	rBV	86520	83609	10.20%	1.379%
22	12.727	1769	1775	1779	rBV	99112	119999	14.64%	1.979%
23	12.857	1794	1797	1802	rBV	374446	310200	37.85%	5.116%
24	13.927	1975	1979	1982	rBV	906986	819511	100.00%	13.515%
25	14.010	1990	1993	1998	rBV	180002	184129	22.47%	3.037%
26	15.374	2221	2225	2236	rVB2	482658	596431	72.78%	9.836%




Sum of corrected areas: 6063616

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082522\
Data File : BF130010.D
Acq On : 25 Aug 2022 21:08
Operator : CG\JU
Sample : N4323-01 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TR-05-082322

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

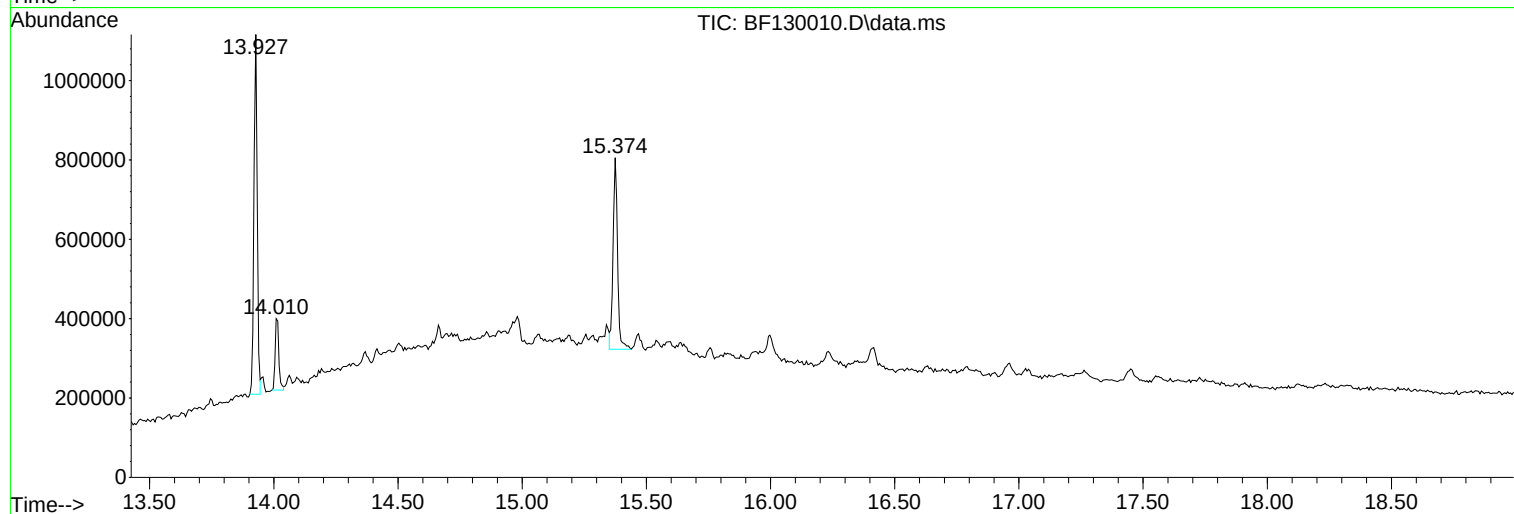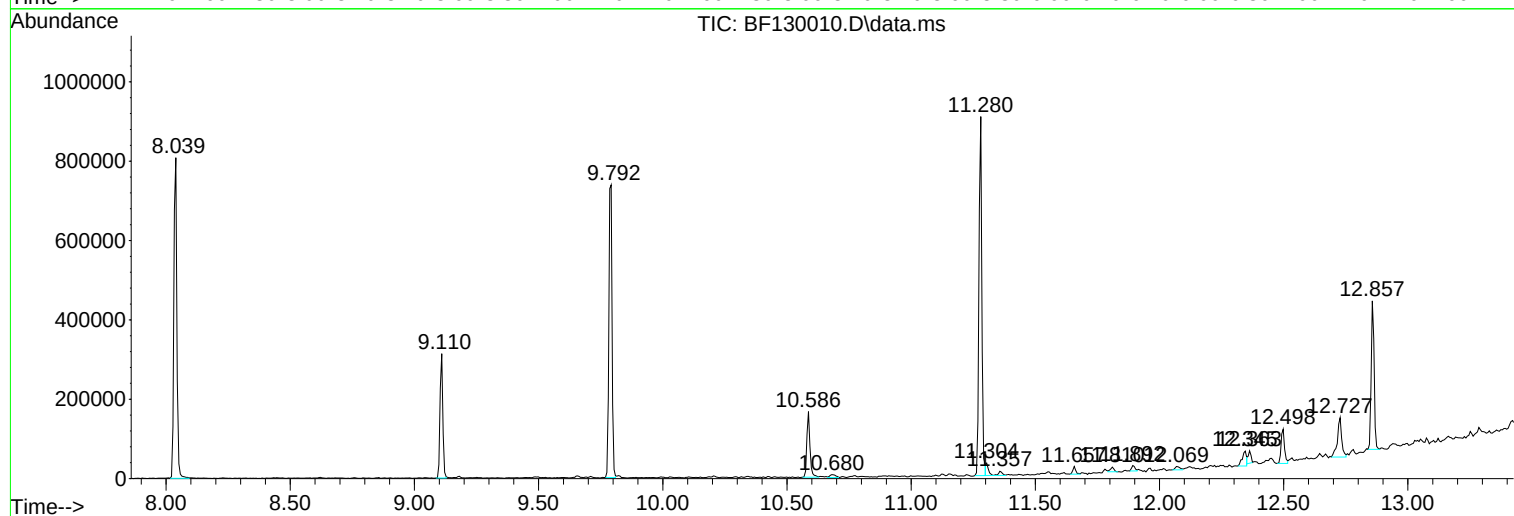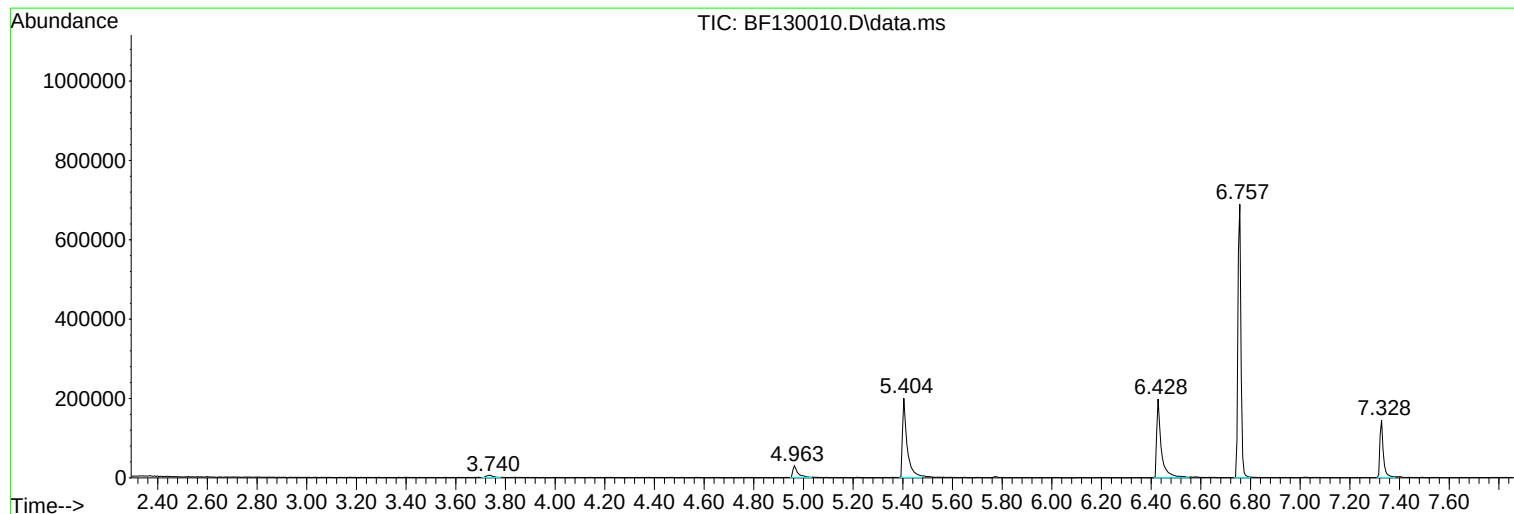

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082522\
Data File : BF130010.D
Acq On : 25 Aug 2022 21:08
Operator : CG\JU
Sample : N4323-01 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TR-05-082322










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.010	4.49 ng	184129	Chrysene-d12	13.927

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	94
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19N03S	1000483-83-4	70
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	45
4			Benzoic acid, 2-(diphenylphosphi...	306	C19H15O2P	017261-28-8	40
5			(Carbethoxymethyl)-triphenylphos...	428	C22H22BrO2P	001530-45-6	40

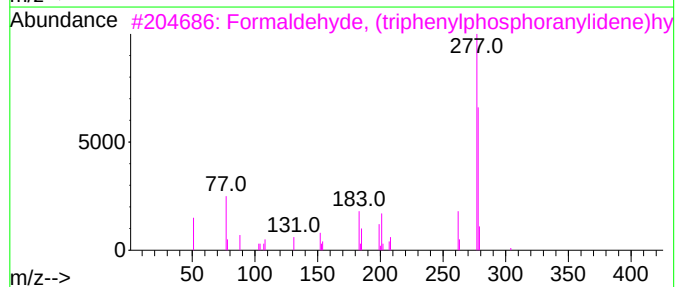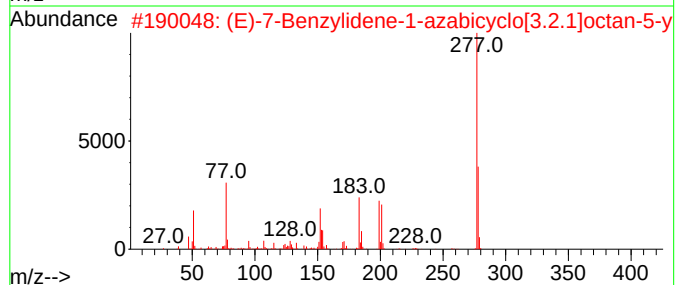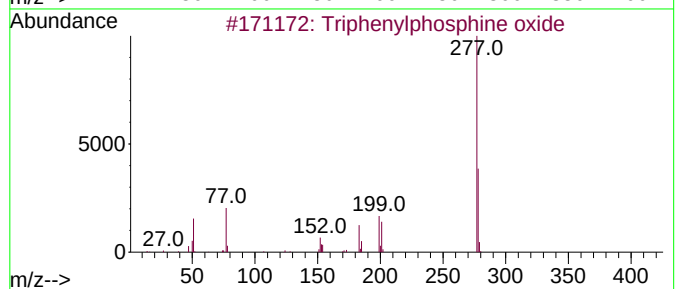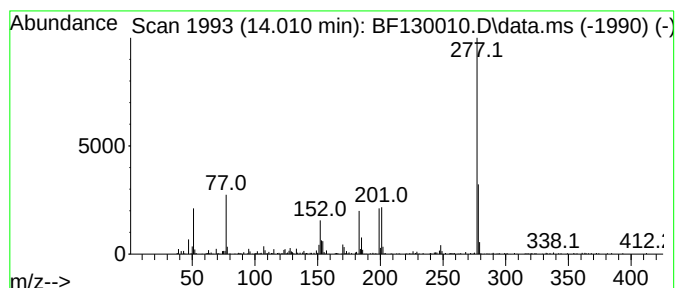

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082522\
Data File : BF130010.D
Acq On : 25 Aug 2022 21:08
Operator : CG\JU
Sample : N4323-01 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TR-05-082322

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.010	4.5	ng	184129	5	13.927	819511	20.0