
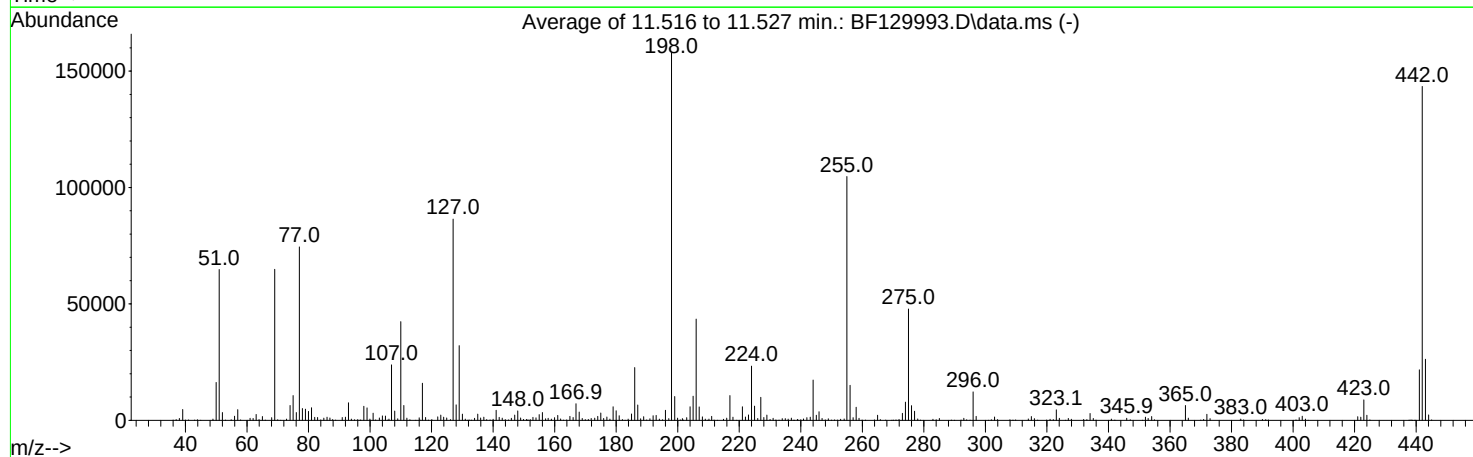


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082522\
 Data File : BF129993.D
 Acq On : 25 Aug 2022 10:41
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 25 14:45:09 2022

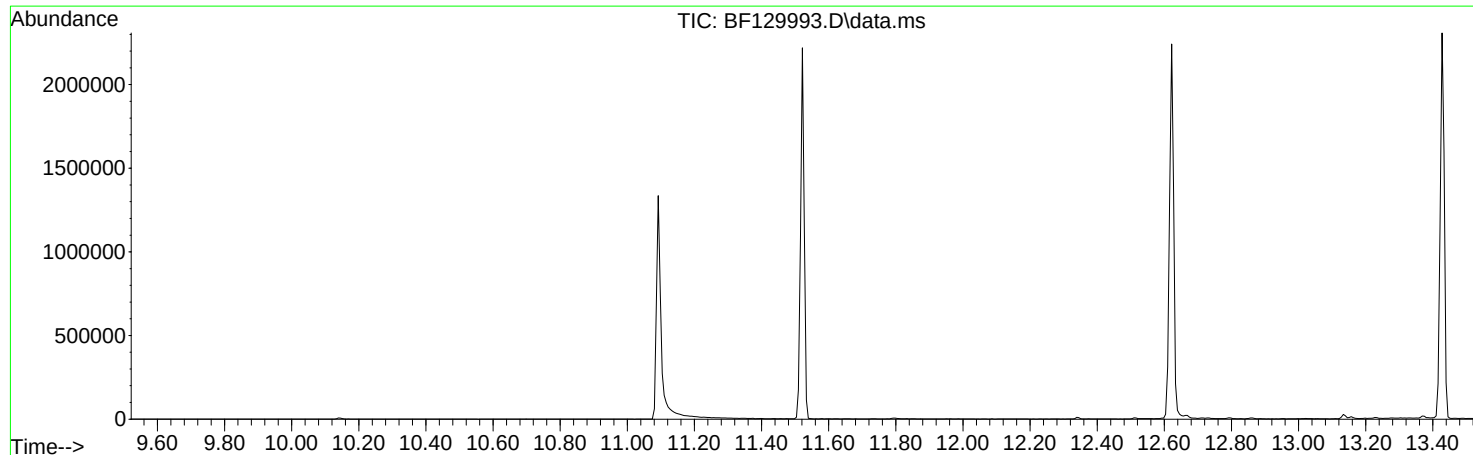




AutoFind: Scans 1569, 1570, 1571; Background Corrected with Scan 1564

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	64795	PASS
68	69	0.00	2	1.7	1126	PASS
69	198	0.00	100	41.0	64869	PASS
70	69	0.00	2	0.4	271	PASS
127	198	10	80	54.7	86453	PASS
197	198	0.00	2	0.5	714	PASS
198	198	100	100	100.0	158029	PASS
199	198	5	9	6.4	10189	PASS
275	198	10	60	30.2	47781	PASS
365	198	1	100	4.0	6397	PASS
441	198	0.01	100	13.7	21672	PASS
442	442	50	100	100.0	143397	PASS
443	442	15	24	18.3	26252	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082522\
Data File : BF129993.D
Acq On : 25 Aug 2022 10:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 25 17:23:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 14:45:09 2022
Response via : Initial Calibration

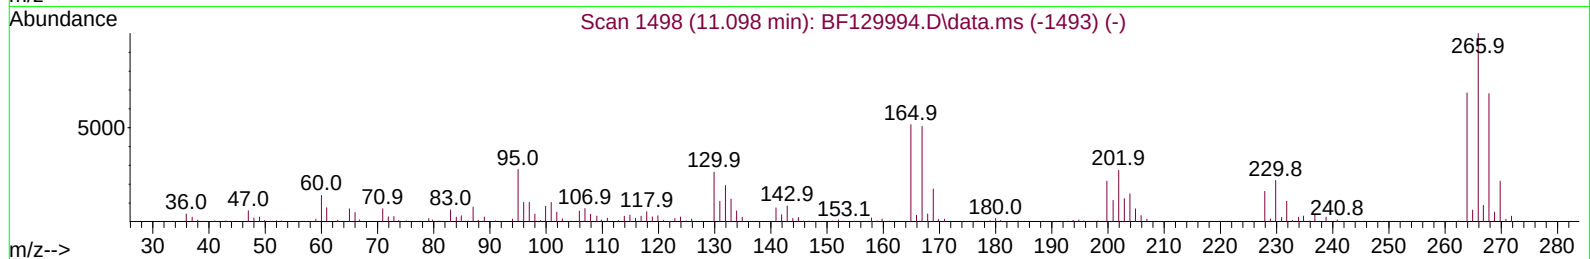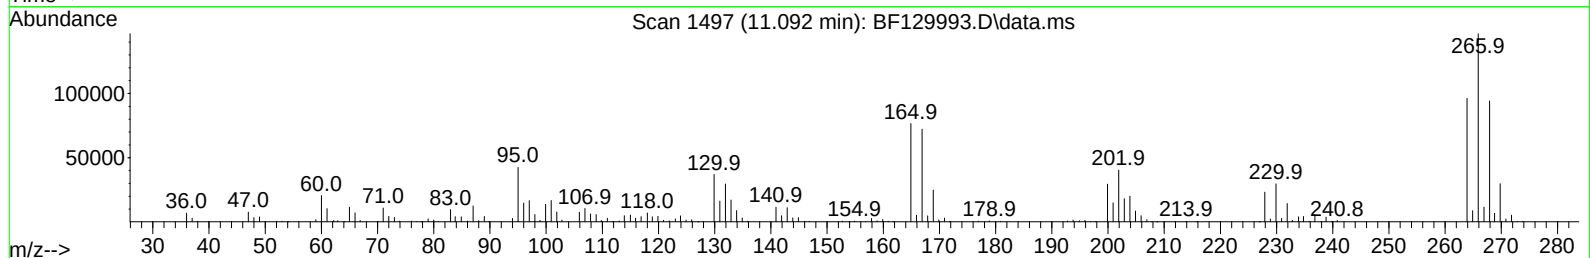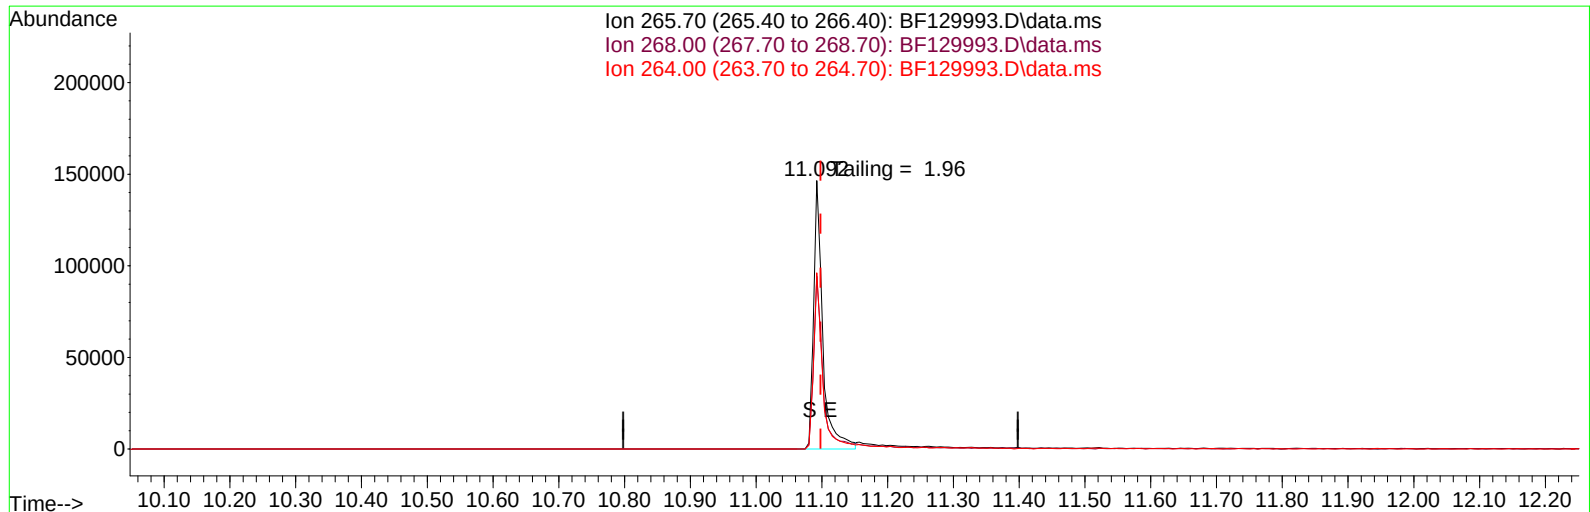

TIC: BF129993.D\data.ms

(70) Pentachlorophenol (C)

11.092min (-0.006) 176679.34 ng




response 153747

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.31
264.00	59.90	65.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082522\
Data File : BF129993.D
Acq On : 25 Aug 2022 10:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 25 17:23:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 14:45:09 2022
Response via : Initial Calibration

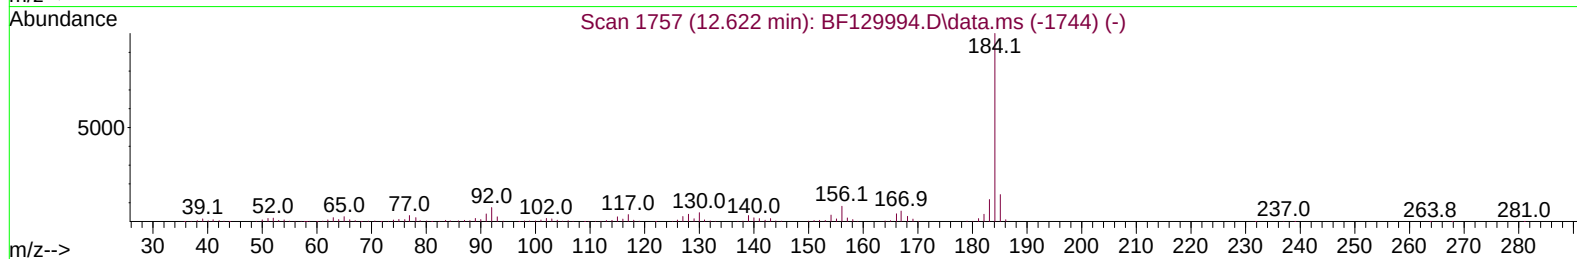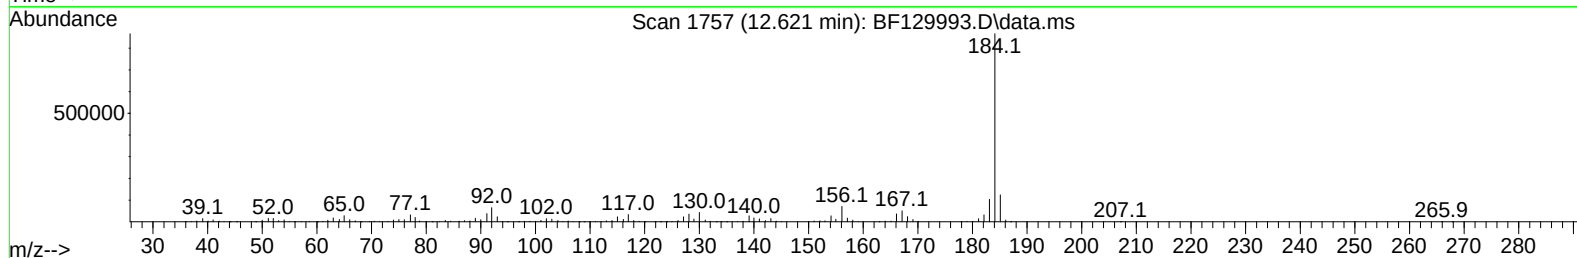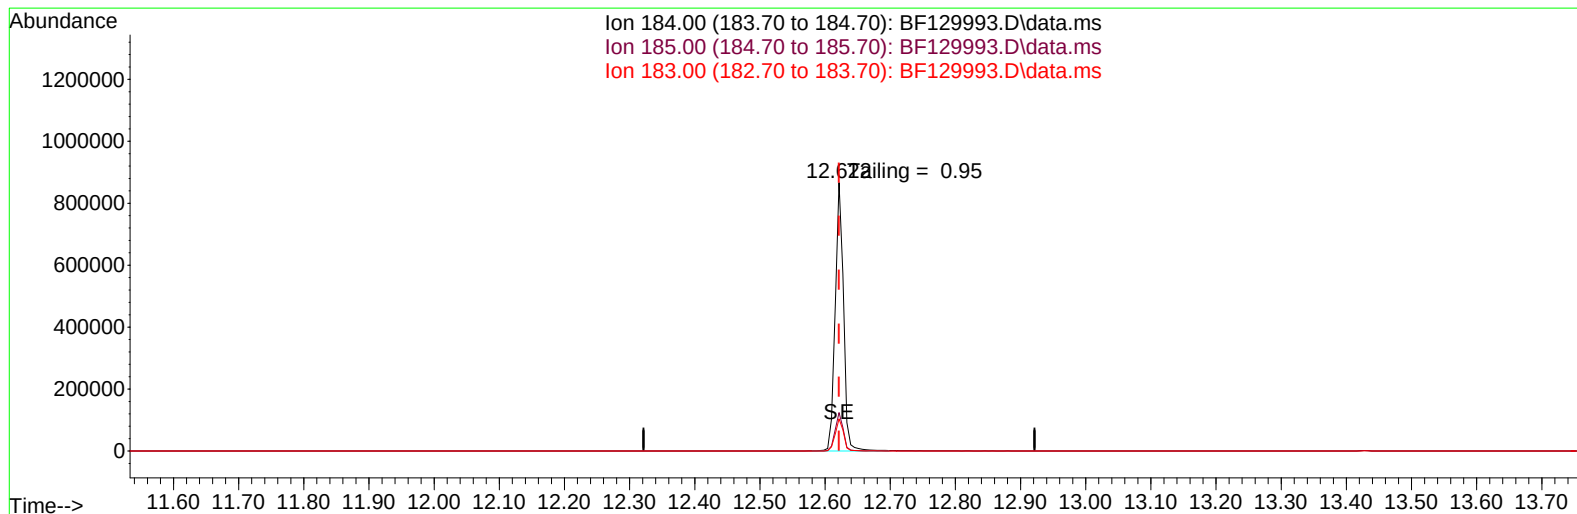

TIC: BF129993.D\data.ms

(77) Benzidine

12.621min (-0.000) 69900.05 ng

response 777516

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.35
183.00	11.80	11.97
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/25/2022	BNA_F	<u>BF129993.D</u>
Compound Name	Response	Retention Time
DDT	366495	13.42
DDD	4507	13.13
DDE	1025	12.79
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5532	372027	1.49

Instrument :
BNA_F
ClientSampleId :
DFTPP