
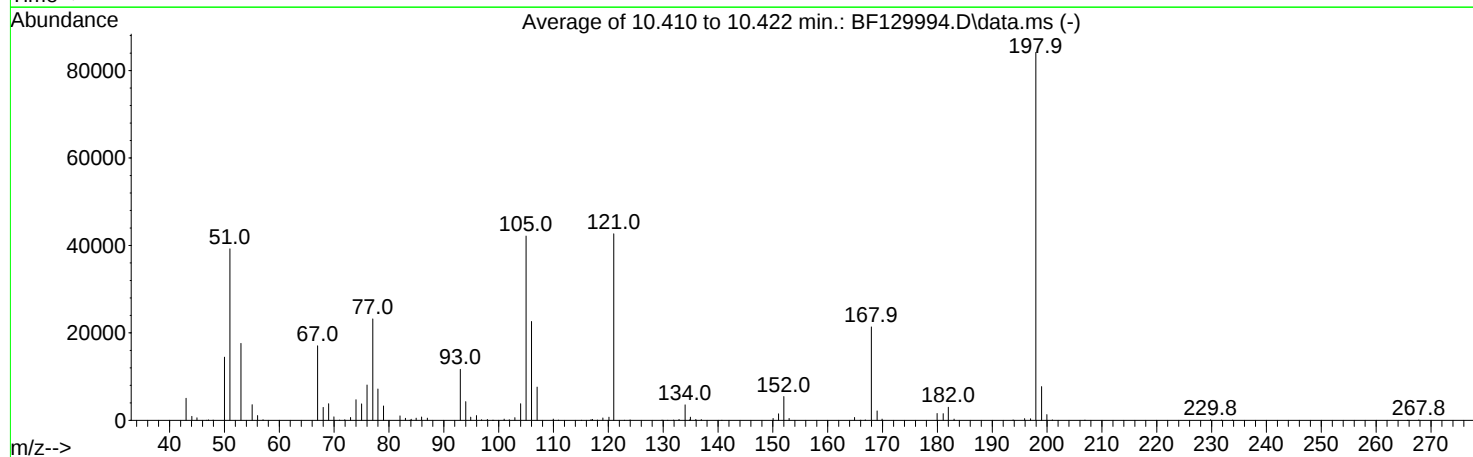


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082522\
 Data File : BF129994.D
 Acq On : 25 Aug 2022 11:49
 Operator : CG\JU
 Sample : SSTDCCC040
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_F
 LabSampleId :
 SSTDCCC040

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 25 14:45:09 2022

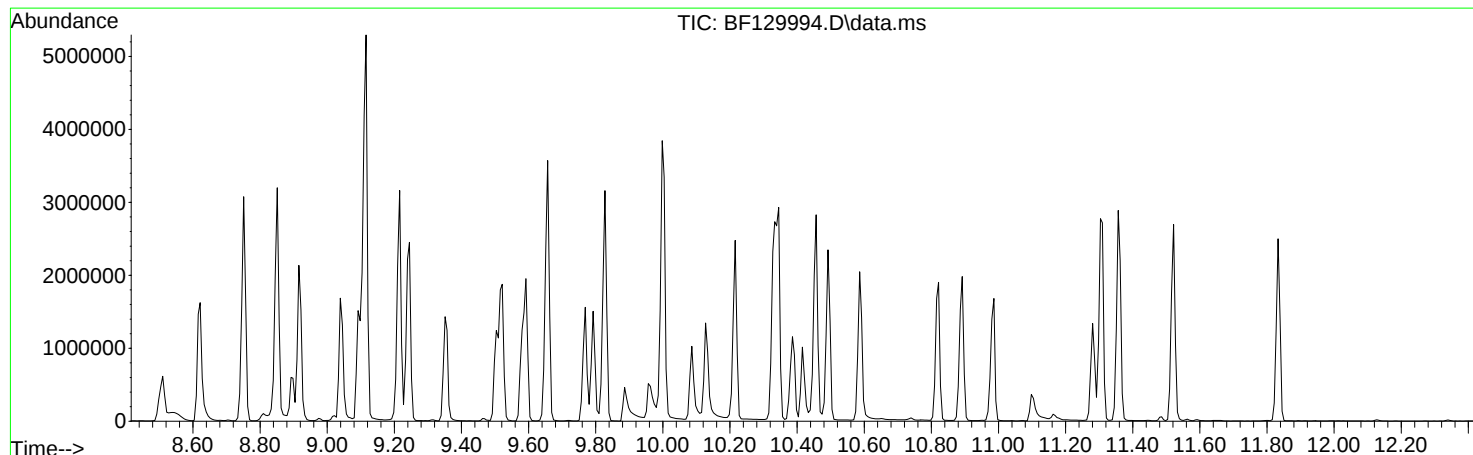

AutoFind: Scans 1381, 1382, 1383; Background Corrected with Scan 1378

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.6	39227	PASS
68	69	0.00	2	77.7	2958	FAIL*
69	198	0.00	100	4.5	3807	PASS
70	69	0.00	2	21.1	805	FAIL*
127	198	10	80	0.0	0	FAIL*
197	198	0.00	2	0.4	373	PASS
198	198	100	100	100.0	84130	PASS
199	198	5	9	9.2	7721	FAIL*
275	198	10	60	0.0	0	FAIL*
365	198	1	100	0.0	0	FAIL*
441	198	0.01	100	0.0	0	FAIL*
442.00	442.00	COMPARISON MASS IS NOT PRESENT!!!				
443.00	442.00	COMPARISON MASS IS NOT PRESENT!!!				