


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082523\
Data File : BF134936.D
Acq On : 25 Aug 2023 11:48
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 28 02:45:19 2023

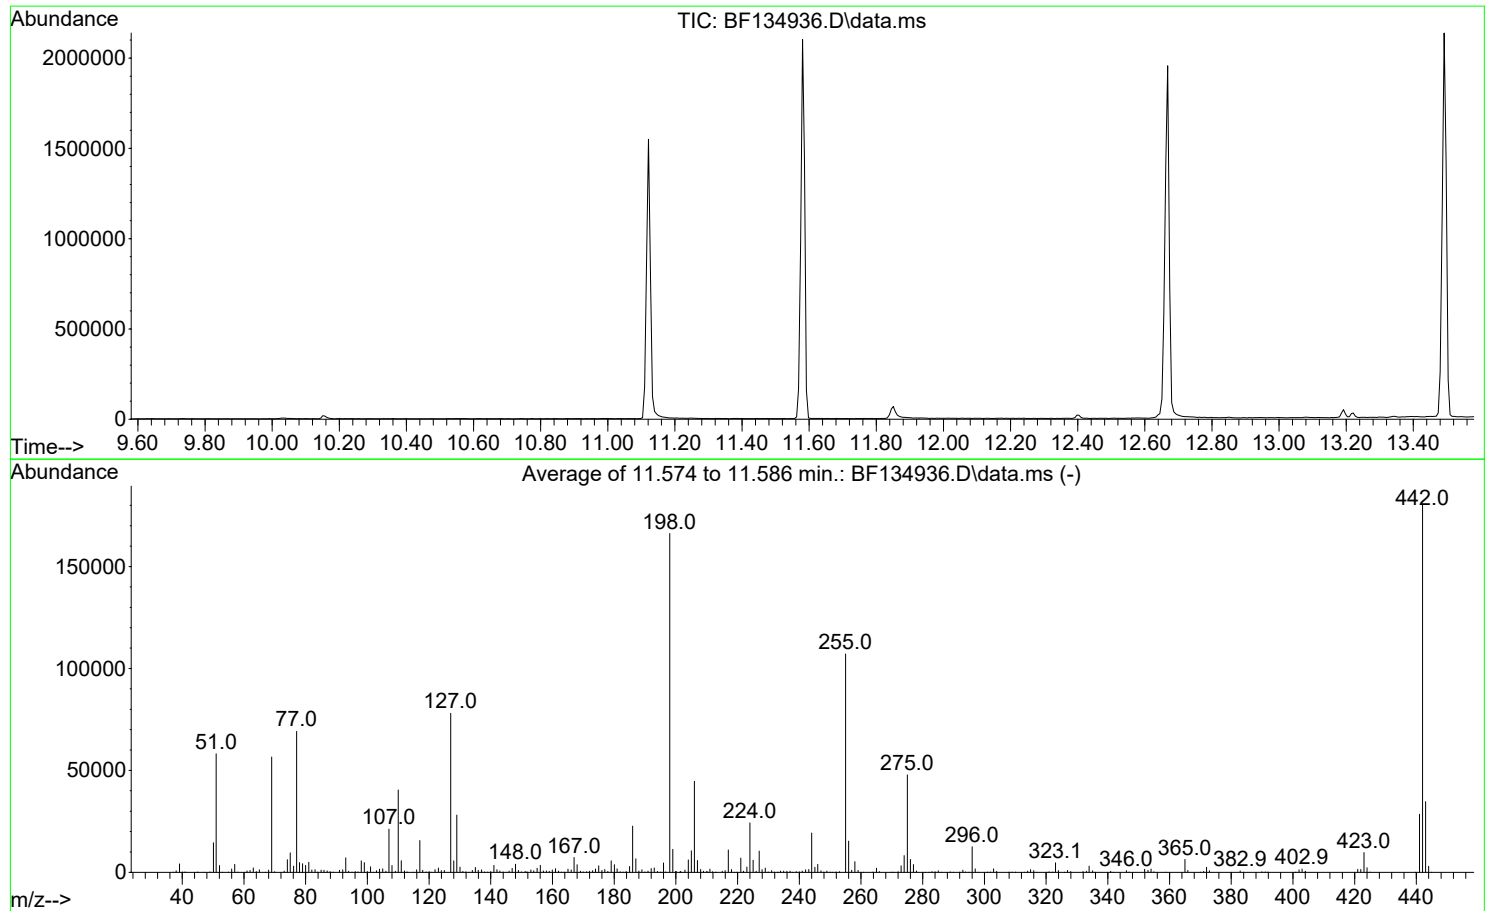




AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	58137	PASS
68	69	0.00	2	1.9	1094	PASS
69	198	0.00	100	34.0	56597	PASS
70	69	0.00	2	0.6	318	PASS
127	198	10	80	46.9	78035	PASS
197	198	0.00	2	0.2	278	PASS
198	198	100	100	100.0	166240	PASS
199	198	5	9	6.8	11295	PASS
275	198	10	60	28.7	47760	PASS
365	198	1	100	3.8	6339	PASS
441	198	0.01	100	17.1	28508	PASS
442	442	50	100	100.0	180429	PASS
443	442	15	24	19.2	34706	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082523\
Data File : BF134936.D
Acq On : 25 Aug 2023 11:48
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 25 14:11:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 22 19:33:25 2023
Response via : Initial Calibration

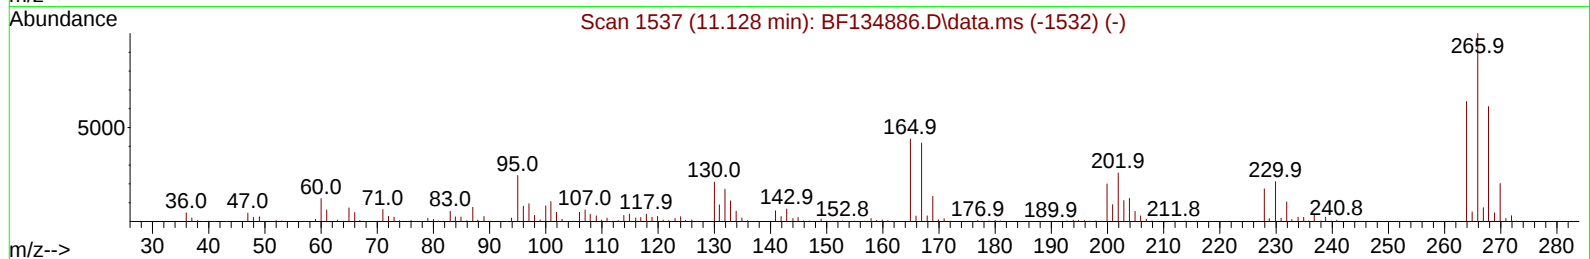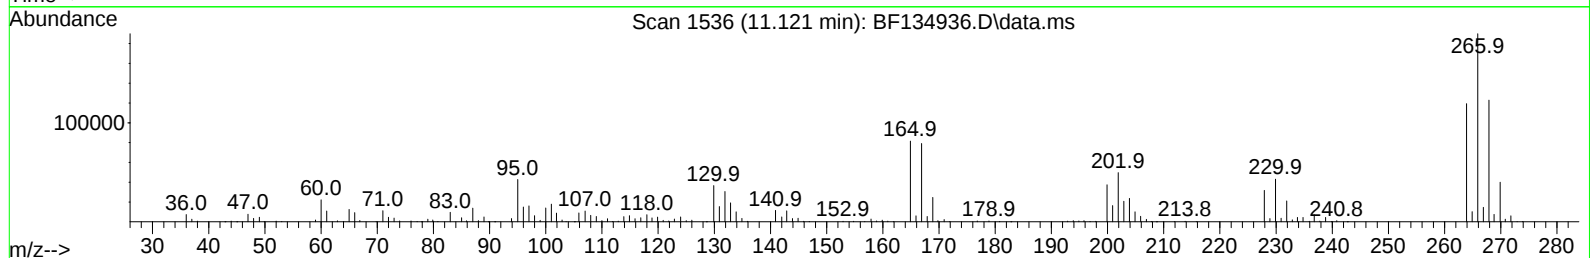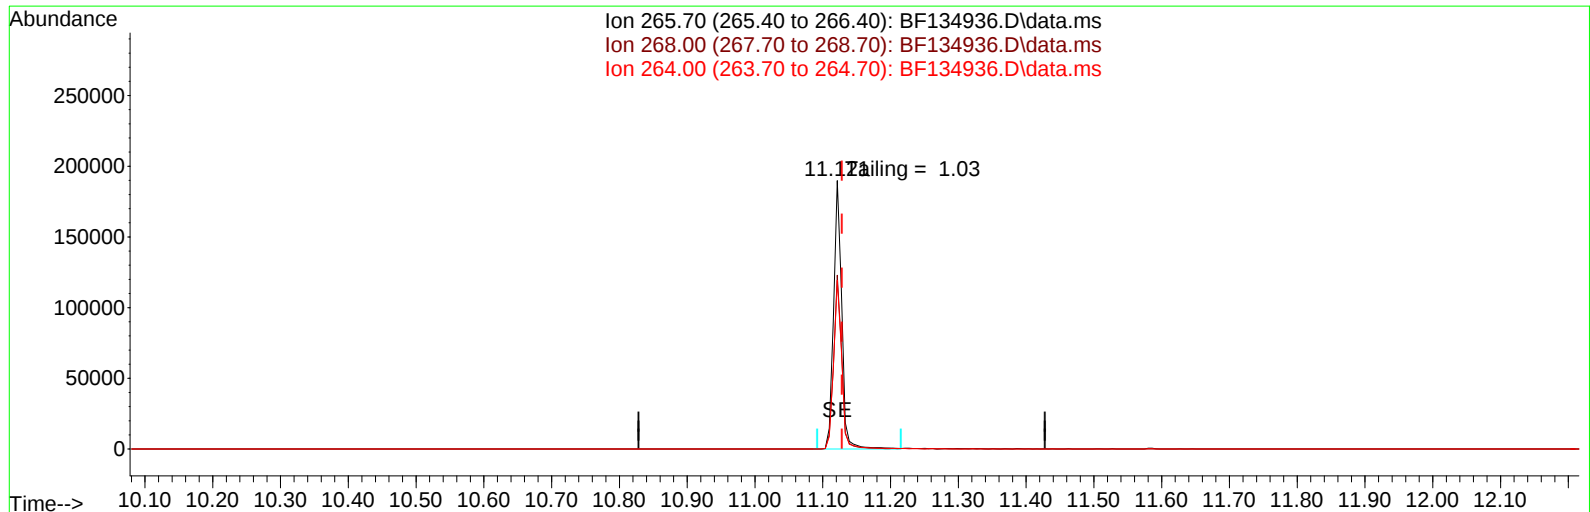

TIC: BF134936.D\data.ms

(70) Pentachlorophenol (C)

11.121min (-0.007) 30827.24 ng




response 158661

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	64.73
264.00	63.80	62.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082523\
Data File : BF134936.D
Acq On : 25 Aug 2023 11:48
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 25 14:11:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 22 19:33:25 2023
Response via : Initial Calibration

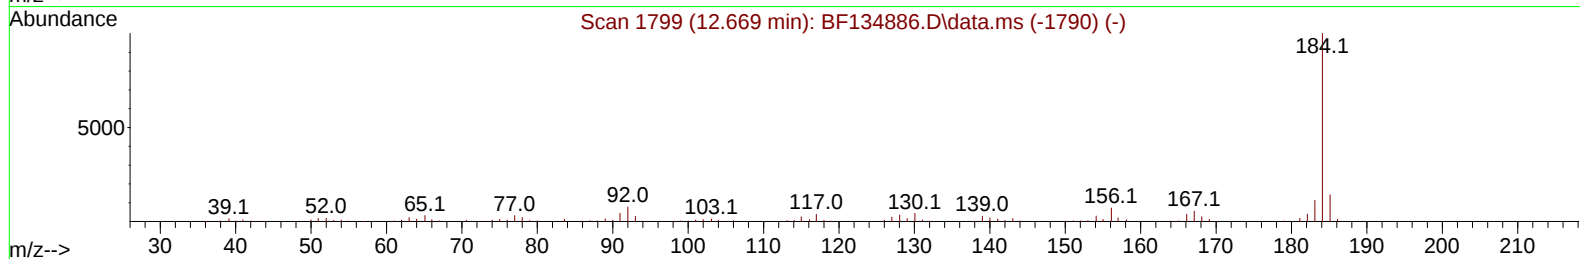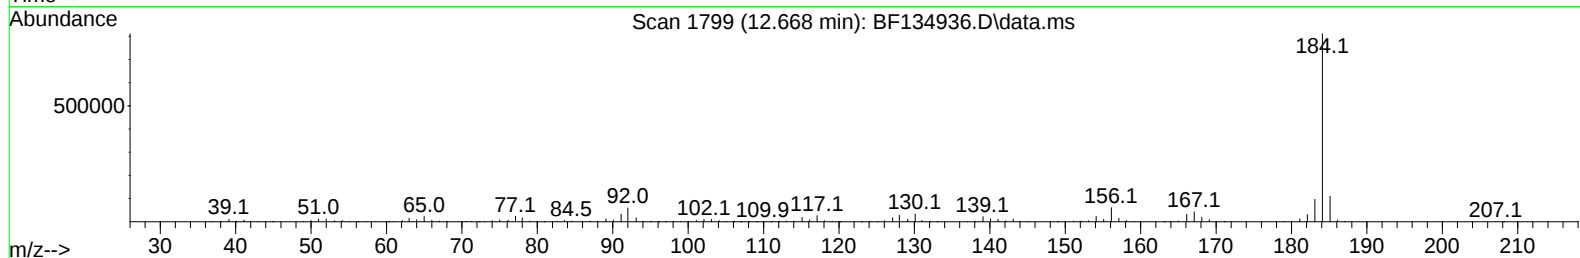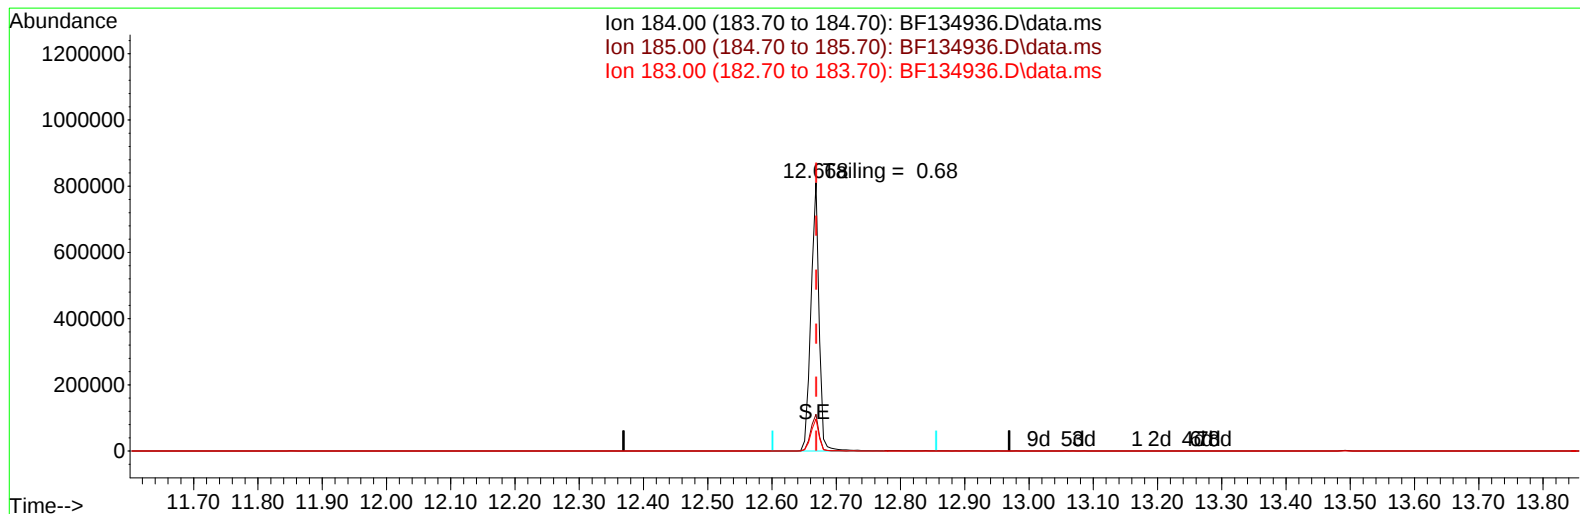

TIC: BF134936.D\data.ms

(77) Benzidine

12.668min (-0.001) 839434.57 ng m

response 721844

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.64
183.00	11.20	11.93
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/25/2023	BNA_F	<u>BF134936.D</u>
Compound Name	Response	Retention Time
DDT	369568	13.492
DDD	11465	13.192
DDE	511	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11976	381544	3.14

Instrument :
BNA_F
ClientSampleId :
DFTPP