

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082718\
 Data File : BF108521.D
 Acq On : 27 Aug 2018 20:03
 Operator : JU/SJ
 Sample : J4652-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Aug 28 01:36:48 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 22 11:01:45 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.00	152	119995	20.00	ng	-0.01
21) Naphthalene-d8	8.28	136	457791	20.00	ng	0.00
38) Acenaphthene-d10	10.04	164	218332	20.00	ng	-0.01
63) Phenanthrene-d10	11.54	188	352158	20.00	ng	-0.01
75) Chrysene-d12	14.19	240	290927	20.00	ng	-0.01
86) Perylene-d12	15.75	264	263073	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.62	112	476737	71.93	ng	0.00
7) Phenol-d6	6.62	99	640319	72.70	ng	-0.01
23) Nitrobenzene-d5	7.56	82	381695	46.53	ng	-0.01
41) 2,4,6-Tribromophenol	10.84	330	144824	66.50	ng	-0.01
44) 2-Fluorobiphenyl	9.35	172	656438	48.27	ng	-0.01
78) Terphenyl-d14	13.12	244	403213	35.24	ng	-0.01
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.56	70	50876	8.542	ng	# 82
25) Isophorone	7.56	82	381691	24.409	ng	# 64
49) Dimethylphthalate	9.75	163	212421	13.967	ng	# 98
56) 2,4-Dinitrotoluene	10.04	165	27489	6.712	ng	# 23
64) 4,6-Dinitro-2-methylphenol	10.84	198	271	5.541	ng	# 1
66) 4-Bromophenyl-phenylether	10.84	248	9445	2.468	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082718\
Data File : BF108521.D
Acq On : 27 Aug 2018 20:03
Operator : JU/SJ
Sample : J4652-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Aug 28 01:36:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 22 11:01:45 2018
Response via : Initial Calibration

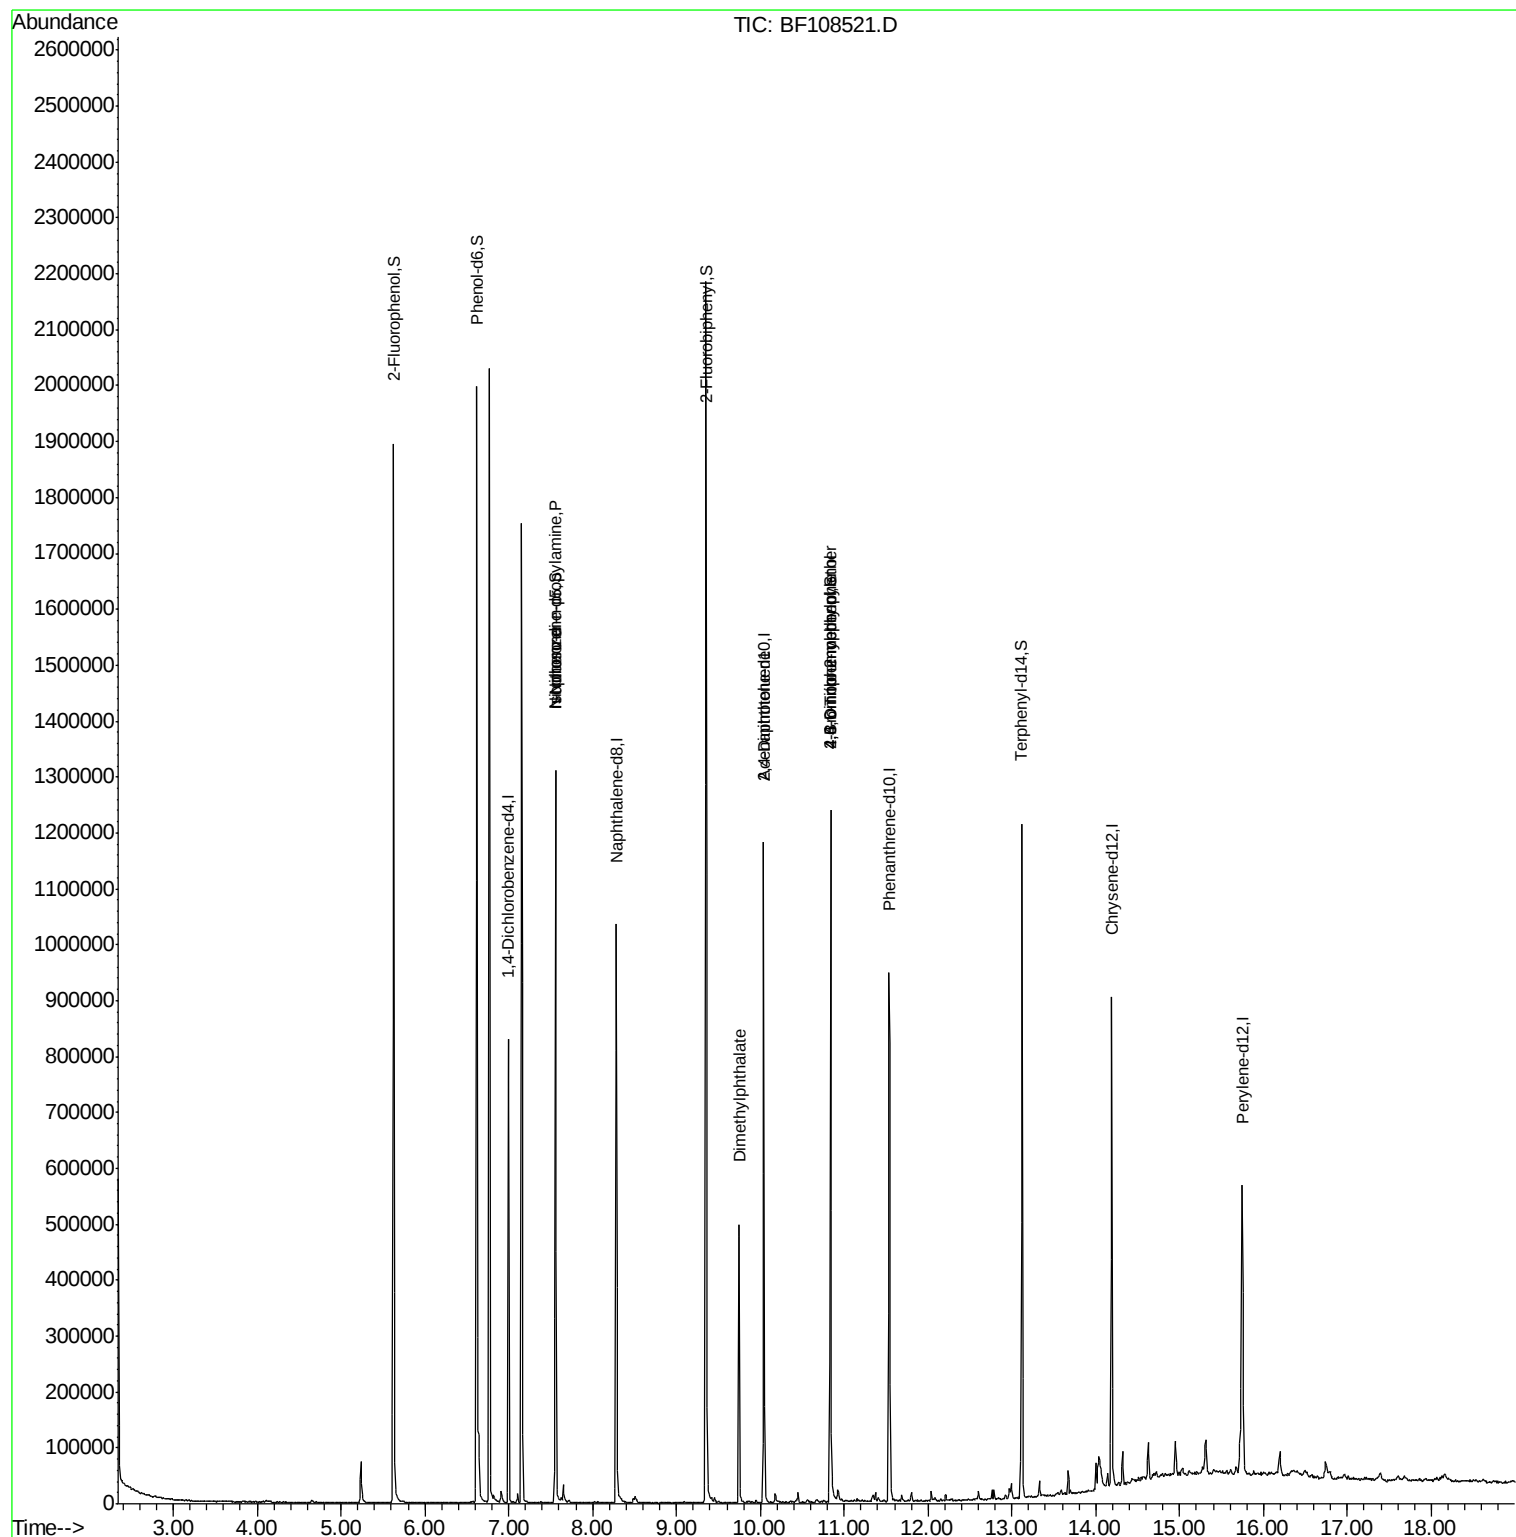




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.00 min Scan# 792
Delta R.T. -0.01 min
Lab File: BF108521.D
Acq: 27 Aug 2018 20:03

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	154.5	124.6	186.8
115	61.6	50.1	75.1



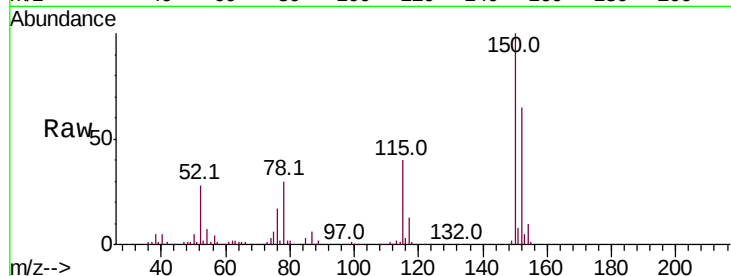


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

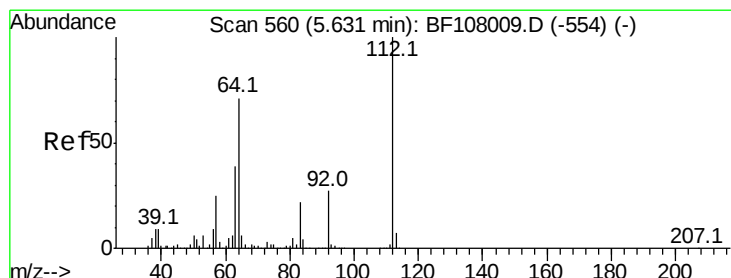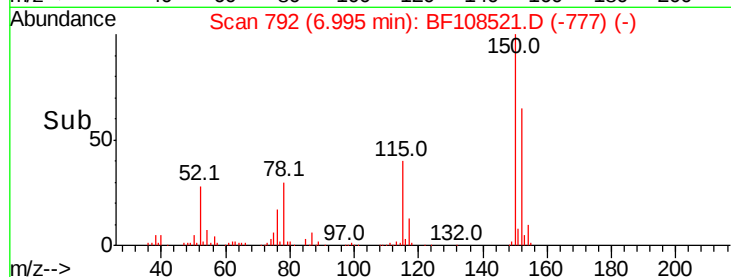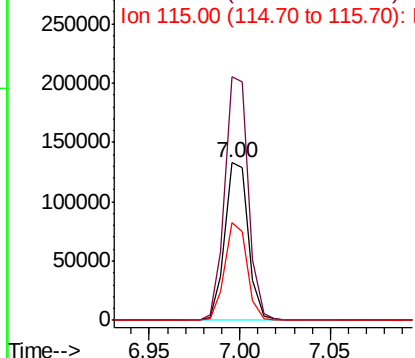

#5

2-Fluorophenol
Concen: 71.929 ng
RT: 5.62 min Scan# 559
Delta R.T. -0.01 min
Lab File: BF108521.D
Acq: 27 Aug 2018 20:03

Tgt Ion	Ratio	Lower	Upper
112	100		
64	70.7	47.9	71.9
63	37.5	23.7	35.5#


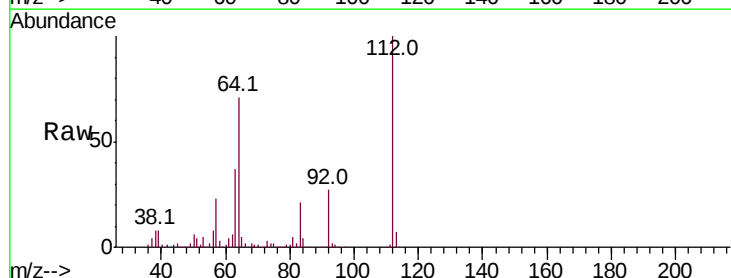


Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

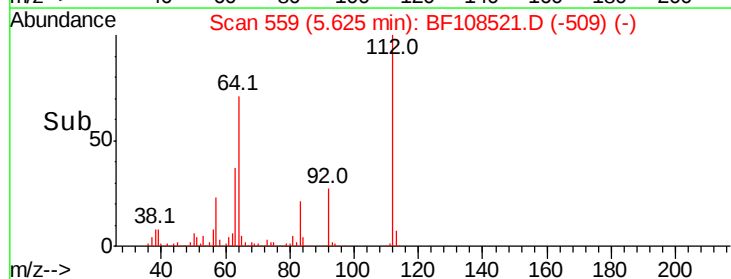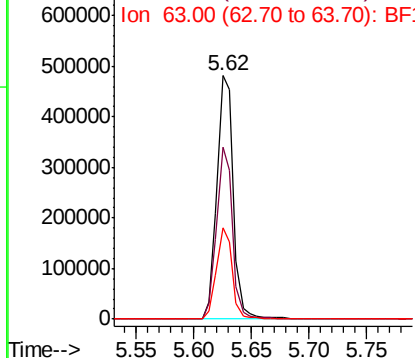



#7

Phenol-d6

Concen: 72.701 ng

RT: 6.62 min Scan# 728

Delta R.T. -0.01 min

Lab File: BF108521.D

Acq: 27 Aug 2018 20:03

Instrument :

BNA_F

ClientSampled :


Tot Ion: 99 Resp: 640319

Ion Ratio Lower Upper




99 100

42 23.5 14.5 21.7#

71 37.1 25.4 38.0

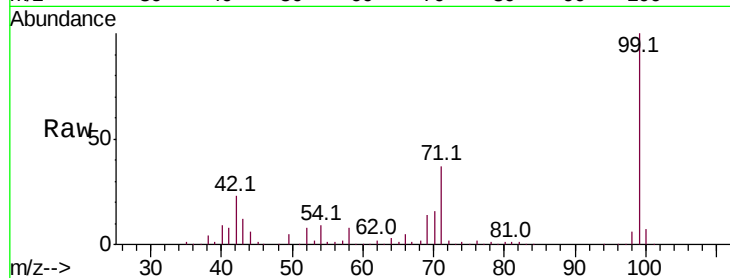

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

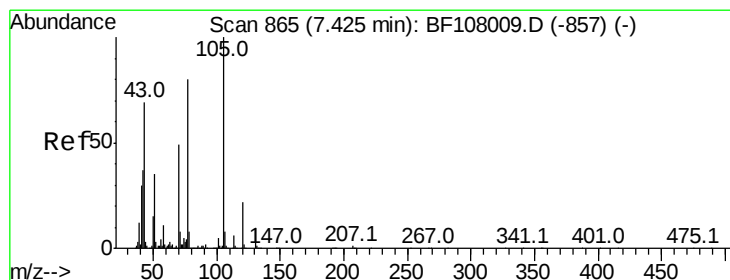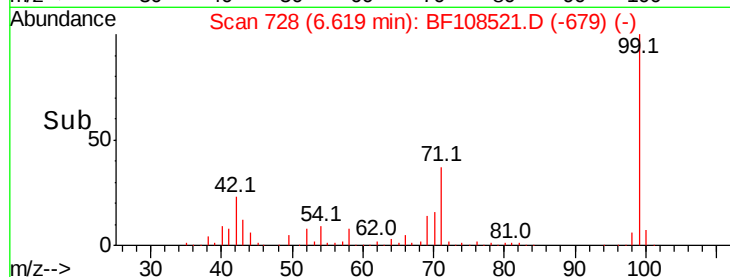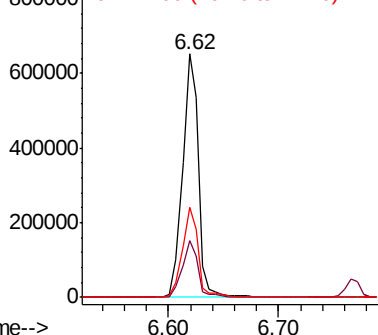

#19

n-Nitroso-di-n-propylamine

Concen: 8.542 ng

RT: 7.56 min Scan# 888

Delta R.T. 0.15 min

Lab File: BF108521.D

Acq: 27 Aug 2018 20:03

Tgt Ion: 70 Resp: 50876


Ion Ratio Lower Upper

70 100



42 52.1 47.5 71.3


101 0.0 7.4 11.2#

130 2.2 16.6 25.0#

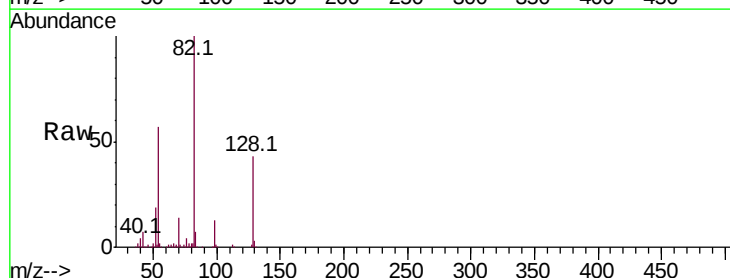

Abundance Ion 70.00 (69.70 to 70.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 101.00 (100.70 to 101.70): BF1
Ion 130.00 (129.70 to 130.70): BF1

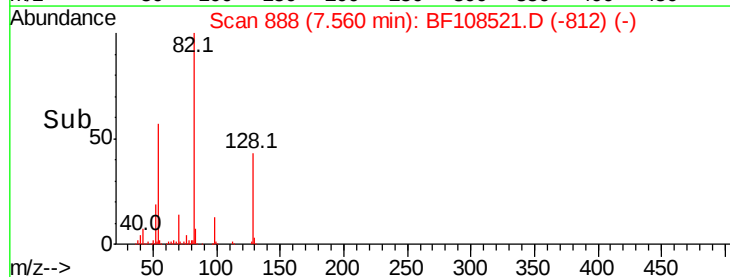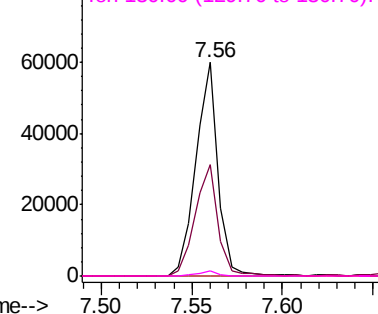

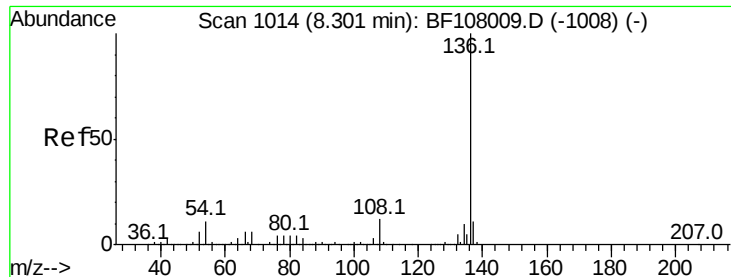

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.28 min Scan# 1011

Delta R.T. -0.01 min

Lab File: BF108521.D

Acq: 27 Aug 2018 20:03

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136 Resp: 457791


Ion Ratio Lower Upper

136 100

137 10.8 8.9 13.3

54 8.9 6.6 9.8

68 5.4 5.0 7.4



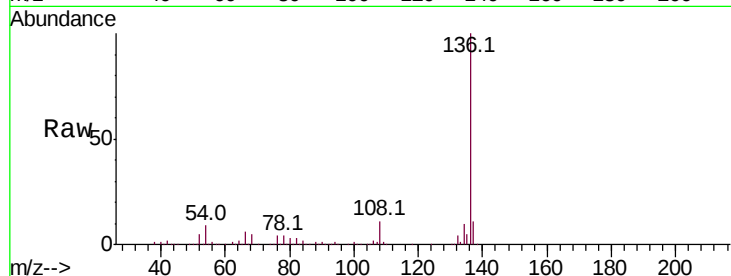


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

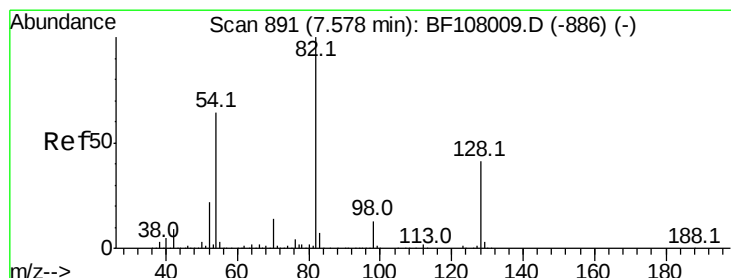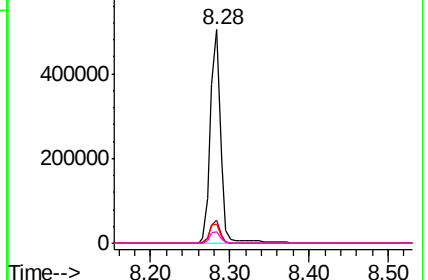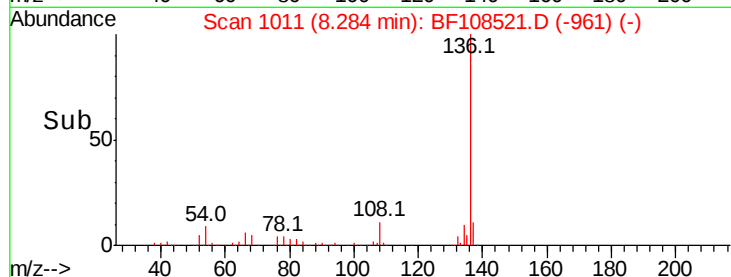

#23

Nitrobenzene-d5

Concen: 46.526 ng

RT: 7.56 min Scan# 888

Delta R.T. -0.01 min

Lab File: BF108521.D

Acq: 27 Aug 2018 20:03


Tgt Ion: 82 Resp: 381695

Ion Ratio Lower Upper

82 100

128 42.8 36.1 54.1



54 57.3 41.4 62.2

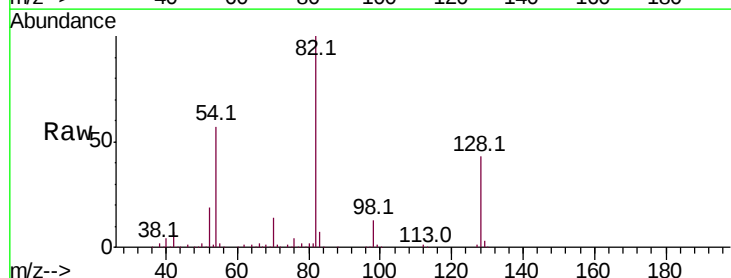


Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

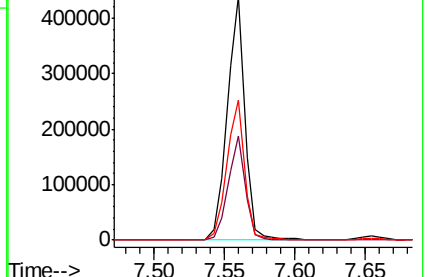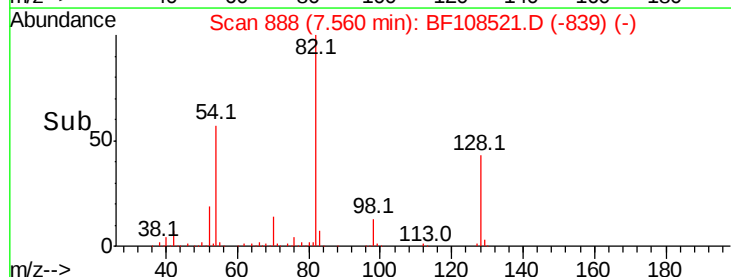

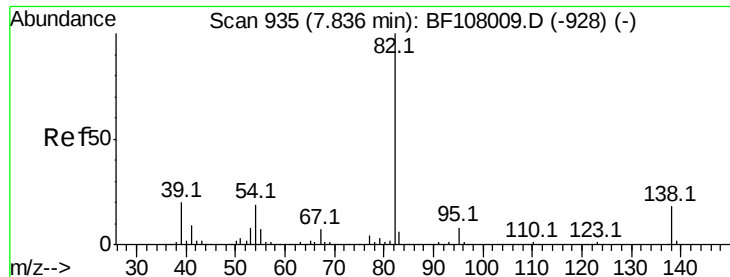

#25

Isophorone

Concen: 24.409 ng

RT: 7.56 min Scan# 888

Delta R.T. -0.26 min

Lab File: BF108521.D

Acq: 27 Aug 2018 20:03

Instrument :

BNA_F

ClientSampled :


Tot Ion: 82 Resp: 381691

Ion Ratio Lower Upper




82 100

95 0.0 5.2 7.8#

138 0.0 14.9 22.3#

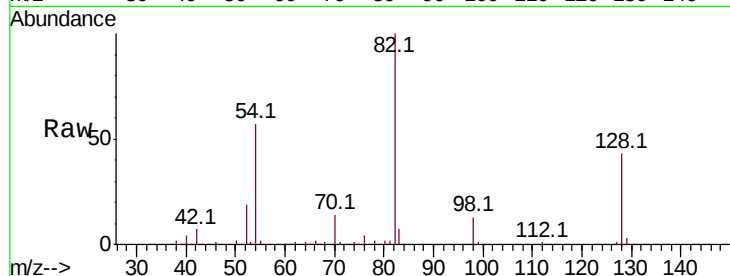

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): E

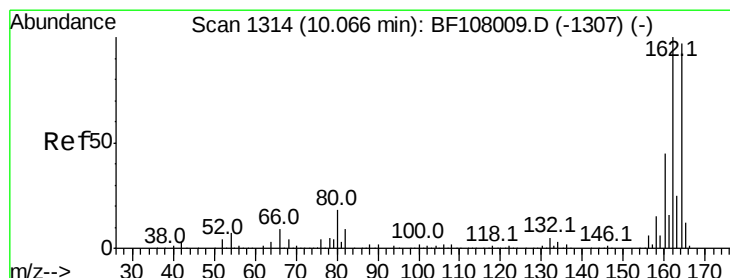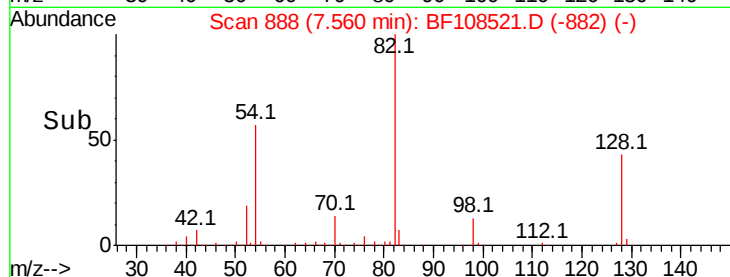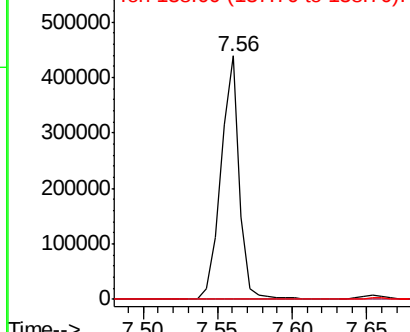

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.04 min Scan# 1310

Delta R.T. -0.01 min

Lab File: BF108521.D

Acq: 27 Aug 2018 20:03


Tgt Ion: 164 Resp: 218332

Ion Ratio Lower Upper



164 100


162 101.4 86.1 129.1

160 45.5 38.3 57.5

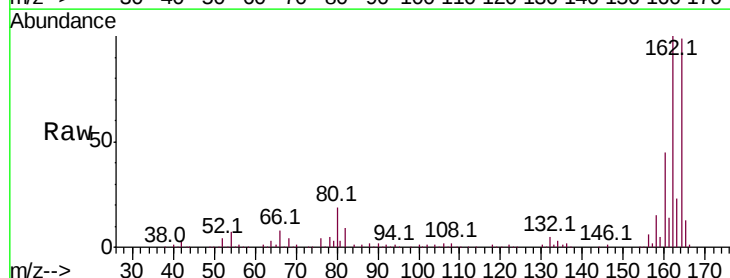

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

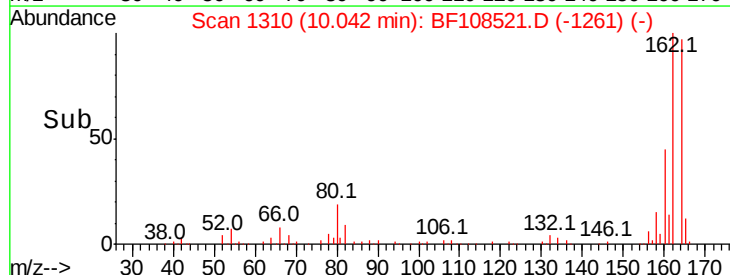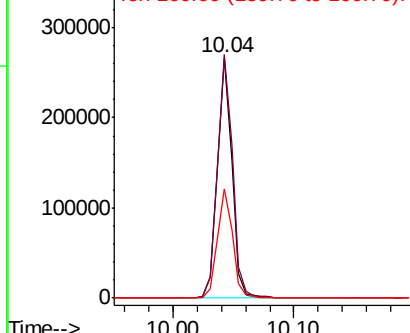


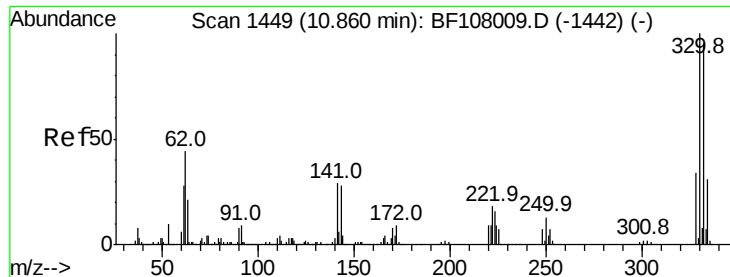




#41
 2,4,6-Tribromophenol
 Concen: 66.500 ng
 RT: 10.84 min Scan# 1445
 Delta R.T. -0.01 min
 Lab File: BF108521.D
 Acq: 27 Aug 2018 20:03

Instrument :
 BNA_F
 ClientSampled :

Tot Ion:330 Resp: 144824
 Ion Ratio Lower Upper
 330 100
 332 96.8 77.0 115.6
 141 32.8 29.9 44.9

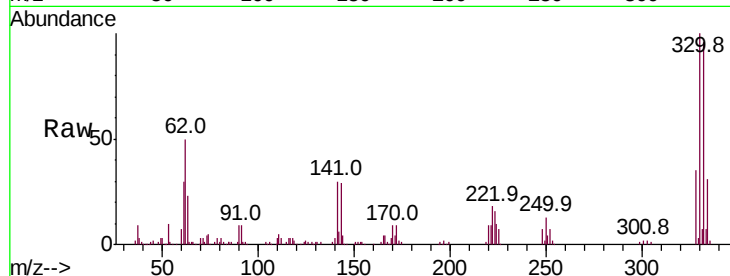


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

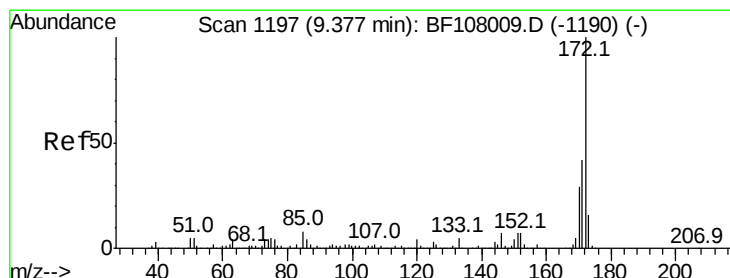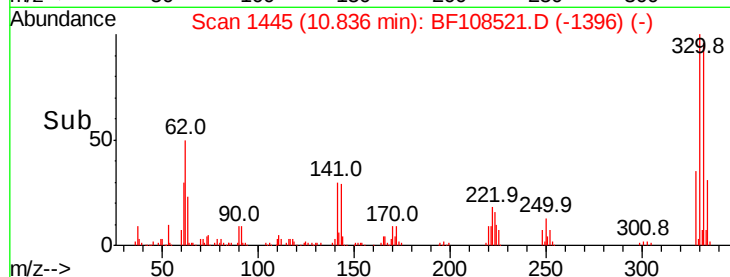
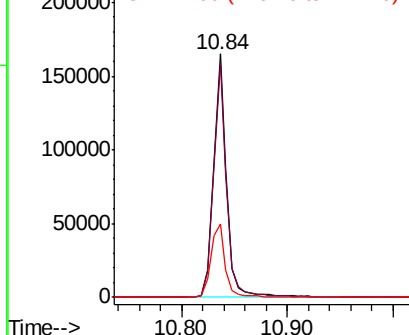



#44
 2-Fluorobiphenyl
 Concen: 48.270 ng
 RT: 9.35 min Scan# 1193
 Delta R.T. -0.01 min
 Lab File: BF108521.D
 Acq: 27 Aug 2018 20:03

Tgt Ion:172 Resp: 656438
 Ion Ratio Lower Upper
 172 100
 171 35.1 29.7 44.5
 170 23.5 19.6 29.4

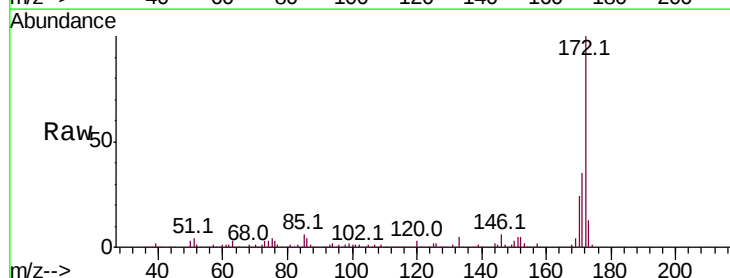

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



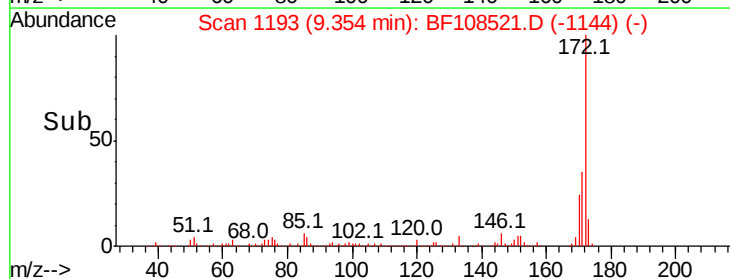
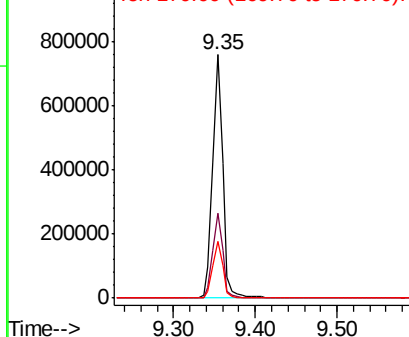


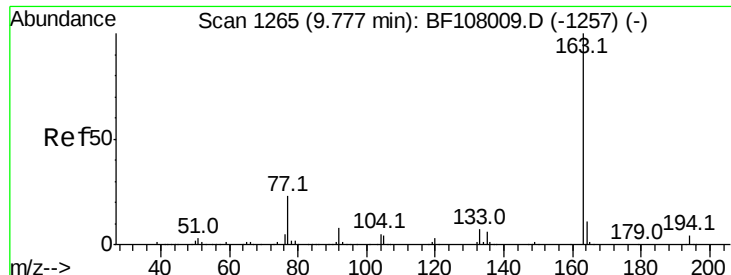

#49
Dimethylphthalate
Concen: 13.967 ng
RT: 9.75 min Scan# 1260
Delta R.T. -0.02 min
Lab File: BF108521.D
Acq: 27 Aug 2018 20:03




Instrument :
BNA_F
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
163	100		
194	4.1	2.7	4.1#
164	9.4	8.2	12.2

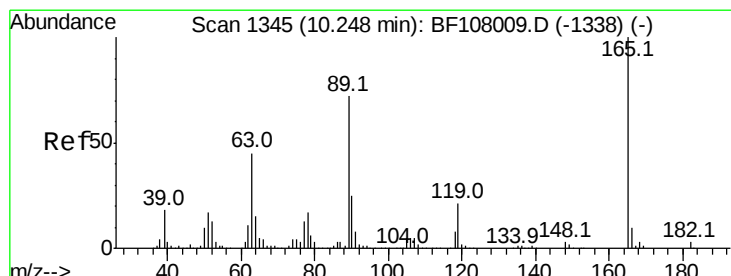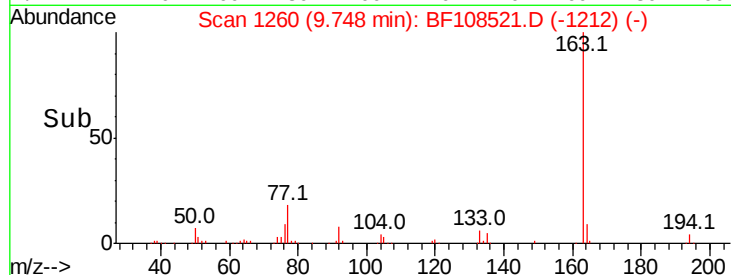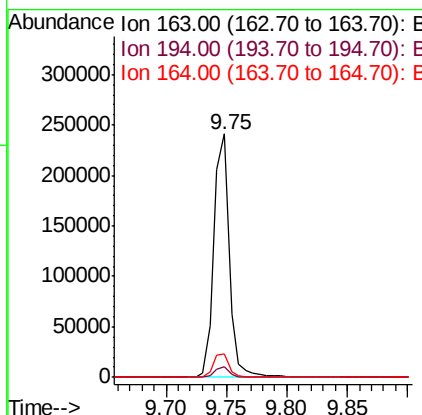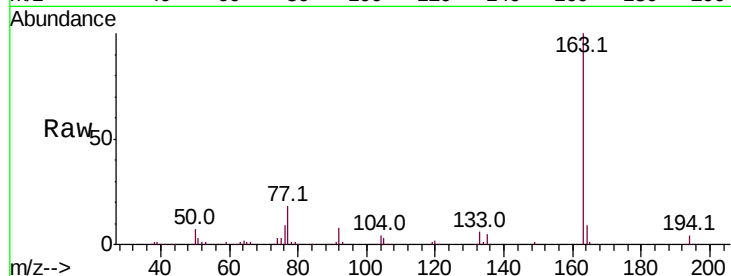

#56
2,4-Dinitrotoluene
Concen: 6.712 ng
RT: 10.04 min Scan# 1310
Delta R.T. -0.19 min
Lab File: BF108521.D
Acq: 27 Aug 2018 20:03

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.3	36.4	54.6#
89	1.2	57.8	86.6#
182	0.0	1.6	2.4#

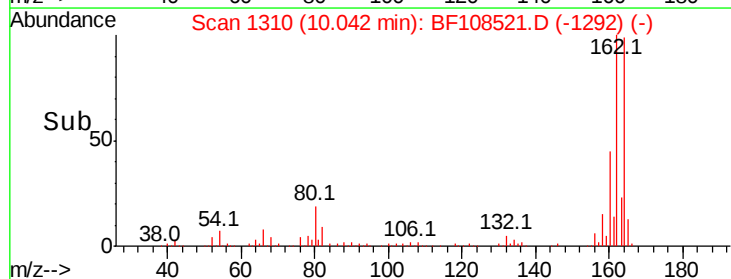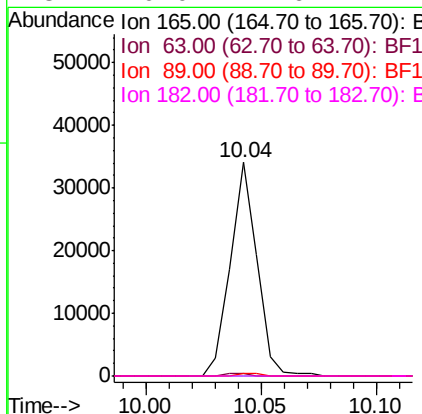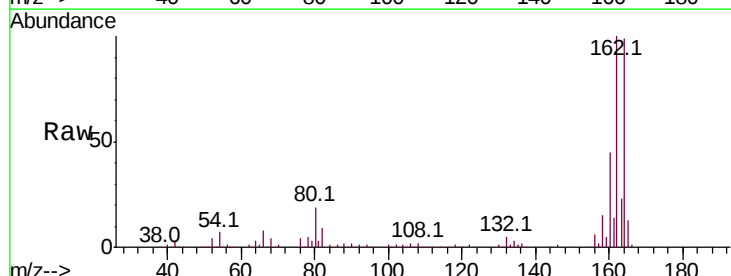


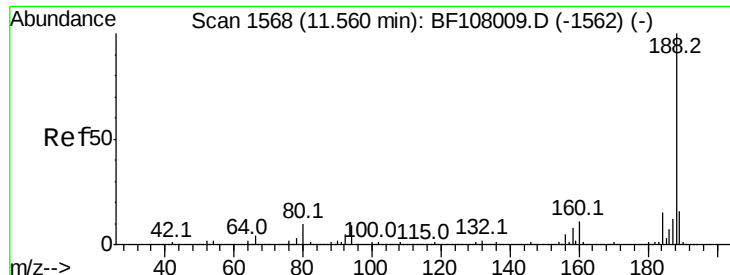




#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.54 min Scan# 1564
 Delta R.T. -0.01 min
 Lab File: BF108521.D
 Acq: 27 Aug 2018 20:03

Instrument :
 BNA_F
 ClientSampled :

Tot Ion:188 Resp: 352158
 Ion Ratio Lower Upper
 188 100
 94 9.1 8.5 12.7
 80 10.5 9.2 13.8

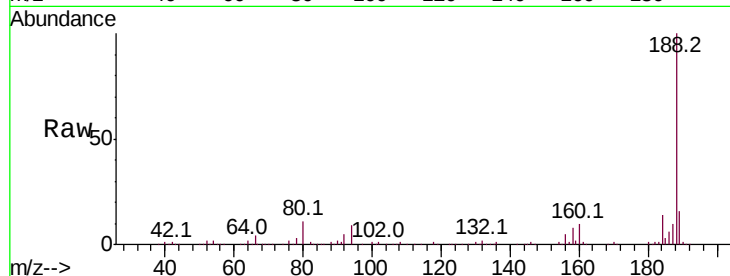


Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF1
 Ion 80.00 (79.70 to 80.70): BF1

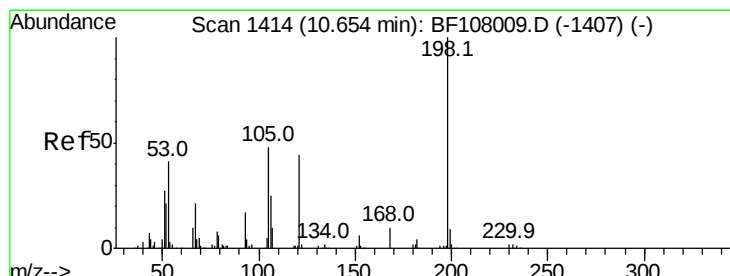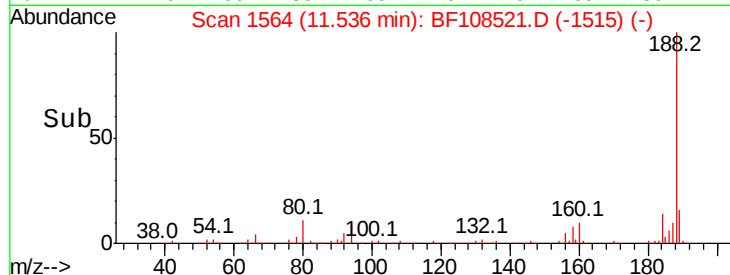
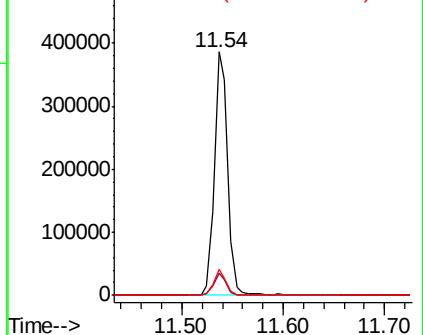



#64
 4,6-Dinitro-2-methylphenol
 Concen: 5.541 ng
 RT: 10.84 min Scan# 1445
 Delta R.T. 0.19 min
 Lab File: BF108521.D
 Acq: 27 Aug 2018 20:03

Tgt Ion:198 Resp: 271
 Ion Ratio Lower Upper
 198 100
 51 157.1 37.7 77.7#
 105 141.8 36.3 76.3#

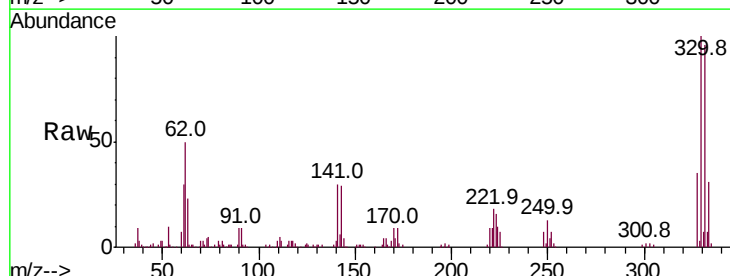

Abundance Ion 198.00 (197.70 to 198.70): E
 Ion 51.00 (50.70 to 51.70): BF1
 Ion 105.00 (104.70 to 105.70): E

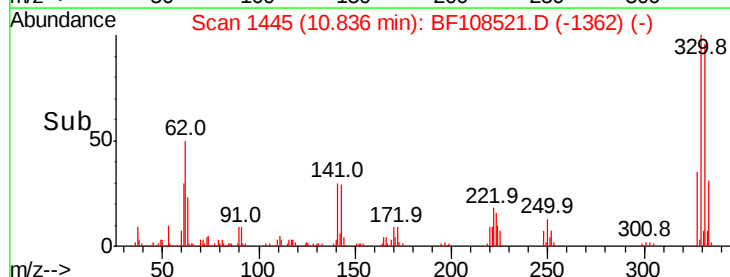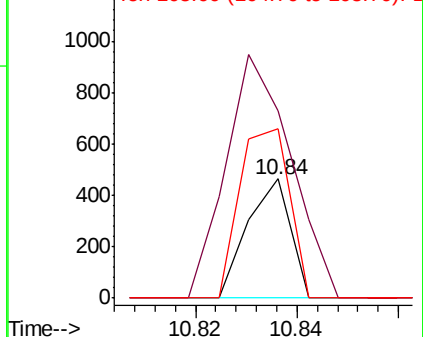


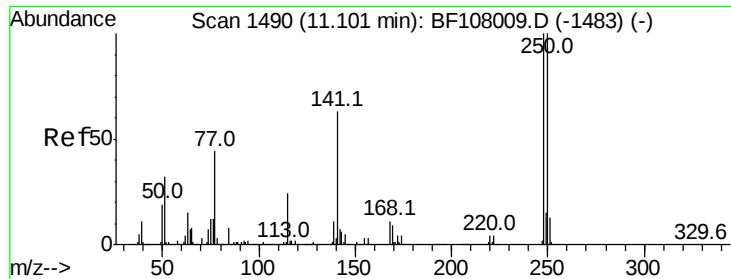




#66
 4-Bromophenyl-phenylether
 Concen: 2.468 ng
 RT: 10.84 min Scan# 1445
 Delta R.T. -0.25 min
 Lab File: BF108521.D
 Acq: 27 Aug 2018 20:03

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:248 Resp: 9445
 Ion Ratio Lower Upper
 248 100
 250 195.9 76.9 115.3#
 141 445.3 74.4 111.6#

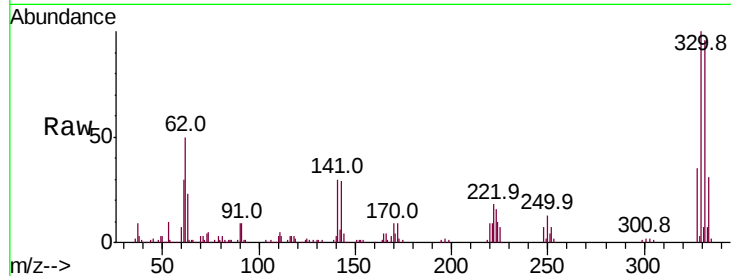


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

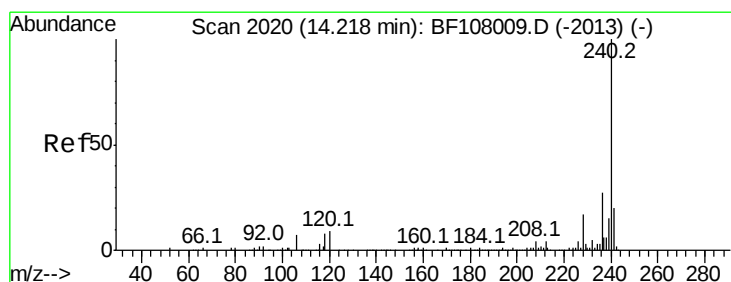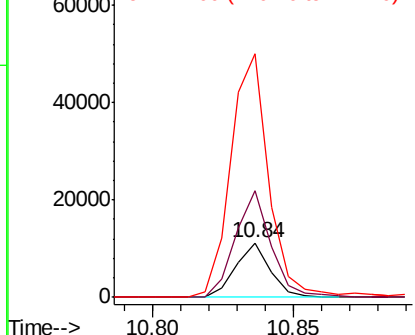
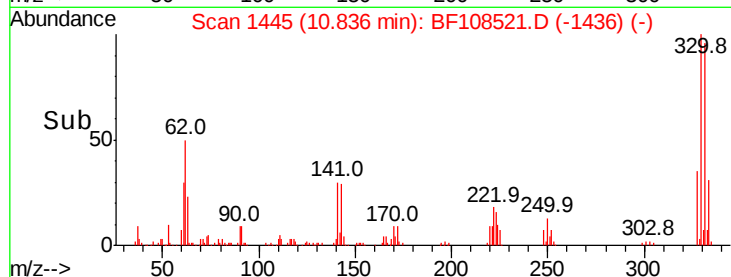



#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 14.19 min Scan# 2015
 Delta R.T. -0.01 min
 Lab File: BF108521.D
 Acq: 27 Aug 2018 20:03

Tgt Ion:240 Resp: 290927
 Ion Ratio Lower Upper
 240 100
 120 10.5 9.5 14.3
 236 26.3 20.7 31.1

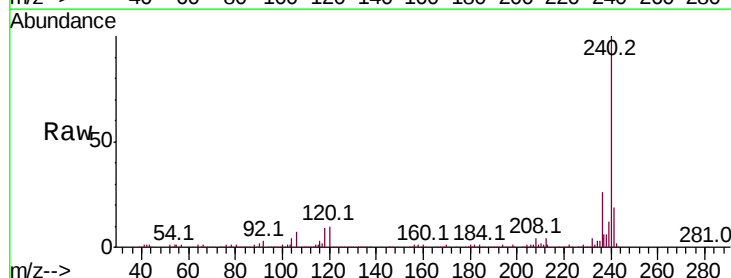

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

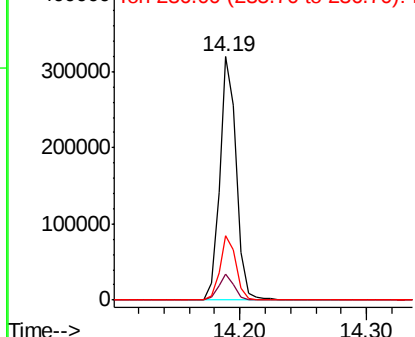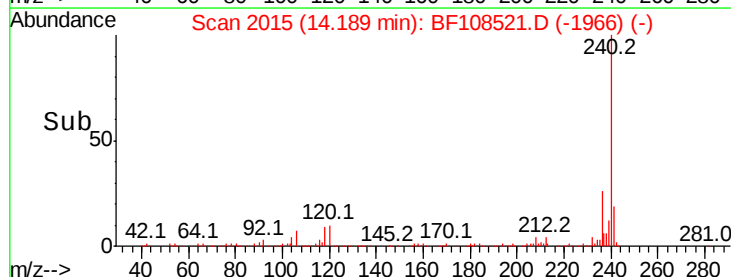

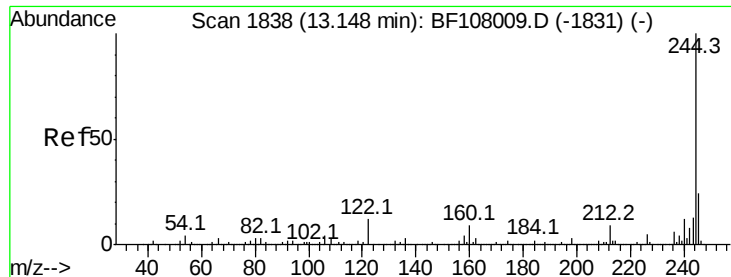

#78

Terphenyl-d14

Concen: 35.239 ng

RT: 13.12 min Scan# 1833

Delta R.T. -0.01 min

Lab File: BF108521.D

Acq: 27 Aug 2018 20:03

Instrument :

BNA_F

ClientSampleId :


Tot Ion:244 Resp: 403213

Ion Ratio Lower Upper

244 100

212 6.7 5.4 8.0




122 10.3 11.0 16.4#

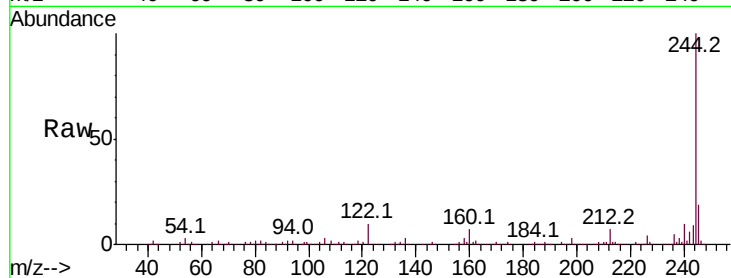

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

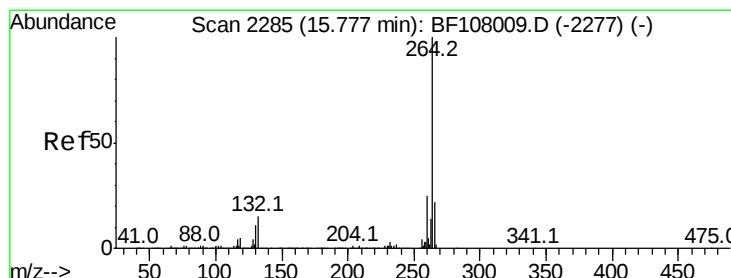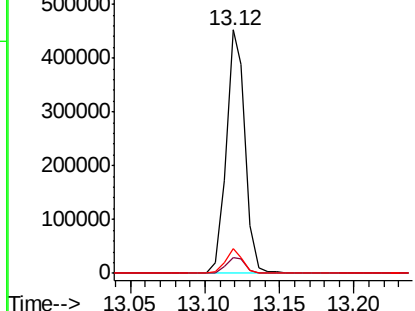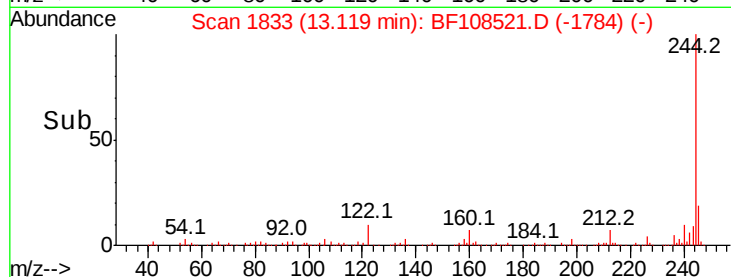

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.75 min Scan# 2280

Delta R.T. -0.01 min

Lab File: BF108521.D

Acq: 27 Aug 2018 20:03


Tgt Ion:264 Resp: 263073

Ion Ratio Lower Upper

264 100

260 23.8 19.2 28.8

265 21.4 17.5 26.3

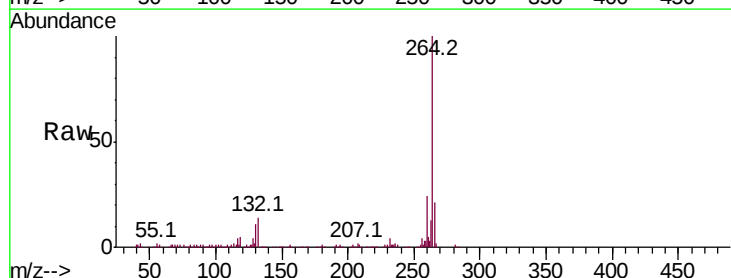

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

