

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082718\
 Data File : BF108550.D
 Acq On : 28 Aug 2018 9:59
 Operator : JU/SJ
 Sample : J4660-05
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Aug 28 10:45:58 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 22 11:01:45 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.00	152	102411	20.00	ng	-0.01
21) Naphthalene-d8	8.28	136	344837	20.00	ng	0.00
38) Acenaphthene-d10	10.04	164	138469	20.00	ng	-0.01
63) Phenanthrene-d10	11.54	188	239636	20.00	ng	-0.01
75) Chrysene-d12	14.19	240	259702	20.00	ng	-0.01
86) Perylene-d12	15.75	264	177842	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	265570	46.95	ng	0.00
7) Phenol-d6	6.61	99	221240	29.43	ng	-0.02
23) Nitrobenzene-d5	7.56	82	669956	108.41	ng	-0.01
41) 2,4,6-Tribromophenol	10.84	330	135699	98.25	ng	-0.01
44) 2-Fluorobiphenyl	9.35	172	1188102	137.75	ng	-0.01
78) Terphenyl-d14	13.12	244	1056722	103.46	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.56	70	89800	17.666	ng	# 84
25) Isophorone	7.56	82	669946	56.877	ng	# 64
49) Dimethylphthalate	9.75	163	29662	3.075	ng	# 99
50) 2,6-Dinitrotoluene	10.04	165	17716	8.779	ng	# 26
56) 2,4-Dinitrotoluene	10.04	165	17716	6.820	ng	# 24
64) 4,6-Dinitro-2-methylphenol	10.84	198	267	5.622	ng	# 1
66) 4-Bromophenyl-phenylether	10.84	248	8952	3.438	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082718\
Data File : BF108550.D
Acq On : 28 Aug 2018 9:59
Operator : JU/SJ
Sample : J4660-05
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Aug 28 10:45:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 22 11:01:45 2018
Response via : Initial Calibration

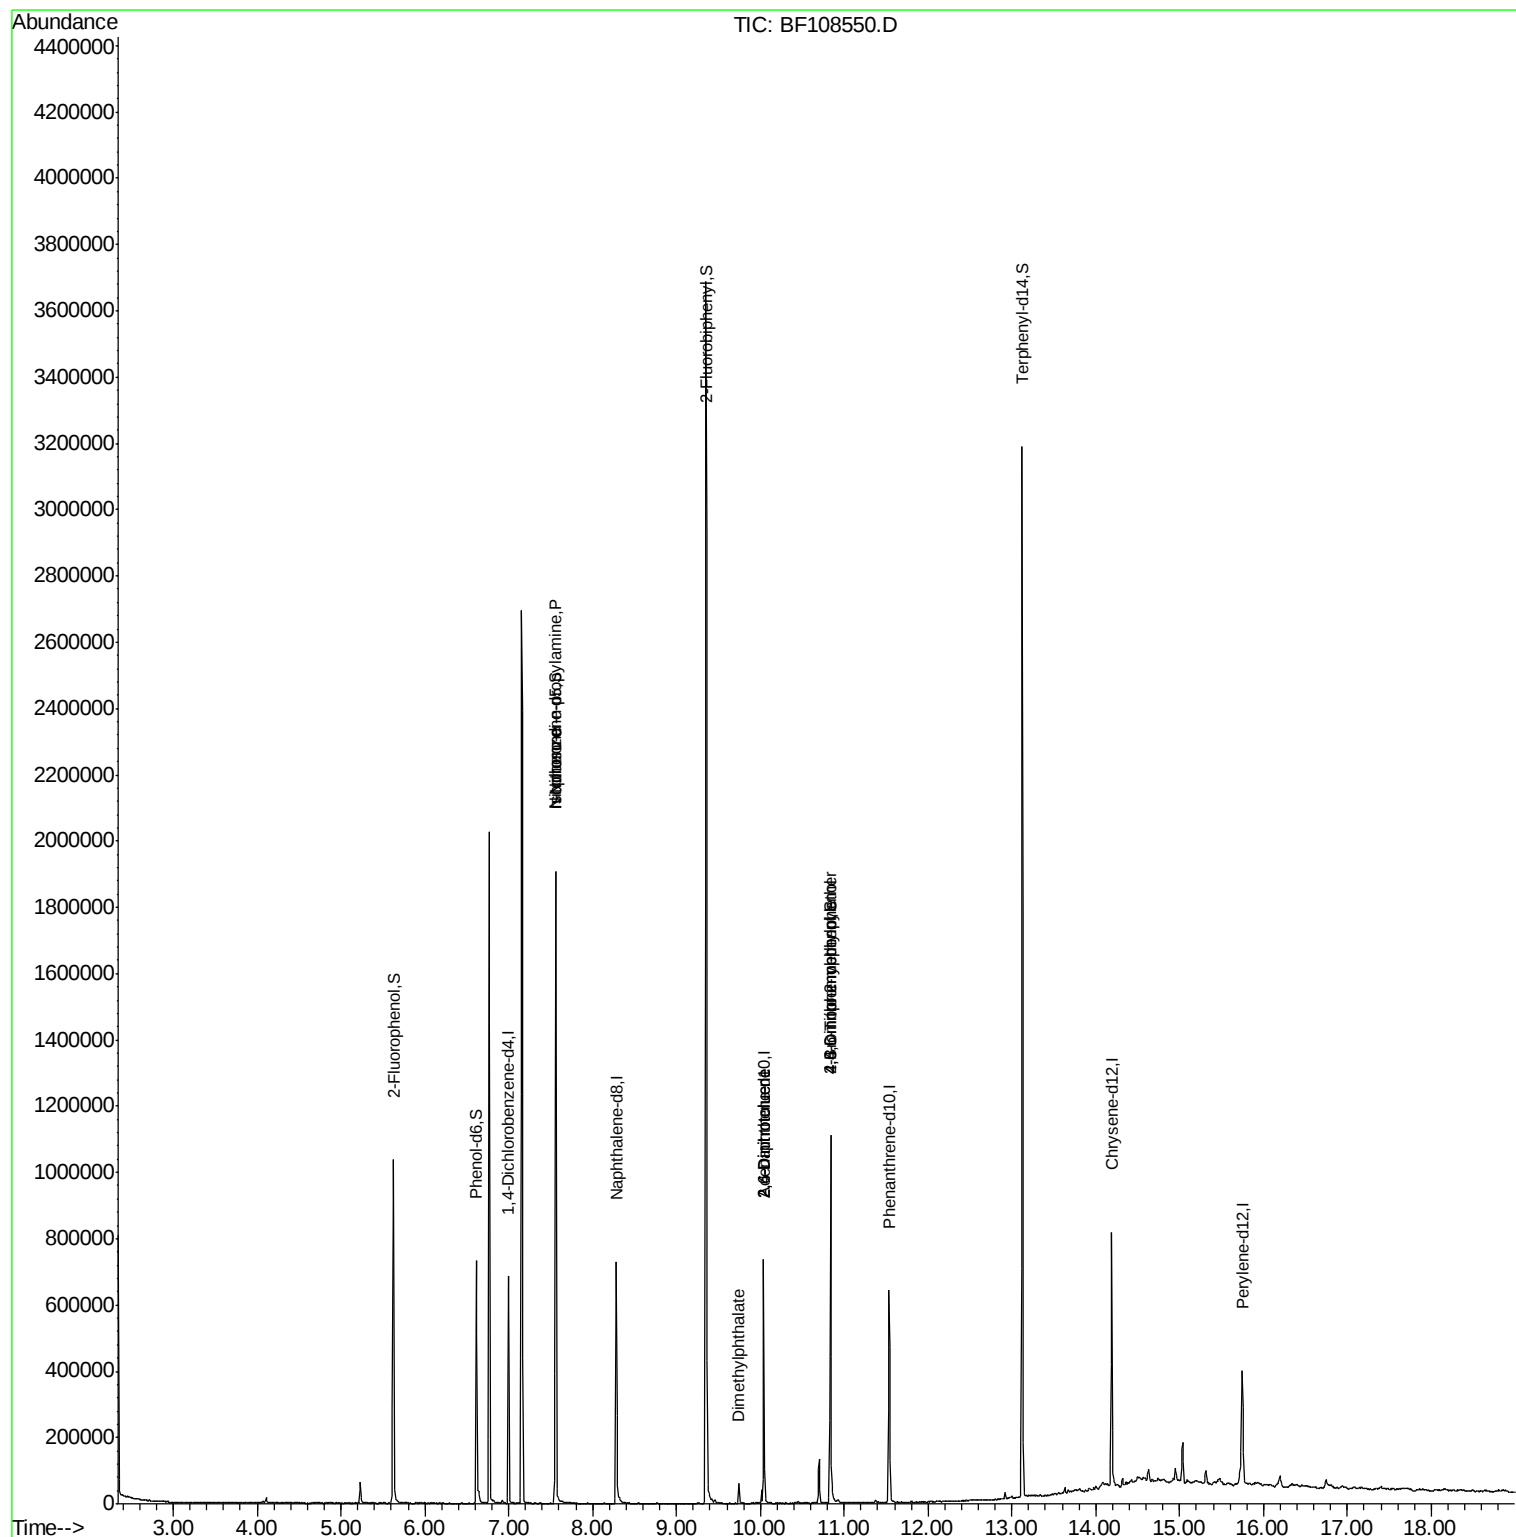




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.00 min Scan# 792
Delta R.T. -0.01 min
Lab File: BF108550.D
Acq: 28 Aug 2018 9:59

Instrument :
BNA_F
ClientSampled :

Tot Ion	Ratio	Lower	Upper
152	100		
150	155.6	124.6	186.8
115	61.4	50.1	75.1

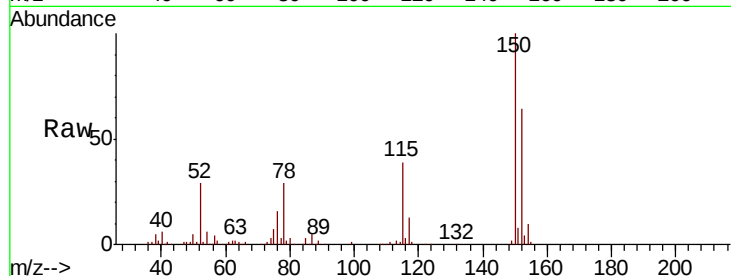


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

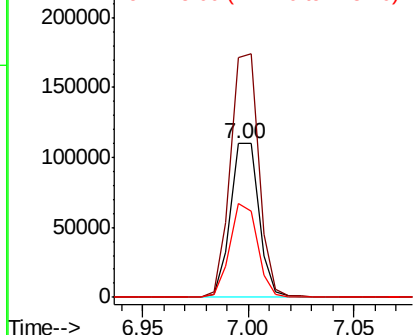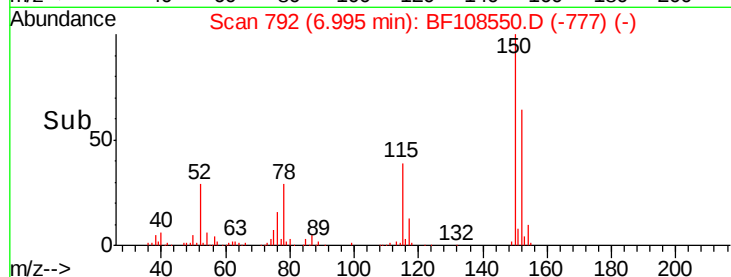



#5

2-Fluorophenol
Concen: 46.948 ng
RT: 5.63 min Scan# 559
Delta R.T. -0.01 min
Lab File: BF108550.D
Acq: 28 Aug 2018 9:59

Tgt Ion	Ratio	Lower	Upper
112	100		
64	66.5	47.9	71.9
63	34.2	23.7	35.5

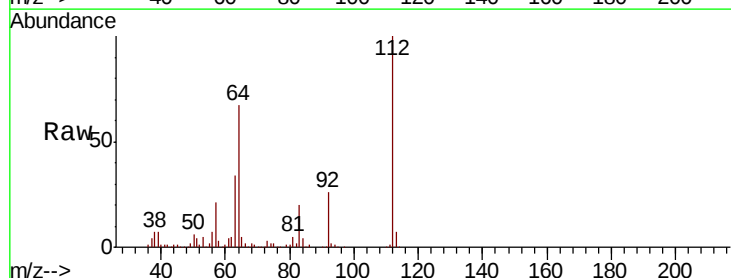

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

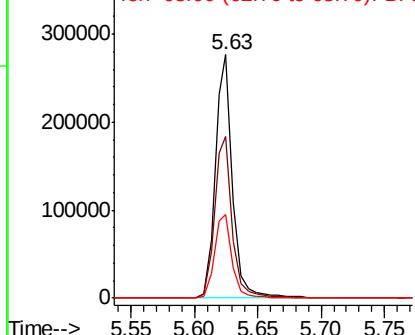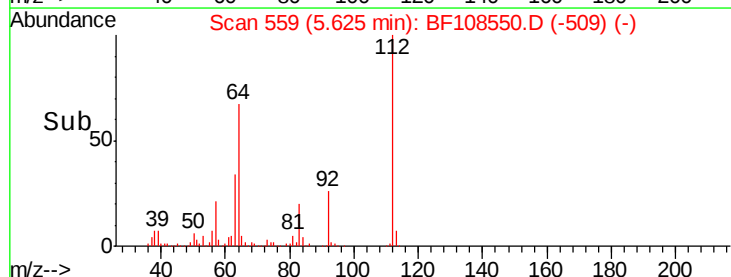



#7

Phenol-d6

Concen: 29.432 ng

RT: 6.61 min Scan# 727

Delta R.T. -0.02 min

Lab File: BF108550.D

Acq: 28 Aug 2018 9:59

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 221240

Ion Ratio Lower Upper




99 100

42 22.4 14.5 21.7#

71 35.6 25.4 38.0



Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

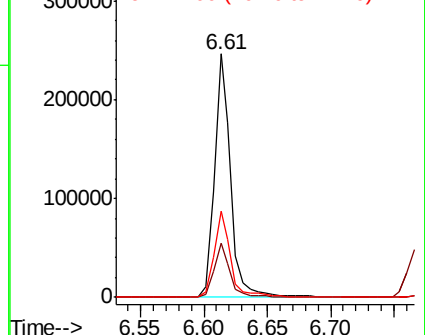

#19

n-Nitroso-di-n-propylamine

Concen: 17.666 ng

RT: 7.56 min Scan# 888

Delta R.T. 0.15 min

Lab File: BF108550.D

Acq: 28 Aug 2018 9:59

Tgt Ion: 70 Resp: 89800


Ion Ratio Lower Upper

70 100



42 54.7 47.5 71.3


101 0.0 7.4 11.2#

130 2.2 16.6 25.0#



Abundance Ion 70.00 (69.70 to 70.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 101.00 (100.70 to 101.70): BF1
Ion 130.00 (129.70 to 130.70): BF1

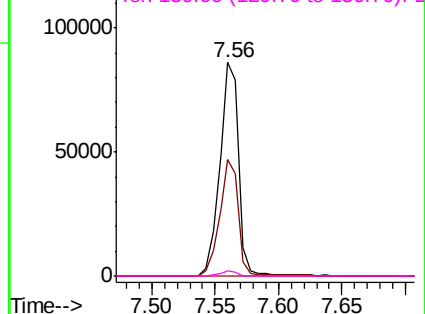

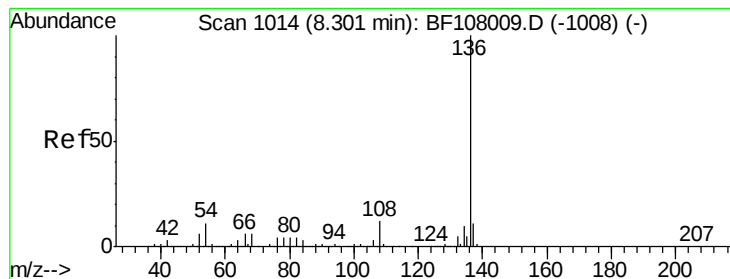

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.28 min Scan# 1011

Delta R.T. -0.01 min

Lab File: BF108550.D

Acq: 28 Aug 2018 9:59

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136 Resp: 344837



Ion Ratio Lower Upper

136 100

137 11.0 8.9 13.3

54 9.2 6.6 9.8

68 5.8 5.0 7.4





Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

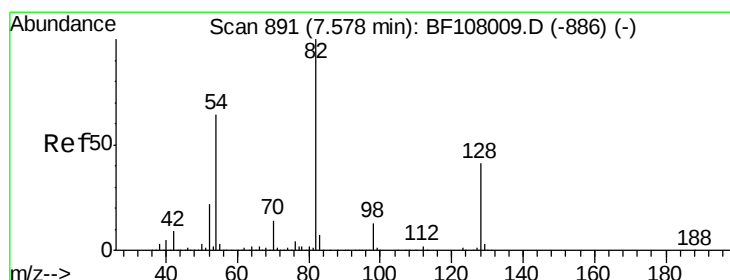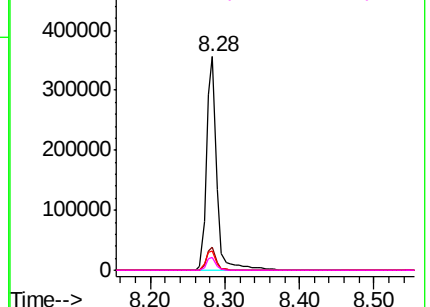

#23

Nitrobenzene-d5

Concen: 108.412 ng

RT: 7.56 min Scan# 888

Delta R.T. -0.01 min

Lab File: BF108550.D

Acq: 28 Aug 2018 9:59



Tgt Ion: 82 Resp: 669956

Ion Ratio Lower Upper

82 100

128 39.9 36.1 54.1


54 58.9 41.4 62.2



Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

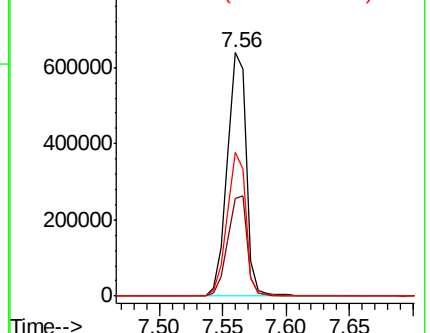



#25

Isophorone

Concen: 56.877 ng

RT: 7.56 min Scan# 888

Delta R.T. -0.26 min

Lab File: BF108550.D

Acq: 28 Aug 2018 9:59

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 669946

Ion Ratio Lower Upper




82 100

95 0.0 5.2 7.8#

138 0.0 14.9 22.3#



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): BF1

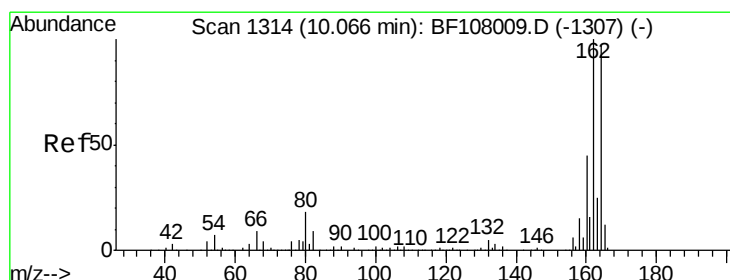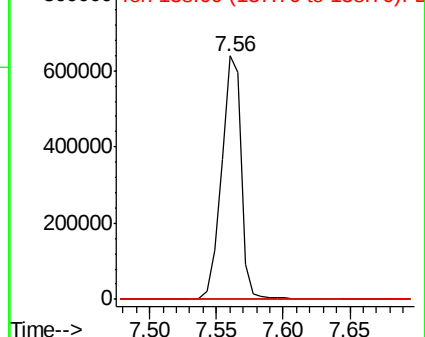

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.04 min Scan# 1310

Delta R.T. -0.01 min

Lab File: BF108550.D

Acq: 28 Aug 2018 9:59


Tgt Ion: 164 Resp: 138469

Ion Ratio Lower Upper



164 100

162 103.3 86.1 129.1

160 46.4 38.3 57.5



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

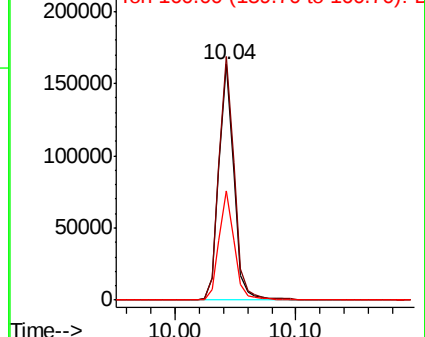




#41
 2,4,6-Tribromophenol
 Concen: 98.248 ng
 RT: 10.84 min Scan# 1445
 Delta R.T. -0.01 min
 Lab File: BF108550.D
 Acq: 28 Aug 2018 9:59

Instrument :
 BNA_F
 ClientSampled :

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.5	77.0	115.6
141	32.6	29.9	44.9


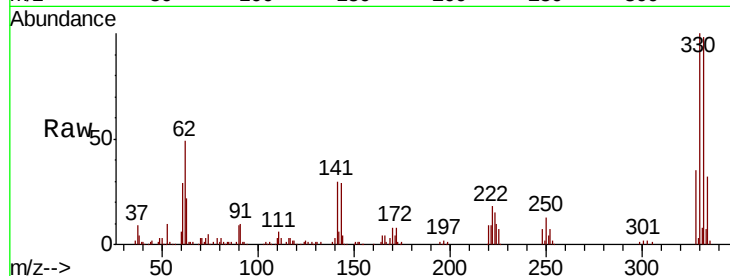


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

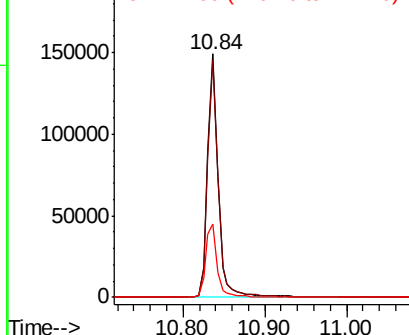

#44
 2-Fluorobiphenyl
 Concen: 137.754 ng
 RT: 9.35 min Scan# 1193
 Delta R.T. -0.01 min
 Lab File: BF108550.D
 Acq: 28 Aug 2018 9:59

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.6	29.7	44.5
170	24.0	19.6	29.4






Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

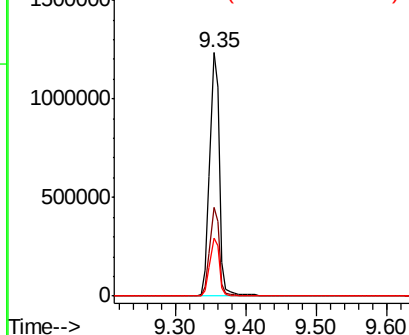


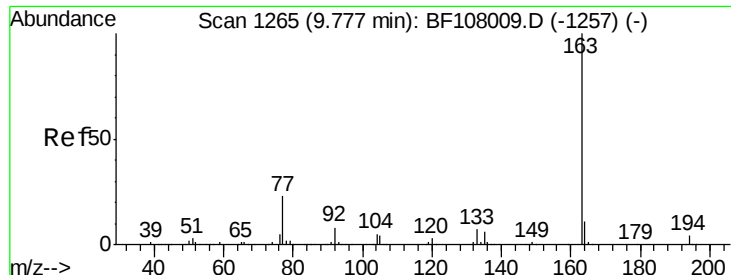



#49
Dimethylphthalate
Concen: 3.075 ng
RT: 9.75 min Scan# 1260
Delta R.T. -0.02 min
Lab File: BF108550.D
Acq: 28 Aug 2018 9:59

Instrument :
BNA_F
ClientSampleId :

Tot Ion:163 Resp: 29662
Ion Ratio Lower Upper
163 100
194 4.2 2.7 4.1#
164 10.5 8.2 12.2

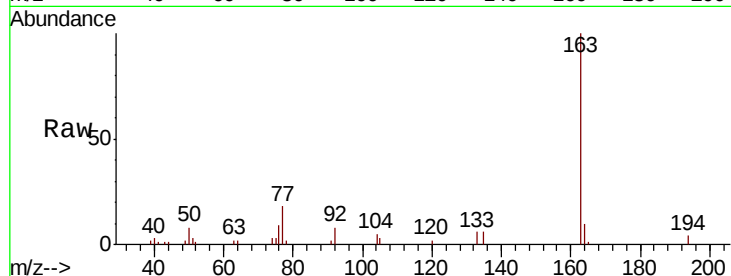


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E


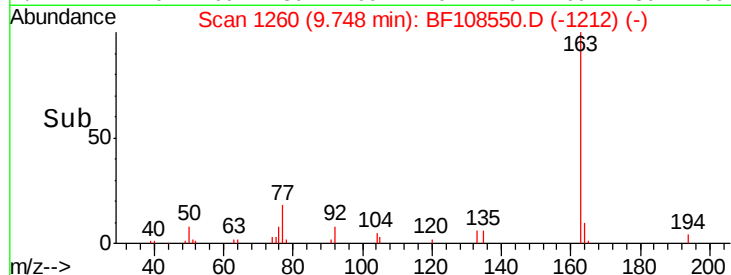
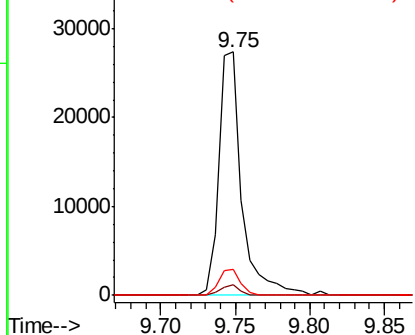



#50
2,6-Dinitrotoluene
Concen: 8.779 ng
RT: 10.04 min Scan# 1310
Delta R.T. 0.21 min
Lab File: BF108550.D
Acq: 28 Aug 2018 9:59

Tgt Ion:165 Resp: 17716
Ion Ratio Lower Upper
165 100
63 1.8 44.7 67.1#
89 1.7 44.0 66.0#

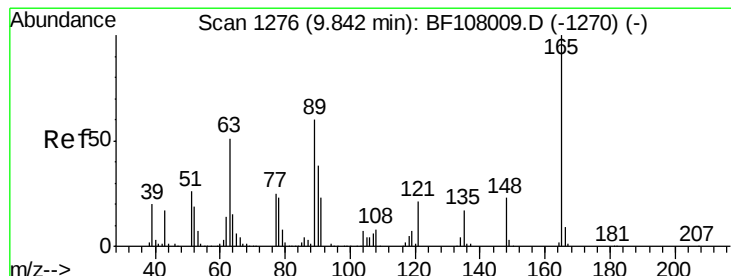

Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF1
Ion 89.00 (88.70 to 89.70): BF1

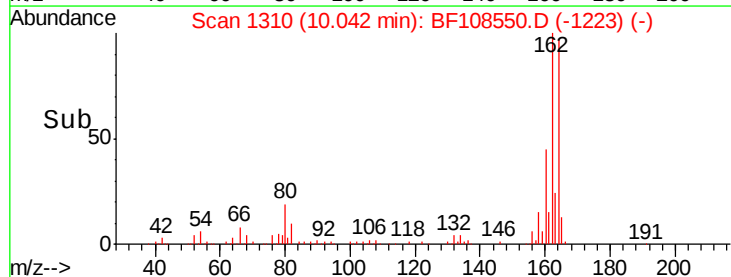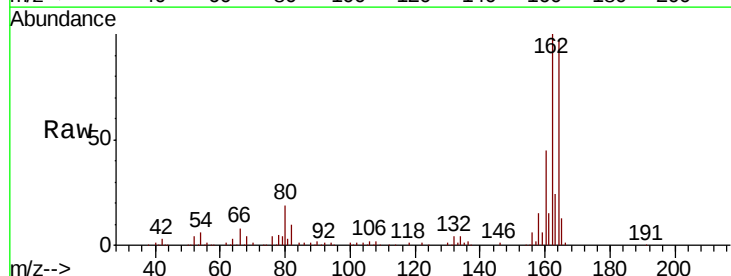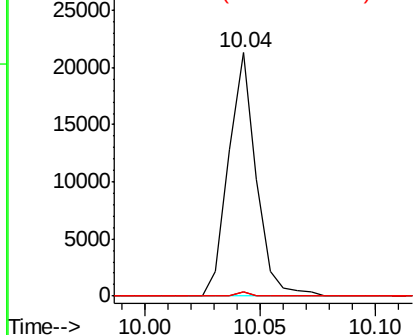


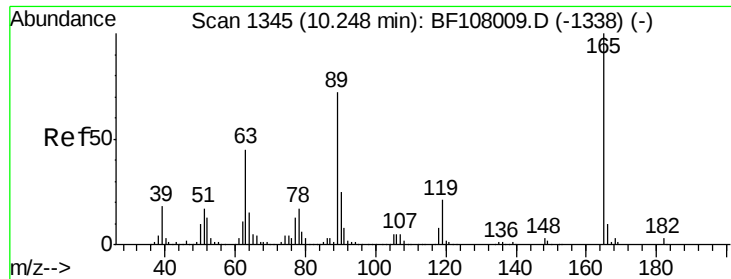

#56
 2,4-Dinitrotoluene
 Concen: 6.820 ng
 RT: 10.04 min Scan# 1310
 Delta R.T. -0.19 min
 Lab File: BF108550.D
 Acq: 28 Aug 2018 9:59

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
63	1.8	36.4	54.6#
89	1.7	57.8	86.6#
182	0.0	1.6	2.4#



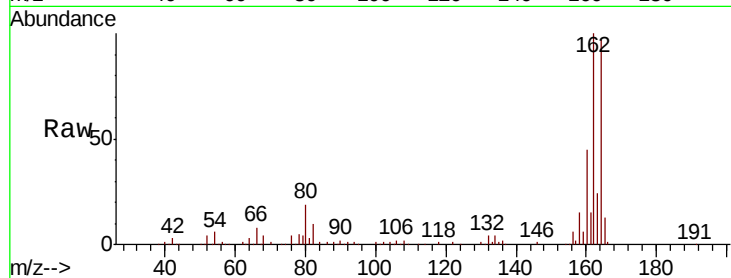


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1


Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E

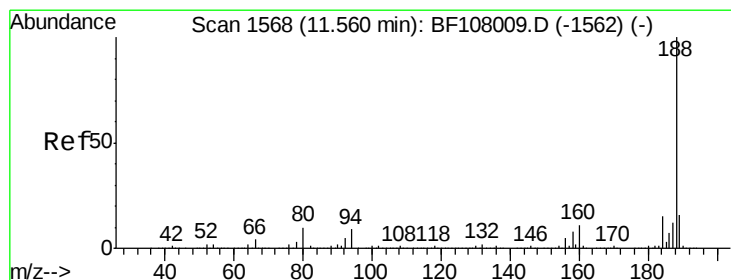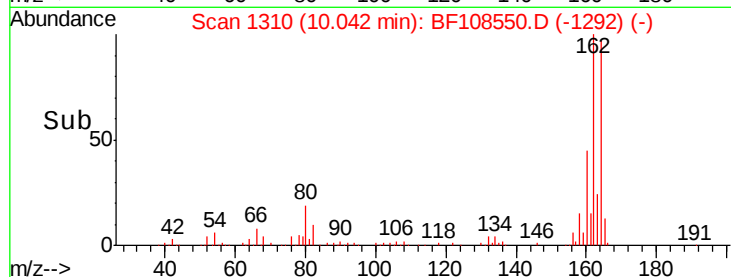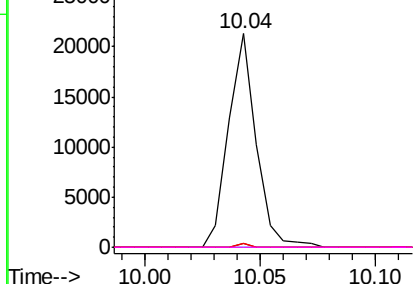

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.54 min Scan# 1564
 Delta R.T. -0.01 min
 Lab File: BF108550.D
 Acq: 28 Aug 2018 9:59



Tgt Ion	Ratio	Lower	Upper
188	100		
94	9.1	8.5	12.7
80	9.7	9.2	13.8

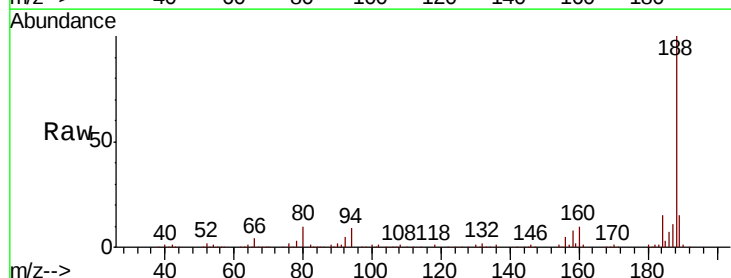

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

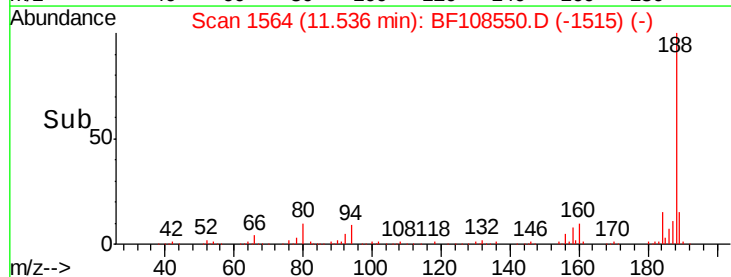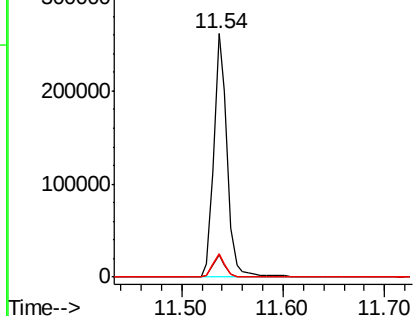



#64

4,6-Dinitro-2-methylphenol

Concen: 5.622 ng

RT: 10.84 min Scan# 1445

Delta R.T. 0.19 min

Lab File: BF108550.D

Acq: 28 Aug 2018 9:59

Instrument :

BNA_F

ClientSampled :


Tot Ion:198 Resp: 267

Ion Ratio Lower Upper

198 100

51 178.2 37.7 77.7#




105 175.2 36.3 76.3#

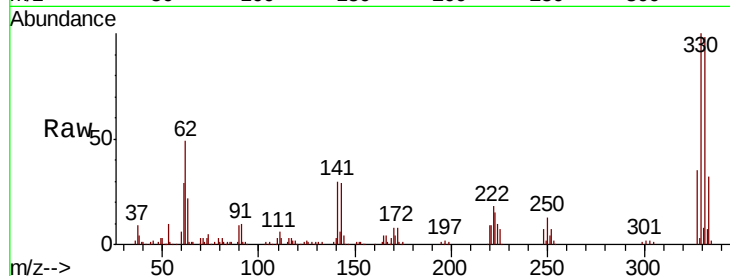

Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BF1

Ion 105.00 (104.70 to 105.70): E

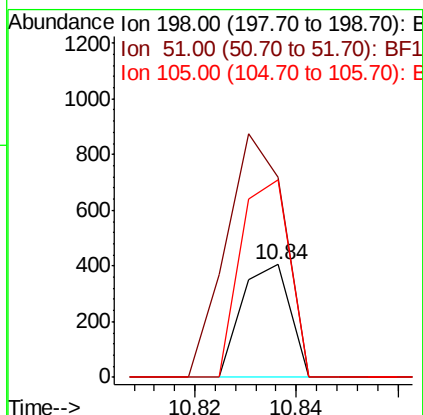

#66

4-Bromophenyl-phenylether

Concen: 3.438 ng

RT: 10.84 min Scan# 1445

Delta R.T. -0.25 min

Lab File: BF108550.D

Acq: 28 Aug 2018 9:59


Tgt Ion:248 Resp: 8952

Ion Ratio Lower Upper

248 100

250 191.1 76.9 115.3#



141 434.9 74.4 111.6#




Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

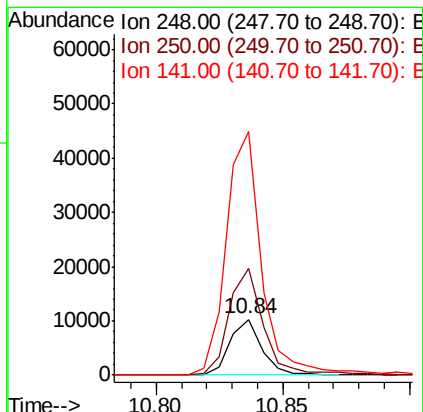

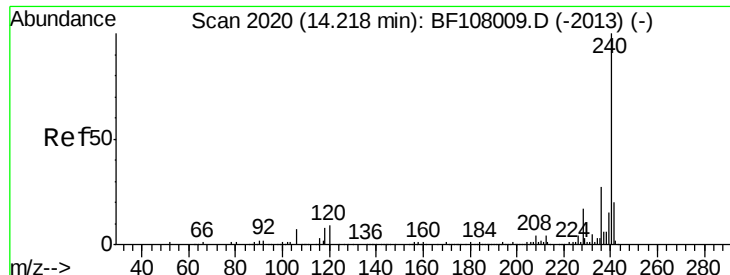

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.19 min Scan# 2015

Delta R.T. -0.01 min

Lab File: BF108550.D

Acq: 28 Aug 2018 9:59

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 259702

Ion Ratio Lower Upper

240 100

120 10.2 9.5 14.3




236 26.3 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

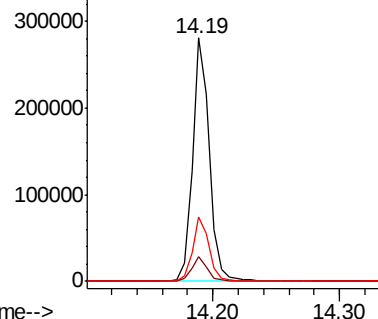

#78

Terphenyl-d14

Concen: 103.457 ng

RT: 13.12 min Scan# 1834

Delta R.T. -0.01 min

Lab File: BF108550.D

Acq: 28 Aug 2018 9:59


Tgt Ion:244 Resp: 1056722

Ion Ratio Lower Upper

244 100

212 7.4 5.4 8.0



122 9.6 11.0 16.4#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

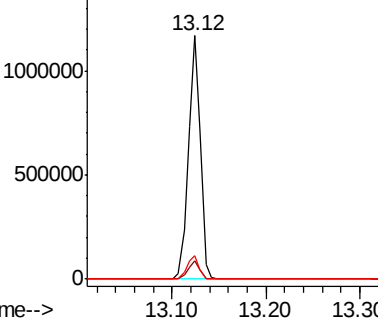

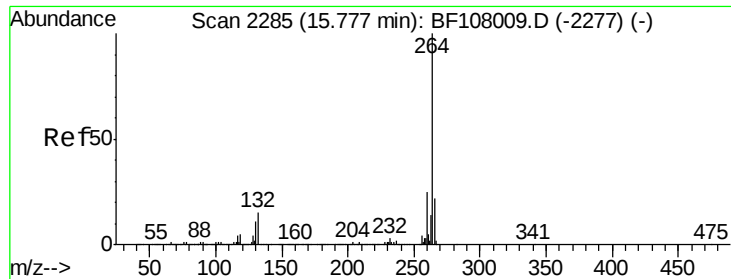

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.75 min Scan# 2280
Delta R.T. -0.01 min
Lab File: BF108550.D
Acq: 28 Aug 2018 9:59

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.8	19.2	28.8
265	21.4	17.5	26.3

