
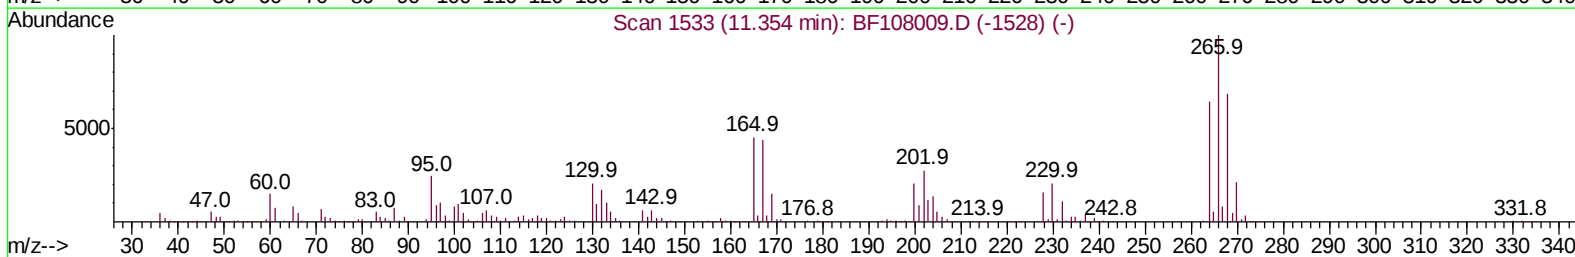
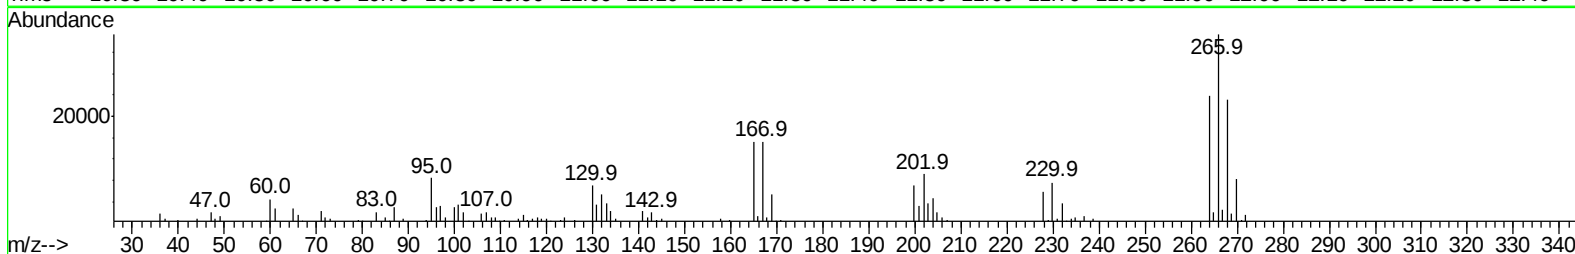


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082718\
Data File : BF108524.D
Acq On : 27 Aug 2018 21:52
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 05:47:15 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 22 11:01:45 2018
Response via : Initial Calibration

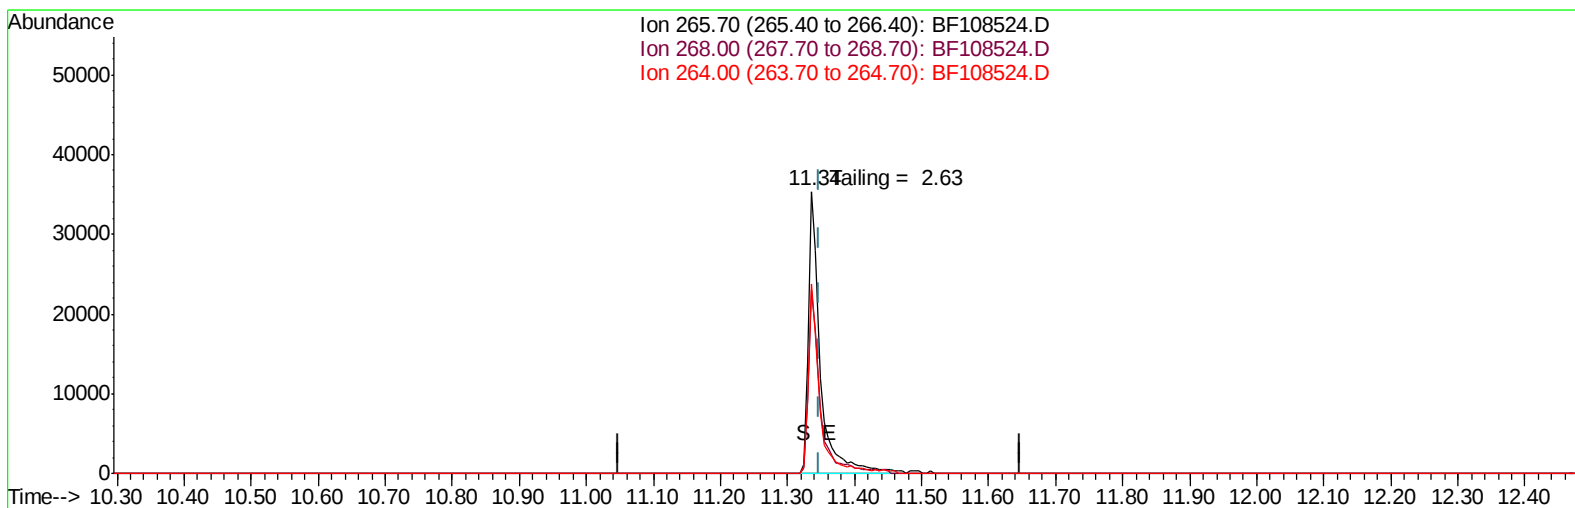

TIC: BF108524.D

(69) Pentachlorophenol (C)




11.336min (-0.012) 27381.16ng

response 43008

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.14
264.00	61.90	67.18
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082718\
 Data File : BF108524.D
 Acq On : 27 Aug 2018 21:52
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 05:47:15 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 22 11:01:45 2018
 Response via : Initial Calibration

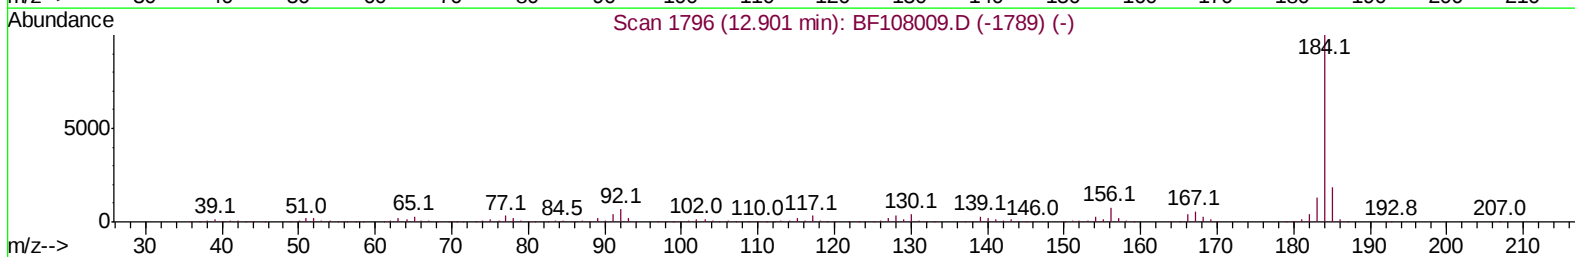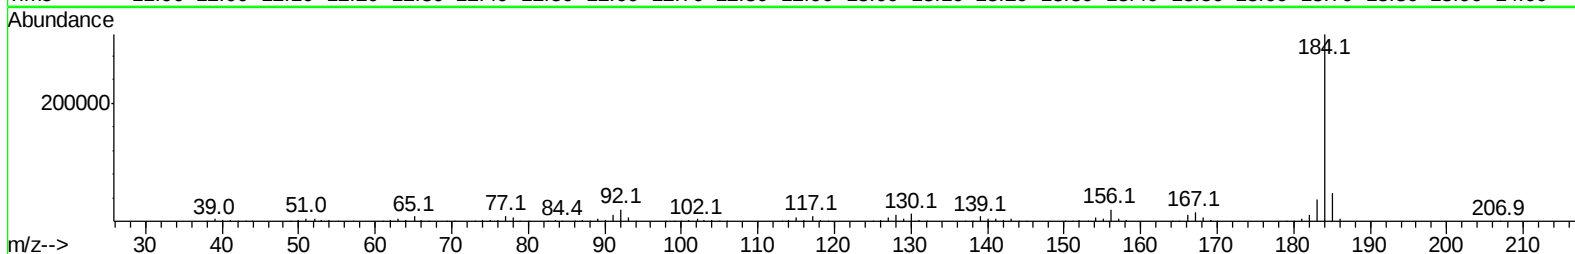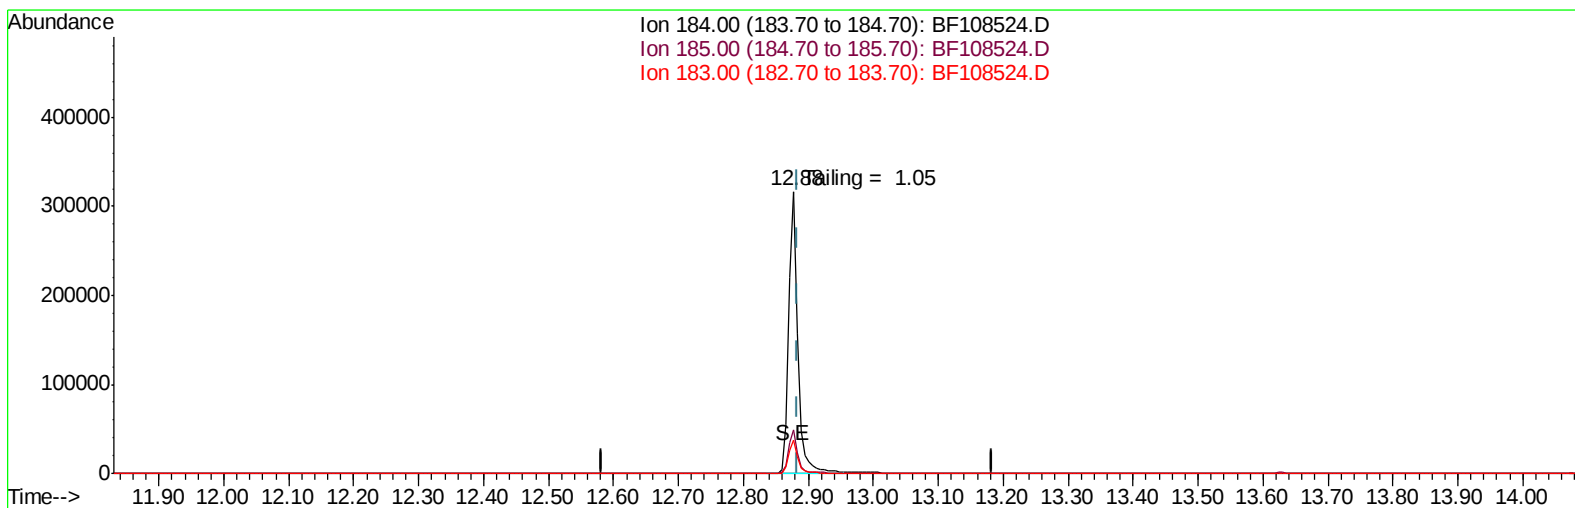

TIC: BF108524.D

(76) Benzidine

12.877min (-0.006) 69503.16ng

response 311617

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.34
183.00	11.60	11.75
0.00	0.00	0.00