

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082718\
 Data File : BF108514.D
 Acq On : 27 Aug 2018 16:54
 Operator : JU/SJ
 Sample : J4538-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 VSS1

Quant Time: Aug 27 18:07:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 22 11:01:45 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.00	152	125961	20.00	ng	0.00
21) Naphthalene-d8	8.28	136	472398	20.00	ng	0.00
38) Acenaphthene-d10	10.04	164	232932	20.00	ng	-0.01
63) Phenanthrene-d10	11.54	188	387086	20.00	ng	-0.01
75) Chrysene-d12	14.19	240	286960	20.00	ng	-0.01
86) Perylene-d12	15.75	264	253043	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	724692	104.16	ng	0.00
7) Phenol-d6	6.62	99	977695	105.75	ng	0.00
23) Nitrobenzene-d5	7.56	82	648325	76.58	ng	-0.01
41) 2,4,6-Tribromophenol	10.84	330	256002	110.18	ng	-0.01
44) 2-Fluorobiphenyl	9.35	172	1227479	84.60	ng	-0.01
78) Terphenyl-d14	13.12	244	940066	83.29	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.74	163	91466	5.637	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082718\
Data File : BF108514.D
Acq On : 27 Aug 2018 16:54
Operator : JU/SJ
Sample : J4538-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VSS1

Quant Time: Aug 27 18:07:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 22 11:01:45 2018
Response via : Initial Calibration

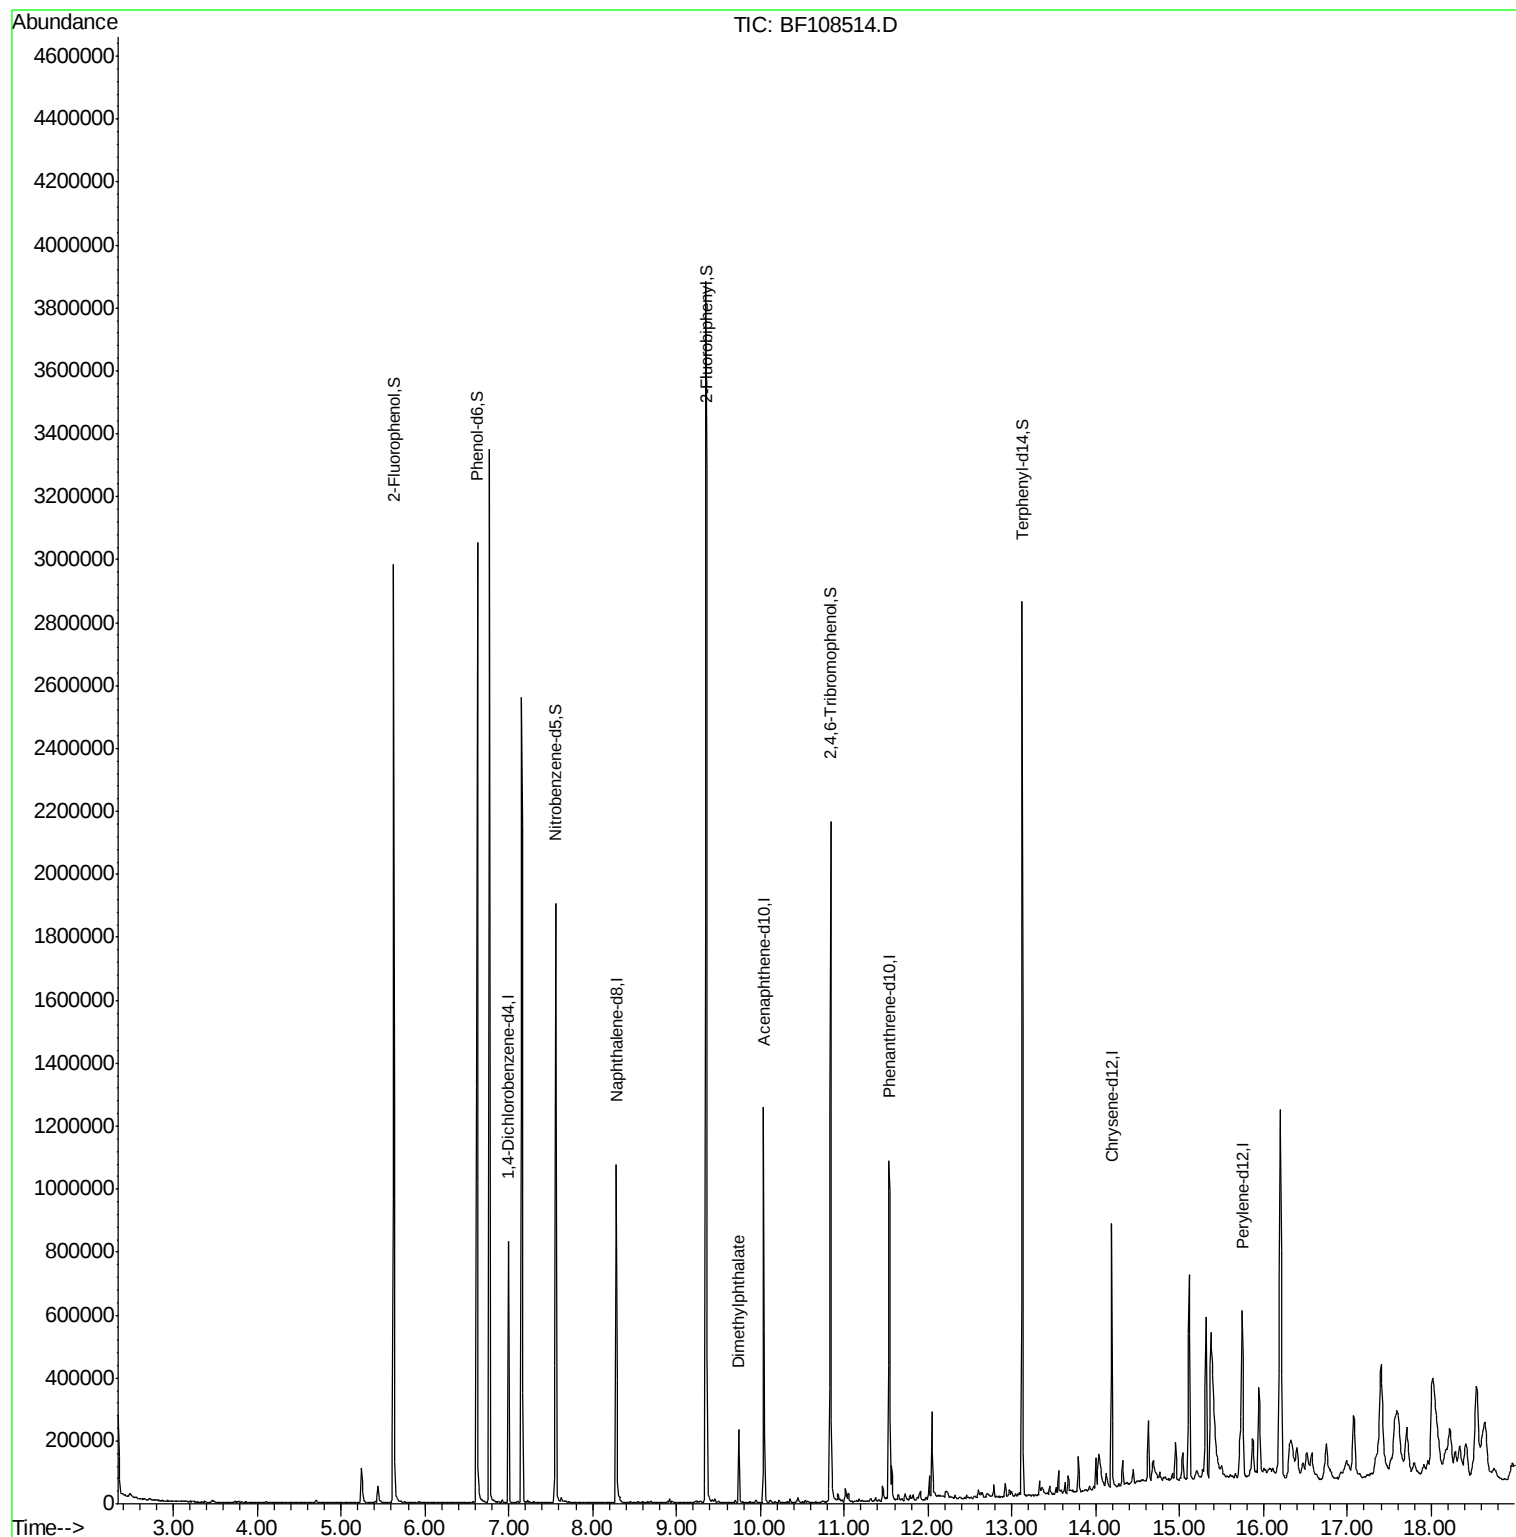

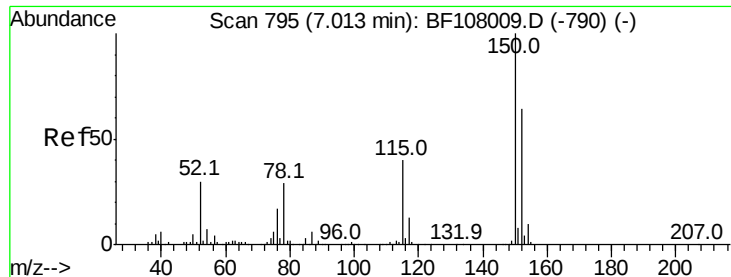


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.00 min Scan# 793
Delta R.T. -0.01 min
Lab File: BF108514.D
Acq: 27 Aug 2018 16:54

Instrument :
BNA_F
ClientSampleId :
VSS1

Tot Ion:152 Resp: 125961
Ion Ratio Lower Upper
152 100
150 149.7 124.6 186.8
115 56.0 50.1 75.1

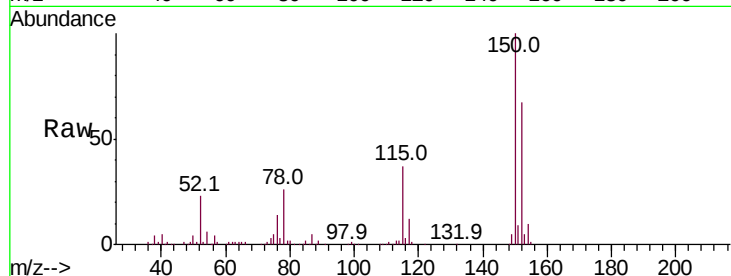



Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

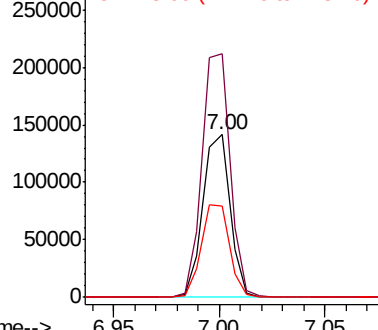



#5


2-Fluorophenol
Concen: 104.161 ng
RT: 5.63 min Scan# 560
Delta R.T. -0.00 min
Lab File: BF108514.D
Acq: 27 Aug 2018 16:54

Tgt Ion:112 Resp: 724692
Ion Ratio Lower Upper
112 100
64 69.4 47.9 71.9
63 36.8 23.7 35.5#

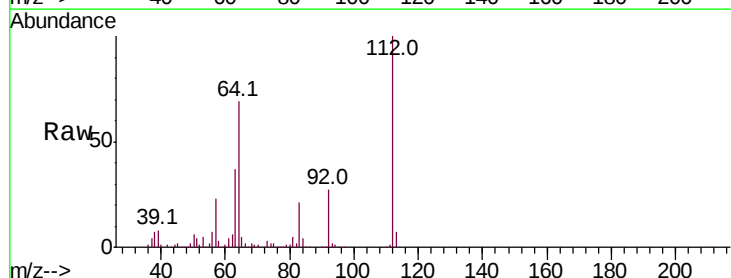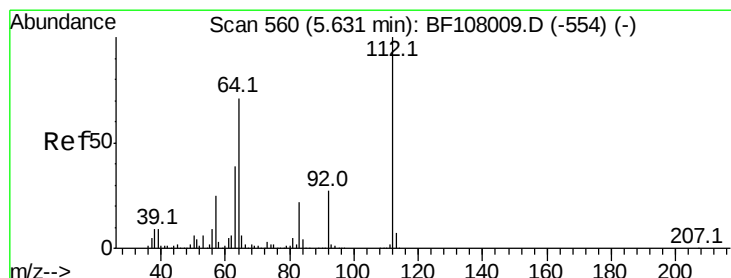

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

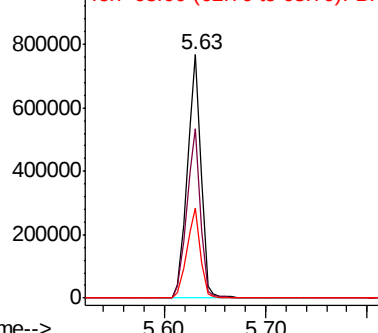

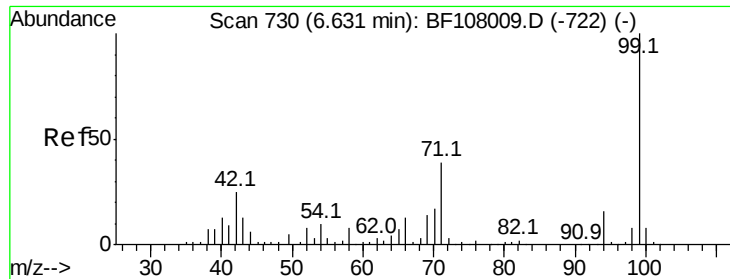

#7

Phenol-d6

Concen: 105.748 ng

RT: 6.62 min Scan# 729

Delta R.T. -0.01 min

Lab File: BF108514.D

Acq: 27 Aug 2018 16:54

Instrument :

BNA_F

ClientSampled :

VSS1


Tot Ion: 99 Resp: 977695

Ion Ratio Lower Upper




99 100

42 22.8 14.5 21.7#

71 36.9 25.4 38.0

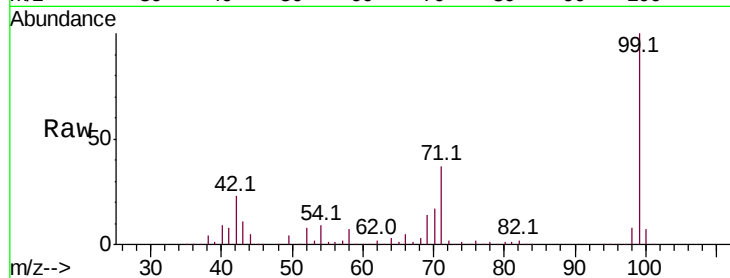

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

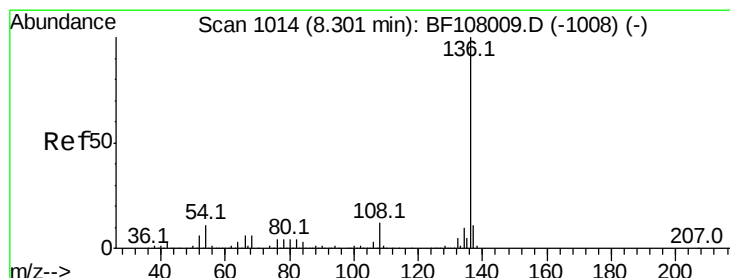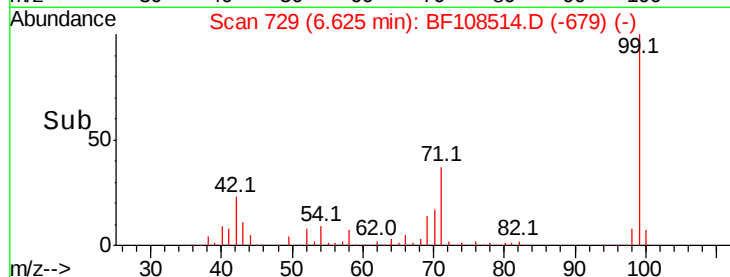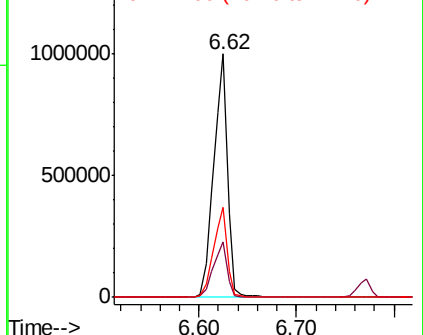

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.28 min Scan# 1011

Delta R.T. -0.01 min

Lab File: BF108514.D

Acq: 27 Aug 2018 16:54

Tgt Ion: 136 Resp: 472398


Ion Ratio Lower Upper

136 100



137 10.9 8.9 13.3


54 9.0 6.6 9.8

68 5.6 5.0 7.4

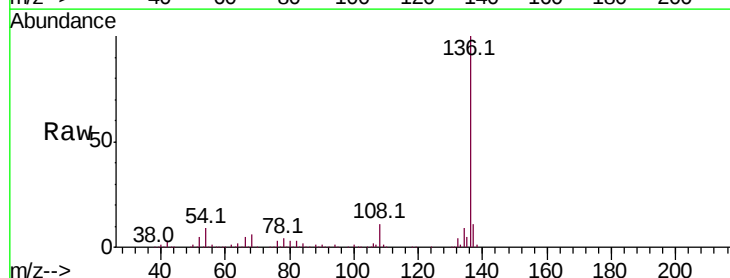

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

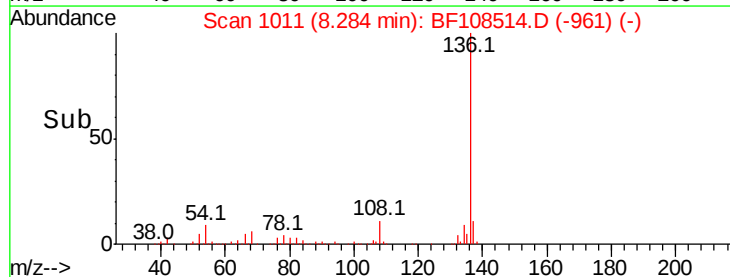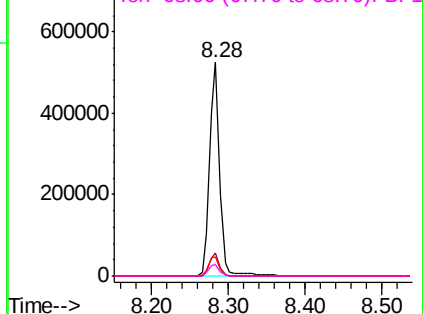


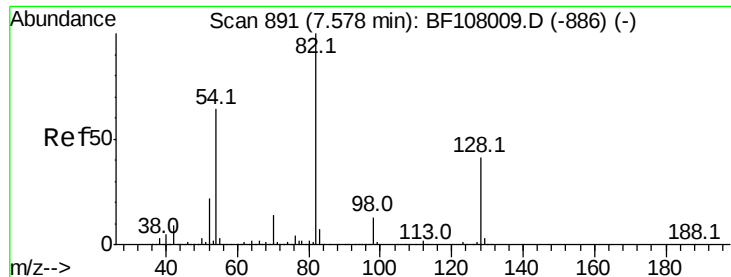




#23
Nitrobenzene-d5
Concen: 76.583 ng
RT: 7.56 min Scan# 888
Delta R.T. -0.01 min
Lab File: BF108514.D
Acq: 27 Aug 2018 16:54

Instrument :
BNA_F
ClientSampleId :
VSS1

Tot Ion: 82 Resp: 648325
Ion Ratio Lower Upper
82 100
128 40.3 36.1 54.1
54 59.9 41.4 62.2

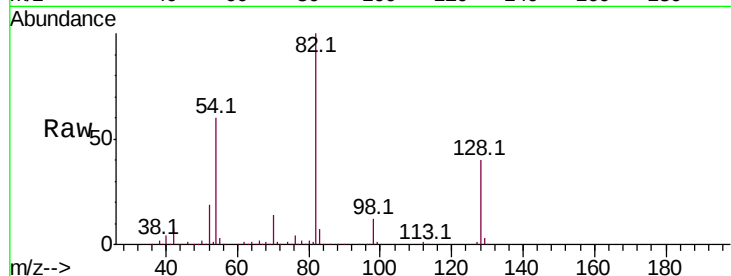


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

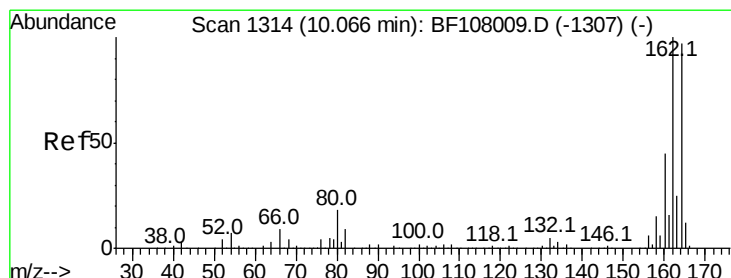
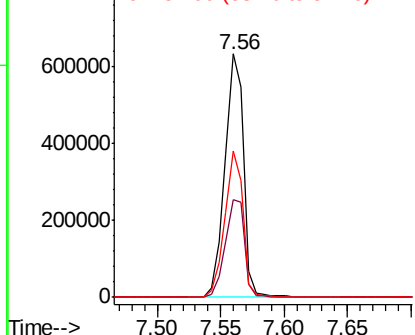



#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.04 min Scan# 1310
Delta R.T. -0.01 min
Lab File: BF108514.D
Acq: 27 Aug 2018 16:54

Tgt Ion:164 Resp: 232932
Ion Ratio Lower Upper
164 100
162 103.9 86.1 129.1
160 46.0 38.3 57.5

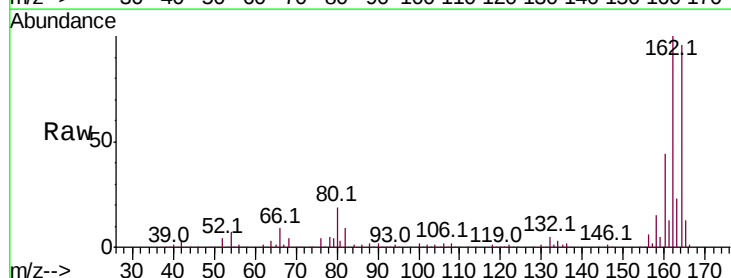

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

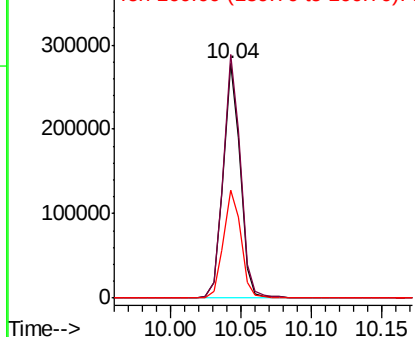


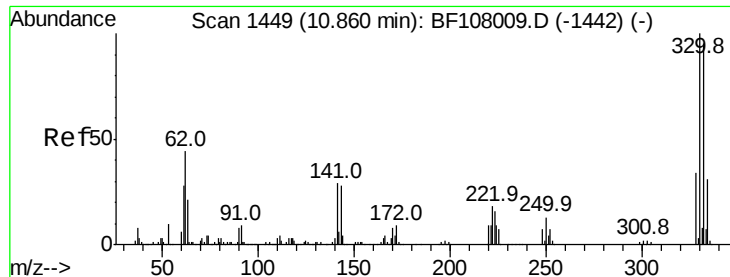




#41
 2,4,6-Tribromophenol
 Concen: 110.182 ng
 RT: 10.84 min Scan# 1445
 Delta R.T. -0.01 min
 Lab File: BF108514.D
 Acq: 27 Aug 2018 16:54

Instrument :
 BNA_F
 ClientSampleId :
 VSS1

Tot Ion:330 Resp: 256002
 Ion Ratio Lower Upper
 330 100
 332 96.4 77.0 115.6
 141 32.0 29.9 44.9

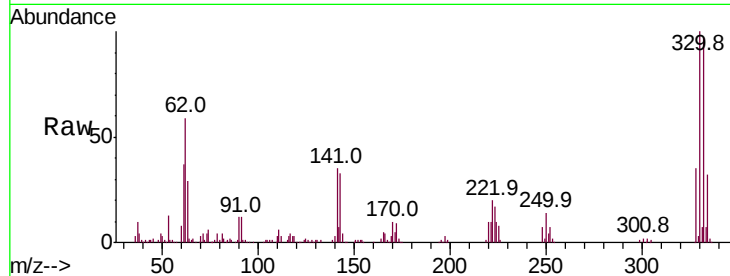


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

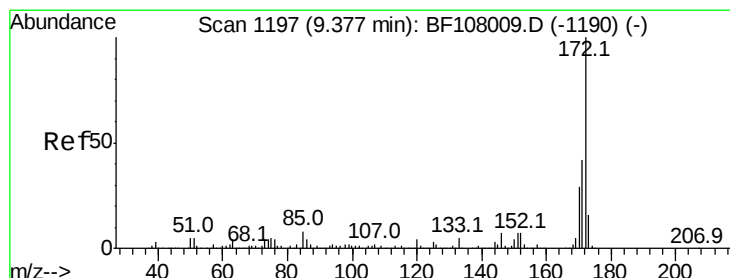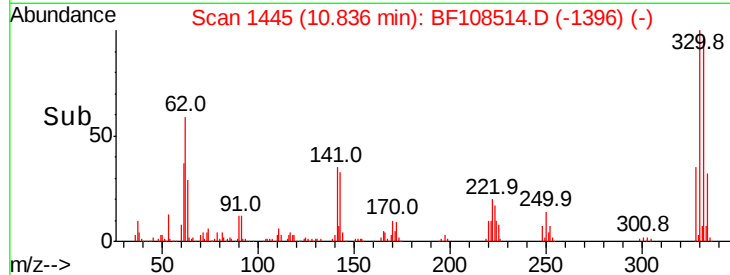
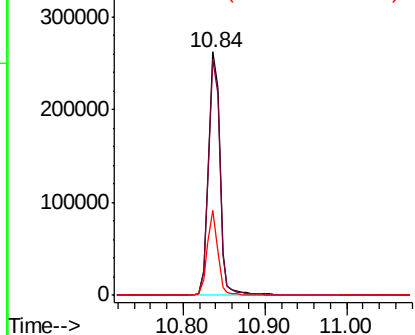



#44
 2-Fluorobiphenyl
 Concen: 84.603 ng
 RT: 9.35 min Scan# 1193
 Delta R.T. -0.01 min
 Lab File: BF108514.D
 Acq: 27 Aug 2018 16:54

Tgt Ion:172 Resp: 1227479
 Ion Ratio Lower Upper
 172 100
 171 36.9 29.7 44.5
 170 24.7 19.6 29.4

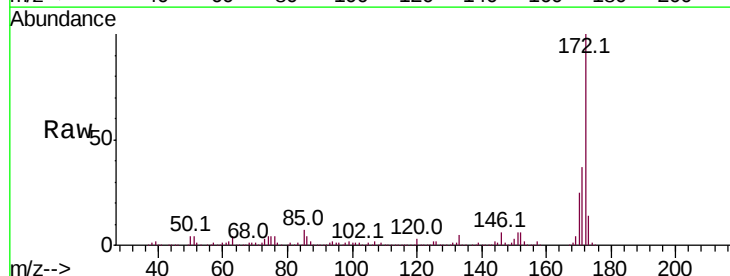

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

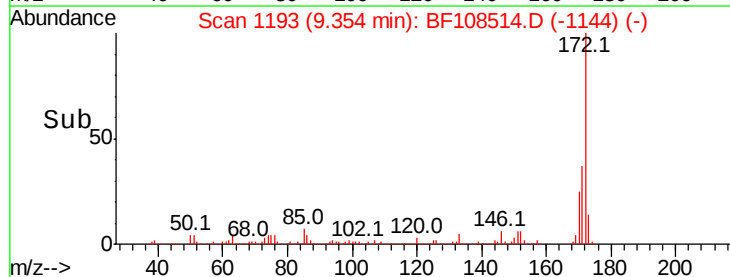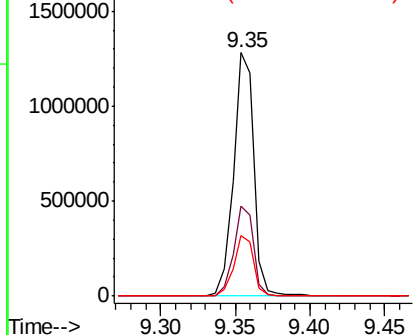


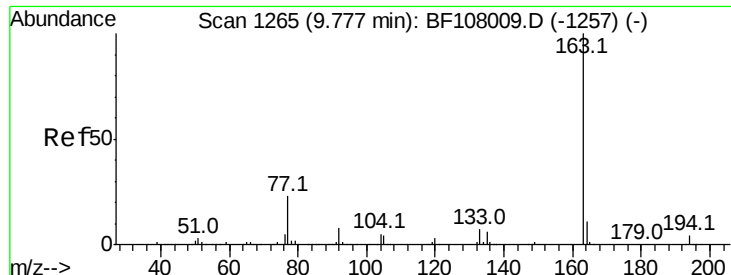




#49
Dimethylphthalate
Concen: 5.637 ng
RT: 9.74 min Scan# 1259
Delta R.T. -0.02 min
Lab File: BF108514.D
Acq: 27 Aug 2018 16:54

Instrument :
BNA_F
ClientSampled :
VSS1

Tot Ion:163 Resp: 91466
Ion Ratio Lower Upper
163 100
194 3.4 2.7 4.1
164 10.6 8.2 12.2

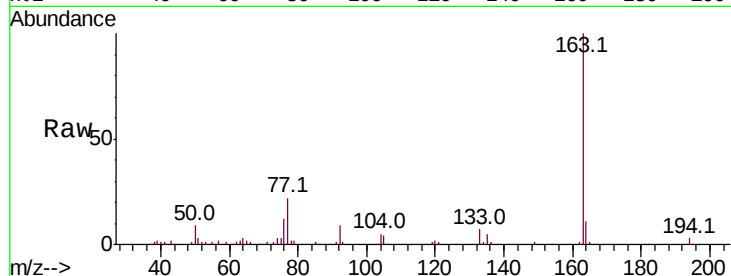


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

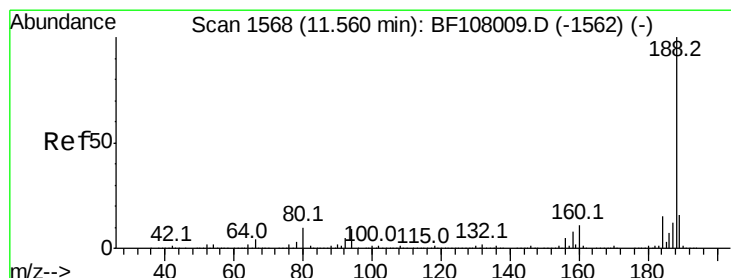
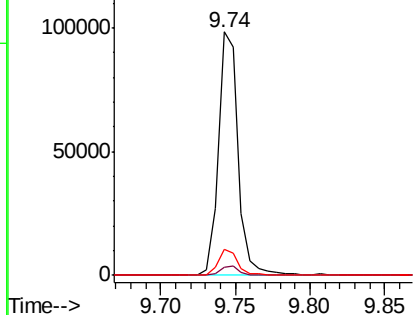



#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.54 min Scan# 1564
Delta R.T. -0.01 min
Lab File: BF108514.D
Acq: 27 Aug 2018 16:54

Tgt Ion:188 Resp: 387086
Ion Ratio Lower Upper
188 100
94 8.9 8.5 12.7
80 9.9 9.2 13.8

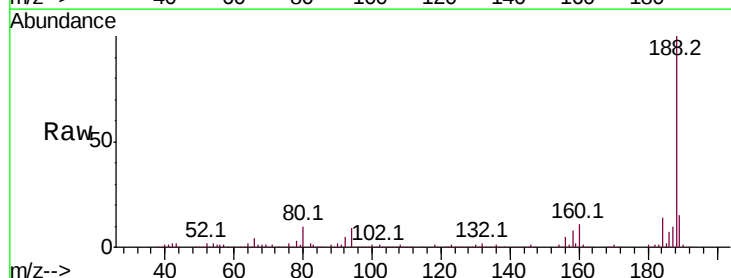

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

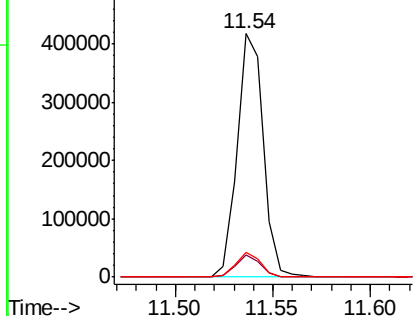



#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.19 min Scan# 2015

Delta R.T. -0.01 min

Lab File: BF108514.D

Acq: 27 Aug 2018 16:54

Instrument :

BNA_F

ClientSampleId :

VSS1


Tot Ion:240 Resp: 286960

Ion Ratio Lower Upper

240 100

120 10.4 9.5 14.3




236 26.4 20.7 31.1

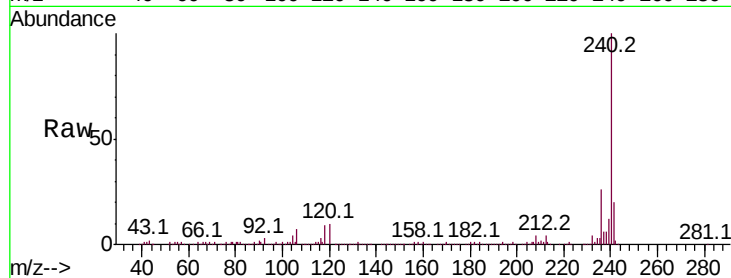

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

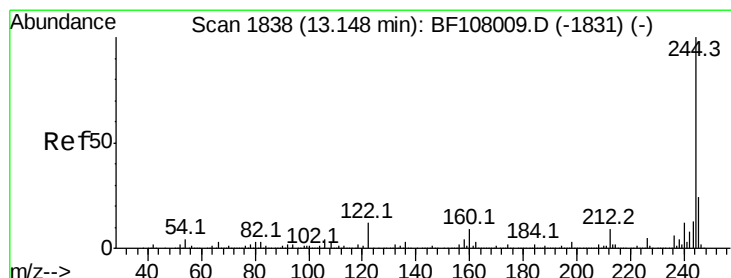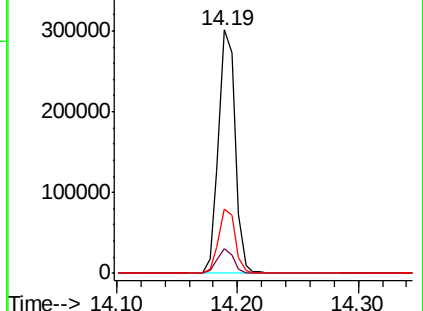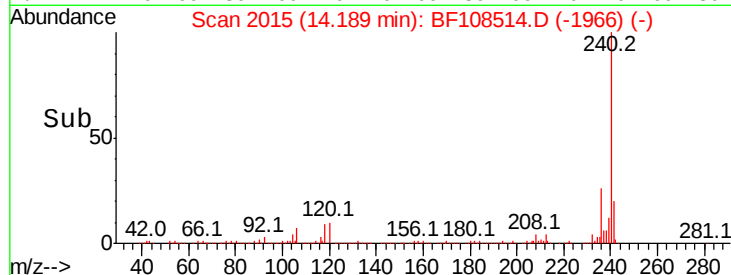

#78

Terphenyl-d14

Concen: 83.293 ng

RT: 13.12 min Scan# 1834

Delta R.T. -0.01 min

Lab File: BF108514.D

Acq: 27 Aug 2018 16:54


Tgt Ion:244 Resp: 940066

Ion Ratio Lower Upper

244 100

212 7.2 5.4 8.0



122 9.6 11.0 16.4#

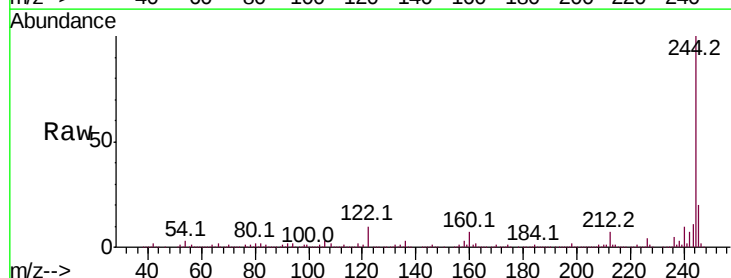


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

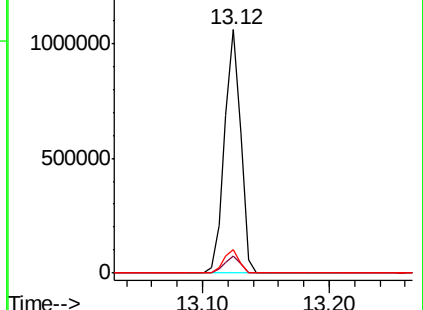

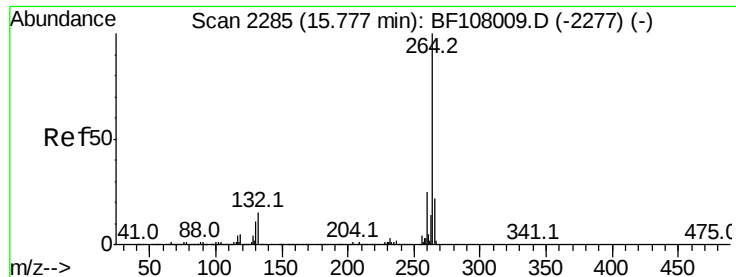

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.75 min Scan# 2280
Delta R.T. -0.01 min
Lab File: BF108514.D
Acq: 27 Aug 2018 16:54

Instrument :
BNA_F
ClientSampleId :
VSS1

Tot Ion	Ratio	Lower	Upper
264	100		
260	25.3	19.2	28.8
265	21.8	17.5	26.3

