

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082718\
 Data File : BF108503.D
 Acq On : 27 Aug 2018 12:02
 Operator : JU/SJ
 Sample : J4282-11 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SU-02-082318-A

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.619	554	558	569	rBV	356962	339812	27.53%	1.911%
2	6.613	723	727	742	rBV	416326	392680	31.81%	2.208%
3	6.766	749	753	760	rBV	466325	393823	31.91%	2.215%
4	6.995	789	792	796	rBV	862848	729506	59.10%	4.102%
5	7.154	815	819	822	rBV	350589	304800	24.69%	1.714%
6	7.554	884	887	895	rBV	265382	249061	20.18%	1.401%
7	8.284	1007	1011	1013	rBV	1099368	1004267	81.36%	5.647%
8	8.301	1013	1014	1021	rVB	390737	269625	21.84%	1.516%
9	8.995	1128	1132	1138	rBV	109232	100601	8.15%	0.566%
10	9.095	1145	1149	1155	rVB	74199	63505	5.15%	0.357%
11	9.354	1189	1193	1201	rBV	571710	488343	39.56%	2.746%
12	9.454	1208	1210	1214	rVB	28188	26186	2.12%	0.147%
13	9.625	1234	1239	1244	rBV	32381	45694	3.70%	0.257%
14	9.695	1247	1251	1254	rVV	57468	57802	4.68%	0.325%
15	9.725	1254	1256	1257	rVV	36121	29994	2.43%	0.169%
16	9.742	1257	1259	1267	rVV	145817	131134	10.62%	0.737%
17	9.813	1267	1271	1279	rVB	24578	32193	2.61%	0.181%
18	9.901	1283	1286	1291	rVB2	37553	32422	2.63%	0.182%
19	10.019	1303	1306	1307	rBV	15394	14904	1.21%	0.084%
20	10.042	1307	1310	1313	rVV2	1257170	1102662	89.34%	6.200%
21	10.072	1313	1315	1319	rVB	180310	168495	13.65%	0.947%
22	10.248	1340	1345	1348	rBV	128900	126079	10.21%	0.709%
23	10.278	1348	1350	1354	rVB	22662	19174	1.55%	0.108%
24	10.354	1358	1363	1366	rBV2	17807	17620	1.43%	0.099%
25	10.448	1373	1379	1385	rBV3	39029	51483	4.17%	0.289%
26	10.589	1400	1403	1409	rBV	221129	212789	17.24%	1.197%
27	10.677	1416	1418	1420	rVB2	25407	20129	1.63%	0.113%
28	10.748	1428	1430	1433	rVB	36595	29703	2.41%	0.167%
29	10.830	1441	1444	1451	rBV	293330	319449	25.88%	1.796%
30	10.936	1457	1462	1471	rVB4	19771	34880	2.83%	0.196%
31	11.142	1491	1497	1499	rBV	42362	48640	3.94%	0.274%
32	11.172	1499	1502	1504	rVV	23613	22898	1.86%	0.129%
33	11.225	1508	1511	1514	rVV	19681	17005	1.38%	0.096%
34	11.266	1514	1518	1520	rVV4	14835	20403	1.65%	0.115%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082718\
 Data File : BF108503.D
 Acq On : 27 Aug 2018 12:02
 Operator : JU/SJ
 Sample : J4282-11 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SU-02-082318-A

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.289	1520	1522	1526	rVV2	18914	20080	1.63%	0.113%
36	11.342	1526	1531	1534	rVV4	12478	17361	1.41%	0.098%
37	11.377	1534	1537	1540	rVV2	29420	30749	2.49%	0.173%
38	11.436	1544	1547	1551	rVB	71130	60455	4.90%	0.340%
39	11.536	1560	1564	1566	rBV	1209546	1119512	90.70%	6.295%
40	11.560	1566	1568	1572	rVV	1043254	953874	77.28%	5.364%
41	11.613	1574	1577	1581	rVV	338144	288528	23.38%	1.622%
42	11.648	1581	1583	1586	rVB	17974	15470	1.25%	0.087%
43	11.766	1599	1603	1607	rBV	92798	97457	7.90%	0.548%
44	11.801	1607	1609	1612	rVB	17658	15699	1.27%	0.088%
45	11.830	1612	1614	1618	rBV3	22572	20059	1.63%	0.113%
46	11.872	1618	1621	1624	rVV	20790	20984	1.70%	0.118%
47	11.907	1624	1627	1630	rVV2	19658	17024	1.38%	0.096%
48	12.042	1646	1650	1652	rBV	106006	101812	8.25%	0.573%
49	12.066	1652	1654	1658	rVV	130514	121492	9.84%	0.683%
50	12.119	1659	1663	1666	rVV	56995	53978	4.37%	0.304%
51	12.154	1666	1669	1672	rVV2	188067	216576	17.55%	1.218%
52	12.177	1672	1673	1676	rVV	69088	37447	3.03%	0.211%
53	12.213	1676	1679	1682	rVB2	18937	17754	1.44%	0.100%
54	12.336	1696	1700	1703	rBV	72365	63788	5.17%	0.359%
55	12.366	1703	1705	1710	rVB5	20468	19230	1.56%	0.108%
56	12.483	1719	1725	1728	rBV4	22693	25380	2.06%	0.143%
57	12.513	1728	1730	1733	rVV	21670	18145	1.47%	0.102%
58	12.595	1739	1744	1746	rBV3	132383	142501	11.55%	0.801%
59	12.619	1746	1748	1755	rVB4	71537	102403	8.30%	0.576%
60	12.677	1755	1758	1768	rVB6	28264	54920	4.45%	0.309%
61	12.760	1768	1772	1775	rBV	979592	829332	67.19%	4.663%
62	12.819	1780	1782	1785	rVB2	21074	16181	1.31%	0.091%
63	12.913	1794	1798	1801	rBV2	29860	35675	2.89%	0.201%
64	12.971	1804	1808	1809	rBV2	154578	168411	13.64%	0.947%
65	12.989	1809	1811	1816	rVB	762939	647786	52.48%	3.643%
66	13.036	1816	1819	1823	rVB3	40001	42386	3.43%	0.238%
67	13.118	1826	1833	1836	rBV	478626	445399	36.09%	2.505%
68	13.148	1836	1838	1843	rVB	29087	28198	2.28%	0.159%
69	13.195	1843	1846	1851	rBV3	47804	85122	6.90%	0.479%
70	13.313	1863	1866	1871	rVB	111001	126722	10.27%	0.713%
71	13.383	1875	1878	1880	rBV	116305	96975	7.86%	0.545%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082718\
 Data File : BF108503.D
 Acq On : 27 Aug 2018 12:02
 Operator : JU/SJ
 Sample : J4282-11 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SU-02-082318-A

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	13.418	1880	1884	1887	rVV2	51534	60332	4.89%	0.339%
73	13.513	1897	1900	1903	rBV	37864	38579	3.13%	0.217%
74	13.548	1903	1906	1912	rVB	41695	53330	4.32%	0.300%
75	13.671	1924	1927	1930	rBV4	25570	27666	2.24%	0.156%
76	13.801	1946	1949	1951	rBV2	18901	19009	1.54%	0.107%
77	13.824	1951	1953	1957	rVV	25120	28337	2.30%	0.159%
78	13.942	1968	1973	1975	rBV2	52753	67527	5.47%	0.380%
79	13.966	1975	1977	1979	rVV	59748	54390	4.41%	0.306%
80	14.001	1979	1983	1986	rVV3	59876	91873	7.44%	0.517%
81	14.036	1986	1989	1996	rVB4	39817	74671	6.05%	0.420%
82	14.189	2008	2015	2018	rBV2	985504	1234295	100.00%	6.941%
83	14.218	2018	2020	2027	rVB	307452	273760	22.18%	1.539%
84	14.301	2031	2034	2036	rBV	70841	72535	5.88%	0.408%
85	14.383	2046	2048	2050	rVB	21304	15831	1.28%	0.089%
86	14.418	2052	2054	2057	rVB	32926	28599	2.32%	0.161%
87	14.448	2057	2059	2061	rBV2	26183	24423	1.98%	0.137%
88	14.577	2079	2081	2084	rVB	52426	41709	3.38%	0.235%
89	14.707	2101	2103	2105	rBV2	26697	23147	1.88%	0.130%
90	14.730	2105	2107	2112	rVB2	43112	42700	3.46%	0.240%
91	14.954	2142	2145	2148	rVB	54506	58451	4.74%	0.329%
92	15.277	2196	2200	2204	rBV	236896	403887	32.72%	2.271%
93	15.395	2217	2220	2224	rBV	53761	79069	6.41%	0.445%
94	15.607	2253	2256	2263	rVB	132011	190643	15.45%	1.072%
95	15.677	2264	2268	2273	rBV	215038	289416	23.45%	1.627%
96	15.748	2273	2280	2284	rBV	618111	910471	73.76%	5.120%
97	16.201	2353	2357	2363	rVB	67724	99059	8.03%	0.557%
98	16.748	2446	2450	2455	rVB2	48643	75374	6.11%	0.424%
99	17.354	2548	2553	2560	rBV2	78299	177506	14.38%	0.998%
100	17.848	2632	2637	2647	rVB2	55110	134290	10.88%	0.755%


Sum of corrected areas: 17783505

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082718\
Data File : BF108503.D
Acq On : 27 Aug 2018 12:02
Operator : JU/SJ
Sample : J4282-11 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-02-082318-A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

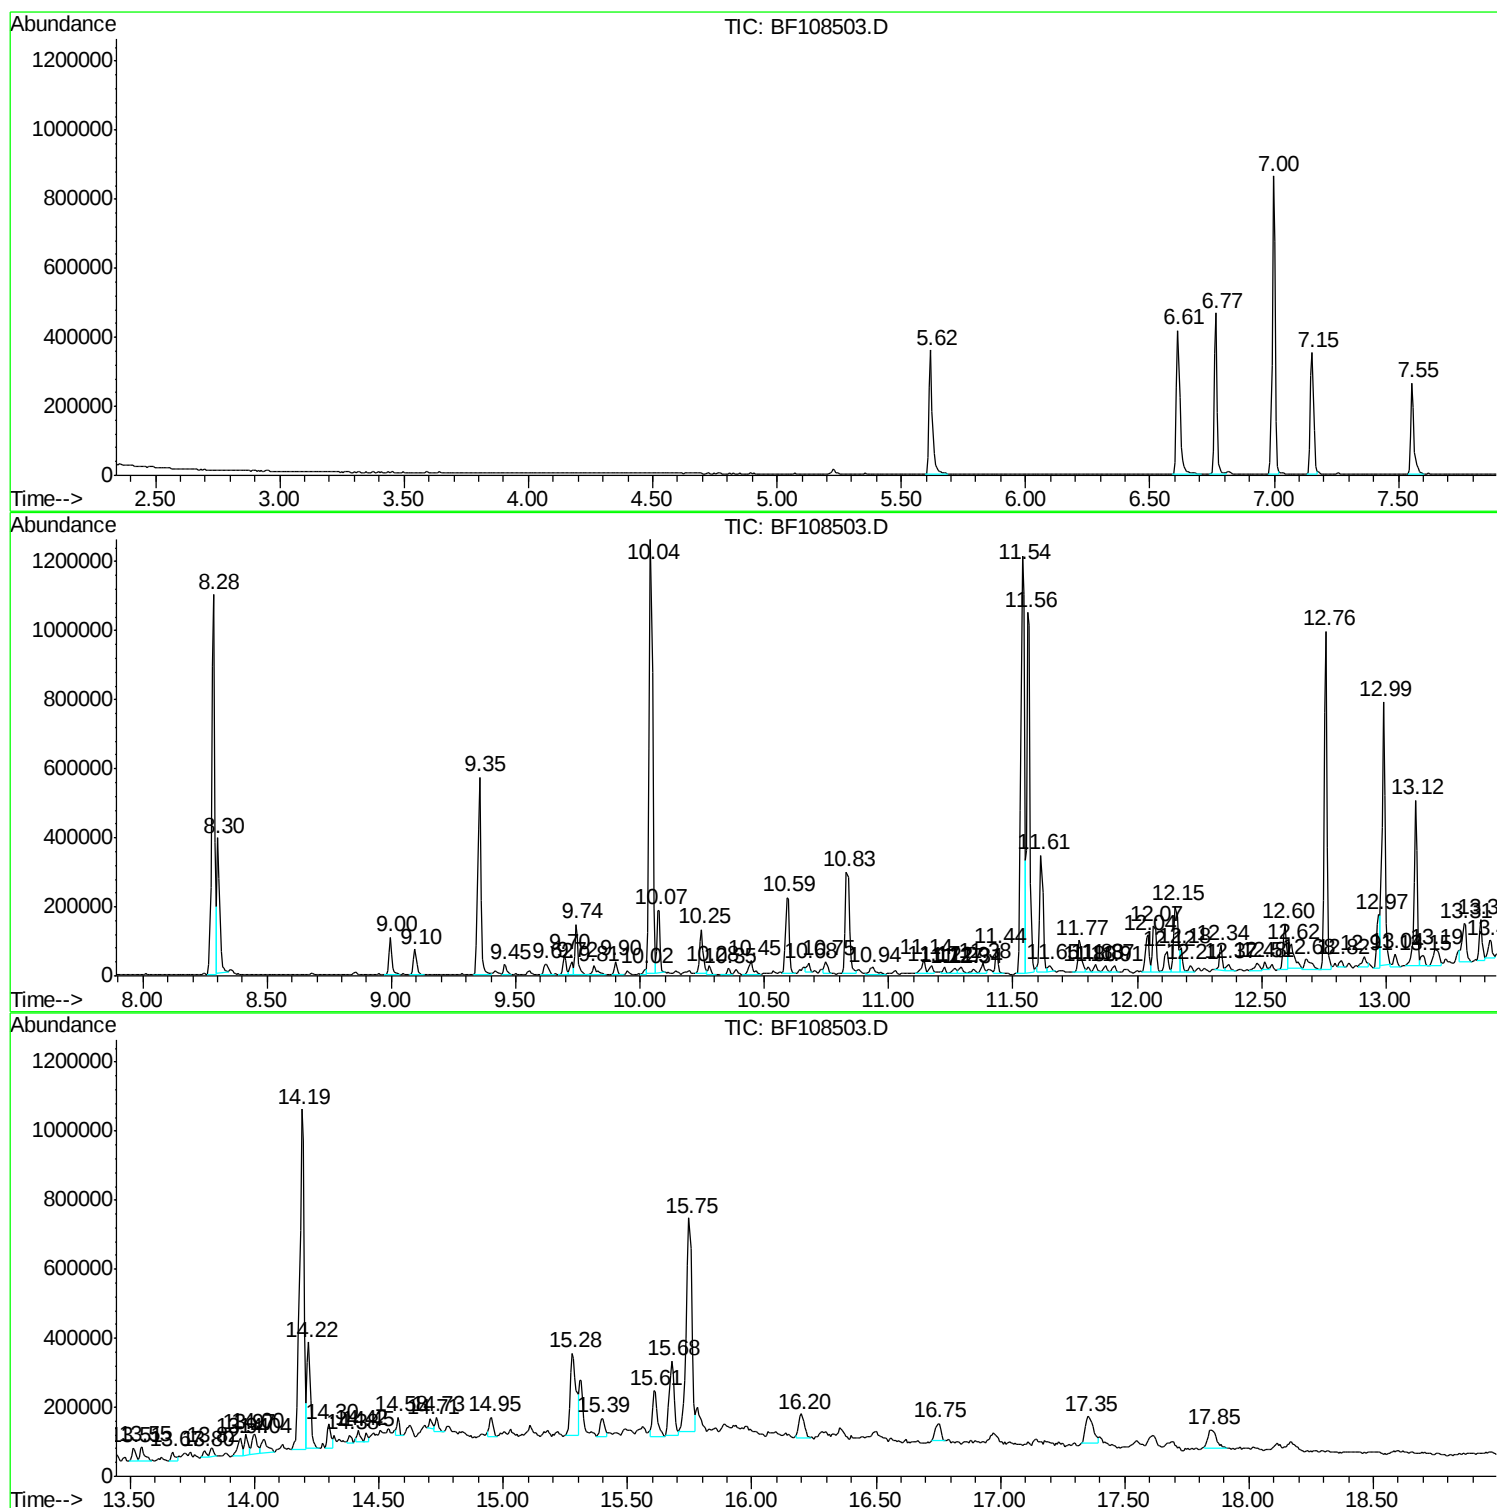

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082718\
Data File : BF108503.D
Acq On : 27 Aug 2018 12:02
Operator : JU/SJ
Sample : J4282-11 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-02-082318-A










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.77 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.77	10.80 ng	393823	1,4-Dichlorobenzene-d4	7.00

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
4		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	9
5		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

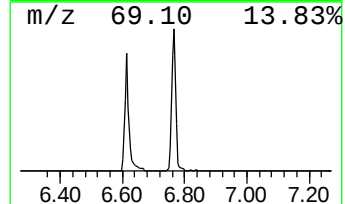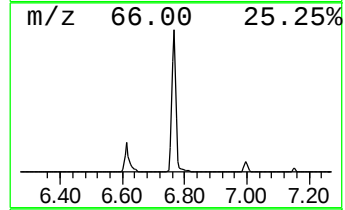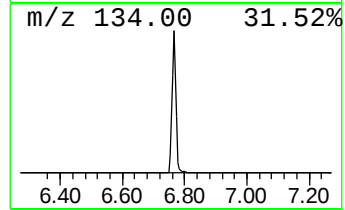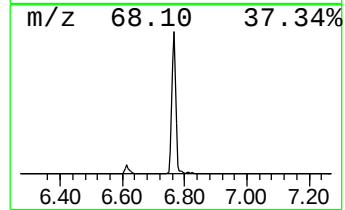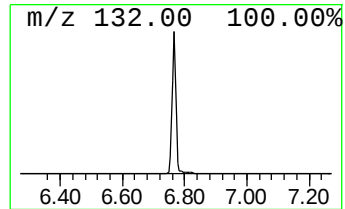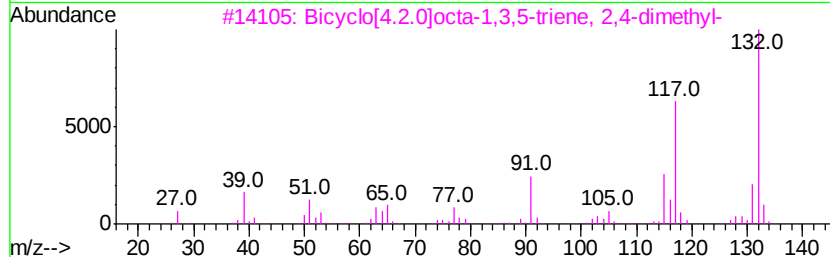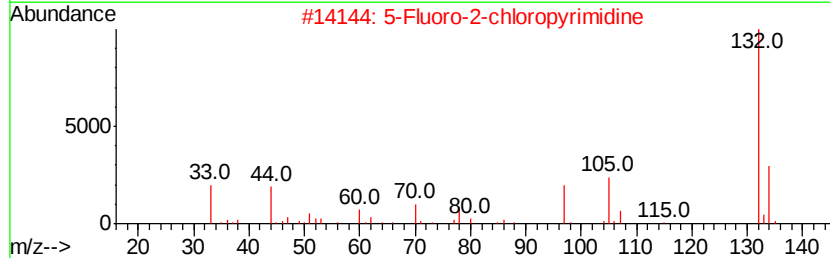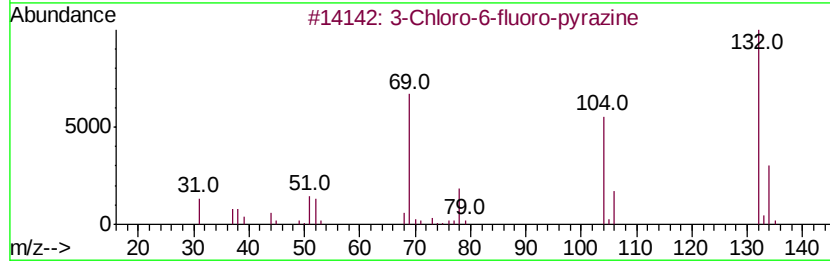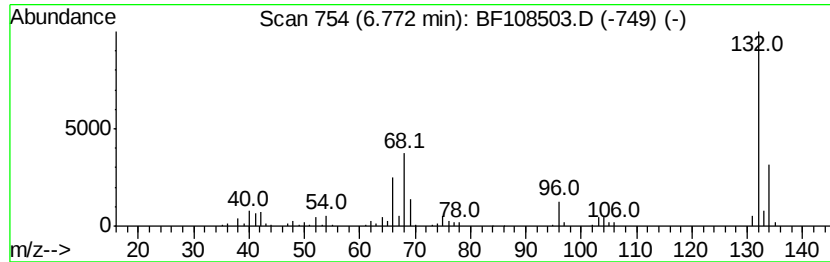

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082718\
Data File : BF108503.D
Acq On : 27 Aug 2018 12:02
Operator : JU/SJ
Sample : J4282-11 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-02-082318-A










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Phenanthrene, 2-methyl- Concentration Rank 7

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.07	2.17 ng	121492	Phenanthrene-d10	11.54

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Phenanthrene, 2-methyl-	192	C15H12	002531-84-2	98
2		Phenanthrene, 1-methyl-	192	C15H12	000832-69-9	96
3		Anthracene, 2-methyl-	192	C15H12	000613-12-7	96
4		Anthracene, 1-methyl-	192	C15H12	000610-48-0	94
5		1H-Indene, 2-phenyl-	192	C15H12	004505-48-0	93

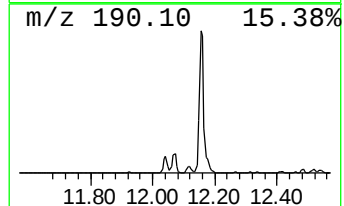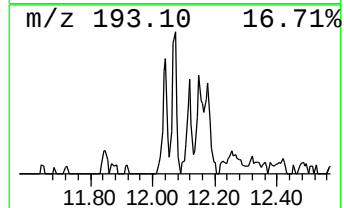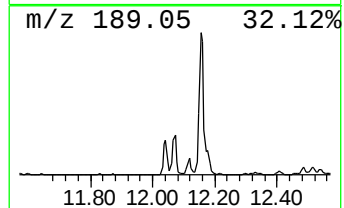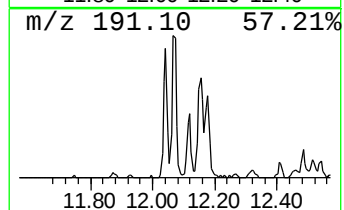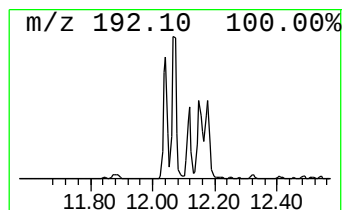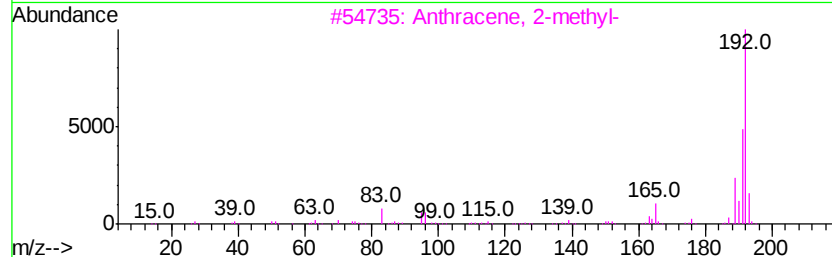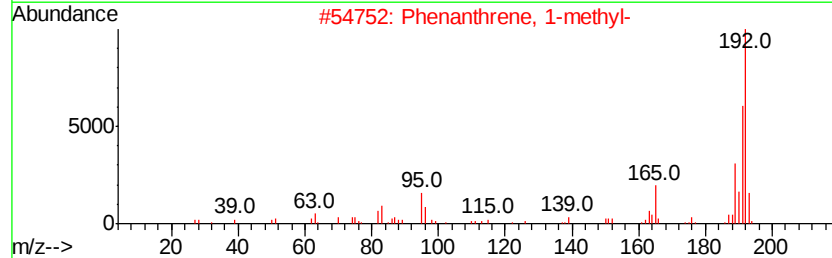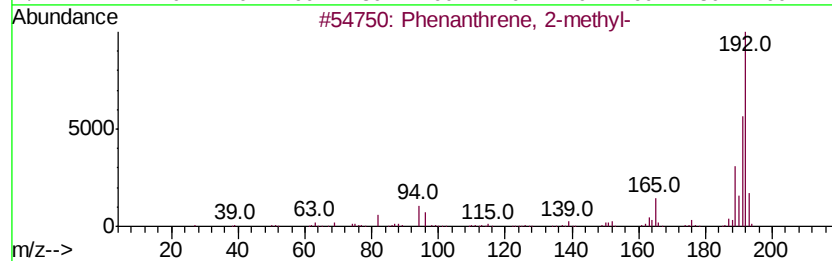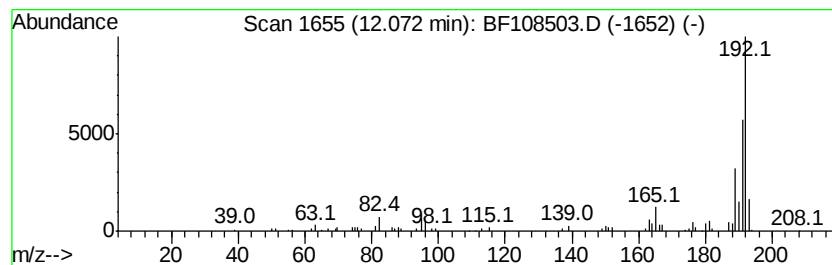

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082718\
Data File : BF108503.D
Acq On : 27 Aug 2018 12:02
Operator : JU/SJ
Sample : J4282-11 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
SU-02-082318-A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 4H-Cyclopenta[def]phenanthrene Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.	
12.15	3.87 ng	216576	Phenanthrene-d10	11.54	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	4H-Cyclopenta[def]phenanthrene	190	C15H10	000203-64-5	87
2	6H-Cyclobuta[ik]phenanthrene	190	C15H10	083469-43-6	72
3	Methyl diselenide	190	C2H6Se2	007101-31-7	55
4	2,2'-Bis(4,5-dimethylimidazole)	190	C10H14N4	069286-06-2	45
5	1,4-Naphthalenedione, 2,5-dihydr...	190	C10H6O4	004923-55-1	25

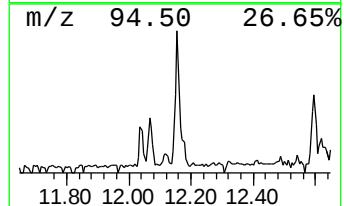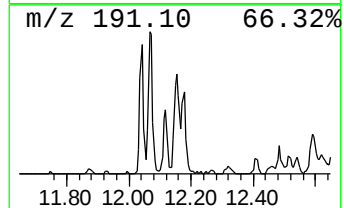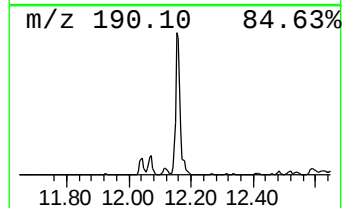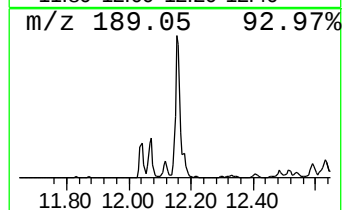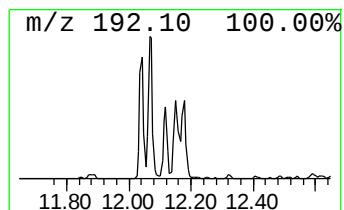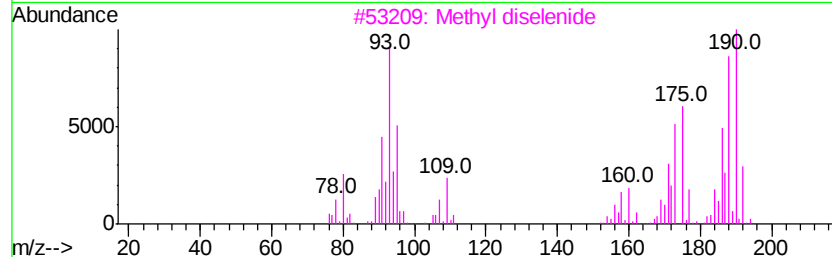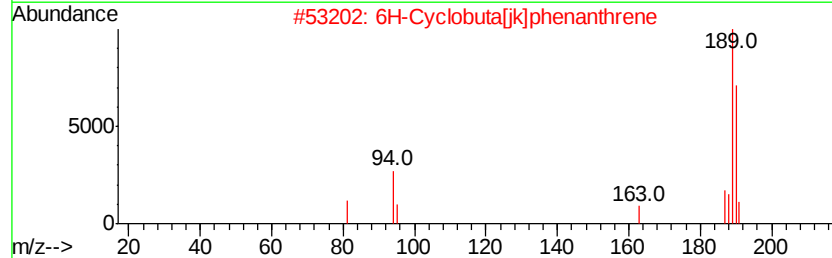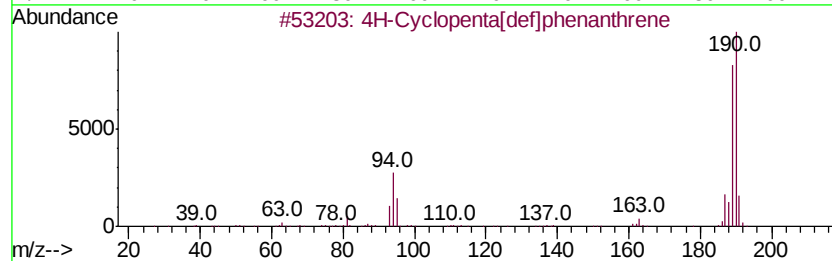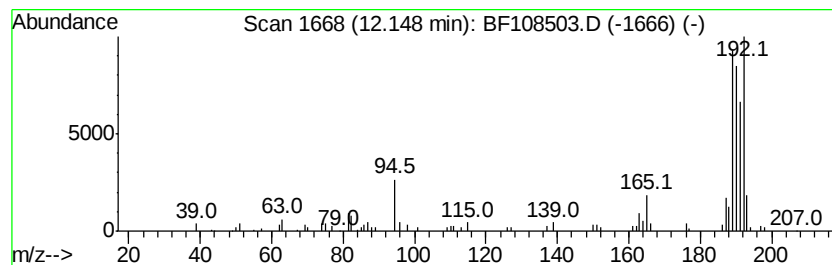

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082718\
Data File : BF108503.D
Acq On : 27 Aug 2018 12:02
Operator : JU/SJ
Sample : J4282-11 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-02-082318-A










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 di-p-Tolylacetylene Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.60	2.55 ng	142501	Phenanthrene-d10	11.54

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	di-p-Tolylacetylene	206	C16H14	002789-88-0	66
2		Phenanthrene, 3,6-dimethyl-	206	C16H14	001576-67-6	66
3		9,10-Dimethylanthracene	206	C16H14	000781-43-1	62
4		Phenanthrene, 2,7-dimethyl-	206	C16H14	001576-69-8	55
5		1,E-8,Z-10-Pentadecatriene	206	C15H26	080625-32-7	53

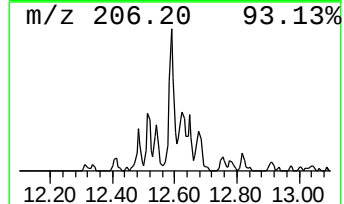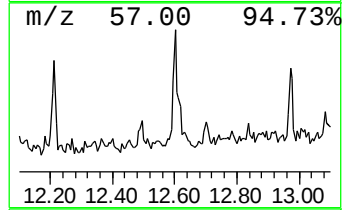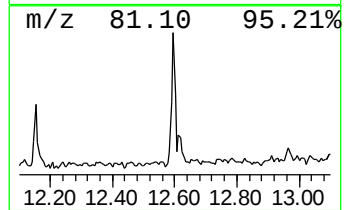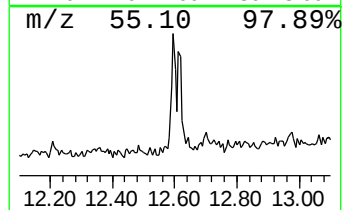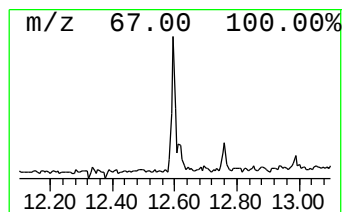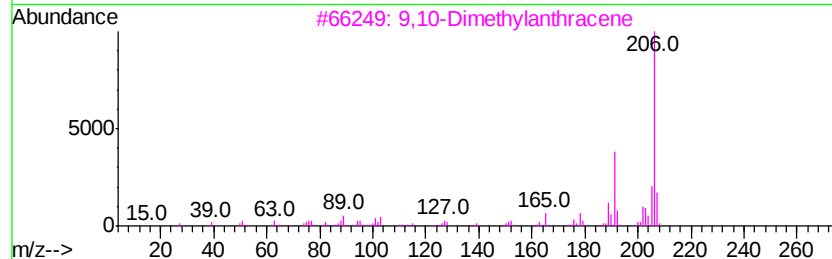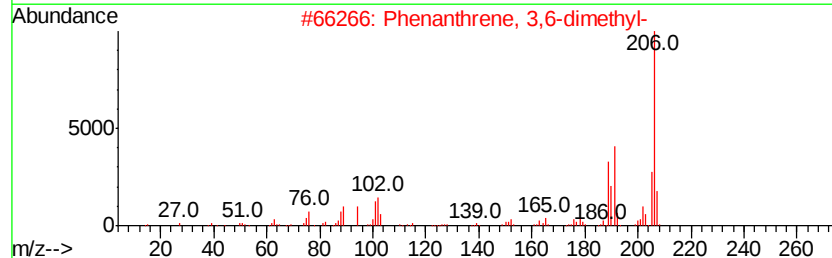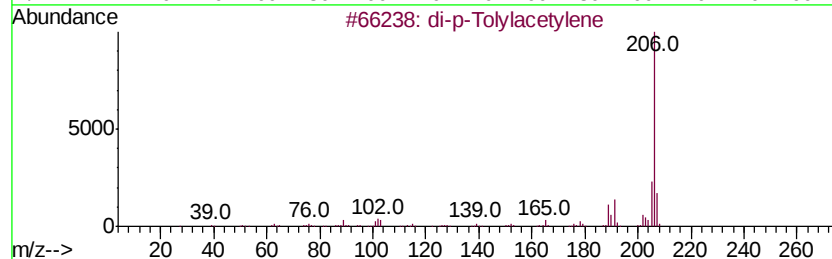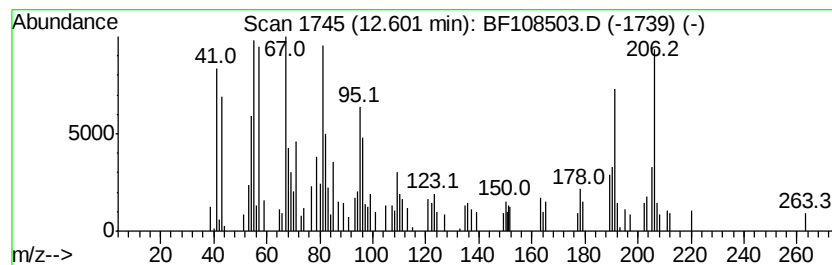

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082718\
Data File : BF108503.D
Acq On : 27 Aug 2018 12:02
Operator : JU/SJ
Sample : J4282-11 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
SU-02-082318-A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 6 11H-Benzo[b]fluorene Concentration Rank 8

R.T.	EstConc	Area	Relative to ISTD		R.T.	
13.31	2.05 ng	126722	Chrysene-d12		14.19	
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		11H-Benzo[b]fluorene	216	C17H12	000243-17-4	90
2		Pyrene, 1-methyl-	216	C17H12	002381-21-7	87
3		Pyrene, 2-methyl-	216	C17H12	003442-78-2	83
4		11H-Benzo[a]fluorene	216	C17H12	000238-84-6	74
5		7H-Benzo[c]fluorene	216	C17H12	000205-12-9	72

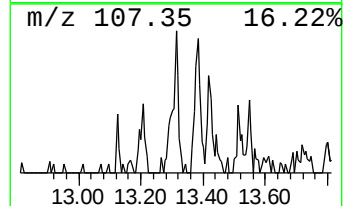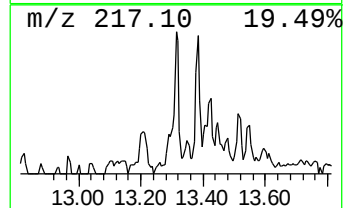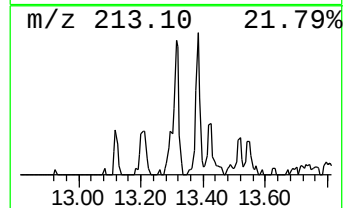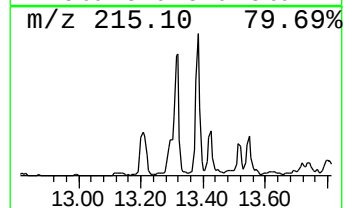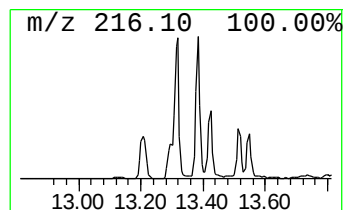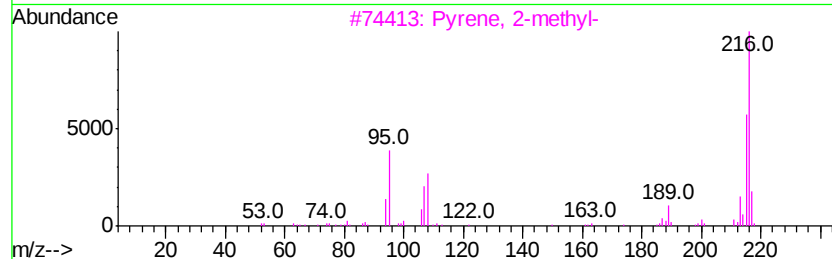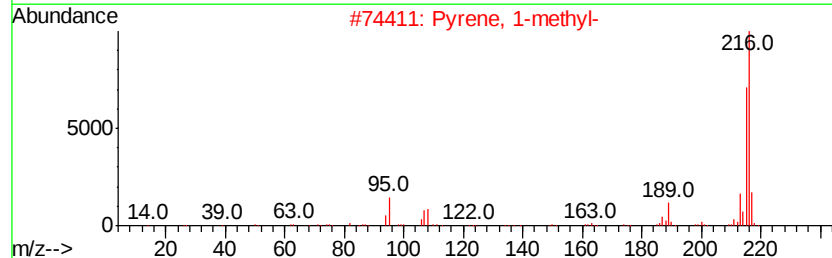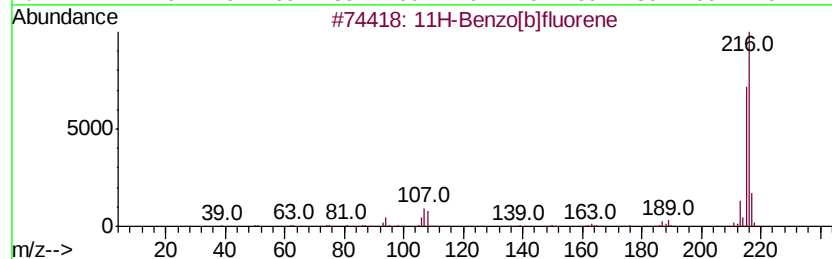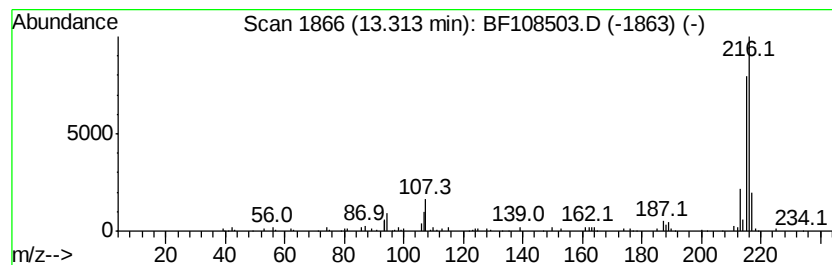

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082718\
Data File : BF108503.D
Acq On : 27 Aug 2018 12:02
Operator : JU/SJ
Sample : J4282-11 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-02-082318-A










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 7 Benzo[e]pyrene Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.61	4.19 ng	190643	Perylene-d12	15.75

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzo[e]pyrene	252	C20H12	000192-97-2	98
2			Benzo[a]pyrene	252	C20H12	000050-32-8	94
3			Perylene	252	C20H12	000198-55-0	94
4			Benzo[e]acephenanthrylene	252	C20H12	000205-99-2	93
5			Benzo[j]fluoranthene	252	C20H12	000205-82-3	93

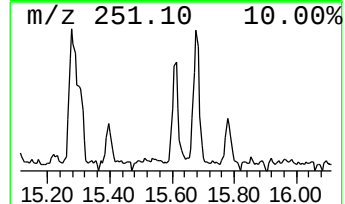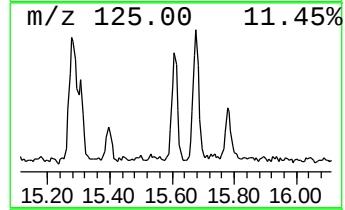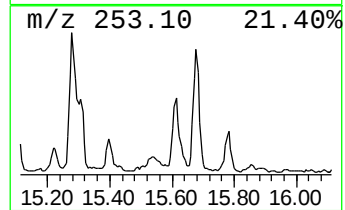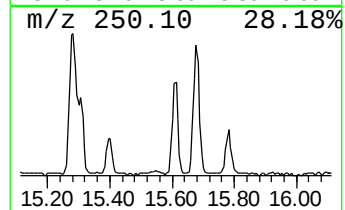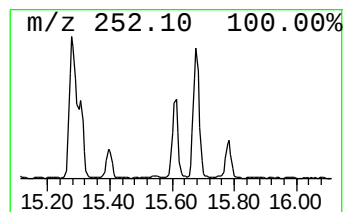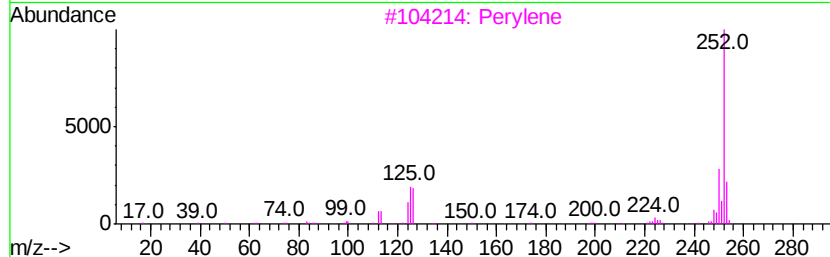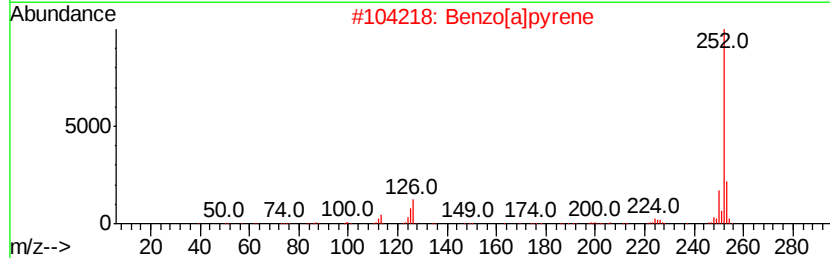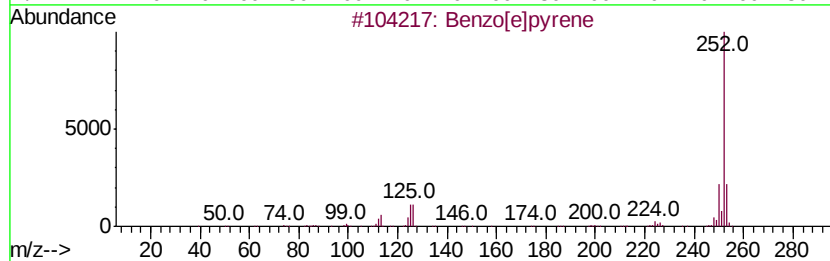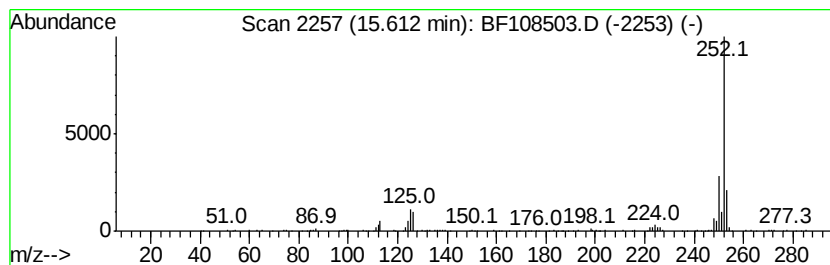

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082718\
Data File : BF108503.D
Acq On : 27 Aug 2018 12:02
Operator : JU/SJ
Sample : J4282-11 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-02-082318-A










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 8 Heptadecane Concentration Rank 6

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.20	2.18 ng	99059	Perylene-d12	15.75

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Heptadecane		240	C17H36	000629-78-7	93
2	Pentadecane		212	C15H32	000629-62-9	92
3	Tridecane, 7-propyl-		226	C16H34	055045-09-5	70
4	Eicosane		282	C20H42	000112-95-8	70
5	Hexacosane		366	C26H54	000630-01-3	68

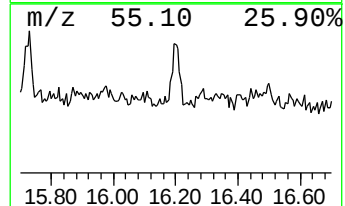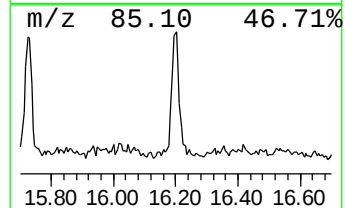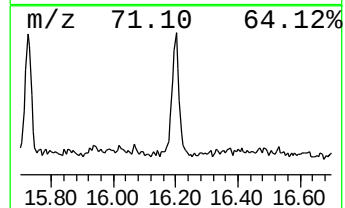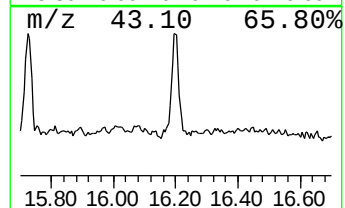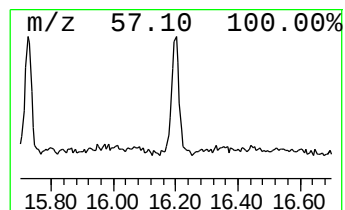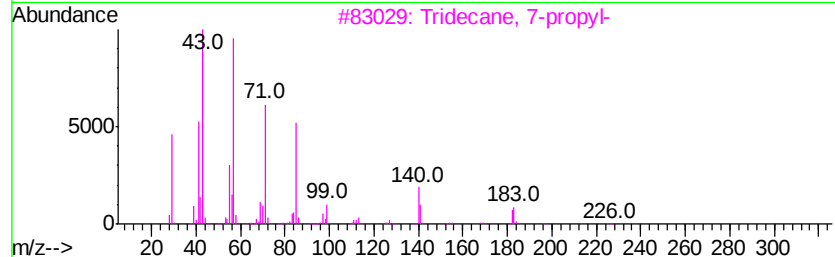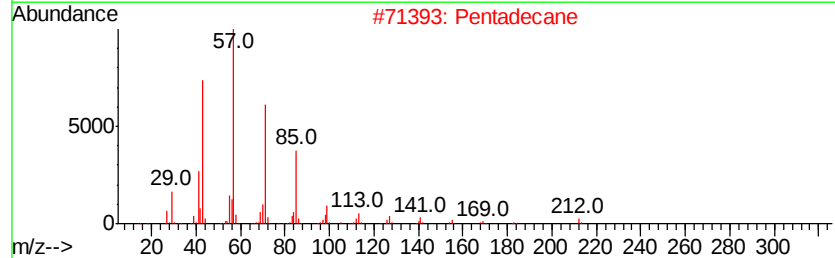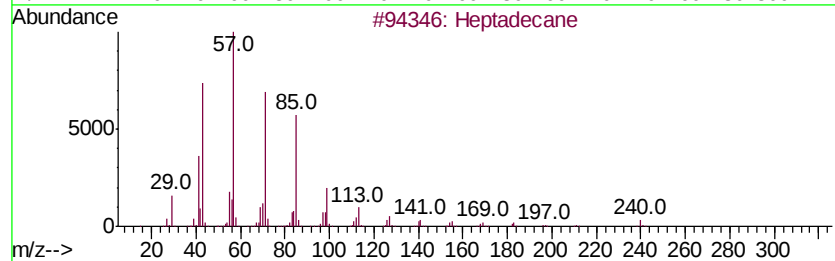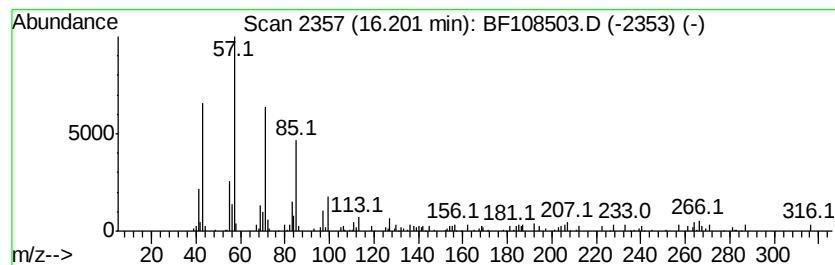

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082718\
Data File : BF108503.D
Acq On : 27 Aug 2018 12:02
Operator : JU/SJ
Sample : J4282-11 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-02-082318-A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.77	6.77	10.8	ng	393823	1	7.00	729506	20.0
Phenanthrene, 2-m...	12.07	2.2	ng	121492	4	11.54	1119510	20.0
4H-Cyclopenta[def...	12.15	3.9	ng	216576	4	11.54	1119510	20.0
di-p-Tolylacetylene	12.60	2.5	ng	142501	4	11.54	1119510	20.0
11H-Benzo[b]fluorene	13.31	2.0	ng	126722	5	14.19	1234300	20.0
Benzo[e]pyrene	15.61	4.2	ng	190643	6	15.75	910471	20.0
Heptadecane	16.20	2.2	ng	99059	6	15.75	910471	20.0