

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082718\
 Data File : BF108533.D
 Acq On : 28 Aug 2018 2:22
 Operator : JU/SJ
 Sample : J4659-06
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 082218-SIDI-E-D-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.231	489	492	500	rVB	41981	43736	1.27%	0.231%
2	5.625	555	559	571	rBV	932754	837250	24.30%	4.422%
3	6.613	724	727	731	rBV	573344	503760	14.62%	2.660%
4	6.766	749	753	757	rBV	1869168	1668286	48.42%	8.811%
5	7.001	789	793	796	rBV	742212	655278	19.02%	3.461%
6	7.154	815	819	823	rBV	2666066	2532414	73.50%	13.374%
7	7.566	883	889	892	rBV	2058742	2031945	58.97%	10.731%
8	8.283	1007	1011	1025	rBV	830788	756955	21.97%	3.998%
9	9.354	1189	1193	1197	rBV	3724307	3445629	100.00%	18.197%
10	9.742	1256	1259	1264	rBV	67498	62120	1.80%	0.328%
11	10.042	1307	1310	1322	rVB	816618	711937	20.66%	3.760%
12	10.701	1419	1422	1426	rBV	70653	57730	1.68%	0.305%
13	10.836	1441	1445	1458	rBV	1086361	1042609	30.26%	5.506%
14	11.536	1561	1564	1578	rVB	698960	629160	18.26%	3.323%
15	13.124	1830	1834	1837	rBV	3190958	2728626	79.19%	14.410%
16	14.189	2011	2015	2025	rBV	727175	727113	21.10%	3.840%
17	15.748	2272	2280	2287	rBV	327234	500553	14.53%	2.644%


Sum of corrected areas: 18935101

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082718\
Data File : BF108533.D
Acq On : 28 Aug 2018 2:22
Operator : JU/SJ
Sample : J4659-06
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082218-SIDI-E-D-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

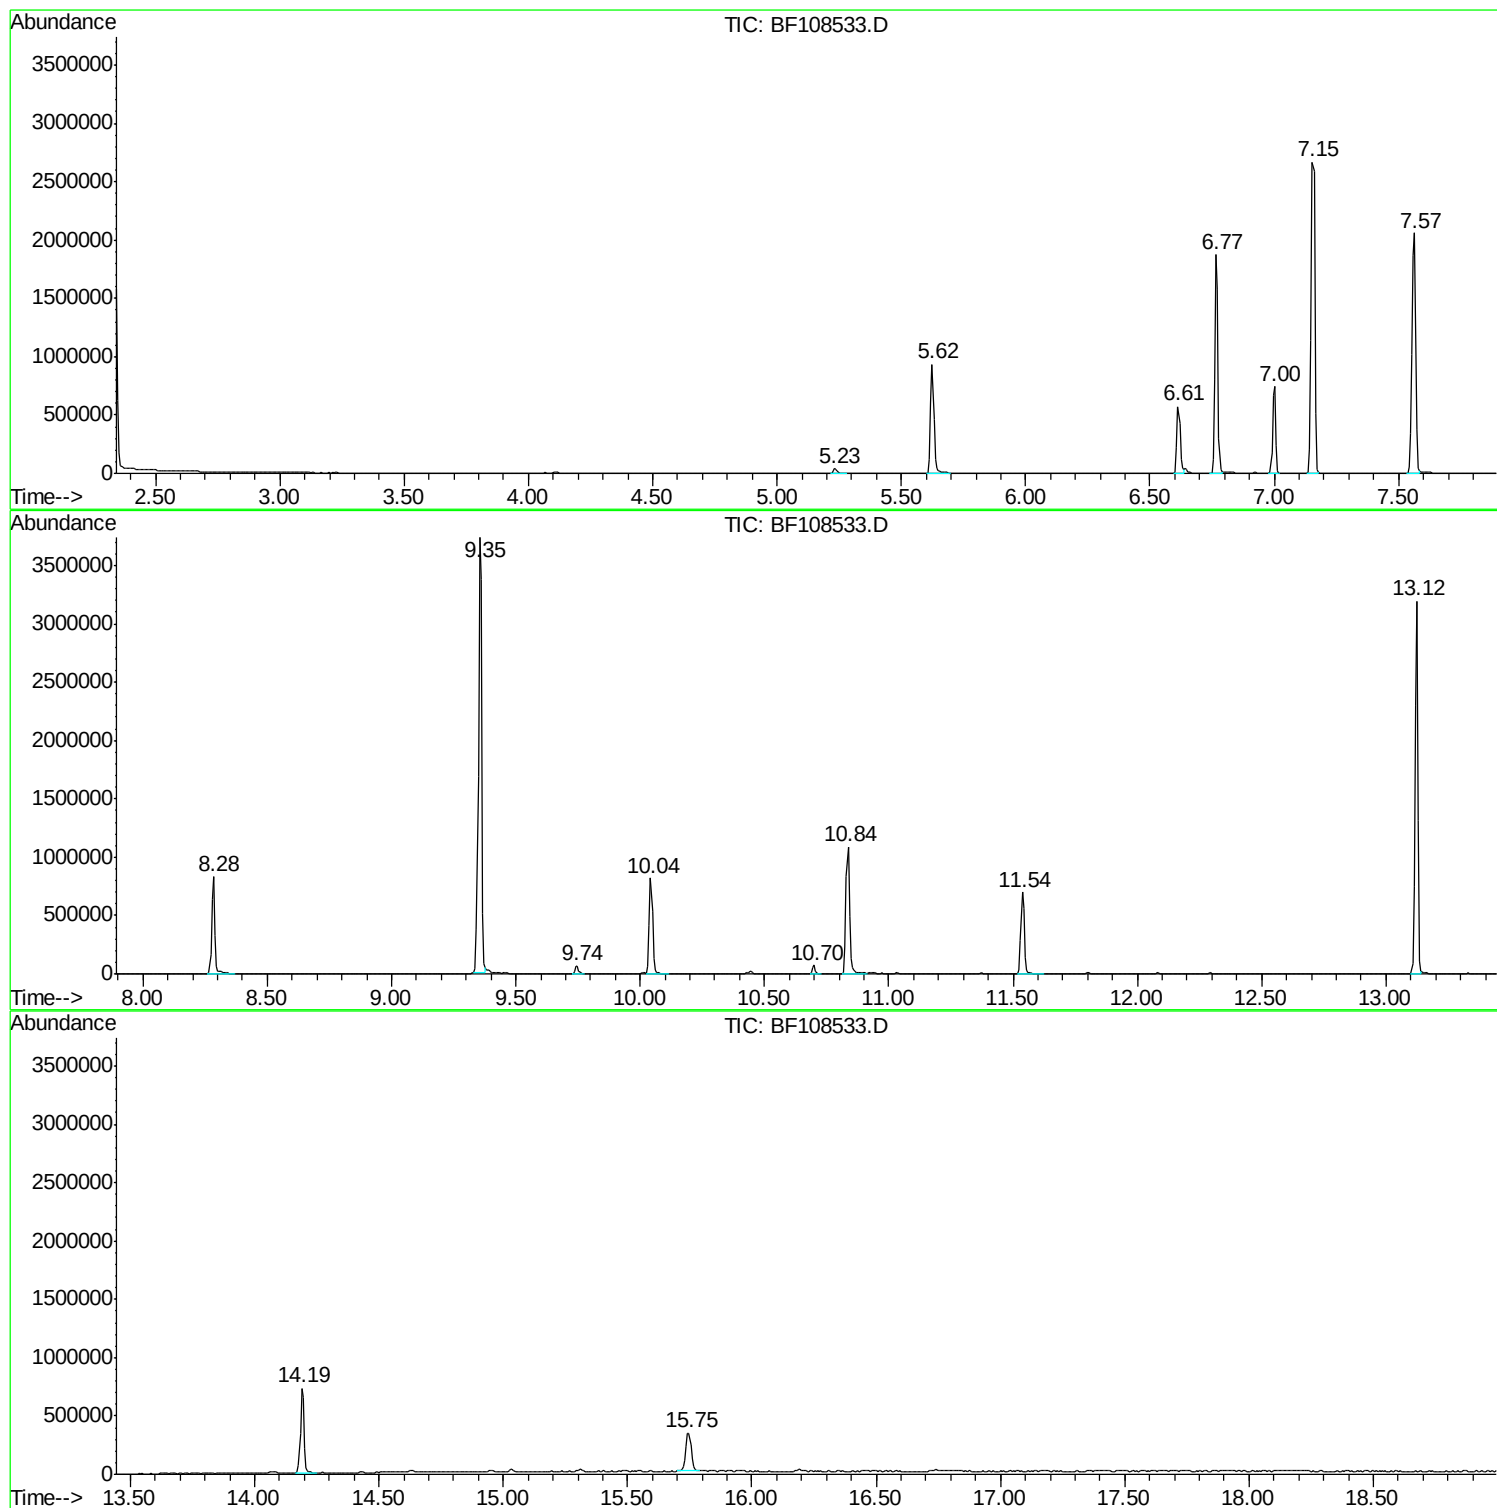

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082718\
Data File : BF108533.D
Acq On : 28 Aug 2018 2:22
Operator : JU/SJ
Sample : J4659-06
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082218-SIDI-E-D-S










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.77 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.77	50.92 ng	1668290	1,4-Dichlorobenzene-d4	7.00

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
2		5-Aminoindole	132	C8H8N2	005192-03-0	12
3		(5-Methyl-2-pyridyl)acetonitrile	132	C8H8N2	1000241-93-9	10
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9

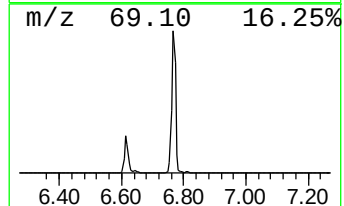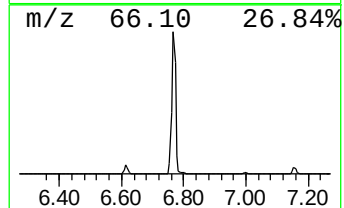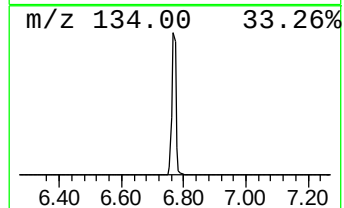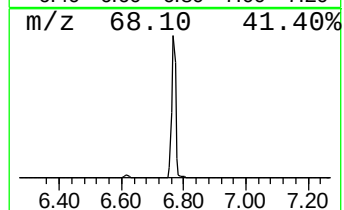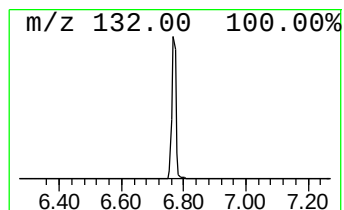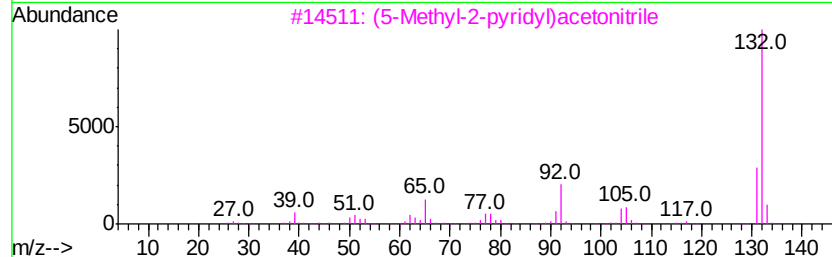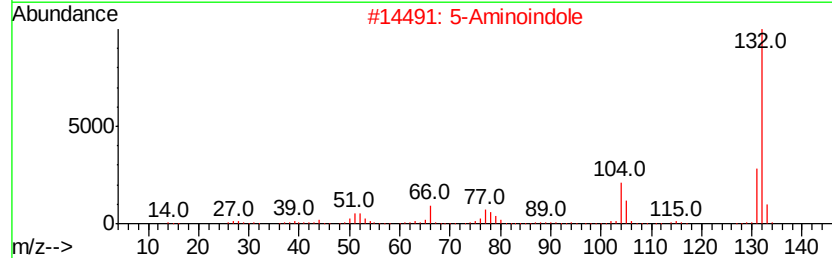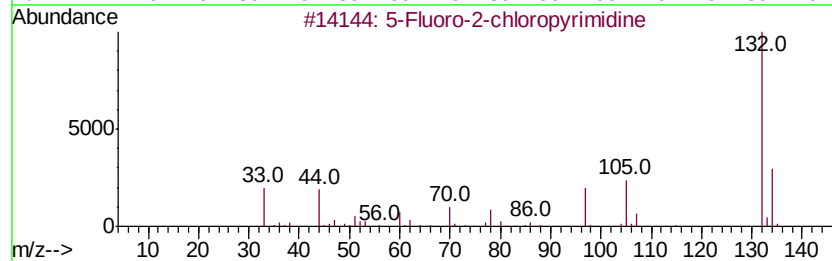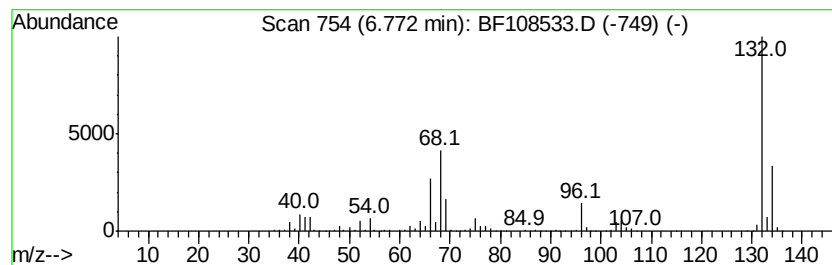

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082718\
Data File : BF108533.D
Acq On : 28 Aug 2018 2:22
Operator : JU/SJ
Sample : J4659-06
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082218-SIDI-E-D-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.77	6.77	50.9	ng	1668290	1	7.00	655278	20.0