


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082718\
 Data File : BF108497.D
 Acq On : 27 Aug 2018 9:19
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 22 11:01:45 2018

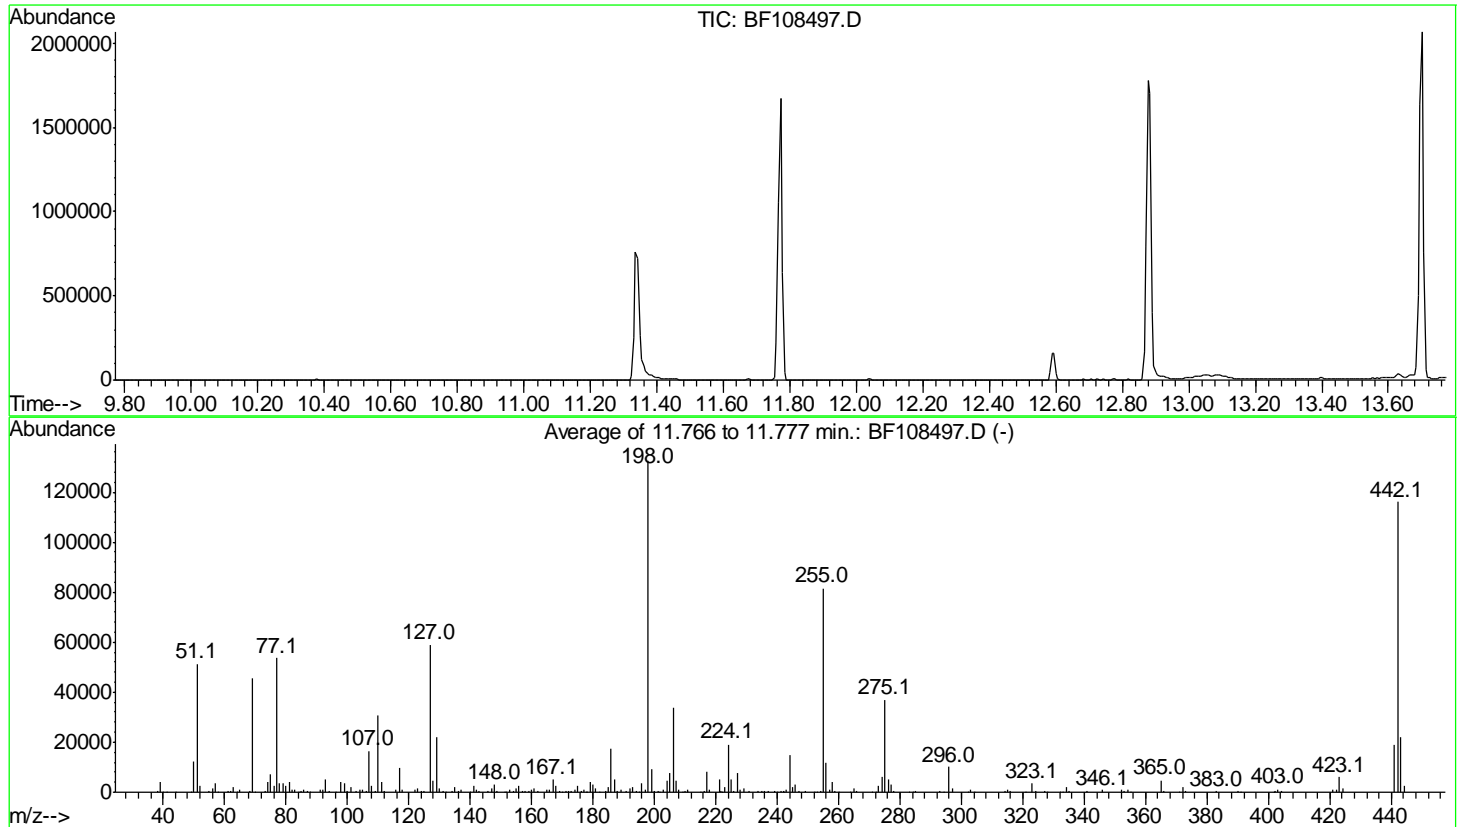

AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	51186	PASS
68	69	0.00	2	1.5	691	PASS
69	198	0.00	100	34.3	45400	PASS
70	69	0.00	2	0.6	260	PASS
127	198	10	80	44.6	59080	PASS
197	198	0.00	2	0.7	862	PASS
198	198	100	100	100.0	132549	PASS
199	198	5	9	6.8	9003	PASS
275	198	10	60	27.8	36914	PASS
365	198	1	100	3.6	4732	PASS
441	198	0.01	100	14.1	18749	PASS
442	198	50	100	87.6	116056	PASS
443	442	15	24	18.8	21842	PASS