


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082718\
 Data File : BF108524.D
 Acq On : 27 Aug 2018 21:52
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 22 11:01:45 2018

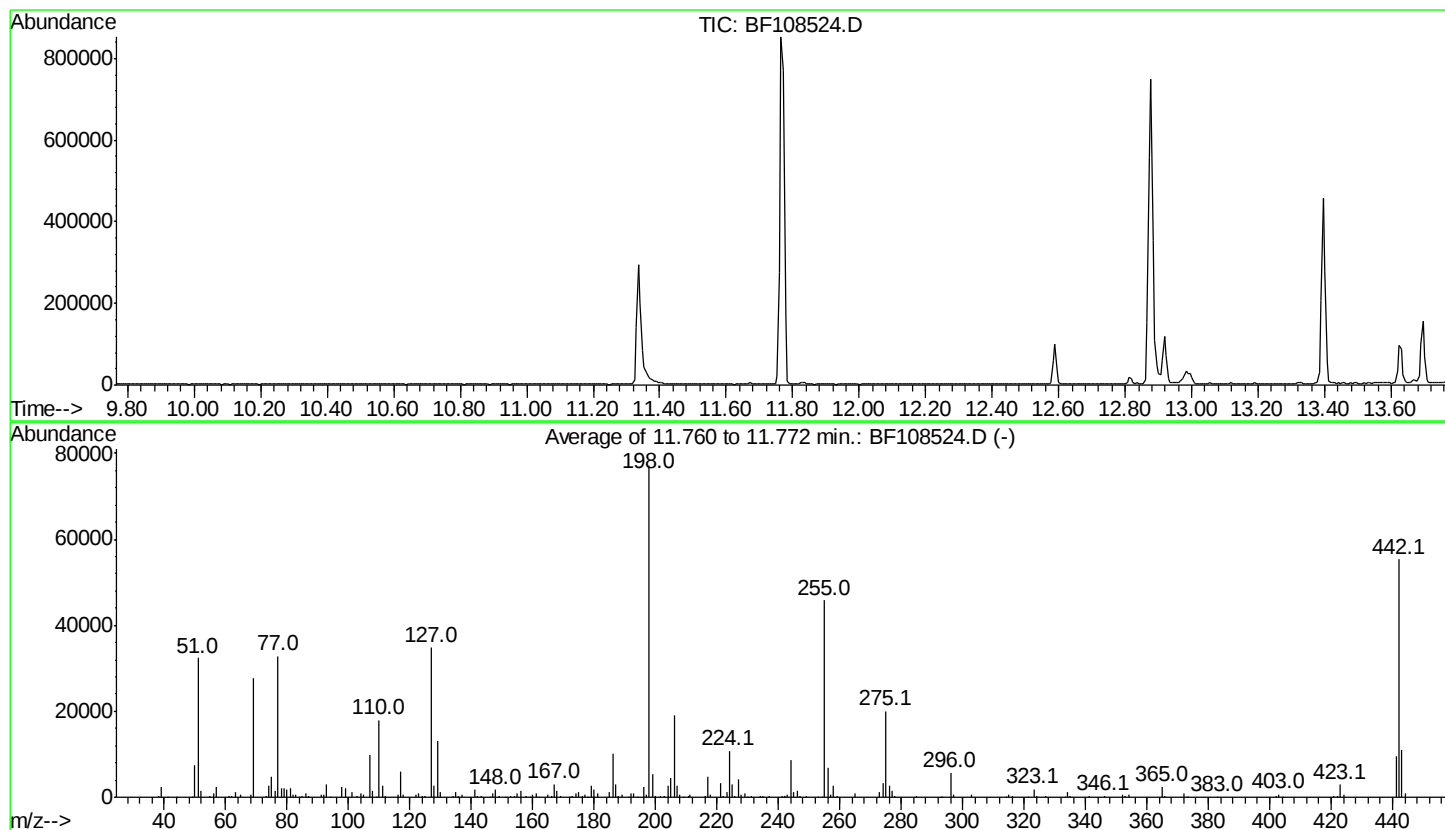

AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	32357	PASS
68	69	0.00	2	1.7	470	PASS
69	198	0.00	100	35.9	27690	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.1	34760	PASS
197	198	0.00	2	0.8	587	PASS
198	198	100	100	100.0	77128	PASS
199	198	5	9	6.9	5311	PASS
275	198	10	60	26.0	20023	PASS
365	198	1	100	3.2	2457	PASS
441	198	0.01	100	12.5	9618	PASS
442	198	50	100	71.7	55315	PASS
443	442	15	24	19.8	10952	PASS