
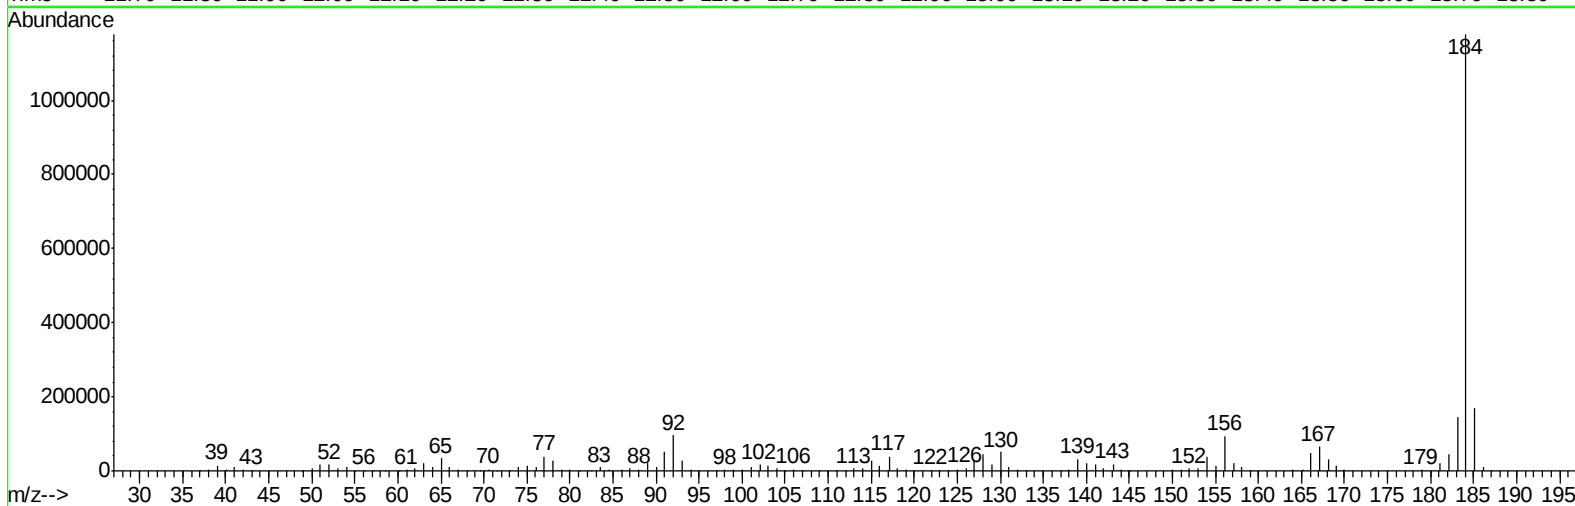


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082719\
Data File : BF116577.D
Acq On : 27 Aug 2019 9:01
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 08:44:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF082319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 23 13:38:31 2019
Response via : Initial Calibration

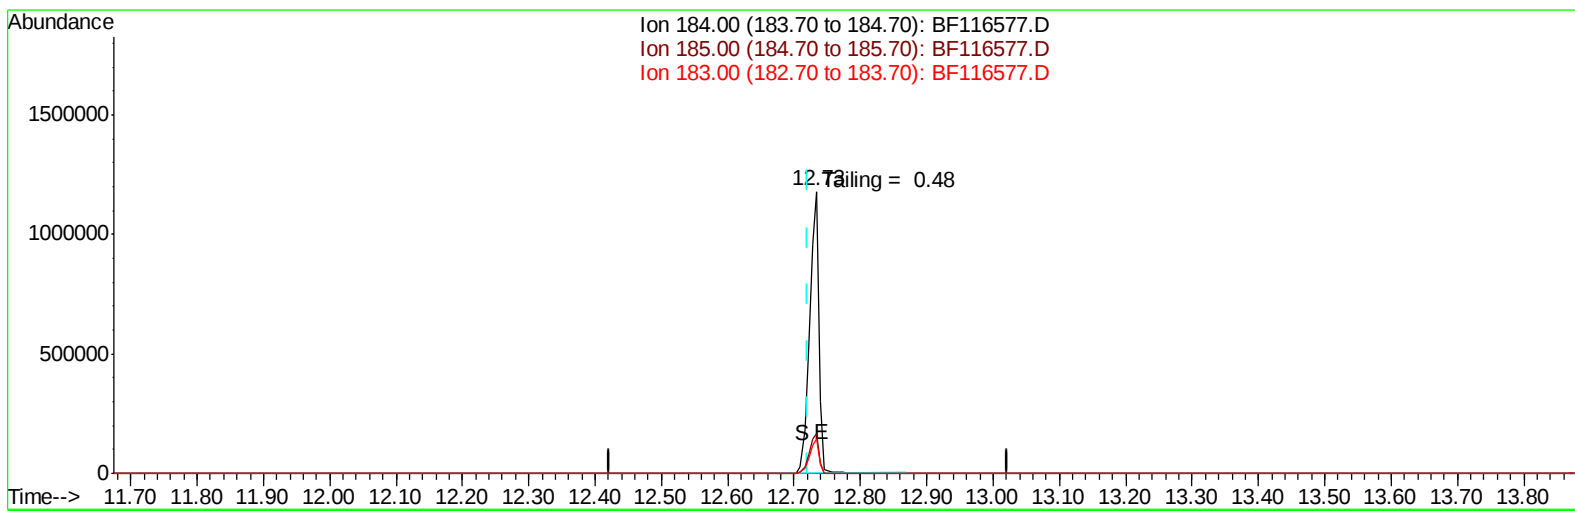

TIC: BF116577.D

(77) Benzidine



12.733min (+0.012) 171118.30ng

response 1149739

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	14.24
183.00	12.20	12.39
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082719\
Data File : BF116577.D
Acq On : 27 Aug 2019 9:01
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 08:44:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF082319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 23 13:38:31 2019
Response via : Initial Calibration

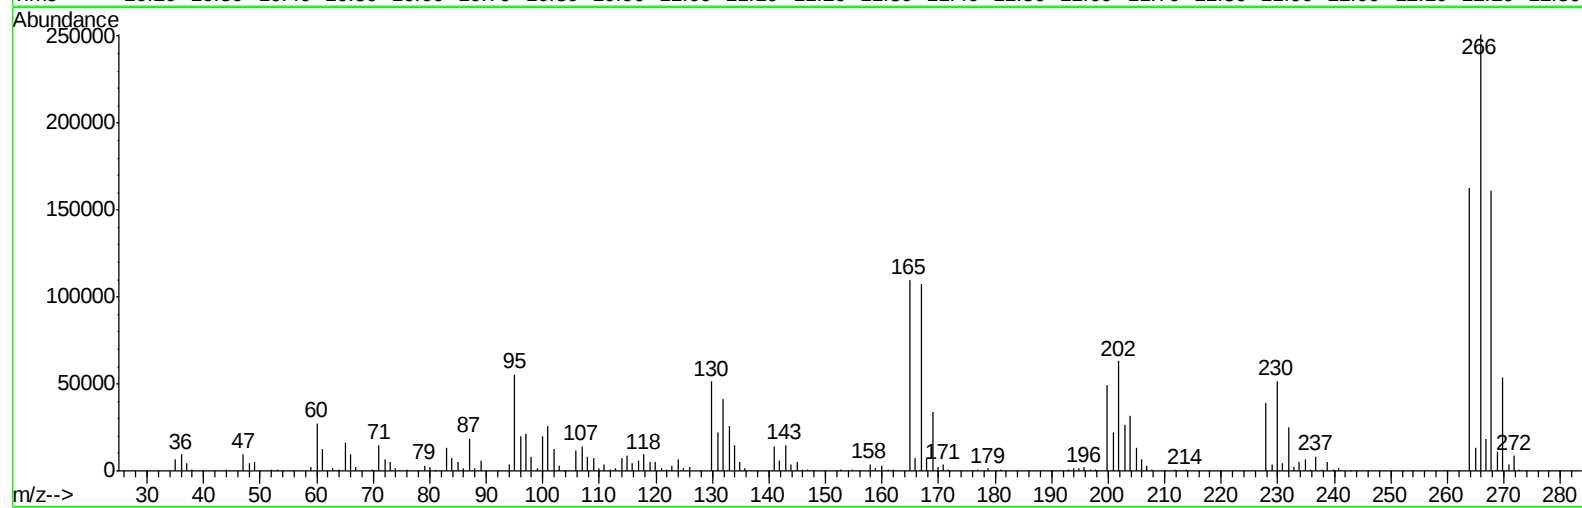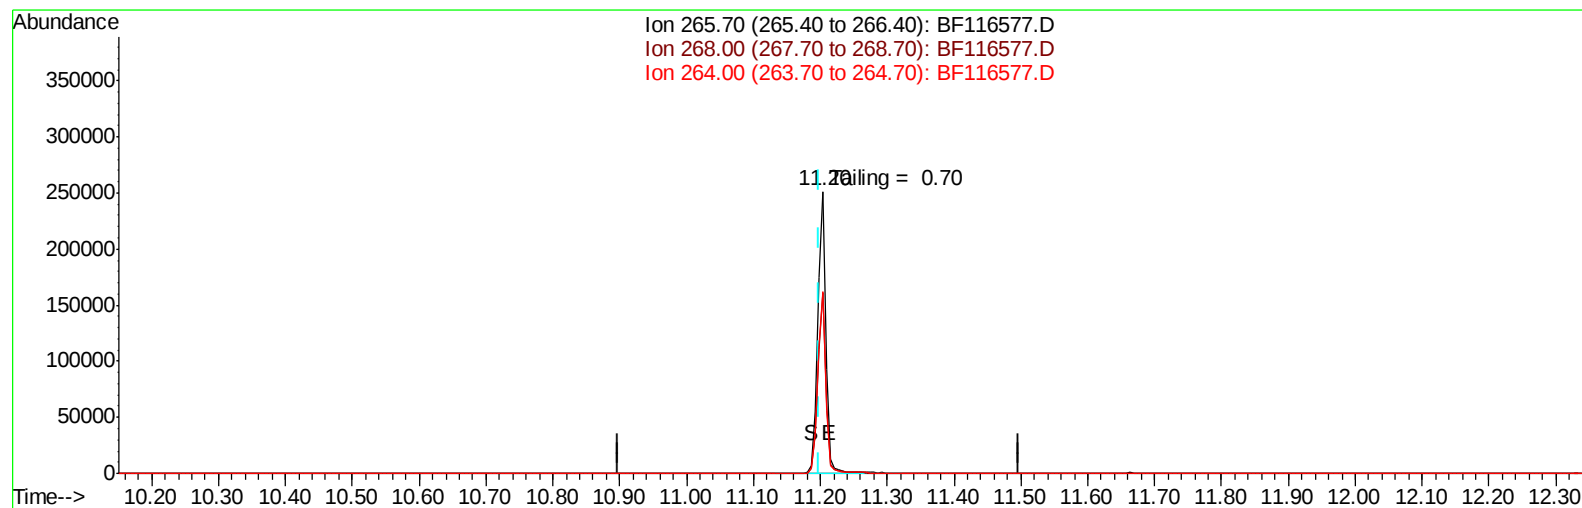

TIC: BF116577.D

(70) Pentachlorophenol (C)

11.204min (+0.006) 93086.54ng

response 217896

Ion	Exp%	Act%
265.70	100	100
268.00	63.40	64.13
264.00	62.50	64.72
0.00	0.00	0.00