
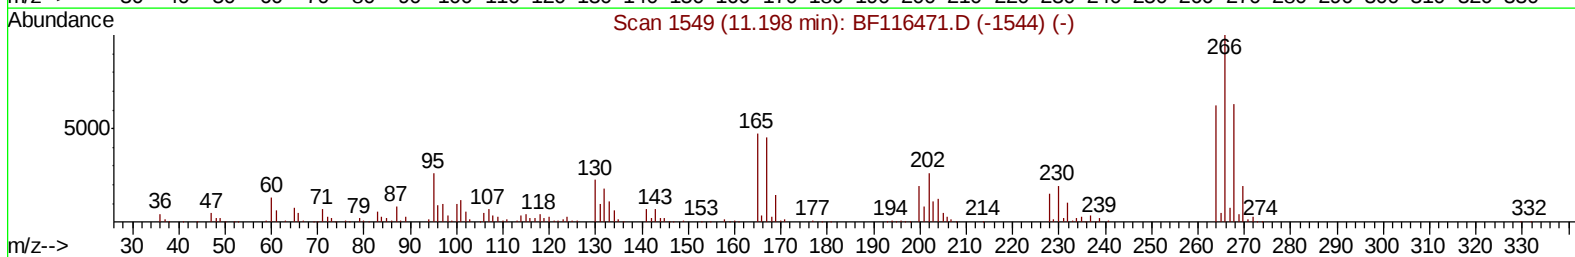
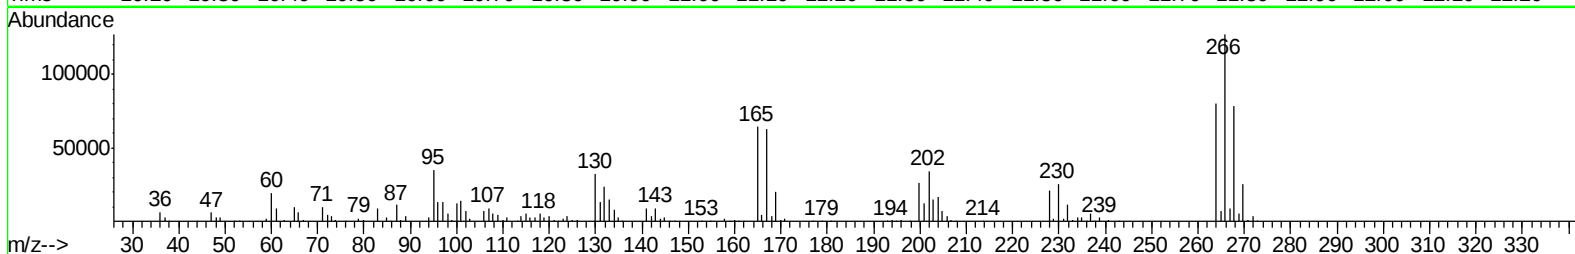


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082719\
Data File : BF116587.D
Acq On : 27 Aug 2019 16:38
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 08:52:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF082319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 23 13:38:31 2019
Response via : Initial Calibration

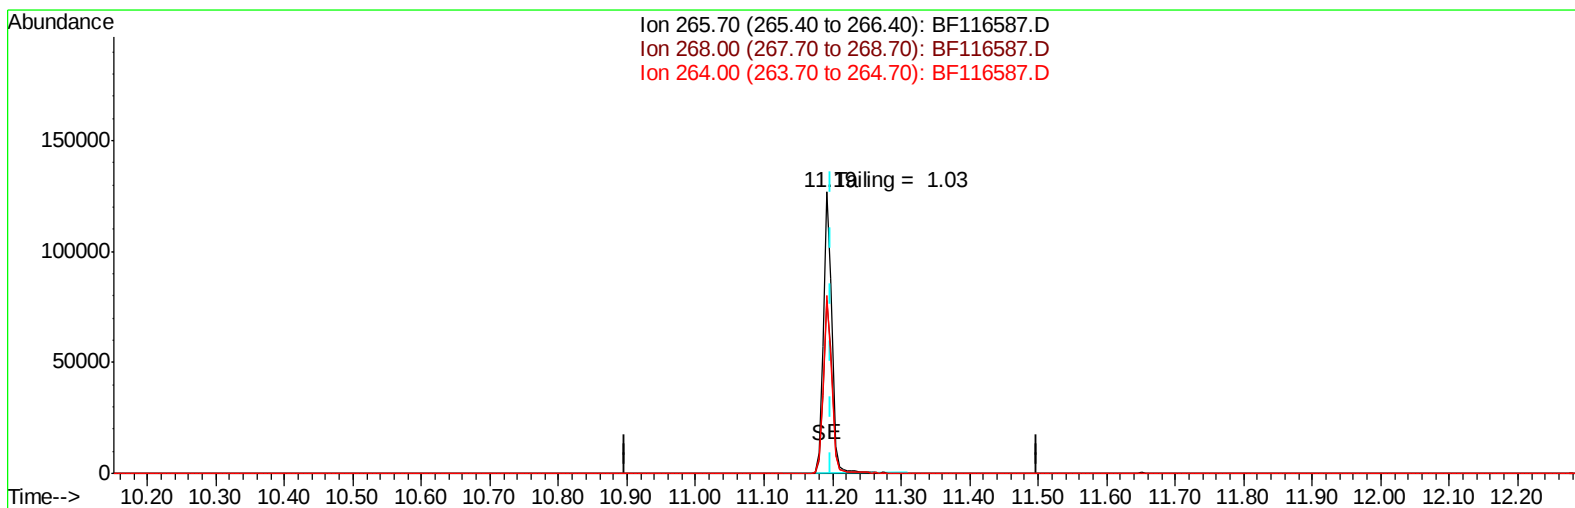

TIC: BF116587.D

(70) Pentachlorophenol (C)




11.192min (-0.006) 57119.76ng

response 107428

Ion	Exp%	Act%
265.70	100	100
268.00	63.40	61.59
264.00	62.50	63.12
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082719\
Data File : BF116587.D
Acq On : 27 Aug 2019 16:38
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 08:52:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF082319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 23 13:38:31 2019
Response via : Initial Calibration

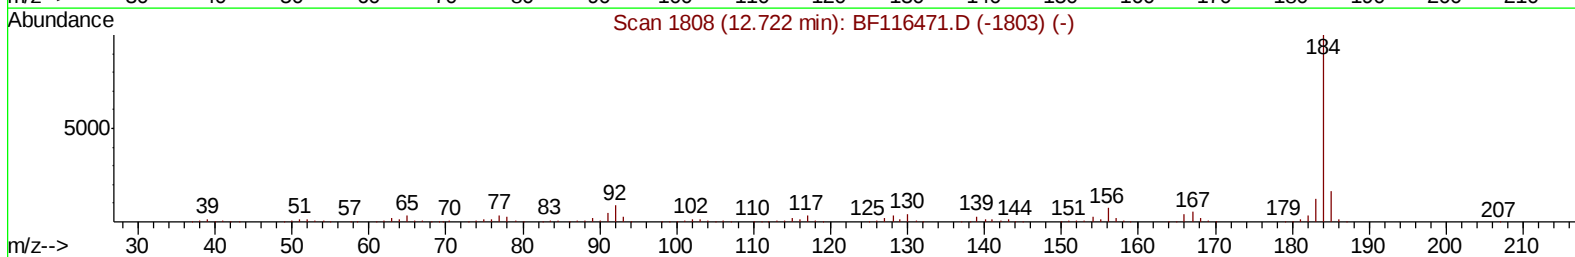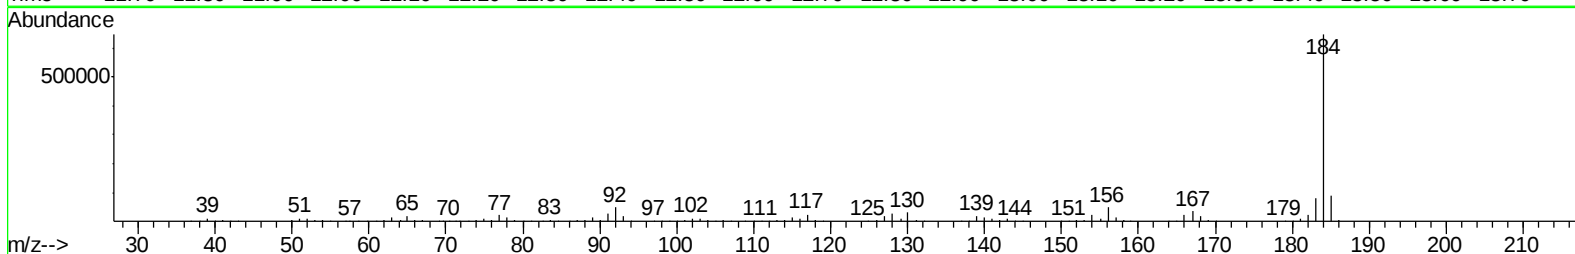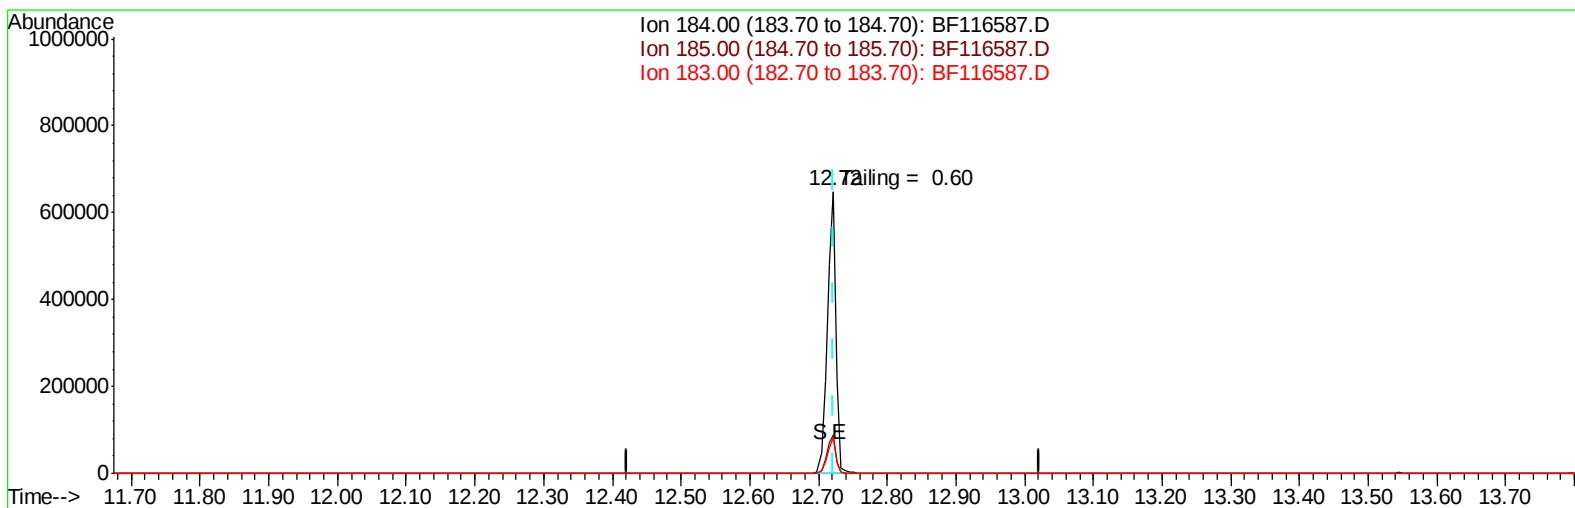

TIC: BF116587.D

(77) Benzidine

12.721min (-0.000) 41899.14ng

response 578210

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	13.61
183.00	12.20	12.71
0.00	0.00	0.00