


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082719\
 Data File : BF116577.D
 Acq On : 27 Aug 2019 9:01
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 23 13:38:31 2019

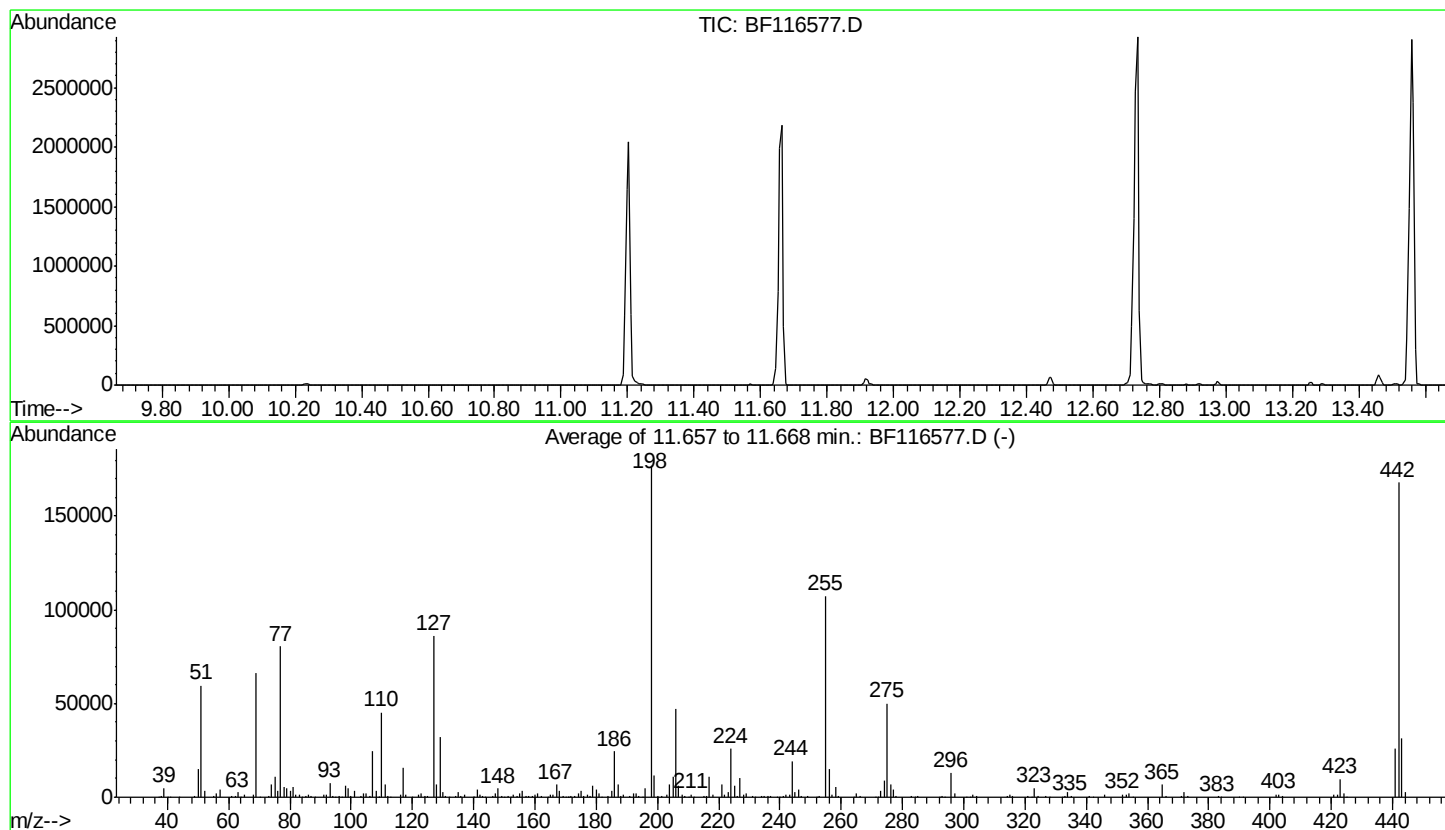

AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	59663	PASS
68	69	0.00	2	1.7	1140	PASS
69	198	0.00	100	37.6	66573	PASS
70	69	0.00	2	0.5	311	PASS
127	198	10	80	48.8	86416	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	176981	PASS
199	198	5	9	6.6	11765	PASS
275	198	10	60	28.2	49949	PASS
365	198	1	100	3.7	6622	PASS
441	198	0.01	100	14.8	26176	PASS
442	198	50	100	94.8	167842	PASS
443	442	15	24	18.6	31266	PASS