


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082719\
 Data File : BF116587.D
 Acq On : 27 Aug 2019 16:38
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 23 13:38:31 2019

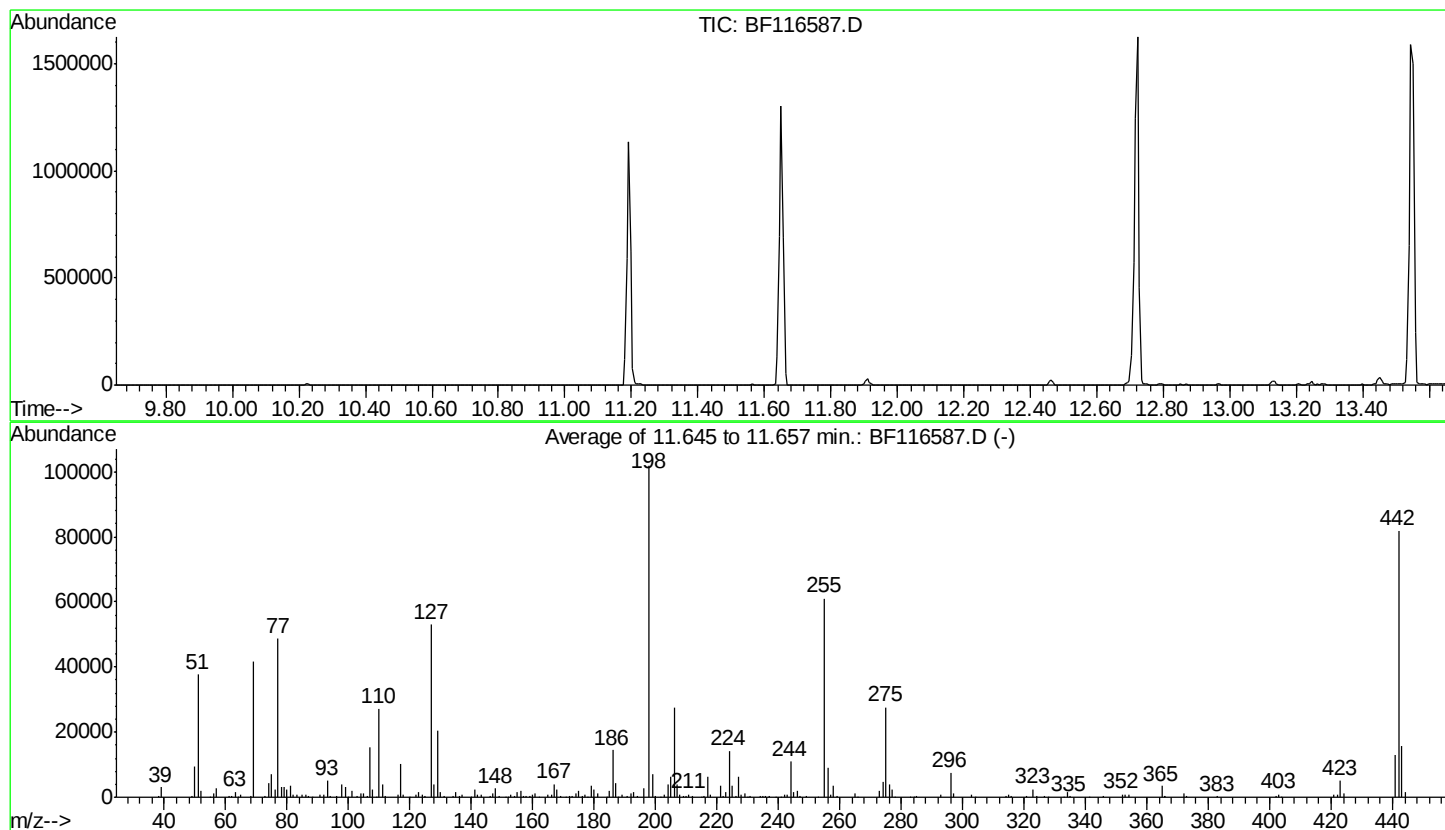

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	37602	PASS
68	69	0.00	2	1.1	461	PASS
69	198	0.00	100	40.9	41680	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.0	52970	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	101858	PASS
199	198	5	9	7.0	7086	PASS
275	198	10	60	27.0	27541	PASS
365	198	1	100	3.4	3510	PASS
441	198	0.01	100	12.8	13087	PASS
442	198	50	100	80.4	81877	PASS
443	442	15	24	19.3	15835	PASS