




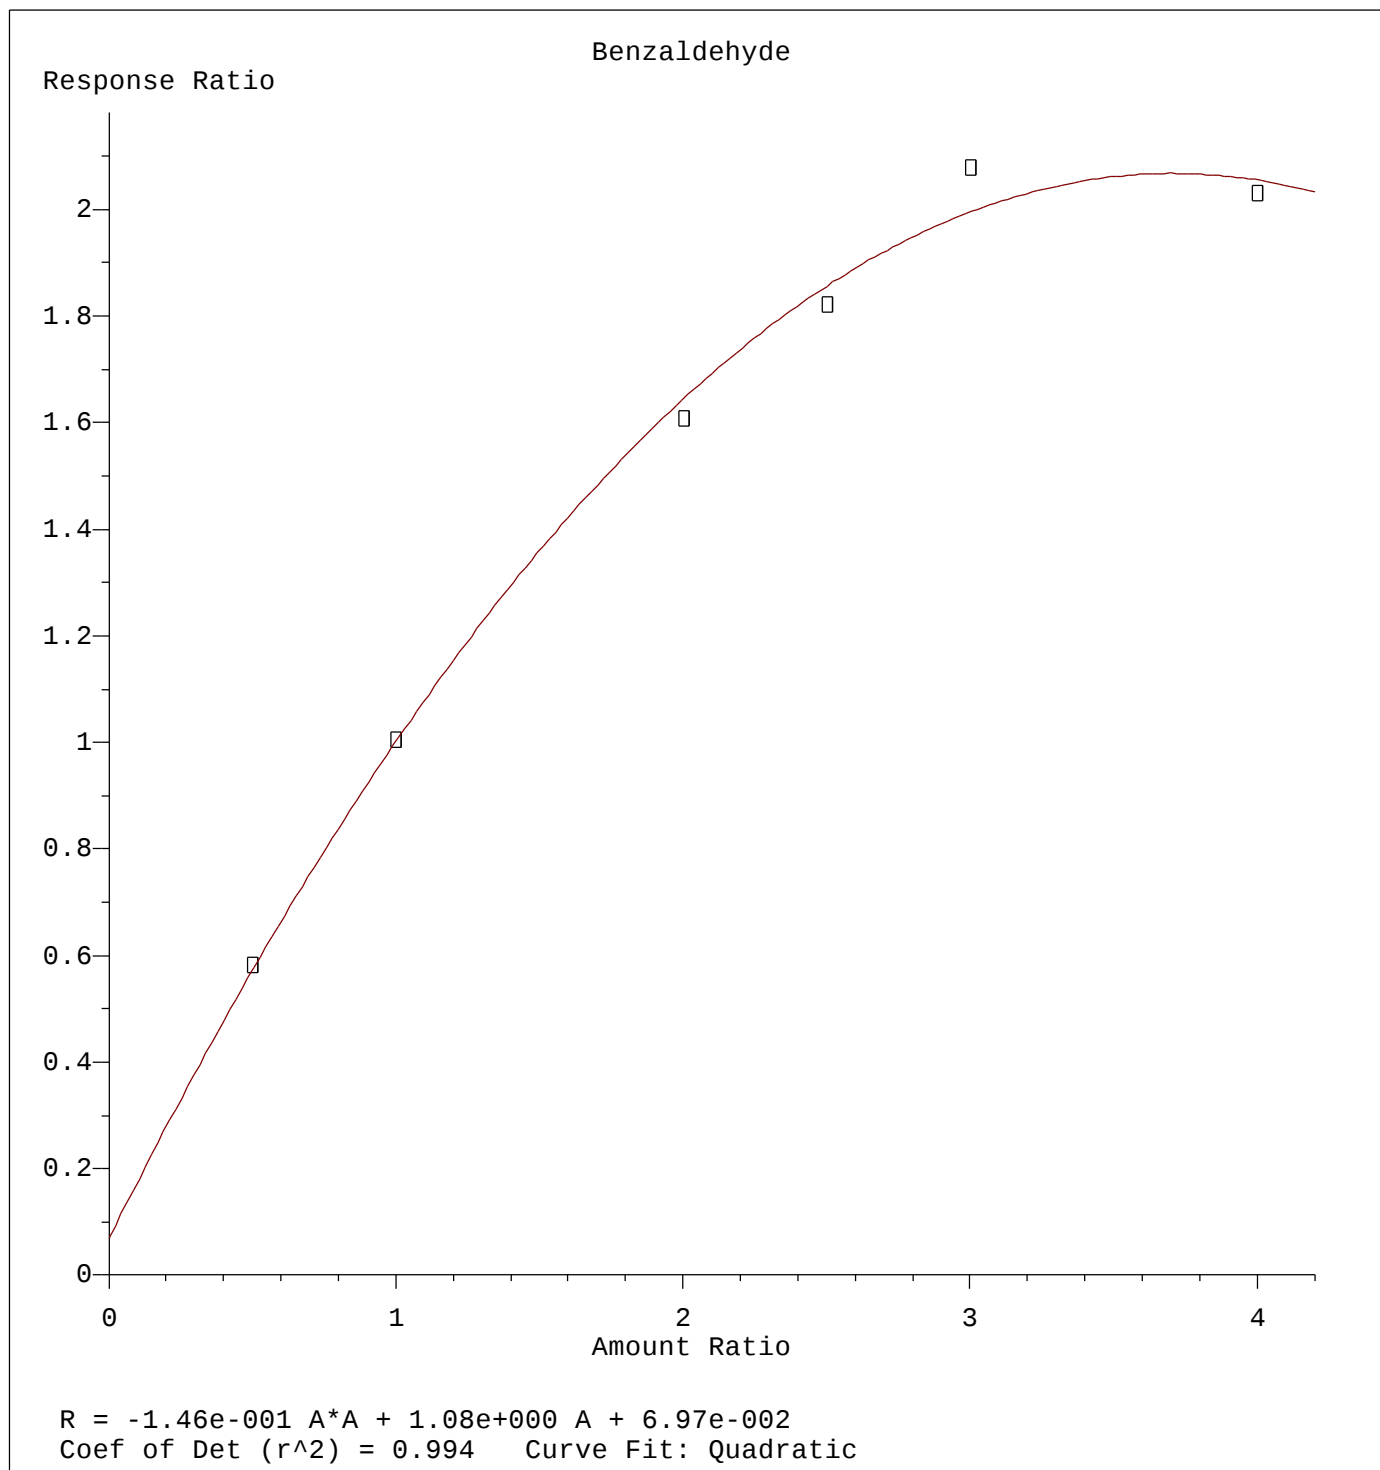

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082720.M
Calibration Table Last Updated: Fri Aug 28 12:42:39 2020

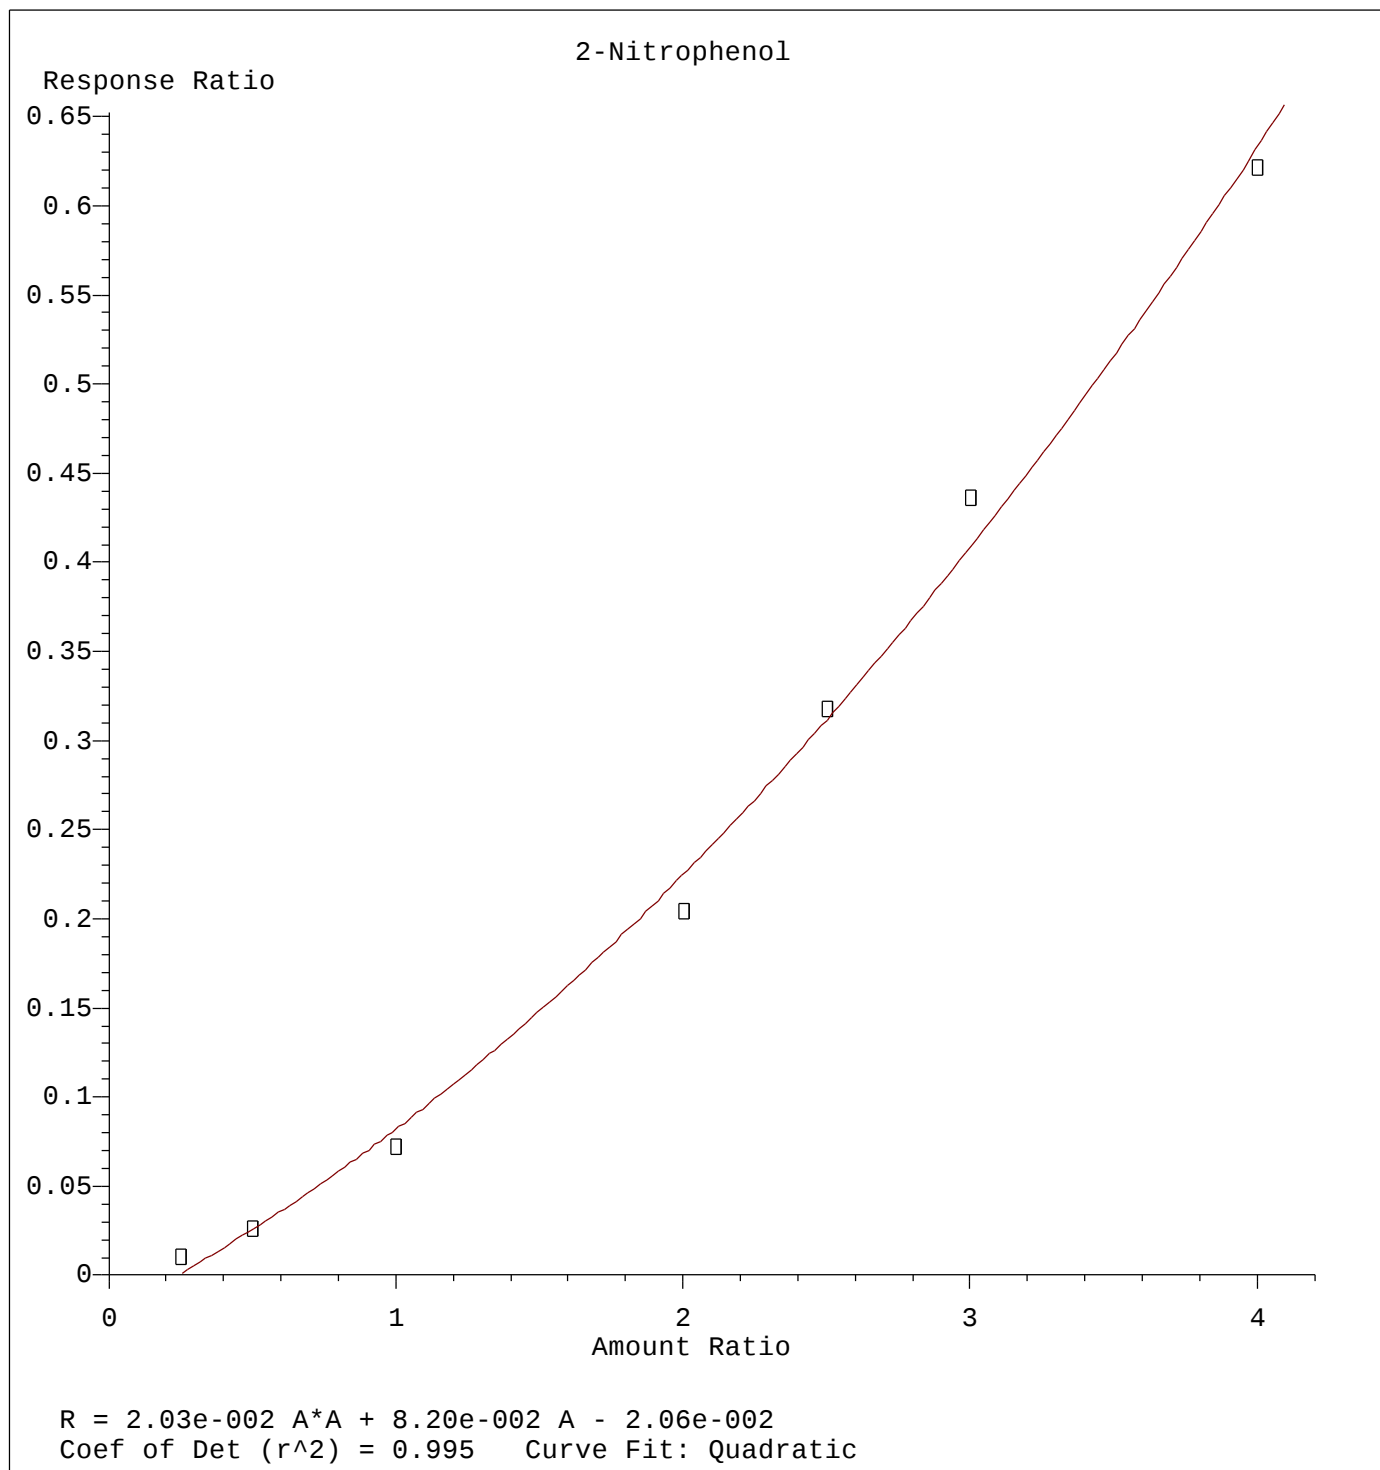


Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082720.M
Calibration Table Last Updated: Fri Aug 28 12:42:39 2020

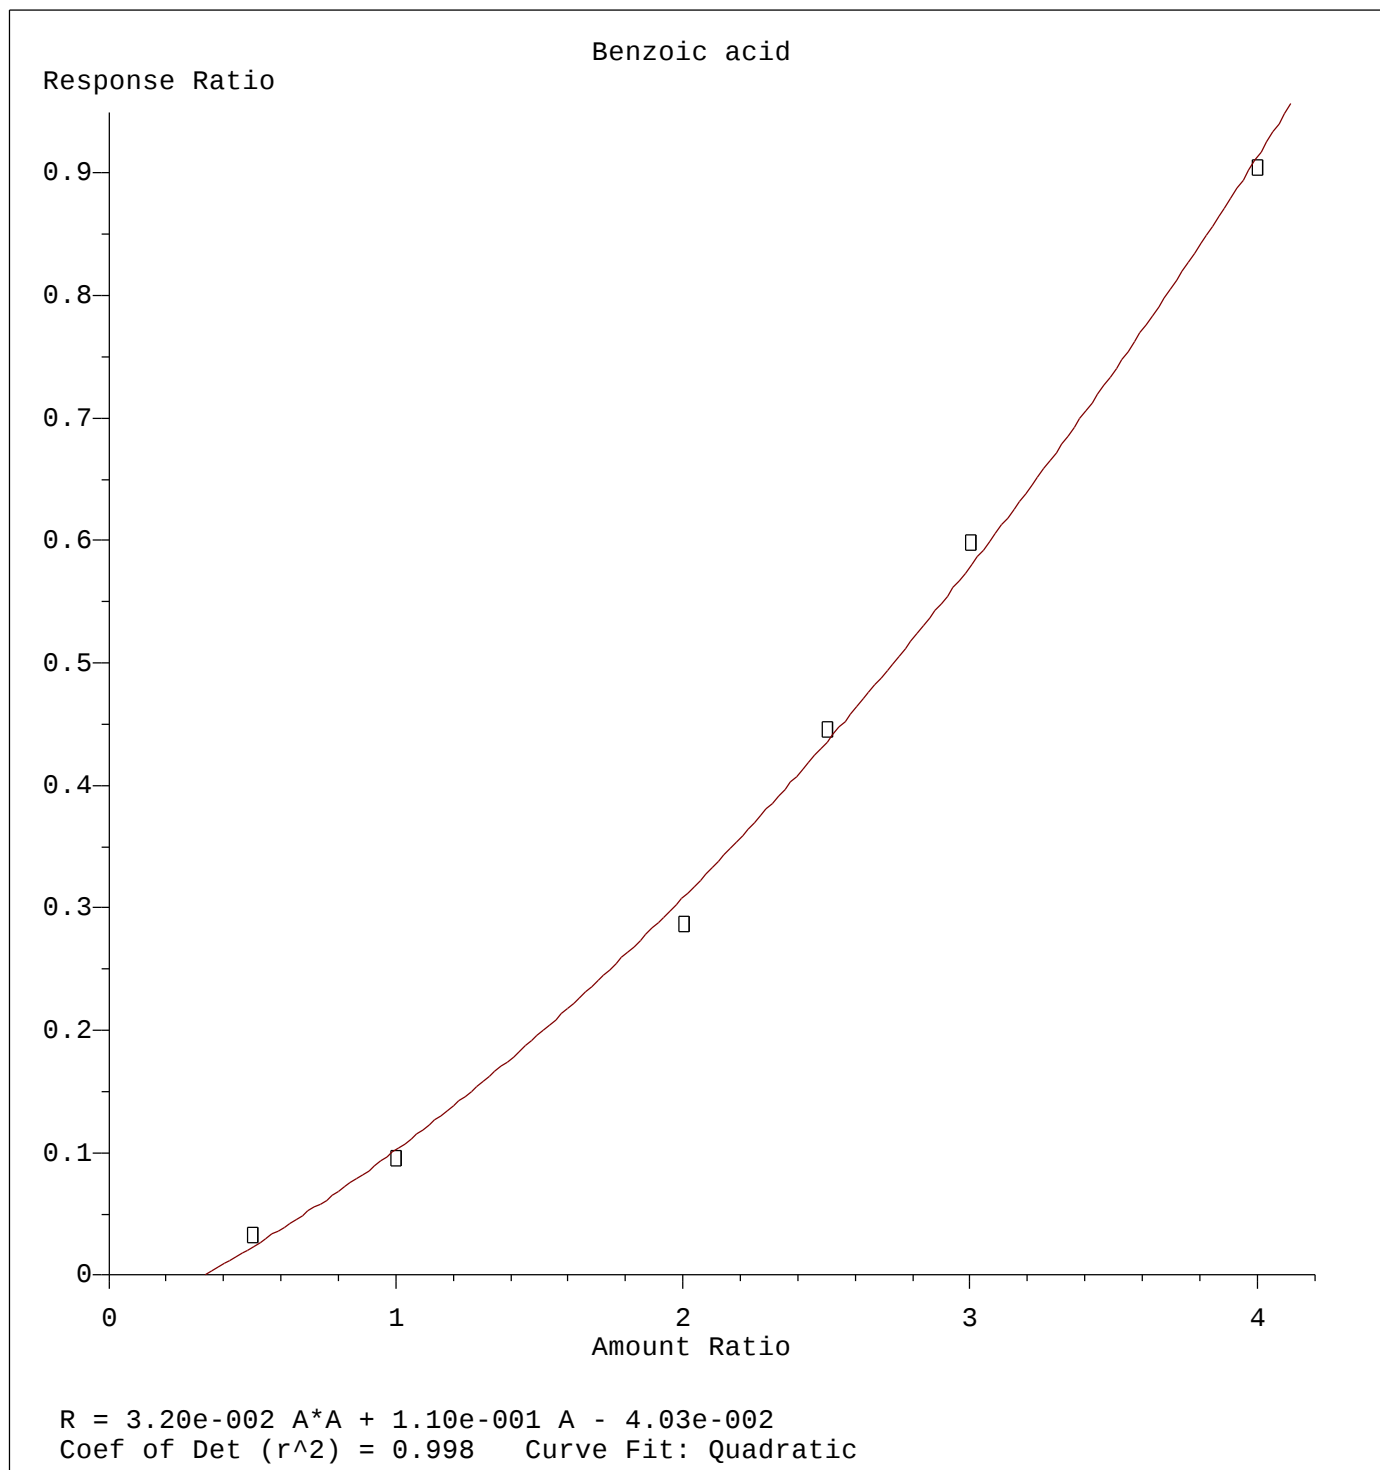

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082720.M
Calibration Table Last Updated: Fri Aug 28 12:42:39 2020

2-Nitroaniline

Response Ratio

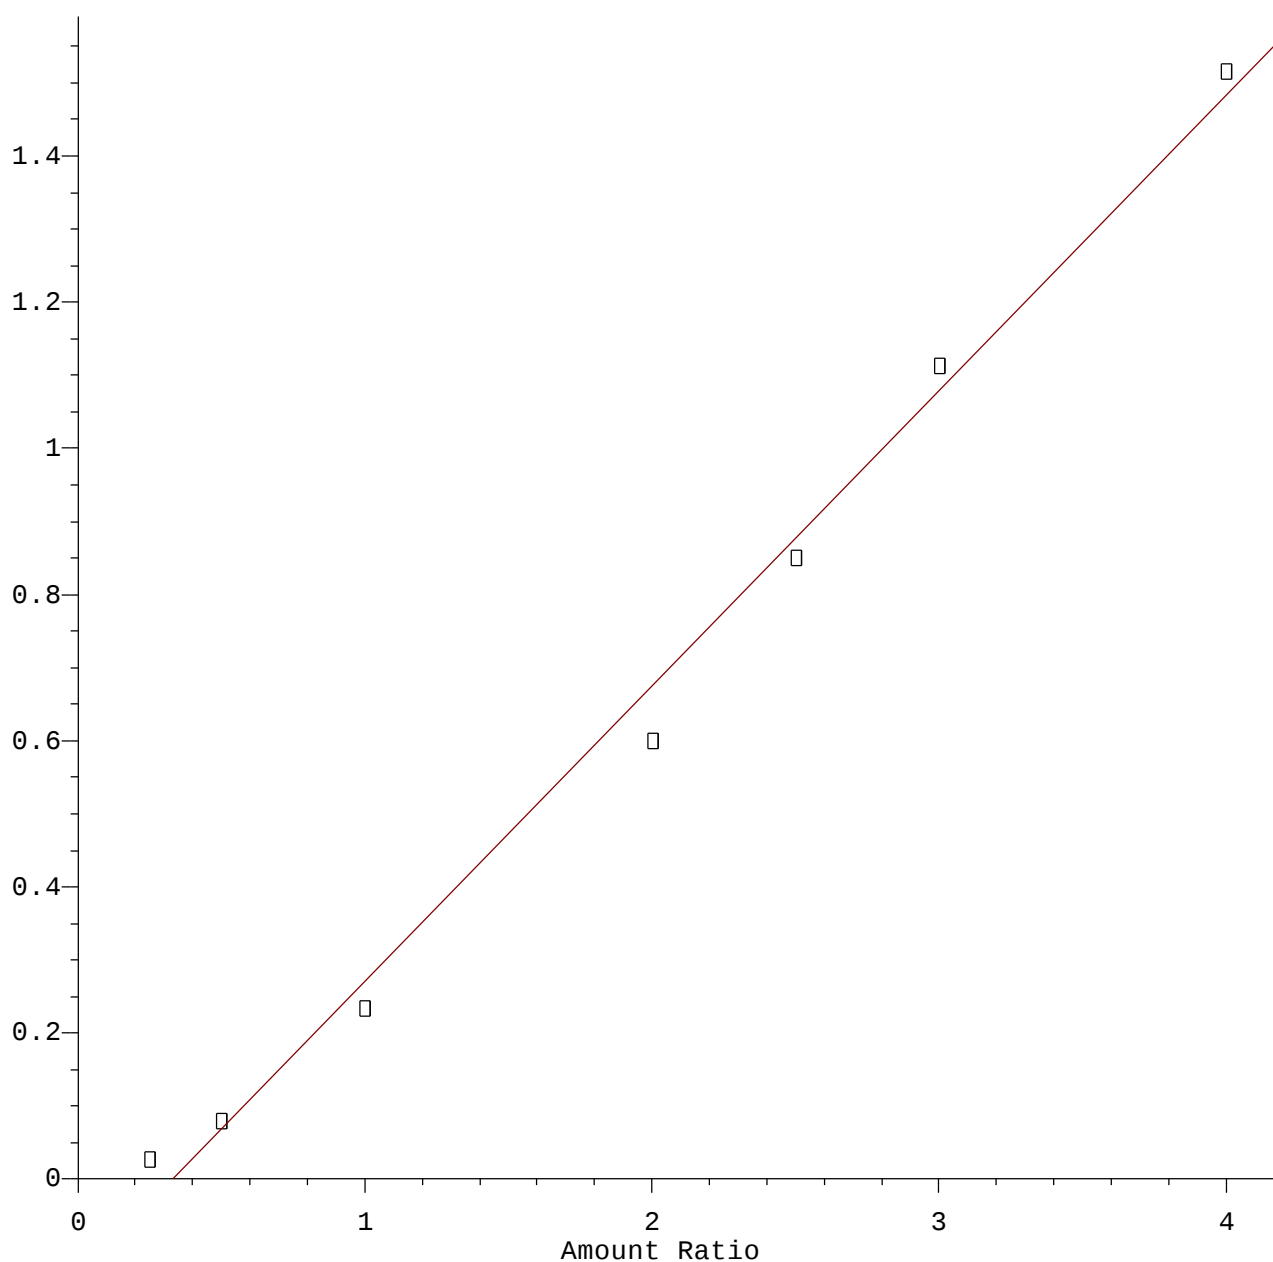


Resp Ratio = $4.04 \times 10^{-1} \times \text{Amt} - 1.34 \times 10^{-1}$
Coef of Det (r^2) = 0.993 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082720.M
Calibration Table Last Updated: Fri Aug 28 12:42:39 2020


2,6-Dinitrotoluene

Response Ratio

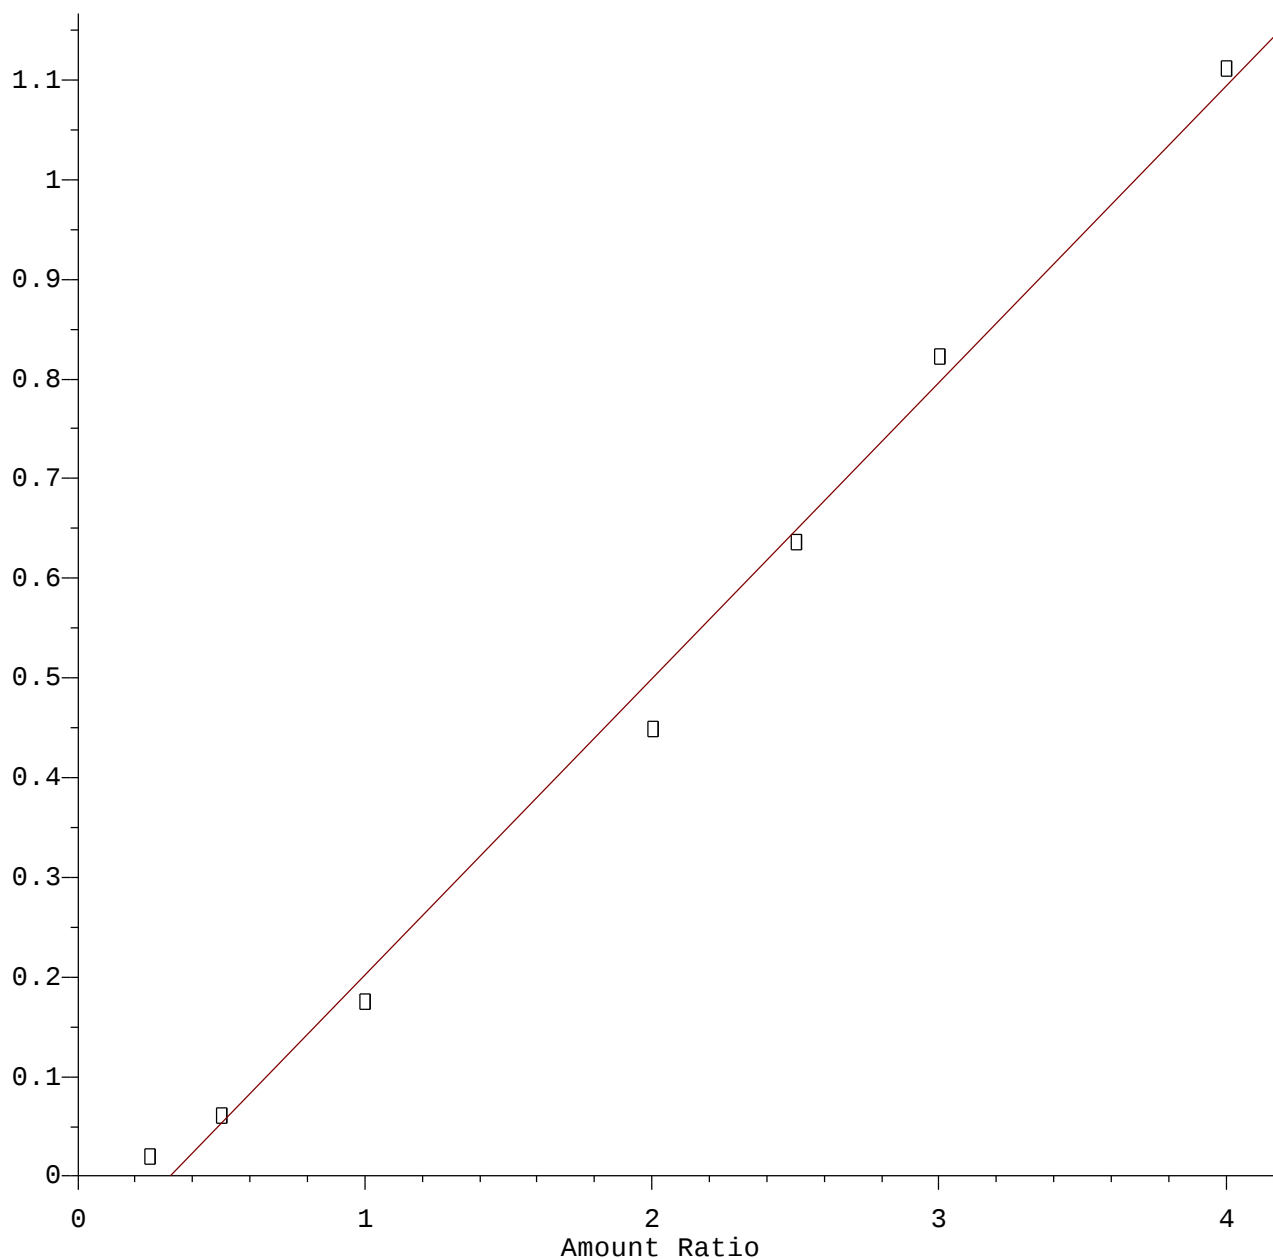


Resp Ratio = $2.97 \times 10^{-1} \times \text{Amt} - 9.54 \times 10^{-2}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear


Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082720.M
Calibration Table Last Updated: Fri Aug 28 12:42:39 2020

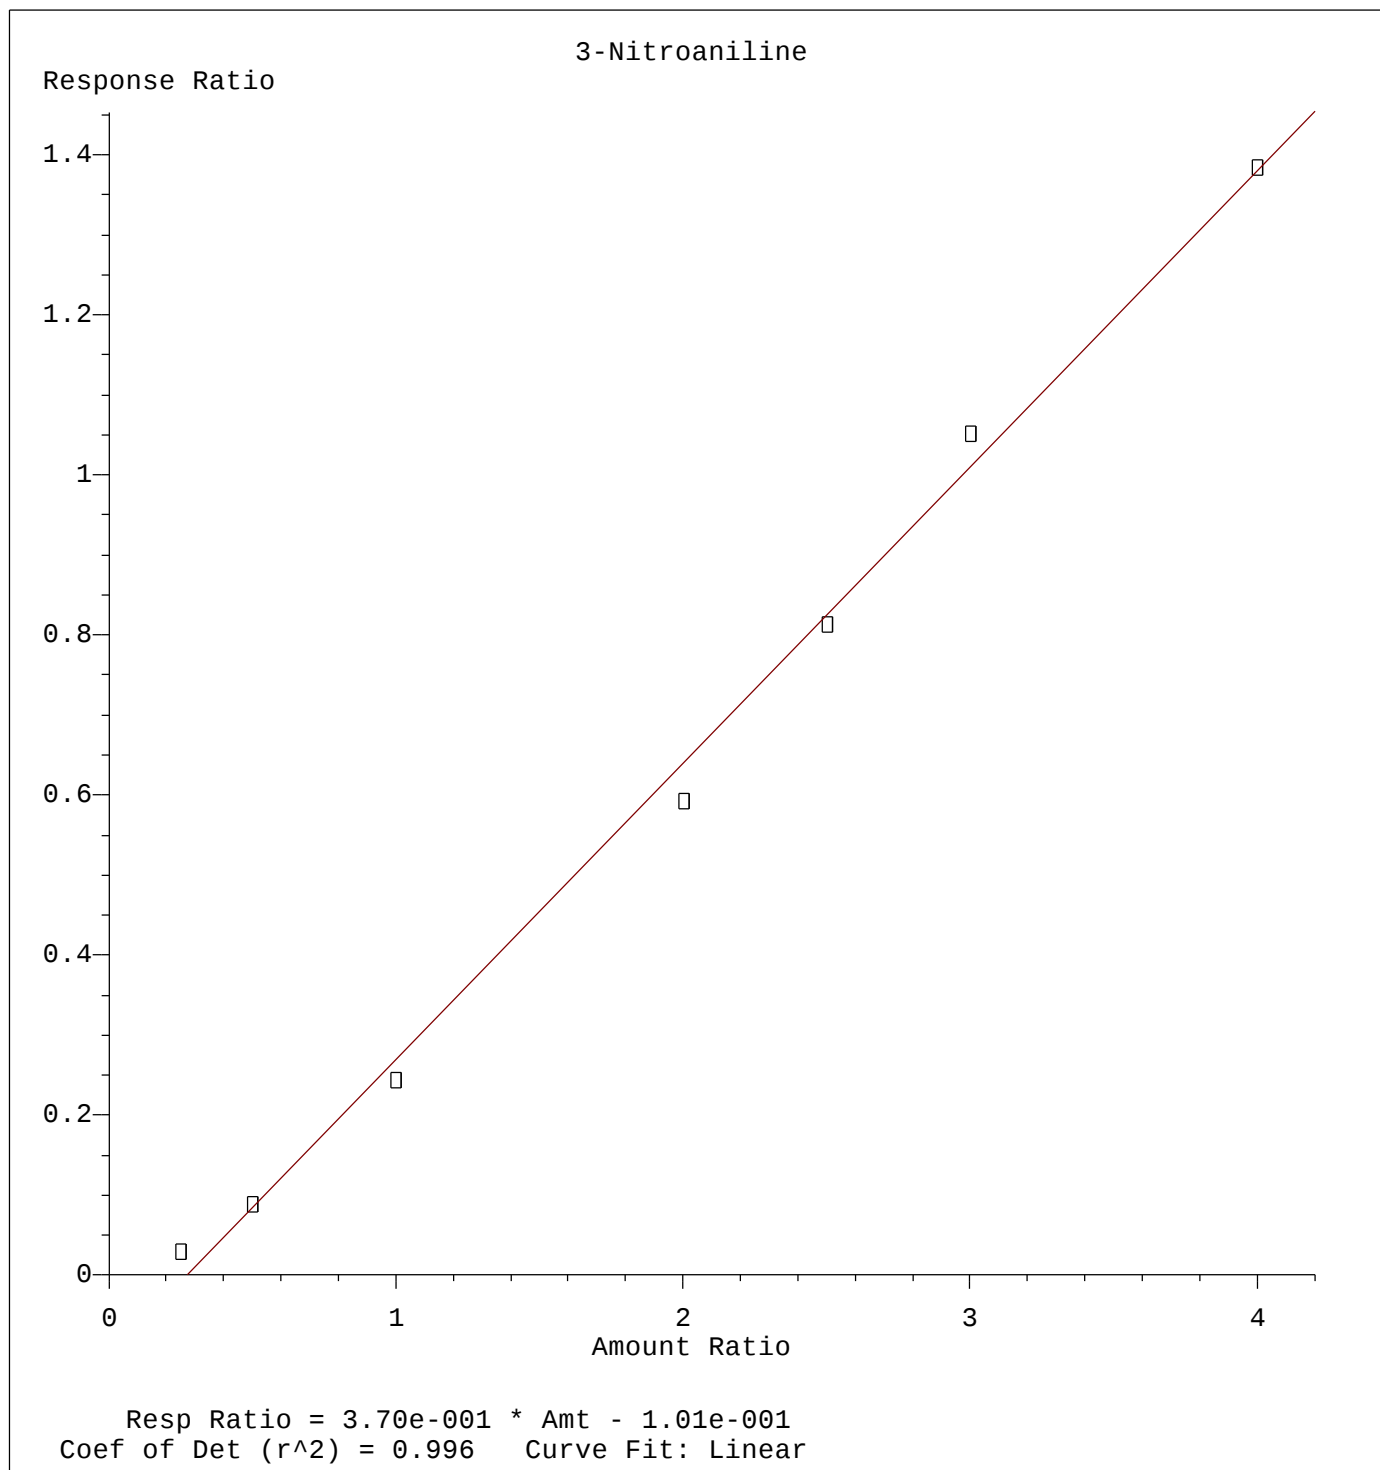

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082720.M
Calibration Table Last Updated: Fri Aug 28 12:42:39 2020

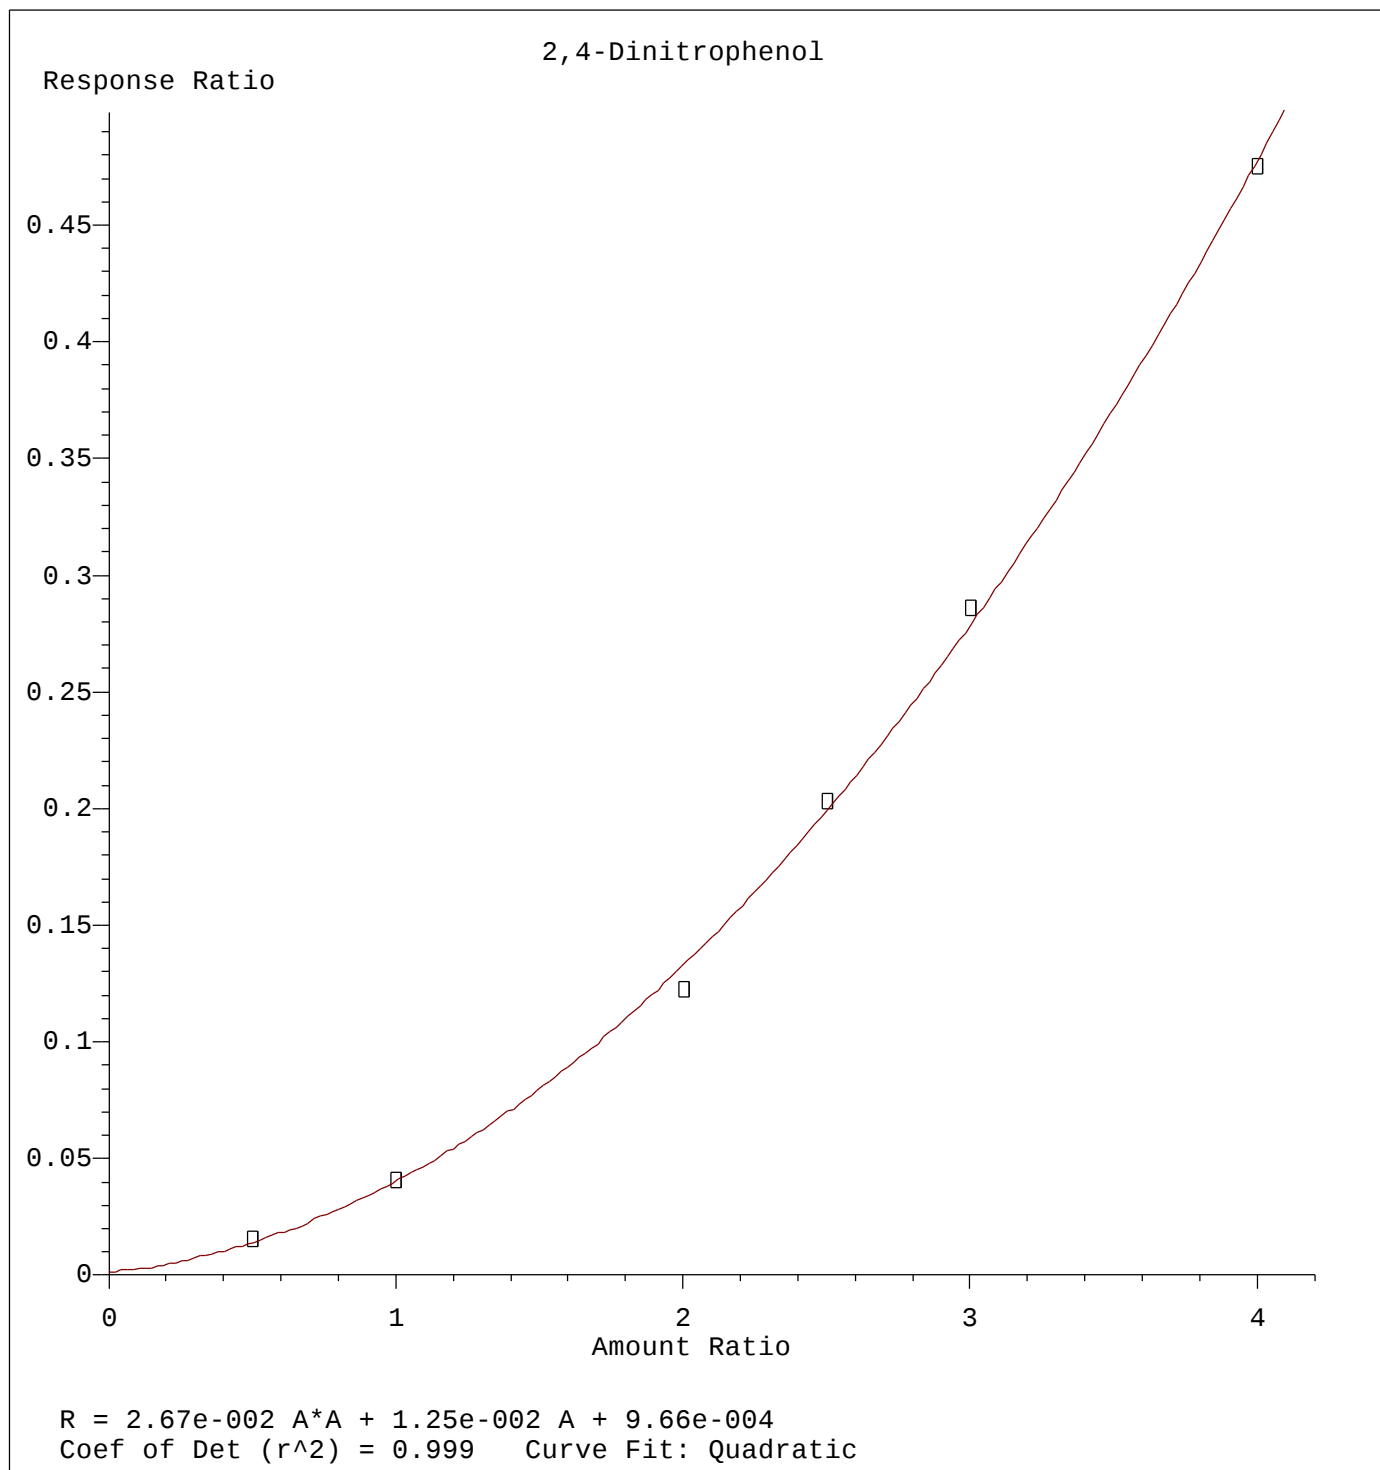


Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082720.M
Calibration Table Last Updated: Fri Aug 28 12:42:39 2020

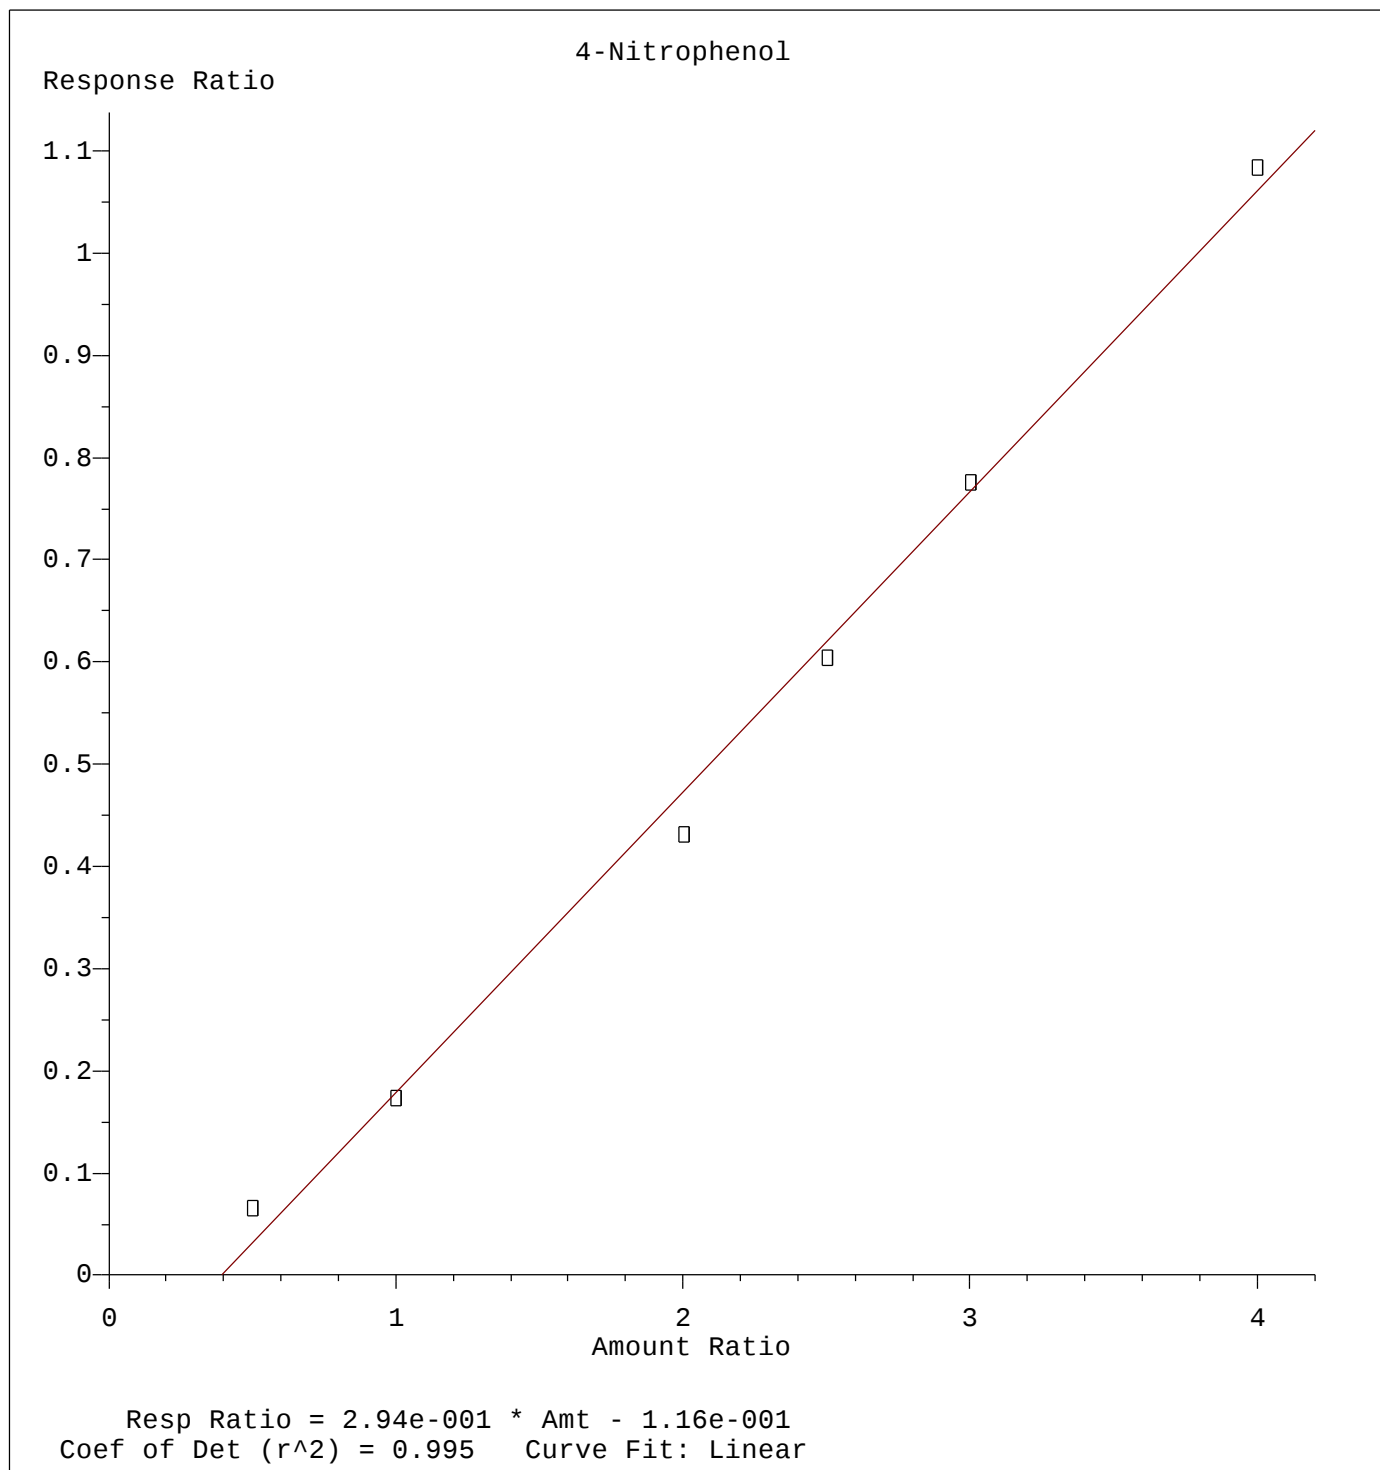

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082720.M
Calibration Table Last Updated: Fri Aug 28 12:42:39 2020


2,4-Dinitrotoluene

Response Ratio

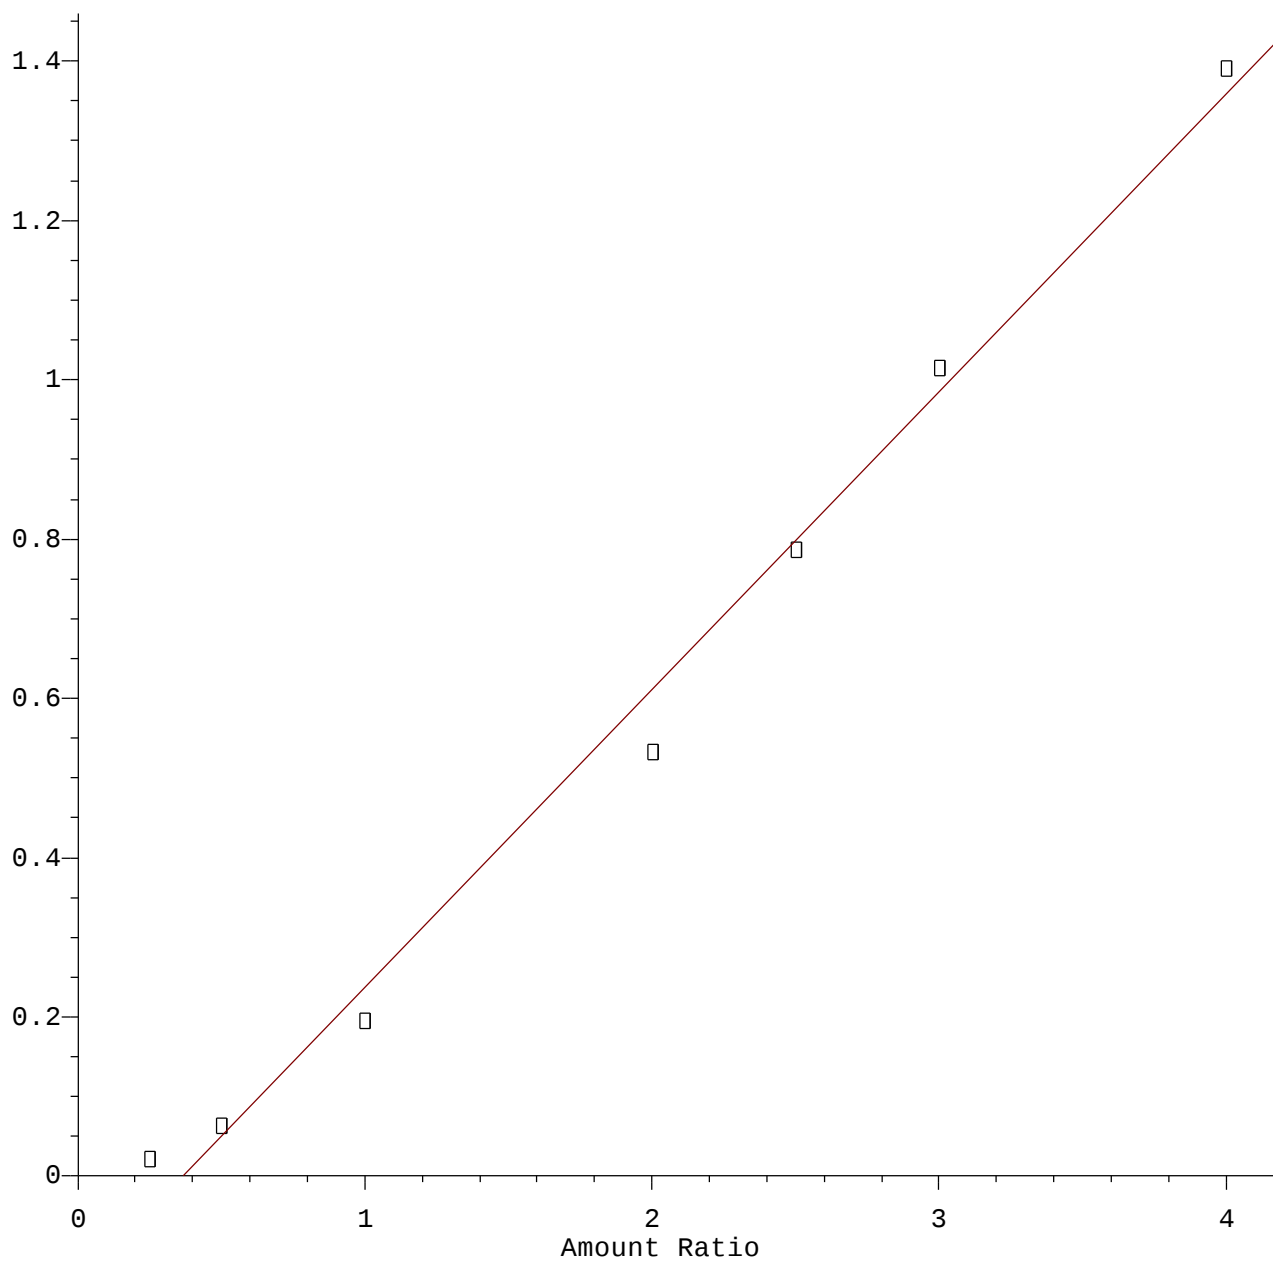


Resp Ratio = $3.74 \times 10^{-1} \times \text{Amt} - 1.36 \times 10^{-1}$
Coef of Det (r^2) = 0.991 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082720.M
Calibration Table Last Updated: Fri Aug 28 12:42:39 2020

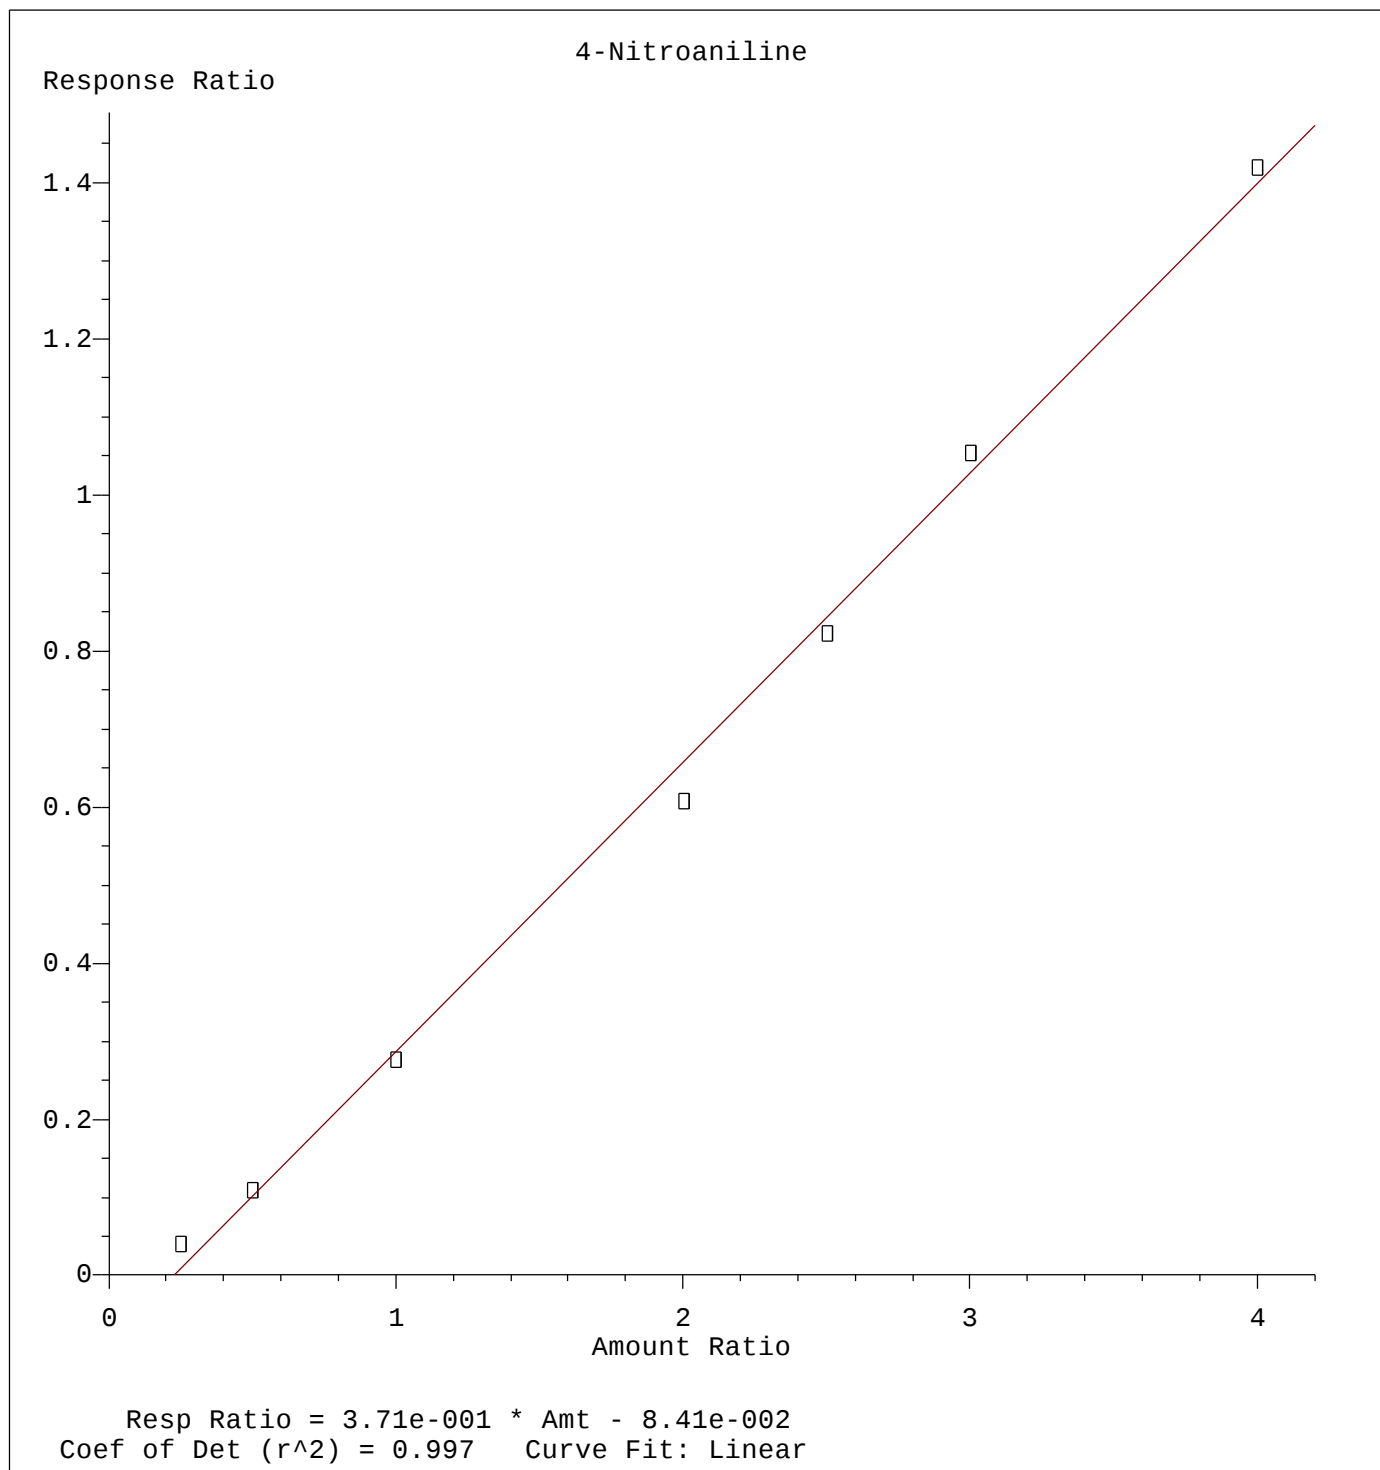

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082720.M
Calibration Table Last Updated: Fri Aug 28 12:42:39 2020

4,6-Dinitro-2-methylphenol

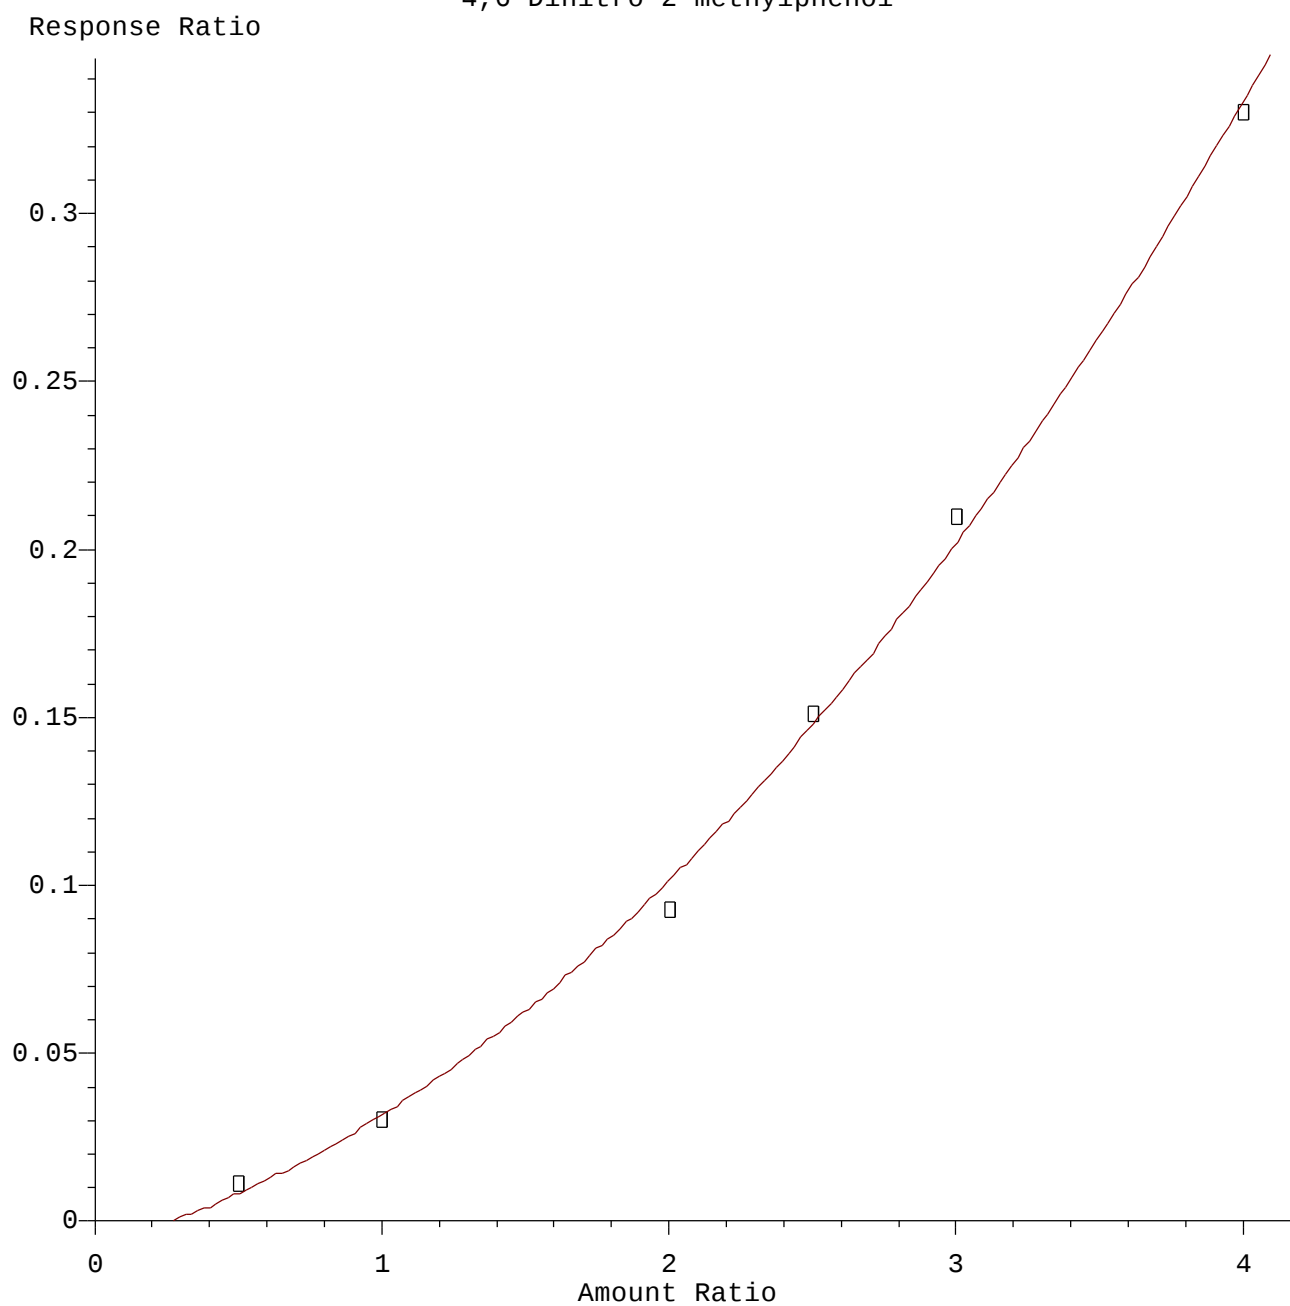

$R = 1.54e-002 A^2 + 2.37e-002 A - 7.48e-003$
Coef of Det (r^2) = 0.998 Curve Fit: Quadratic

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082720.M
Calibration Table Last Updated: Fri Aug 28 12:42:39 2020