


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082720\
 Data File : BF121441.D
 Acq On : 27 Aug 2020 17:33
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 28 09:25:49 2020

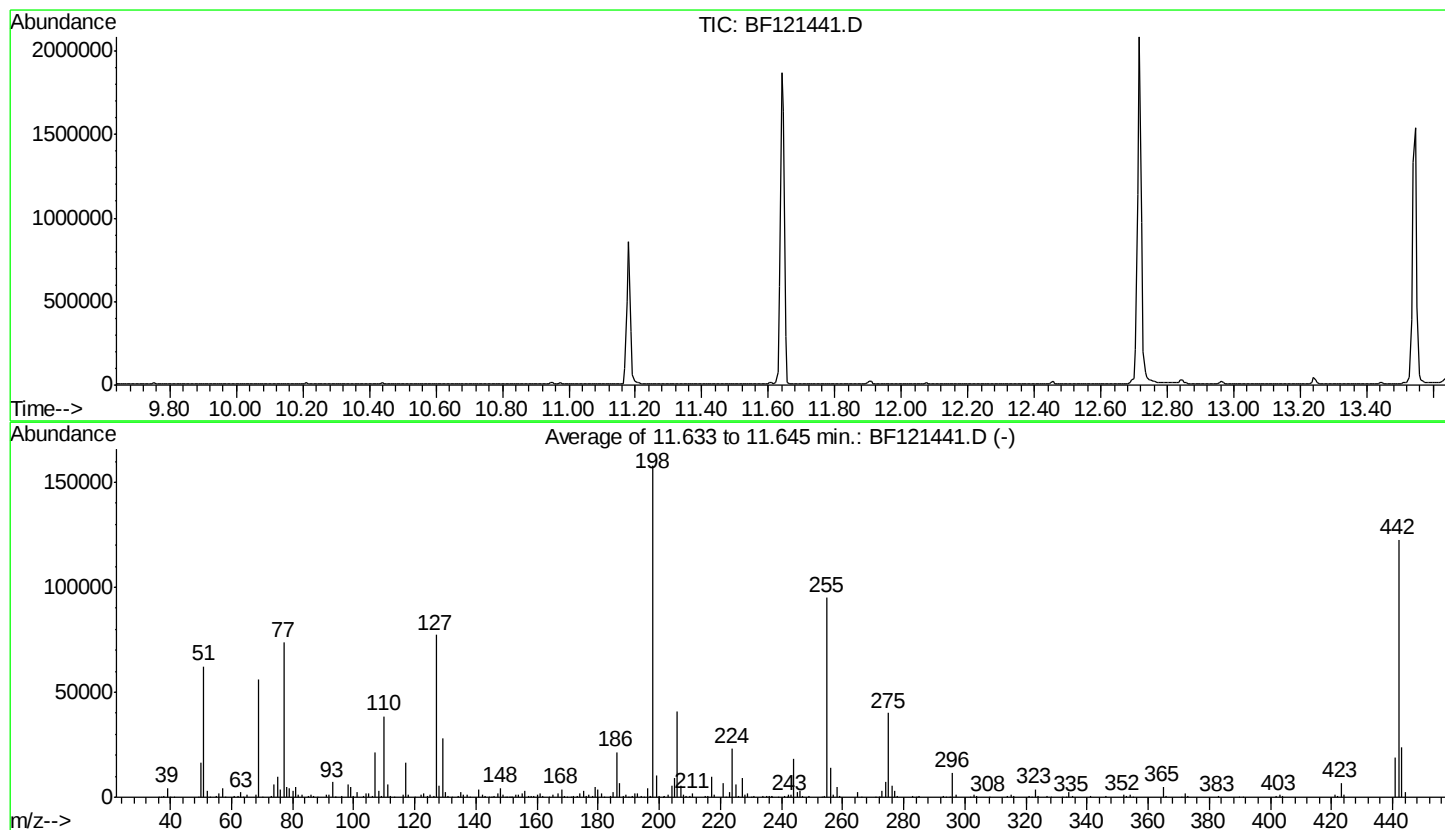

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.5	62398	PASS
68	69	0.00	2	1.9	1086	PASS
69	198	0.00	100	35.7	56400	PASS
70	69	0.00	2	0.3	190	PASS
127	198	10	80	49.0	77381	PASS
197	198	0.00	2	0.5	832	PASS
198	198	100	100	100.0	157984	PASS
199	198	5	9	6.7	10538	PASS
275	198	10	60	25.4	40162	PASS
365	198	1	100	3.2	5102	PASS
441	198	0.01	100	12.1	19087	PASS
442	198	50	100	77.7	122725	PASS
443	442	15	24	19.2	23536	PASS