
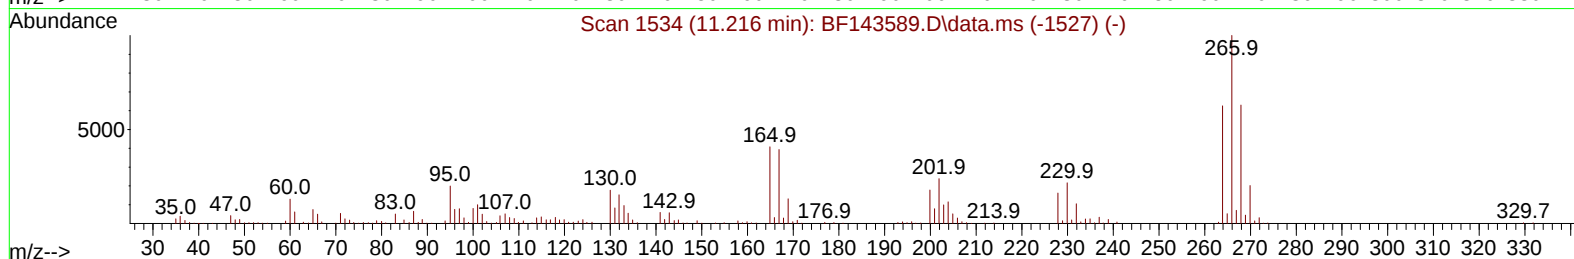
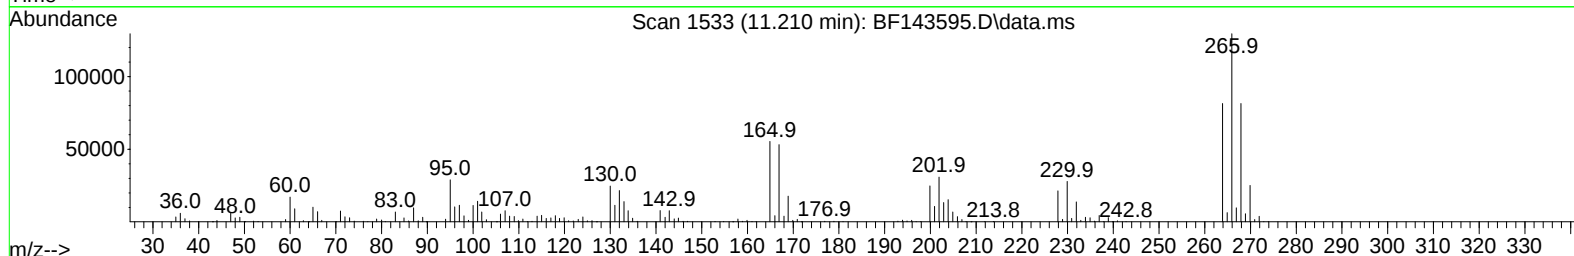


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082725\
Data File : BF143595.D
Acq On : 27 Aug 2025 08:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 27 11:27:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 26 16:30:52 2025
Response via : Initial Calibration

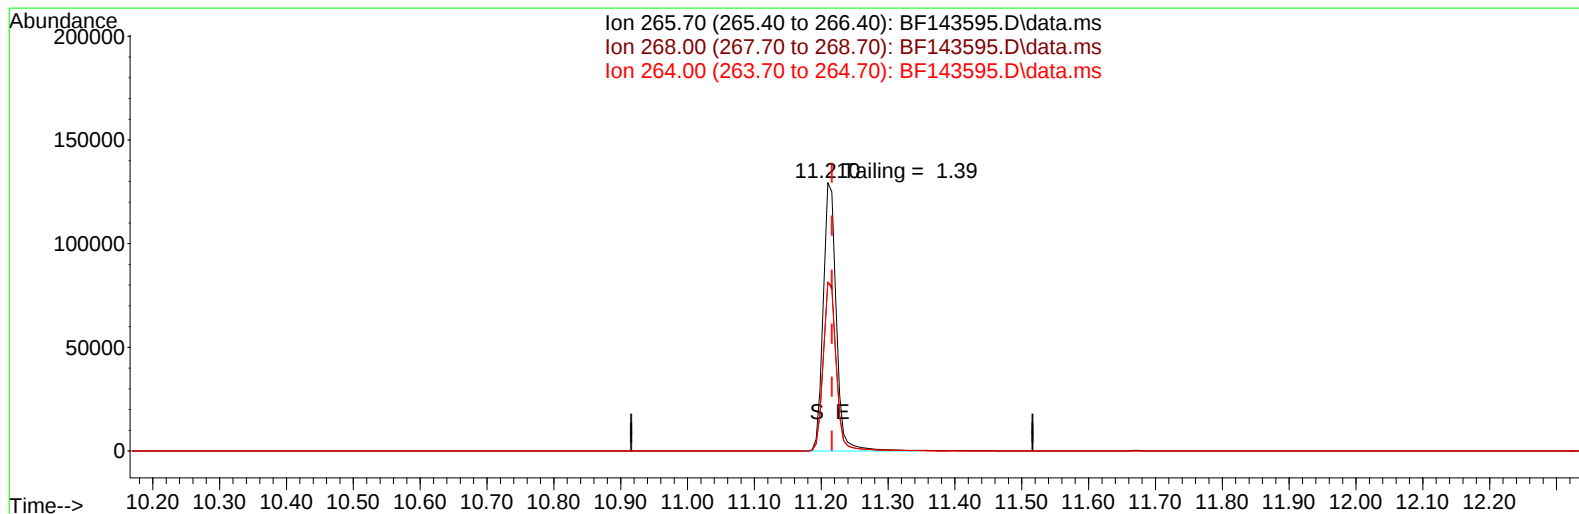

TIC: BF143595.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.006) 54326.76 ng

response 177044

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	62.96
264.00	62.60	62.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082725\
Data File : BF143595.D
Acq On : 27 Aug 2025 08:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 27 11:27:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 26 16:30:52 2025
Response via : Initial Calibration

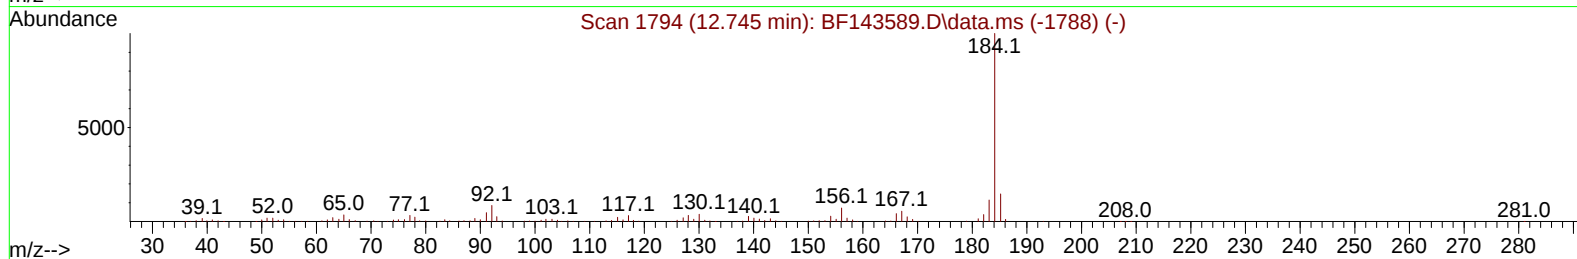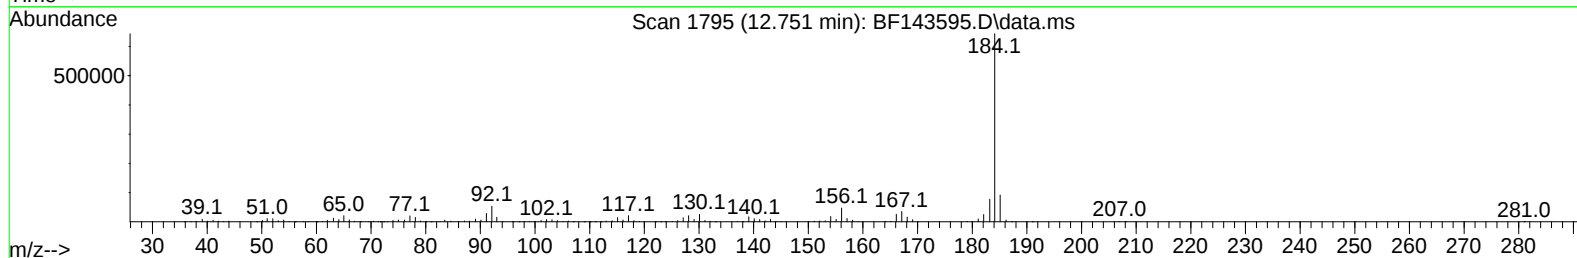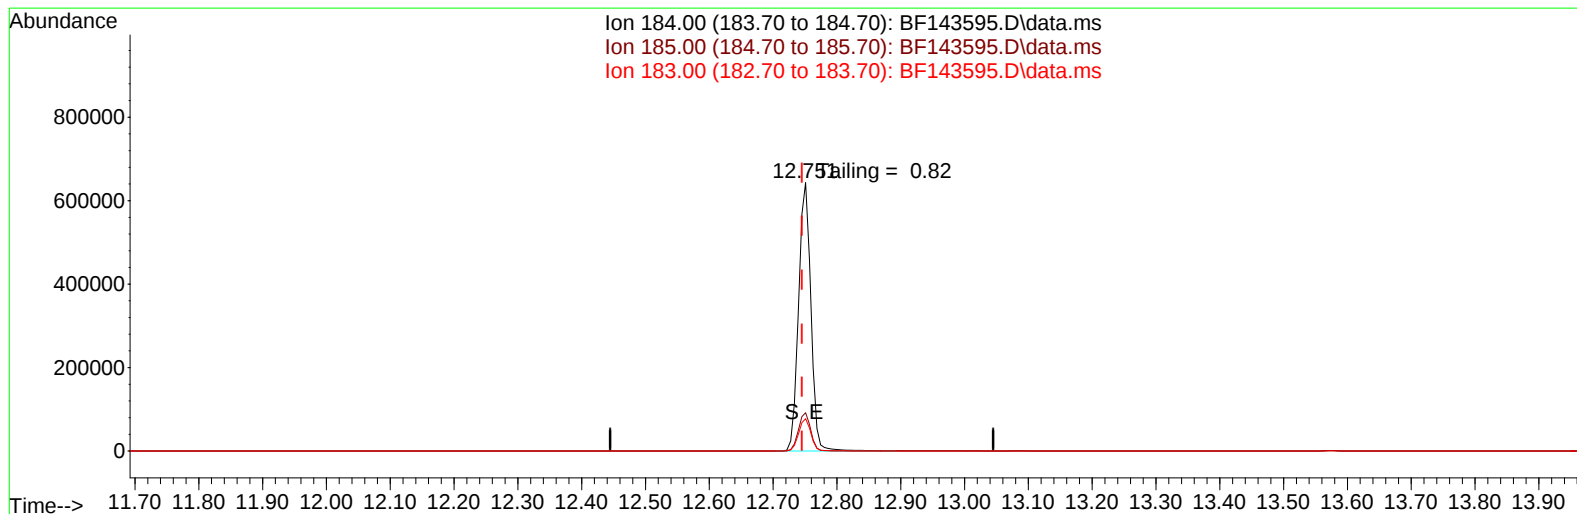

TIC: BF143595.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 57519.20 ng

response 866062

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.27
183.00	11.40	12.04
0.00	0.00	0.00