
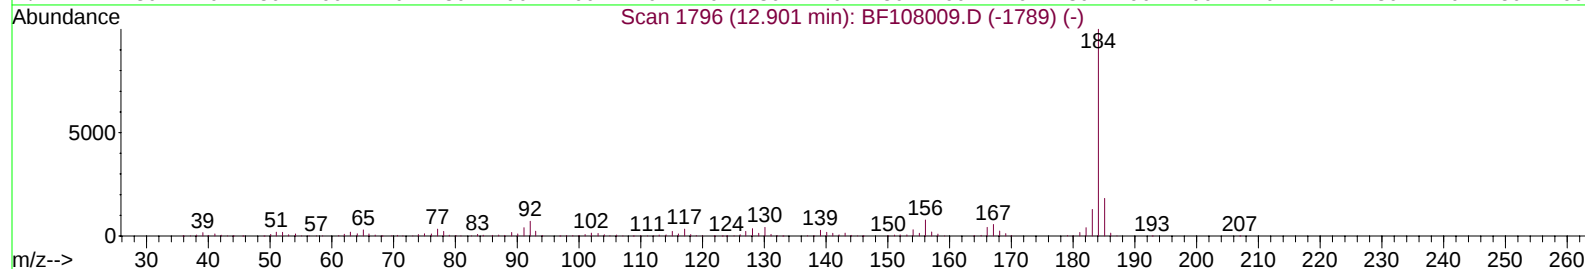
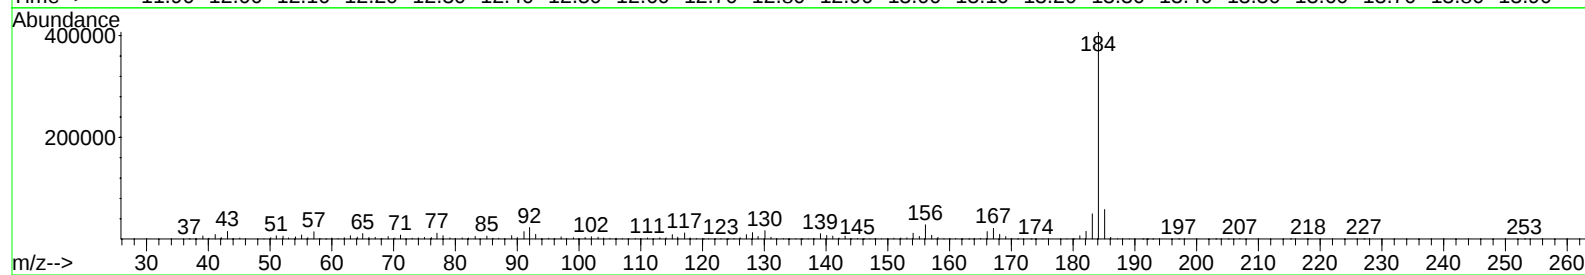


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF082818\
 Data File : BF108551.D
 Acq On : 28 Aug 2018 12:17
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 16:52:35 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 22 11:01:45 2018
 Response via : Initial Calibration

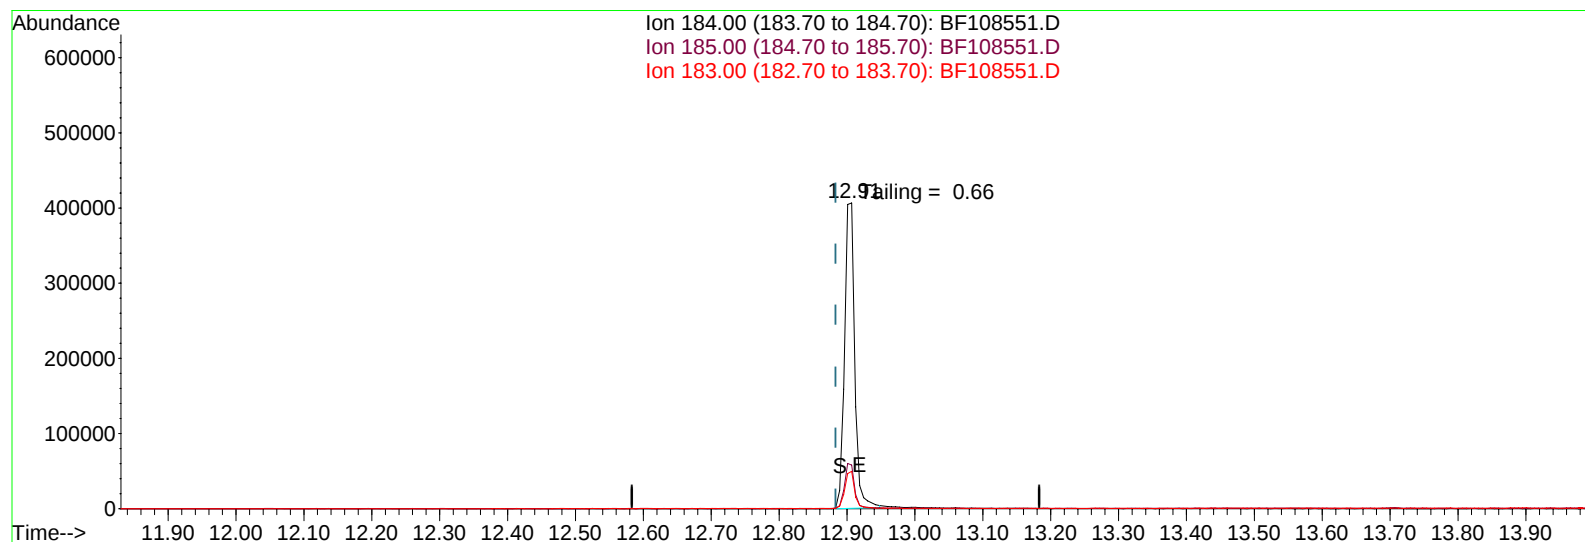

TIC: BF108551.D

(76) Benzidine

12.907min (+0.024) 100226.30ng

response 411917




Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.32
183.00	11.60	12.24
0.00	0.00	0.00

```

Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF082818\
Data File   : BF108551.D
Acq On      : 28 Aug 2018   12:17
Operator    : JU/SJ
Sample      : DFTPP
Misc        :
ALS Vial    : 1      Sample Multiplier: 1

```

Quant Time: Aug 28 16:52:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 22 11:01:45 2018
Response via : Initial Calibration

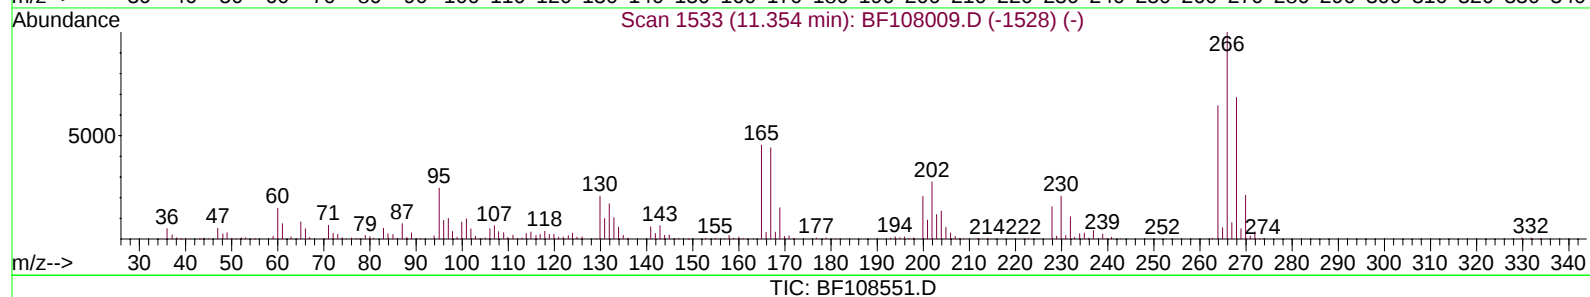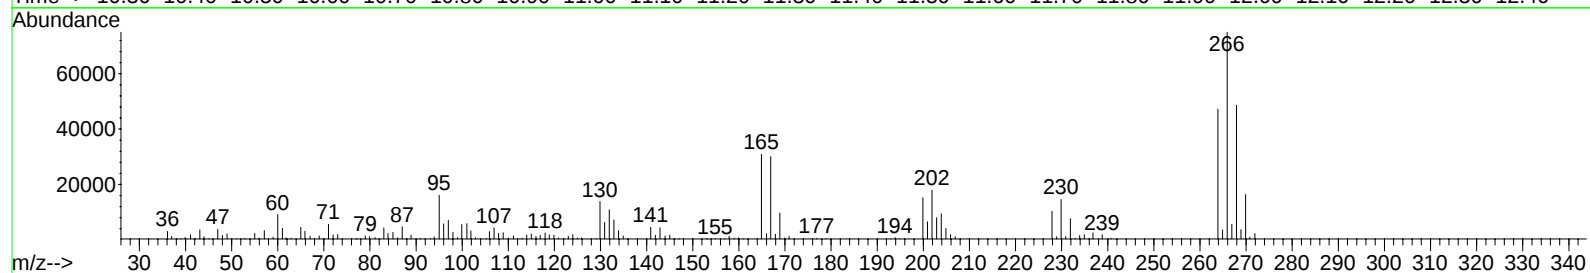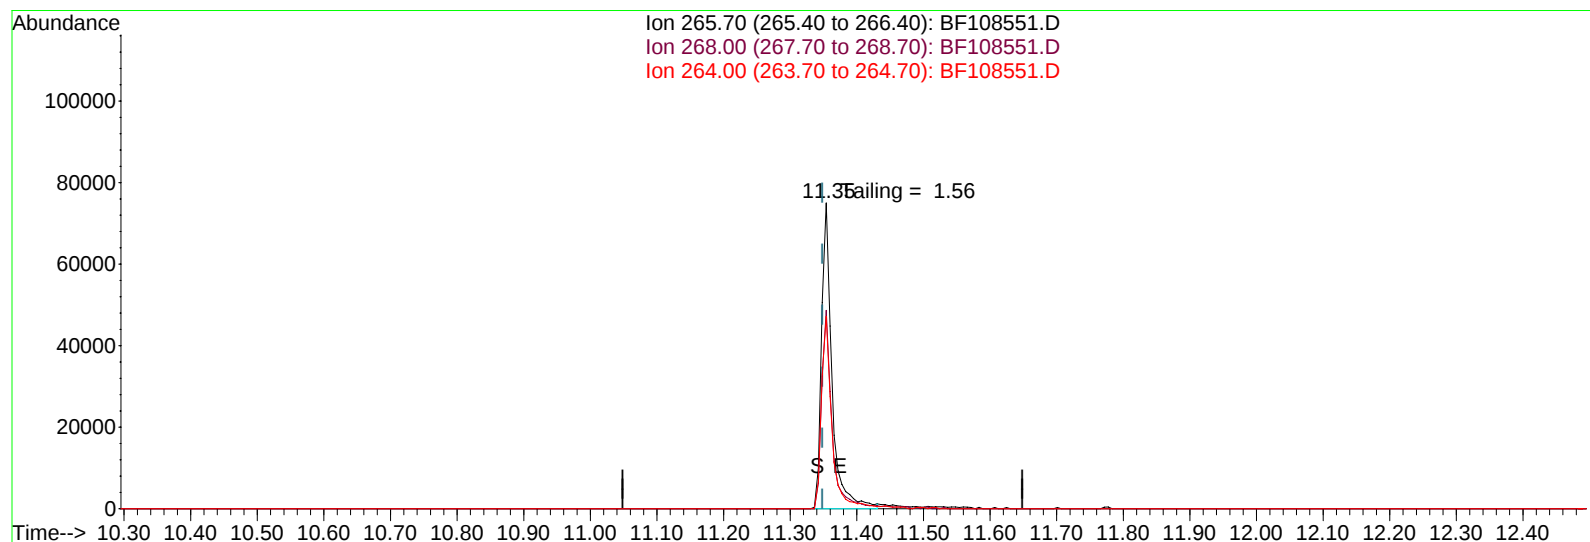

(69) Pentachlorophenol (C)

11.354min (+0.006) 51022.58ng

response 84889

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.87
264.00	61.90	62.92
0.00	0.00	0.00