
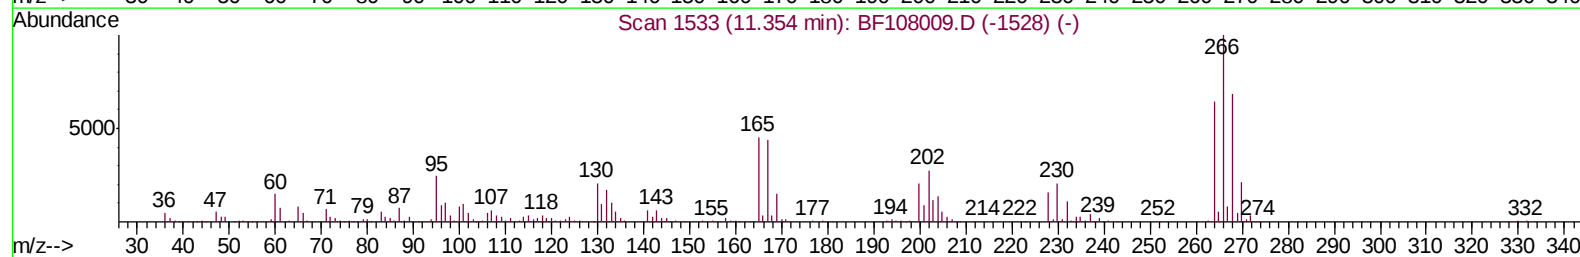
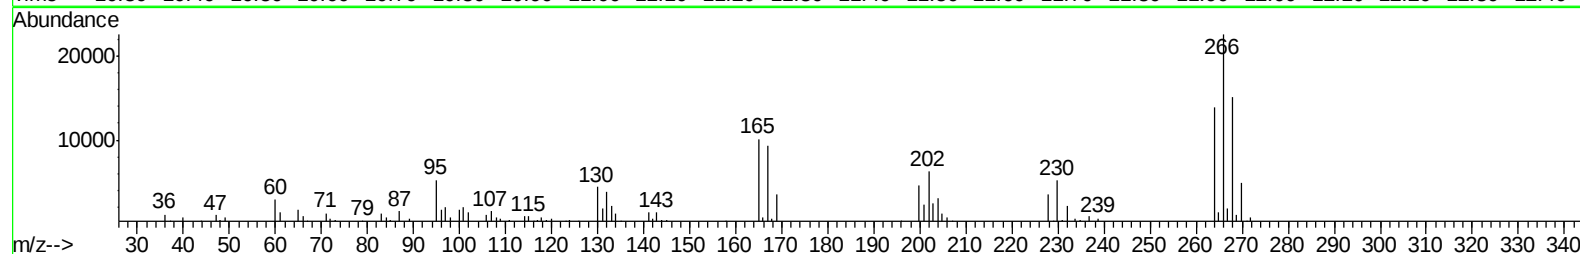


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082818\
Data File : BF108575.D
Acq On : 29 Aug 2018 00:39
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 09:03:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 22 11:01:45 2018
Response via : Initial Calibration

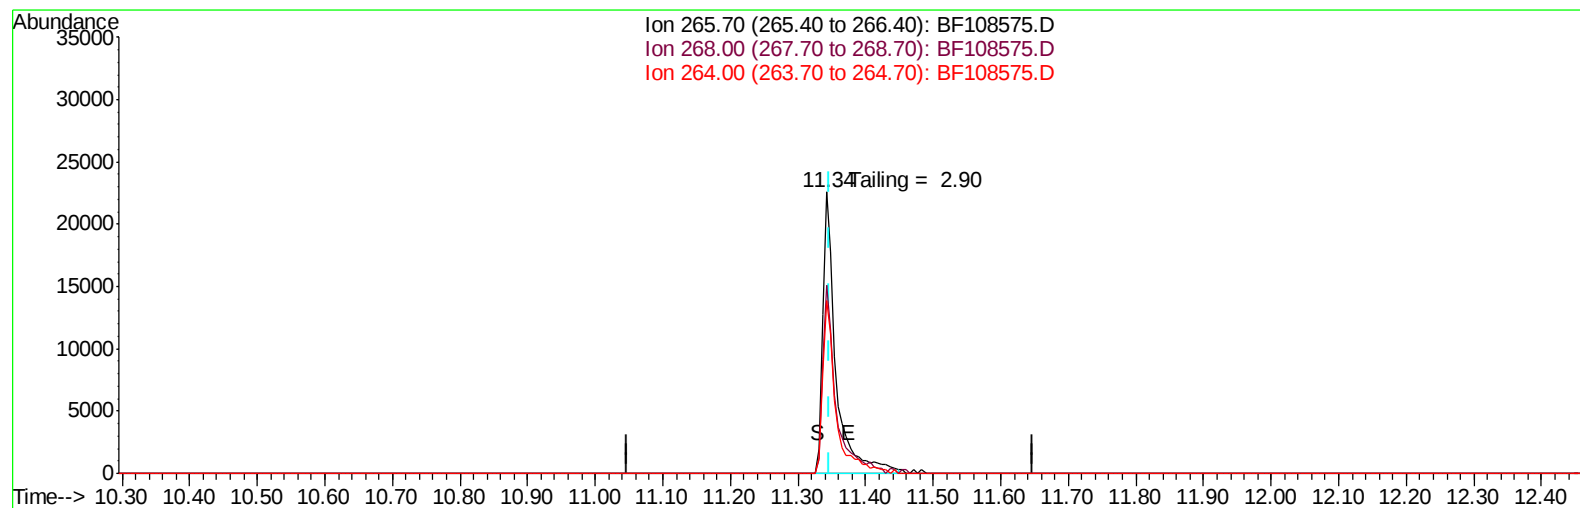

TIC: BF108575.D

(69) Pentachlorophenol (C)




11.342min (-0.006) 46070.13ng

response 31517

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.98
264.00	61.90	61.37
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082818\
Data File : BF108575.D
Acq On : 29 Aug 2018 00:39
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 09:03:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 22 11:01:45 2018
Response via : Initial Calibration

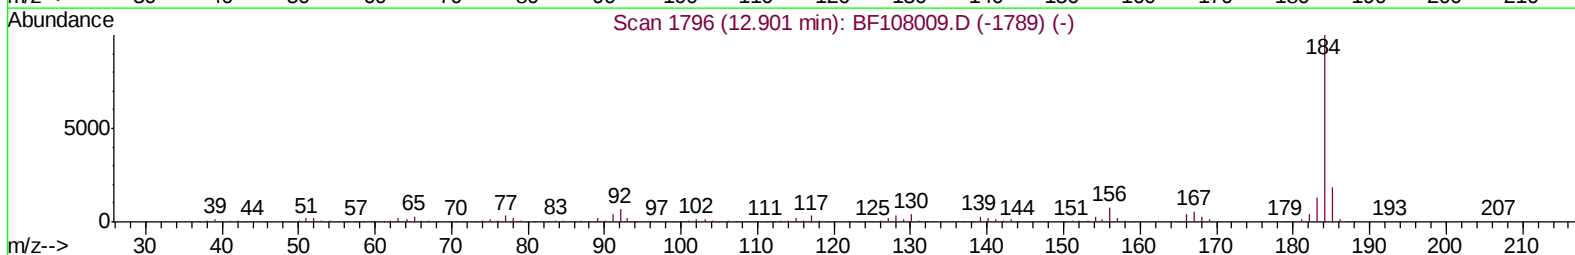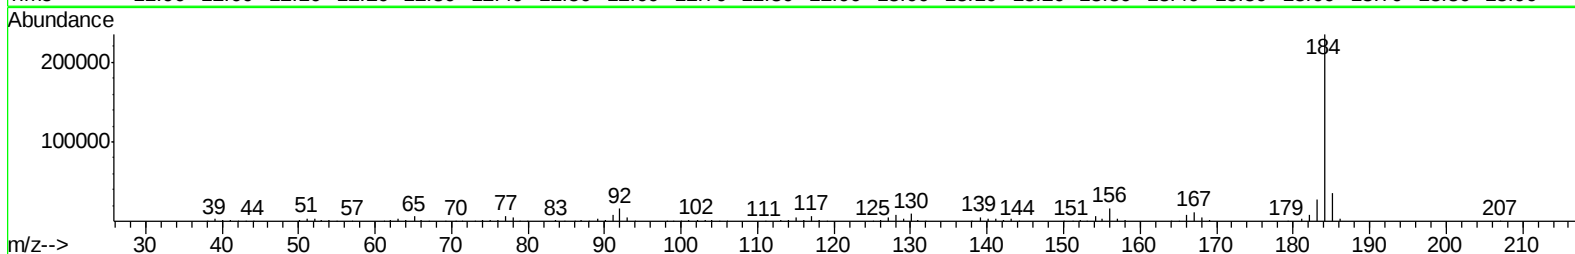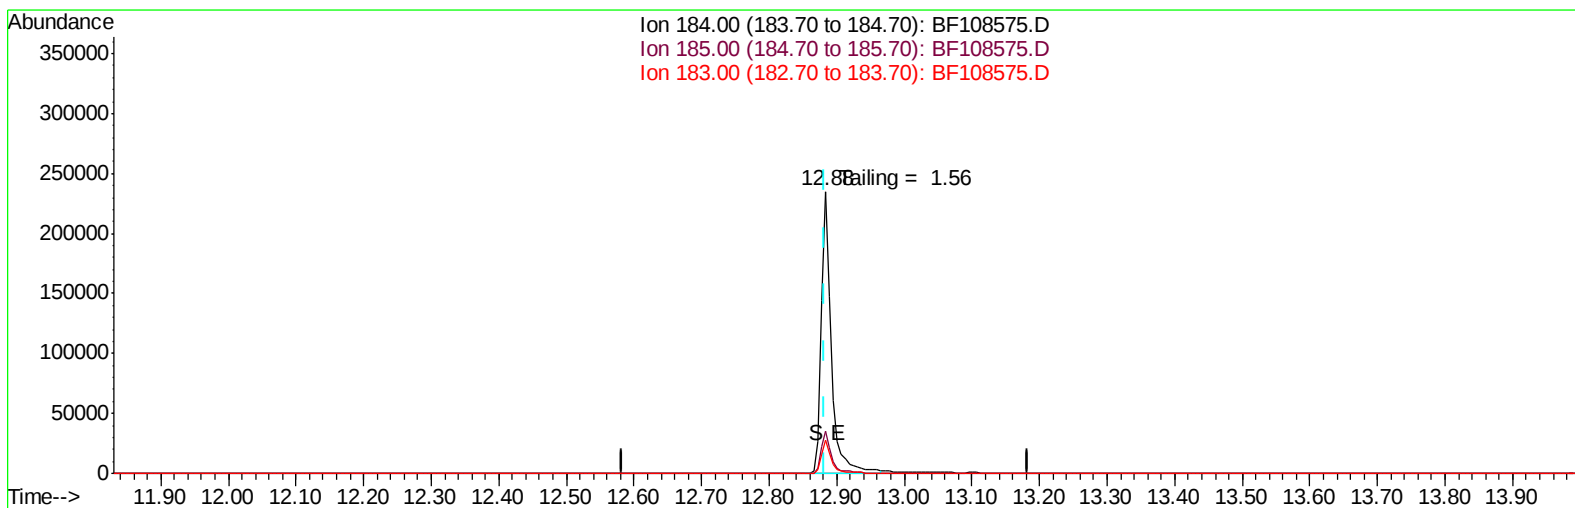

TIC: BF108575.D

(76) Benzidine

12.883min (-0.000) 0.00ng

response 252959

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.19
183.00	11.60	11.66
0.00	0.00	0.00