

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082818\
 Data File : BF108553.D
 Acq On : 28 Aug 2018 14:18
 Operator : JU/SJ
 Sample : J4538-01RE
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 VSS1RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.248	491	495	505	rBV	73374	108350	3.37%	0.257%
2	5.648	558	563	599	rBV	1419069	2685950	83.58%	6.373%
3	6.643	727	732	750	rBV	2158038	2781366	86.55%	6.599%
4	6.778	750	755	768	rVV	2543435	2762000	85.95%	6.553%
5	7.001	789	793	804	rBV	707416	699061	21.75%	1.659%
6	7.154	815	819	830	rBV	2248992	2148554	66.86%	5.098%
7	7.566	884	889	897	rBV	1671490	1783378	55.49%	4.231%
8	8.284	1007	1011	1022	rBV	951760	884078	27.51%	2.098%
9	9.354	1187	1193	1196	rBV	3601756	3213632	100.00%	7.625%
10	9.748	1256	1260	1265	rBV	218085	183115	5.70%	0.434%
11	10.042	1306	1310	1316	rVB2	1128392	997343	31.03%	2.366%
12	10.225	1337	1341	1345	rBV	30753	38577	1.20%	0.092%
13	10.842	1441	1446	1449	rBV	2214910	1966291	61.19%	4.665%
14	11.013	1472	1475	1479	rBV2	49829	60382	1.88%	0.143%
15	11.178	1500	1503	1508	rBV4	39982	50090	1.56%	0.119%
16	11.466	1548	1552	1556	rBV	126677	129664	4.03%	0.308%
17	11.542	1561	1565	1568	rVV	1182118	1040427	32.38%	2.469%
18	11.566	1568	1569	1572	rVB	78075	46509	1.45%	0.110%
19	11.907	1618	1627	1629	rBV5	26401	42759	1.33%	0.101%
20	11.977	1635	1639	1642	rBV2	33681	44686	1.39%	0.106%
21	12.013	1642	1645	1648	rVV	176330	191170	5.95%	0.454%
22	12.054	1648	1652	1663	rVB	629725	658875	20.50%	1.563%
23	12.219	1676	1680	1690	rVB3	51278	98417	3.06%	0.234%
24	12.783	1770	1776	1779	rVB4	41580	74038	2.30%	0.176%
25	12.836	1781	1785	1795	rVV	188566	210057	6.54%	0.498%
26	12.919	1797	1799	1804	rVB3	34440	41702	1.30%	0.099%
27	13.124	1830	1834	1838	rBV	2692061	2520923	78.44%	5.981%
28	13.324	1864	1868	1874	rBV2	66504	86202	2.68%	0.205%
29	13.554	1905	1907	1910	rBV	54527	50550	1.57%	0.120%
30	13.671	1924	1927	1930	rVB	75028	73527	2.29%	0.174%
31	13.795	1945	1948	1955	rVB4	46394	51785	1.61%	0.123%
32	14.007	1980	1984	1995	rBV	270562	381741	11.88%	0.906%
33	14.124	2002	2004	2010	rBV3	28079	41850	1.30%	0.099%
34	14.195	2012	2016	2020	rBV	863637	753267	23.44%	1.787%

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082818\
Data File : BF108553.D
Acq On : 28 Aug 2018 14:18
Operator : JU/SJ
Sample : J4538-01RE
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VSS1RE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	14.319	2033	2037	2046	rBV	137542	156749	4.88%	0.372%
36	14.554	2073	2077	2084	rBV	81869	156993	4.89%	0.372%
37	14.624	2086	2089	2092	rBV	347581	350192	10.90%	0.831%
38	14.954	2140	2145	2148	rBV	391995	453300	14.11%	1.076%
39	15.036	2156	2159	2162	rVB	59824	60875	1.89%	0.144%
40	15.089	2163	2168	2169	rVV	192990	273939	8.52%	0.650%
41	15.113	2169	2172	2178	rVB2	487658	534297	16.63%	1.268%
42	15.313	2202	2206	2210	rBV	756549	905799	28.19%	2.149%
43	15.354	2210	2213	2227	rVB	734269	1223530	38.07%	2.903%
44	15.695	2265	2271	2273	rBV	237351	429678	13.37%	1.019%
45	15.724	2273	2276	2278	rVV	397440	552539	17.19%	1.311%
46	15.754	2278	2281	2290	rVB	547346	735346	22.88%	1.745%
47	15.871	2298	2301	2307	rVB2	93356	126653	3.94%	0.301%
48	15.948	2310	2314	2321	rVB2	186625	301438	9.38%	0.715%
49	16.201	2351	2357	2364	rVB	1166058	1903084	59.22%	4.515%
50	16.277	2365	2370	2378	rBV2	188533	411516	12.81%	0.976%
51	16.395	2384	2390	2397	rVB3	199804	449287	13.98%	1.066%
52	16.577	2418	2421	2430	rVB5	83695	153569	4.78%	0.364%
53	16.748	2447	2450	2464	rVB2	135007	283708	8.83%	0.673%
54	17.083	2501	2507	2515	rVB2	171320	346657	10.79%	0.823%
55	17.354	2545	2553	2557	rBV6	223580	642339	19.99%	1.524%
56	17.536	2576	2584	2594	rBV2	396856	1176122	36.60%	2.791%
57	17.712	2609	2614	2624	rVB5	107788	275658	8.58%	0.654%
58	17.995	2654	2662	2679	rBV3	566782	1750957	54.49%	4.154%
59	18.230	2697	2702	2708	rVB2	128643	277482	8.63%	0.658%
60	18.548	2744	2756	2763	rBV6	363302	1314323	40.90%	3.118%


Sum of corrected areas: 42146346

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082818\
Data File : BF108553.D
Acq On : 28 Aug 2018 14:18
Operator : JU/SJ
Sample : J4538-01RE
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VSS1RE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

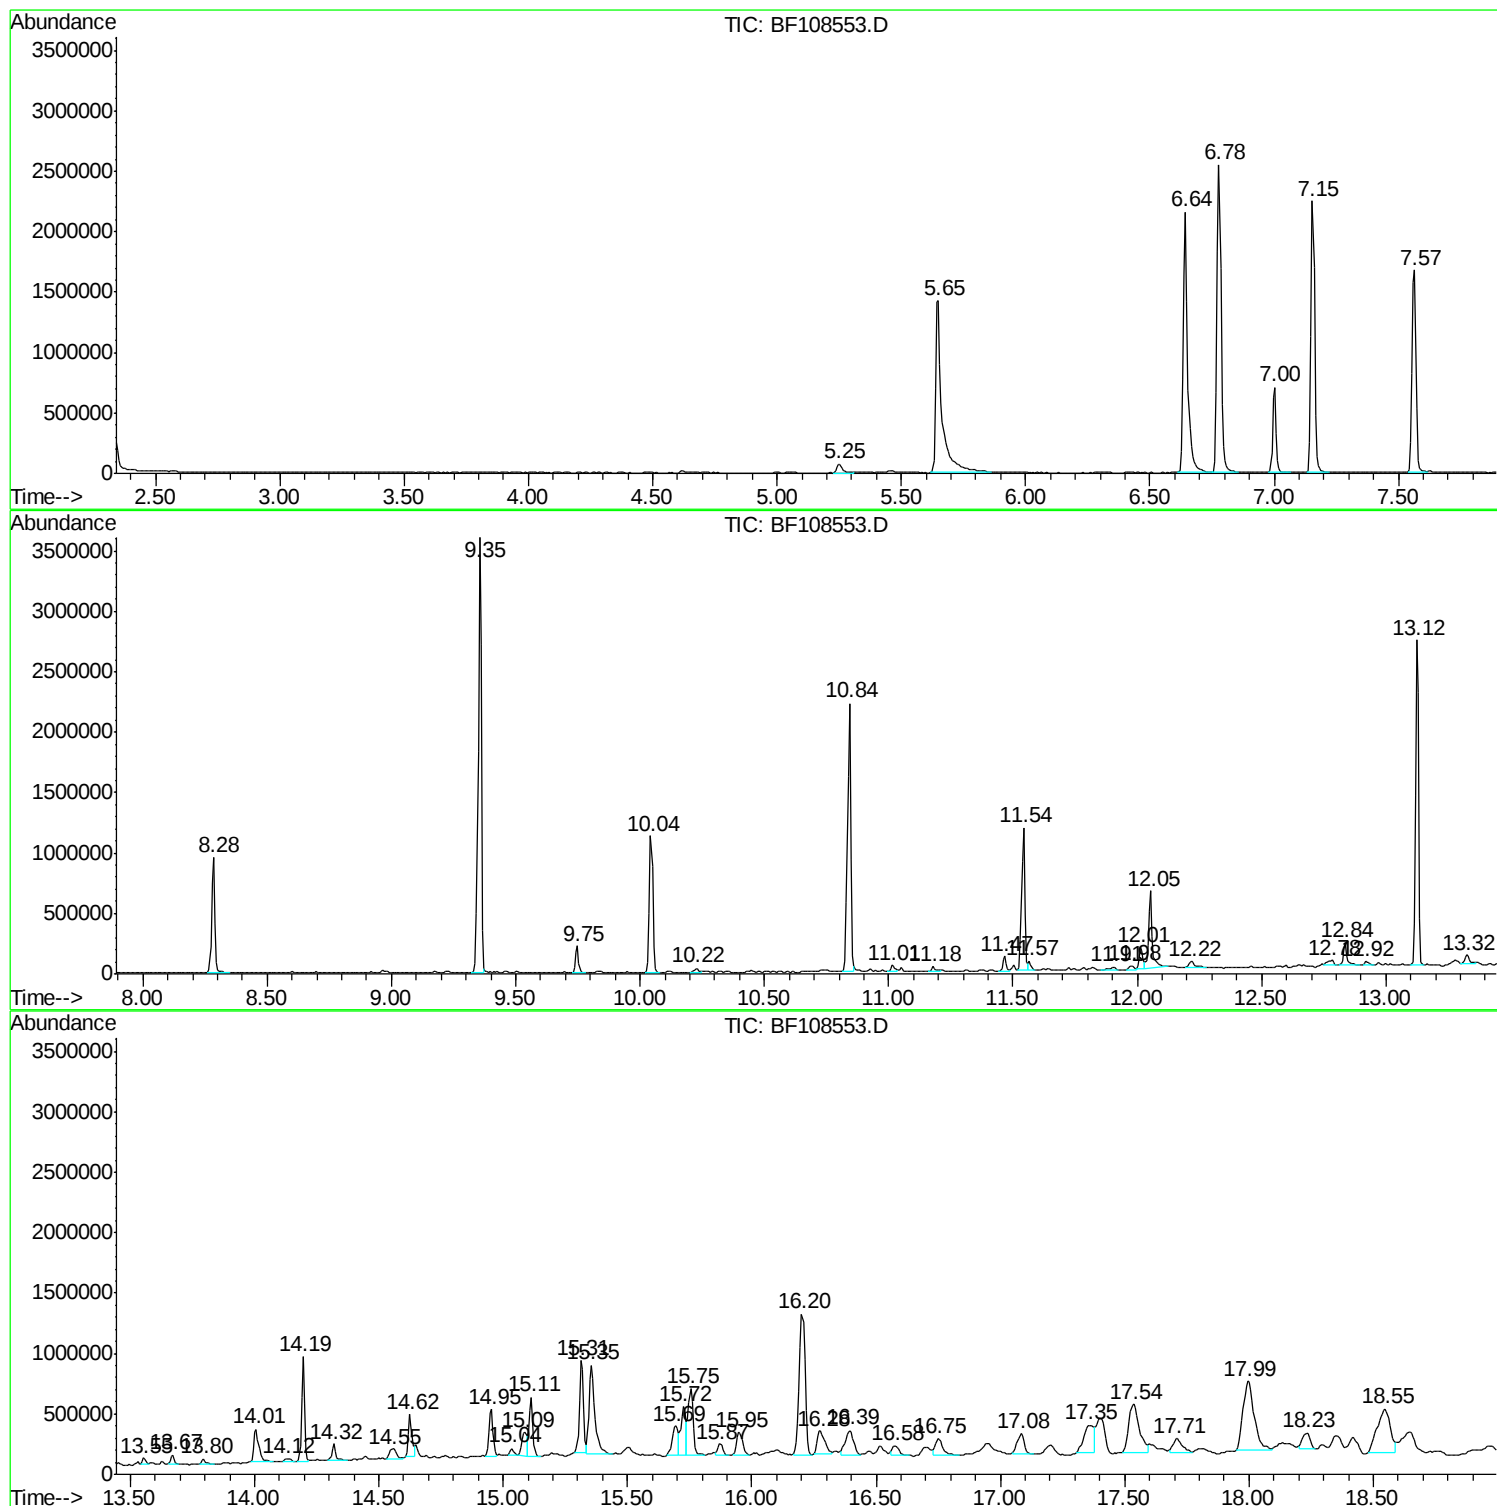

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082818\
Data_File : BF108553.D
Acq_On : 28_Aug_2018_ 14:188
Operator : JU/SJJ
Sample : J4538-01REE
Misc :
ALS_Vial : 3 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
VSS1RE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
