

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082818\
 Data File : BF108554.D
 Acq On : 28 Aug 2018 14:45
 Operator : JU/SJ
 Sample : J4538-02RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 VSS2RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.248	490	495	508	rBV	120767	175366	6.40%	0.693%
2	5.643	559	562	603	rBV	1198067	2248254	82.00%	8.883%
3	6.637	727	731	750	rBV	1726333	2379282	86.78%	9.400%
4	6.778	750	755	776	rVB	2236419	2392290	87.25%	9.452%
5	7.001	789	793	806	rVB	693389	689129	25.13%	2.723%
6	7.154	815	819	831	rBV	1942825	1881009	68.61%	7.432%
7	7.560	884	888	897	rBV	1457954	1543983	56.31%	6.100%
8	8.284	1007	1011	1019	rBV	911525	868904	31.69%	3.433%
9	9.354	1186	1193	1197	rBV	3116995	2741760	100.00%	10.833%
10	9.531	1219	1223	1226	rVB	101708	85600	3.12%	0.338%
11	9.748	1256	1260	1265	rBV	216944	177242	6.46%	0.700%
12	10.042	1297	1310	1314	rBV2	1134650	1041614	37.99%	4.115%
13	10.842	1441	1446	1458	rBV	1727530	1707019	62.26%	6.744%
14	11.542	1561	1565	1568	rBV	1130413	994520	36.27%	3.929%
15	12.042	1646	1650	1656	rBV	117018	121065	4.42%	0.478%
16	13.124	1830	1834	1837	rBV	2409912	2056298	75.00%	8.124%
17	13.671	1924	1927	1933	rVB	29130	31241	1.14%	0.123%
18	14.007	1981	1984	1989	rVB	134471	163490	5.96%	0.646%
19	14.195	2012	2016	2020	rBV	812917	706388	25.76%	2.791%
20	14.318	2034	2037	2040	rBV	49677	46334	1.69%	0.183%
21	14.624	2086	2089	2092	rBV	99981	100672	3.67%	0.398%
22	14.824	2121	2123	2127	rVB	51236	45162	1.65%	0.178%
23	14.954	2141	2145	2149	rVB	160090	176606	6.44%	0.698%
24	15.113	2169	2172	2180	rVB	127086	162589	5.93%	0.642%
25	15.312	2202	2206	2210	rBV	288463	346875	12.65%	1.370%
26	15.360	2210	2214	2225	rVB2	96297	202390	7.38%	0.800%
27	15.724	2271	2276	2278	rBV	247546	355525	12.97%	1.405%
28	15.754	2278	2281	2287	rVB	533333	692652	25.26%	2.737%
29	15.948	2311	2314	2320	rVB3	48221	69045	2.52%	0.273%
30	16.195	2351	2356	2363	rVB	318697	505568	18.44%	1.997%
31	16.748	2446	2450	2461	rVB	102305	208990	7.62%	0.826%
32	17.536	2579	2584	2594	rVB10	51951	133205	4.86%	0.526%
33	17.989	2655	2661	2678	rVB8	82291	260353	9.50%	1.029%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082818\
Data File : BF108554.D
Acq On : 28 Aug 2018 14:45
Operator : JU/SJ
Sample : J4538-02RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VSS2RE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION


Sum of corrected areas: 25310420

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082818\
Data File : BF108554.D
Acq On : 28 Aug 2018 14:45
Operator : JU/SJ
Sample : J4538-02RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VSS2RE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

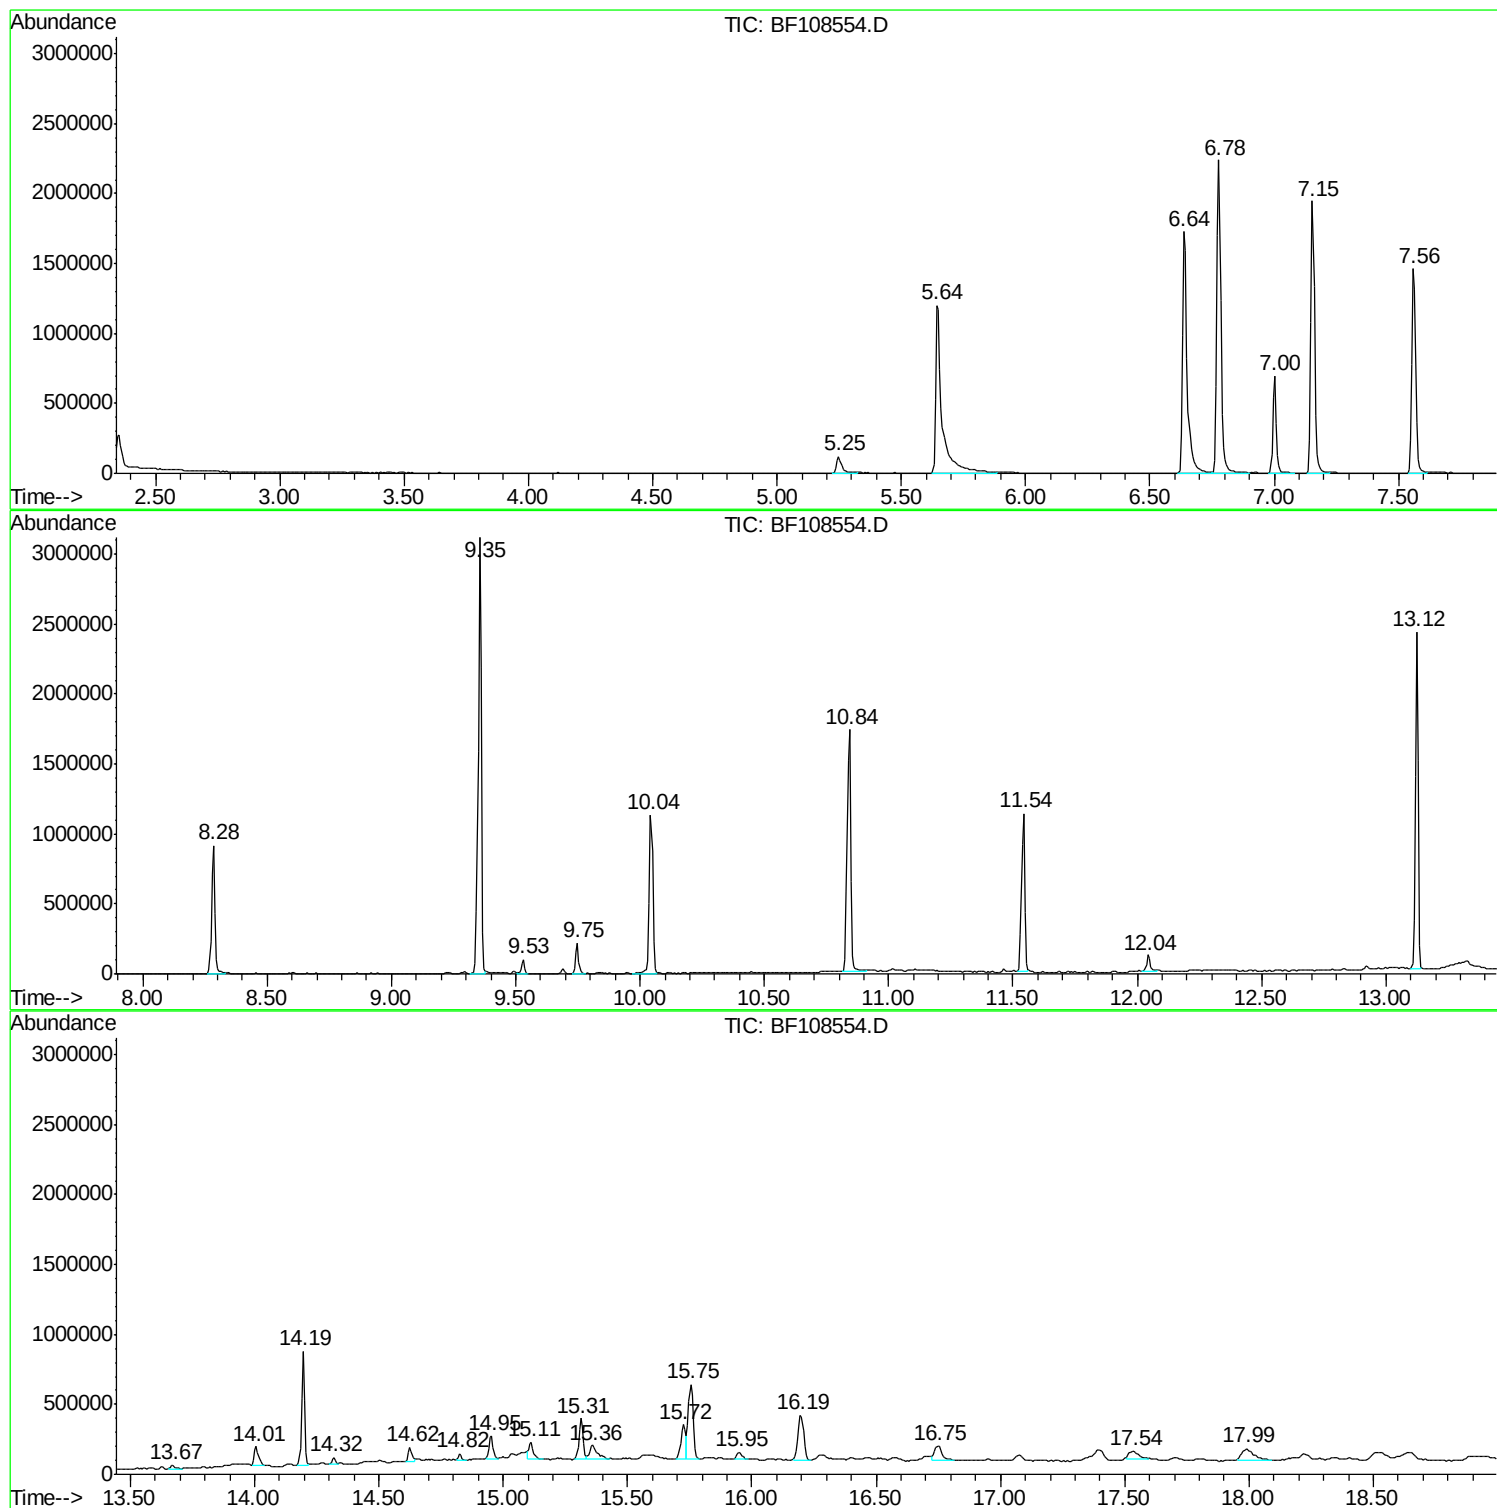

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082818\
Data_File : BF108554.D
Acq_On : 28_Aug_2018_ 14:455
Operator : JU/SJJ
Sample : J4538-02REE
Misc :
ALS_Vial : 4 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
VSS2RE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
